

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072324\
 Data File : PD084053.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2024 07:25
 Operator : AR\AJ
 Sample : P3280-09MS
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 YDZH7MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/23/2024
 Supervised By :Ankita Jodhani 07/23/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 07:38:42 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062624CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 27 04:33:52 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.562	2.771	17840600	103.0E6	17.572	19.013
27)	SA Decachlor...	9.115	7.894	36175306	120.2E6	16.978	17.996m
Target Compounds							
2)	A alpha-BHC	4.019	3.270	92180352	426.6E6	48.725	47.324
3)	MA gamma-BHC...	4.353	3.597	91040246	401.2E6	49.330	46.863m
4)	MA Heptachlor	4.945	3.936	93387655	378.5E6	46.587	44.952
5)	MB Aldrin	5.288	4.215	91888439	372.8E6	45.236	44.188
6)	B beta-BHC	4.550	3.895	36896377	162.1E6	43.927	42.747
7)	B delta-BHC	4.799	4.124	97394628	407.7E6	45.947	44.662
8)	B Heptachlo...	5.714	4.716	90105251	348.7E6	46.282m	44.397
9)	A Endosulfan I	6.102	5.085	88180276	322.3E6	47.610m	46.386
10)	B trans-Chl...	5.973	4.965	90358698	346.7E6	47.457	44.871
11)	B cis-Chlor...	6.051	5.028	93354995	356.8E6	47.693m	45.333
12)	B 4,4'-DDE	6.225	5.216	183.5E6	658.8E6	92.659	87.985
13)	MA Dieldrin	6.379	5.348	195.3E6	699.8E6	97.520	90.391
14)	MA Endrin	6.609	5.622	167.3E6	603.1E6	101.160m	91.072m
15)	B Endosulfa...	6.829	5.916	169.3E6	580.4E6	92.857	86.983m
16)	A 4,4'-DDD	6.743	5.770	140.8E6	535.3E6	97.594	89.857
17)	MA 4,4'-DDT	7.058	6.020	150.9E6	534.6E6	99.816	91.438m
18)	B Endrin al...	6.960	6.097	127.0E6	438.4E6	92.865	87.417
19)	B Endosulfa...	7.195	6.319	163.6E6	557.7E6	92.333	85.843
20)	A Methoxychlor	7.535	6.596	390.1E6	1116.3E6	438.435	377.806
21)	B Endrin ke...	7.682	6.825	183.5E6	619.6E6	93.969	88.203

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072324\
Data File : PD084053.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jul 2024 07:25
Operator : AR\AJ
Sample : P3280-09MS
Misc :
ALS Vial : 29 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 07:38:42 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062624CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 27 04:33:52 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

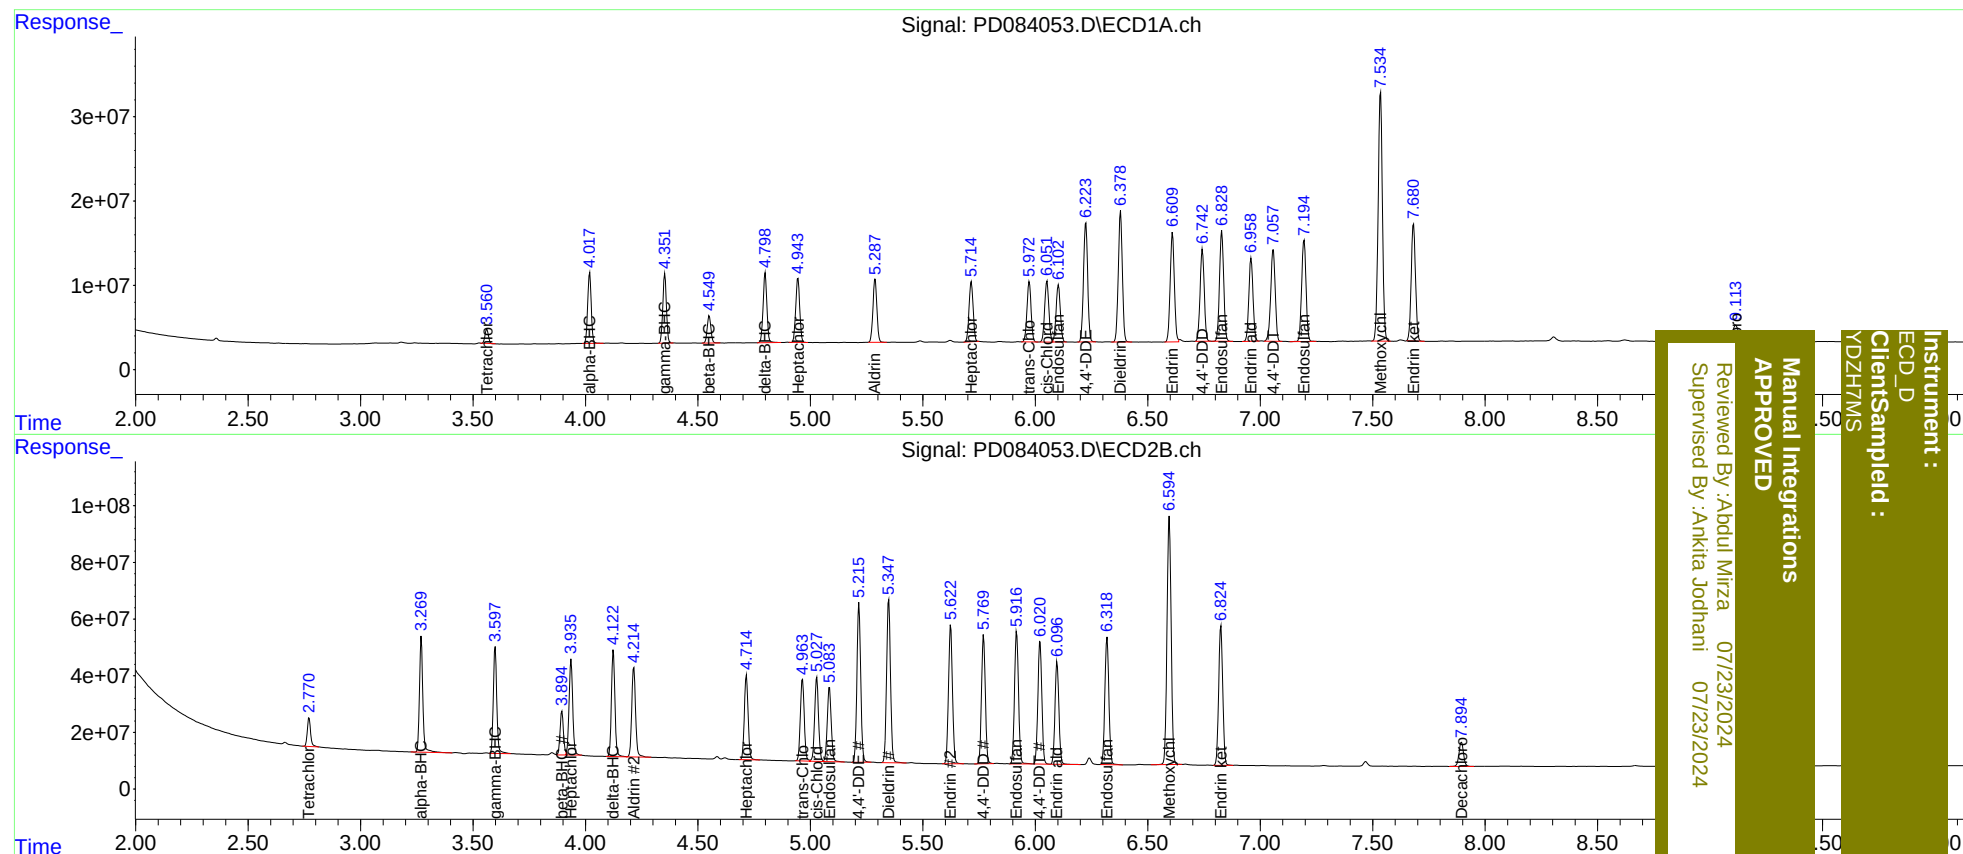

Instrument :
ECD_D
Client Sampled :
VDZHTMS

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 07/23/2024
Supervised By: Ankita Jodhani 07/23/2024