

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072324\
 Data File : PD084054.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2024 07:38
 Operator : AR\AJ
 Sample : P3280-10MSD
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 YDZH7MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/23/2024
 Supervised By :Ankita Jodhani 07/23/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 08:07:49 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062624CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 27 04:33:52 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.560	2.771	18735562	102.8E6	18.453m	18.964
27)	SA Decachlor...	9.114	7.893	35369641	119.0E6	16.600	17.809m
Target Compounds							
2)	A alpha-BHC	4.018	3.271	91154053	423.1E6	48.183	46.929
3)	MA gamma-BHC...	4.352	3.597	90077931	395.6E6	48.809	46.207m
4)	MA Heptachlor	4.944	3.936	92259370	374.0E6	46.024	44.418
5)	MB Aldrin	5.287	4.215	90473783	369.2E6	44.540	43.767
6)	B beta-BHC	4.550	3.896	36527940	159.4E6	43.488	42.039
7)	B delta-BHC	4.799	4.124	95208762	403.9E6	44.915	44.254
8)	B Heptachlo...	5.714	4.716	90567299	345.7E6	46.520m	44.018
9)	A Endosulfan I	6.101	5.086	86672497	318.9E6	46.796m	45.896
10)	B trans-Chl...	5.972	4.965	88829213	343.3E6	46.653	44.424
11)	B cis-Chlor...	6.050	5.029	91581503	353.9E6	46.787m	44.963
12)	B 4,4'-DDE	6.224	5.217	181.2E6	651.8E6	91.501	87.060
13)	MA Dieldrin	6.378	5.349	192.6E6	693.2E6	96.209	89.539
14)	MA Endrin	6.608	5.623	165.4E6	596.8E6	99.978m	90.117m
15)	B Endosulfa...	6.829	5.918	166.9E6	568.7E6	91.563	85.222
16)	A 4,4'-DDD	6.743	5.771	138.7E6	530.0E6	96.146	88.968
17)	MA 4,4'-DDT	7.058	6.021	148.9E6	528.4E6	98.436	90.389
18)	B Endrin al...	6.960	6.096	126.0E6	434.5E6	92.139	86.626m
19)	B Endosulfa...	7.195	6.318	160.8E6	553.6E6	90.742	85.214m
20)	A Methoxychlor	7.534	6.596	384.9E6	1108.7E6	432.655	375.231
21)	B Endrin ke...	7.681	6.825	181.4E6	615.3E6	92.914m	87.593

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072324\
Data File : PD084054.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jul 2024 07:38
Operator : AR\AJ
Sample : P3280-10MSD
Misc :
ALS Vial : 30 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 08:07:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062624CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 27 04:33:52 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

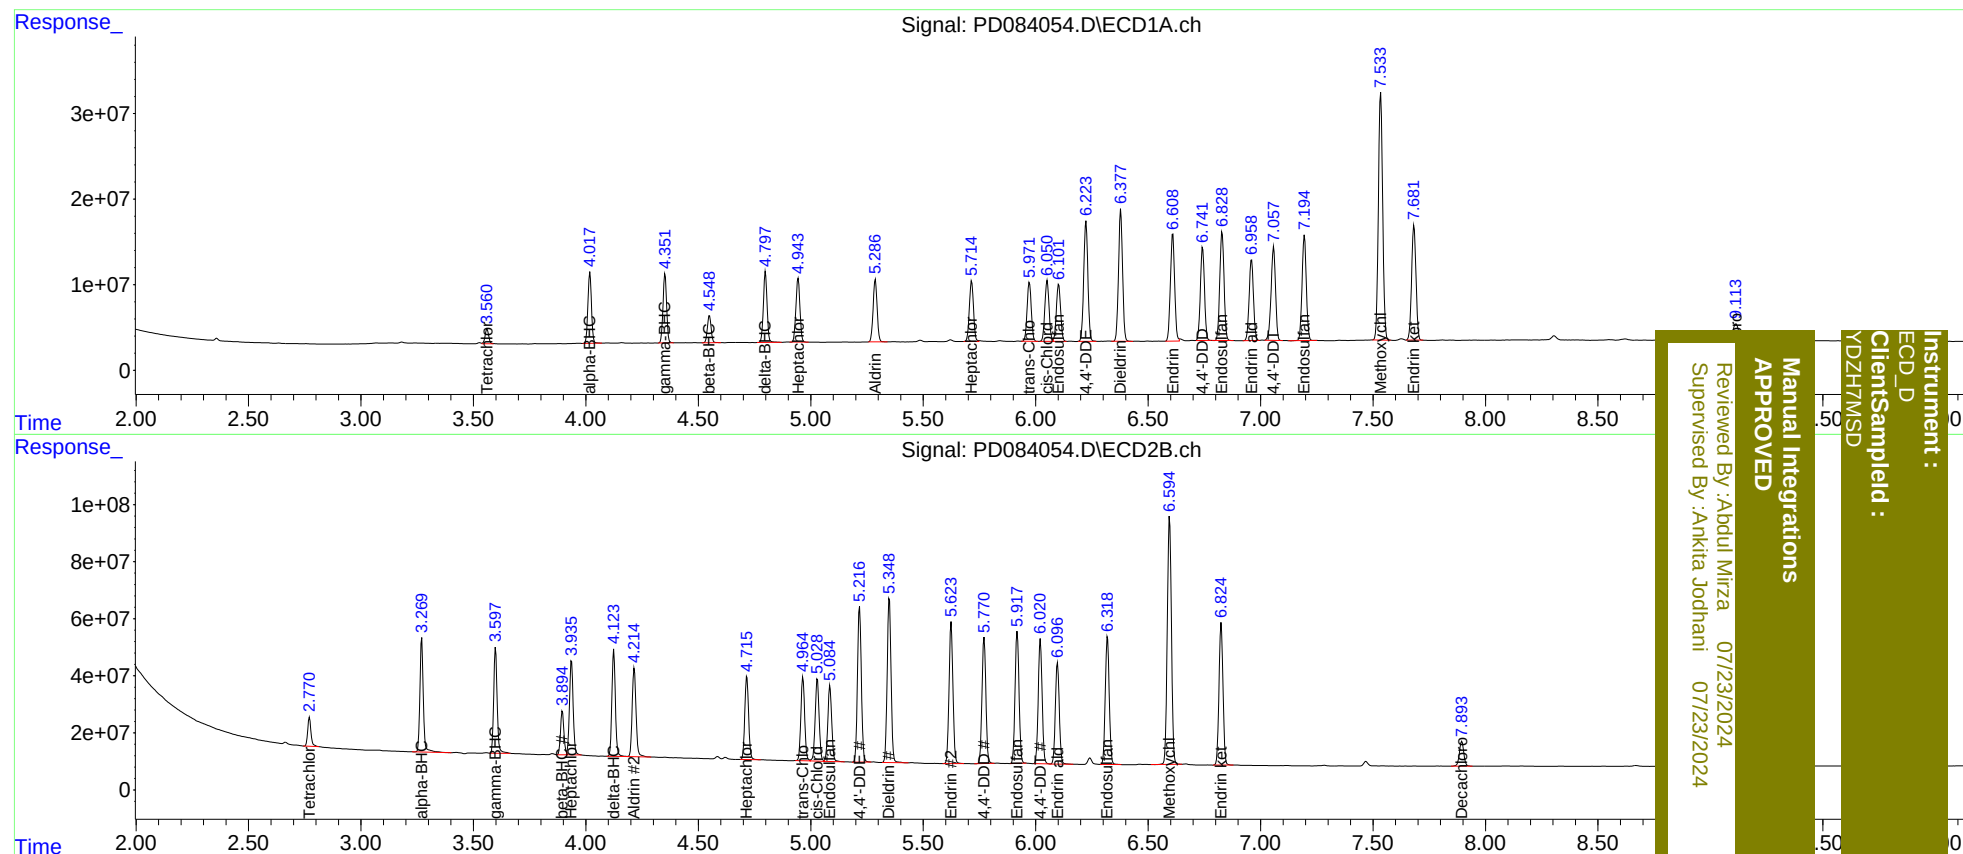

Instrument :
ECD_D
Client Sampled :
YDZHTMSD

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 07/23/2024
Supervised By: Ankita Jodhani 07/23/2024