

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072324\
 Data File : PD084037.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2024 03:53
 Operator : AR\AJ
 Sample : P3300-07MS
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E1G93MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/23/2024
 Supervised By :Ankita Jodhani 07/23/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 06:07:00 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062624CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 27 04:33:52 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.561	2.770	19873029	105.2E6	19.574	19.404m
27)	SA Decachlor...	9.115	7.895	25369554	77452666	11.907	11.593
Target Compounds							
2)	A alpha-BHC	4.019	3.269	102.3E6	462.5E6	54.085	51.305m
3)	MA gamma-BHC...	4.353	3.597	101.5E6	419.7E6	54.977	49.029m
4)	MA Heptachlor	4.945	3.936	103.5E6	385.2E6	51.611	45.750
5)	MB Aldrin	5.288	4.215	101.1E6	389.7E6	49.760	46.188
6)	B beta-BHC	4.549	3.894	40628812	186.6E6	48.370m	49.204m
7)	B delta-BHC	4.799	4.124	100.4E6	446.8E6	47.348	48.948
8)	B Heptachlo...	5.714	4.716	101.8E6	388.5E6	52.275m	49.459
9)	A Endosulfan I	6.102	5.084	97043339	349.5E6	52.395m	50.296m
10)	B trans-Chl...	5.973	4.965	98821000	371.8E6	51.901	48.112
11)	B cis-Chlor...	6.051	5.028	103.7E6	385.3E6	52.981m	48.948m
12)	B 4,4'-DDE	6.225	5.217	201.8E6	719.5E6	101.865	96.099
13)	MA Dieldrin	6.379	5.349	216.0E6	752.0E6	107.876	97.131
14)	MA Endrin	6.611	5.625	181.7E6	652.2E6	109.854	98.487
15)	B Endosulfa...	6.830	5.918	187.5E6	618.8E6	102.844	92.740
16)	A 4,4'-DDD	6.743	5.771	154.0E6	564.6E6	106.742	94.769
17)	MA 4,4'-DDT	7.059	6.022	169.0E6	580.0E6	111.789	99.206
18)	B Endrin al...	6.960	6.098	139.2E6	474.7E6	101.772	94.645
19)	B Endosulfa...	7.196	6.319	180.3E6	603.7E6	101.708	92.931m
20)	A Methoxychlor	7.535	6.596	433.1E6	1175.9E6	486.840	397.948
21)	B Endrin ke...	7.681	6.826	200.1E6	677.6E6	102.484m	96.464

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072324\
Data File : PD084037.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jul 2024 03:53
Operator : AR\AJ
Sample : P3300-07MS
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 06:07:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062624CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 27 04:33:52 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

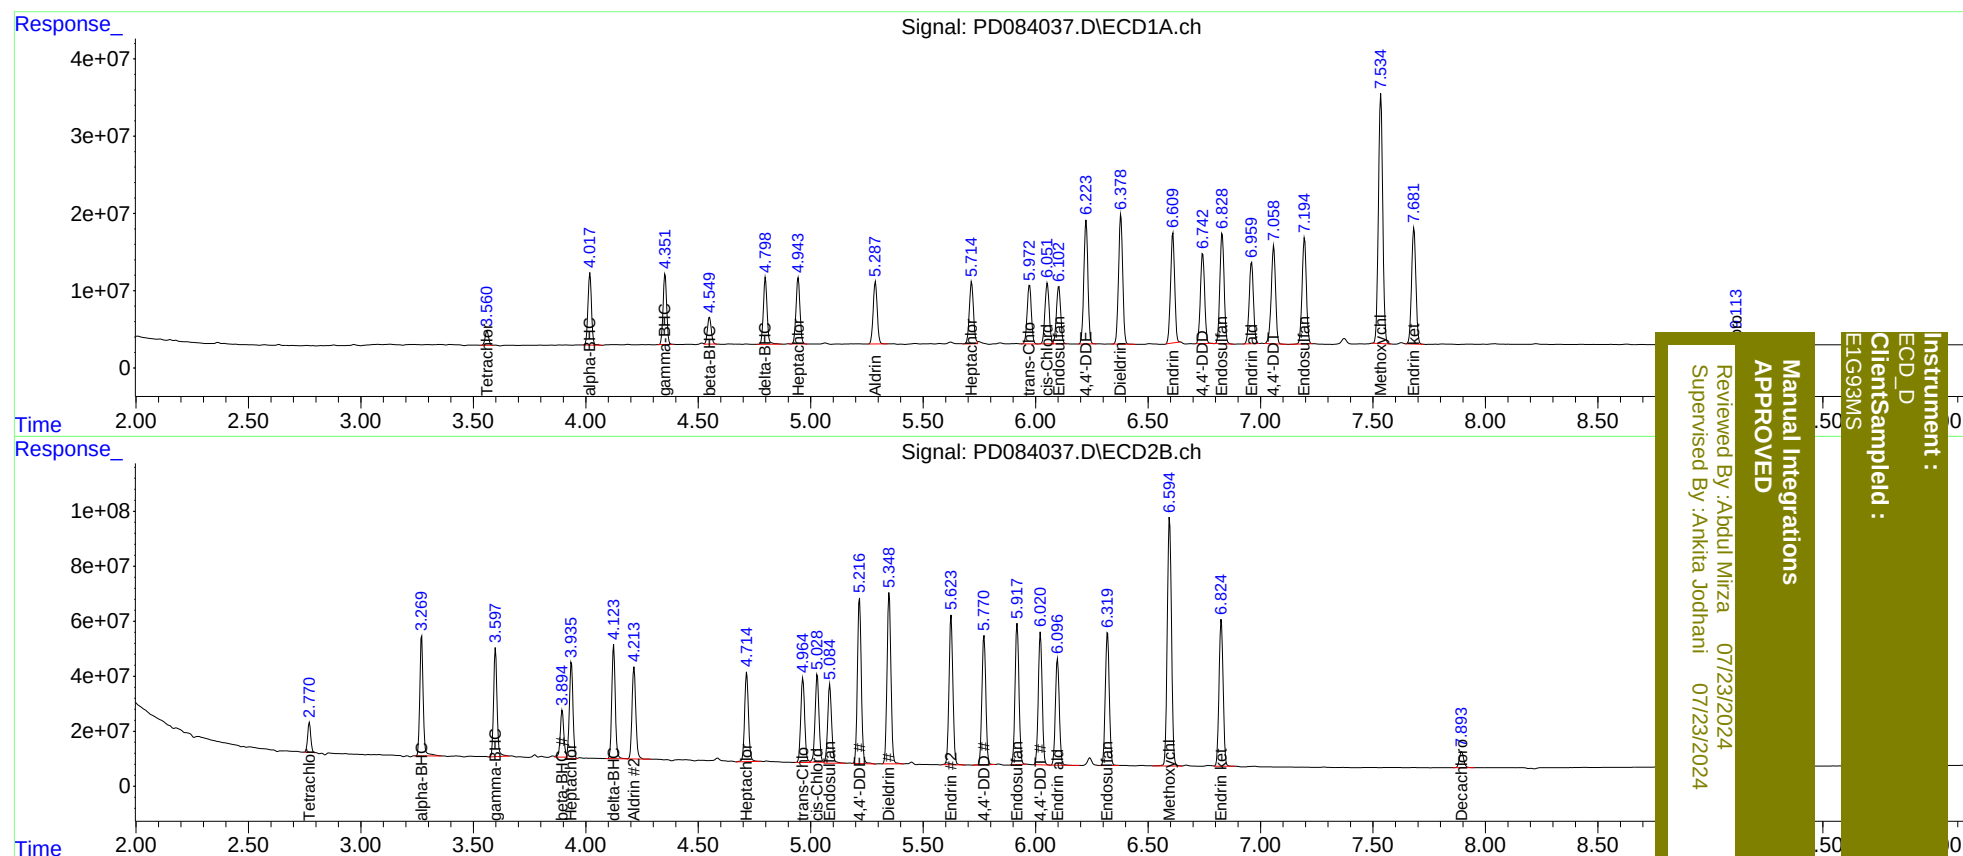

Instrument :
ECD_D
ClientSampled :
E1G93MS

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/23/2024
Supervised By :Ankita Jodhani 07/23/2024