

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072324\
 Data File : PD084038.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2024 04:06
 Operator : AR\AJ
 Sample : P3300-08MSD
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E1G93MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/23/2024
 Supervised By : Ankita Jodhani 07/23/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 06:07:54 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062624CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 27 04:33:52 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.561	2.771	19797363	103.0E6	19.499	18.996
27)	SA Decachlor...	9.116	7.895	25733129	77533776	12.077	11.605
Target Compounds							
2)	A alpha-BHC	4.019	3.271	101.2E6	479.4E6	53.504	53.181
3)	MA gamma-BHC...	4.353	3.597	99570126	412.8E6	53.952	48.226m
4)	MA Heptachlor	4.944	3.937	102.0E6	381.9E6	50.869	45.351
5)	MB Aldrin	5.288	4.215	99602355	384.7E6	49.034	45.596
6)	B beta-BHC	4.549	3.894	41229316	169.0E6	49.085m	44.586m
7)	B delta-BHC	4.799	4.124	100.1E6	438.6E6	47.216	48.056
8)	B Heptachlo...	5.715	4.716	100.4E6	381.9E6	51.592m	48.627
9)	A Endosulfan I	6.102	5.086	96386334	339.6E6	52.040m	48.872
10)	B trans-Chl...	5.973	4.966	97781350	365.4E6	51.355	47.284
11)	B cis-Chlor...	6.050	5.029	102.3E6	384.7E6	52.258m	48.879
12)	B 4,4'-DDE	6.224	5.217	198.8E6	705.9E6	100.340	94.282
13)	MA Dieldrin	6.380	5.349	212.3E6	740.1E6	106.024	95.593
14)	MA Endrin	6.609	5.623	184.6E6	646.6E6	111.631m	97.634m
15)	B Endosulfa...	6.830	5.918	184.8E6	608.8E6	101.366	91.231
16)	A 4,4'-DDD	6.743	5.771	151.7E6	556.5E6	105.115	93.406
17)	MA 4,4'-DDT	7.059	6.021	166.4E6	570.3E6	110.034	97.549
18)	B Endrin al...	6.961	6.097	136.7E6	465.8E6	99.935	92.873
19)	B Endosulfa...	7.195	6.319	176.8E6	591.6E6	99.763m	91.057m
20)	A Methoxychlor	7.536	6.596	426.9E6	1154.9E6	479.799	390.867
21)	B Endrin ke...	7.682	6.824	196.5E6	665.4E6	100.658m	94.722m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072324\
Data File : PD084038.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jul 2024 04:06
Operator : AR\AJ
Sample : P3300-08MSD
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 06:07:54 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062624CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 27 04:33:52 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

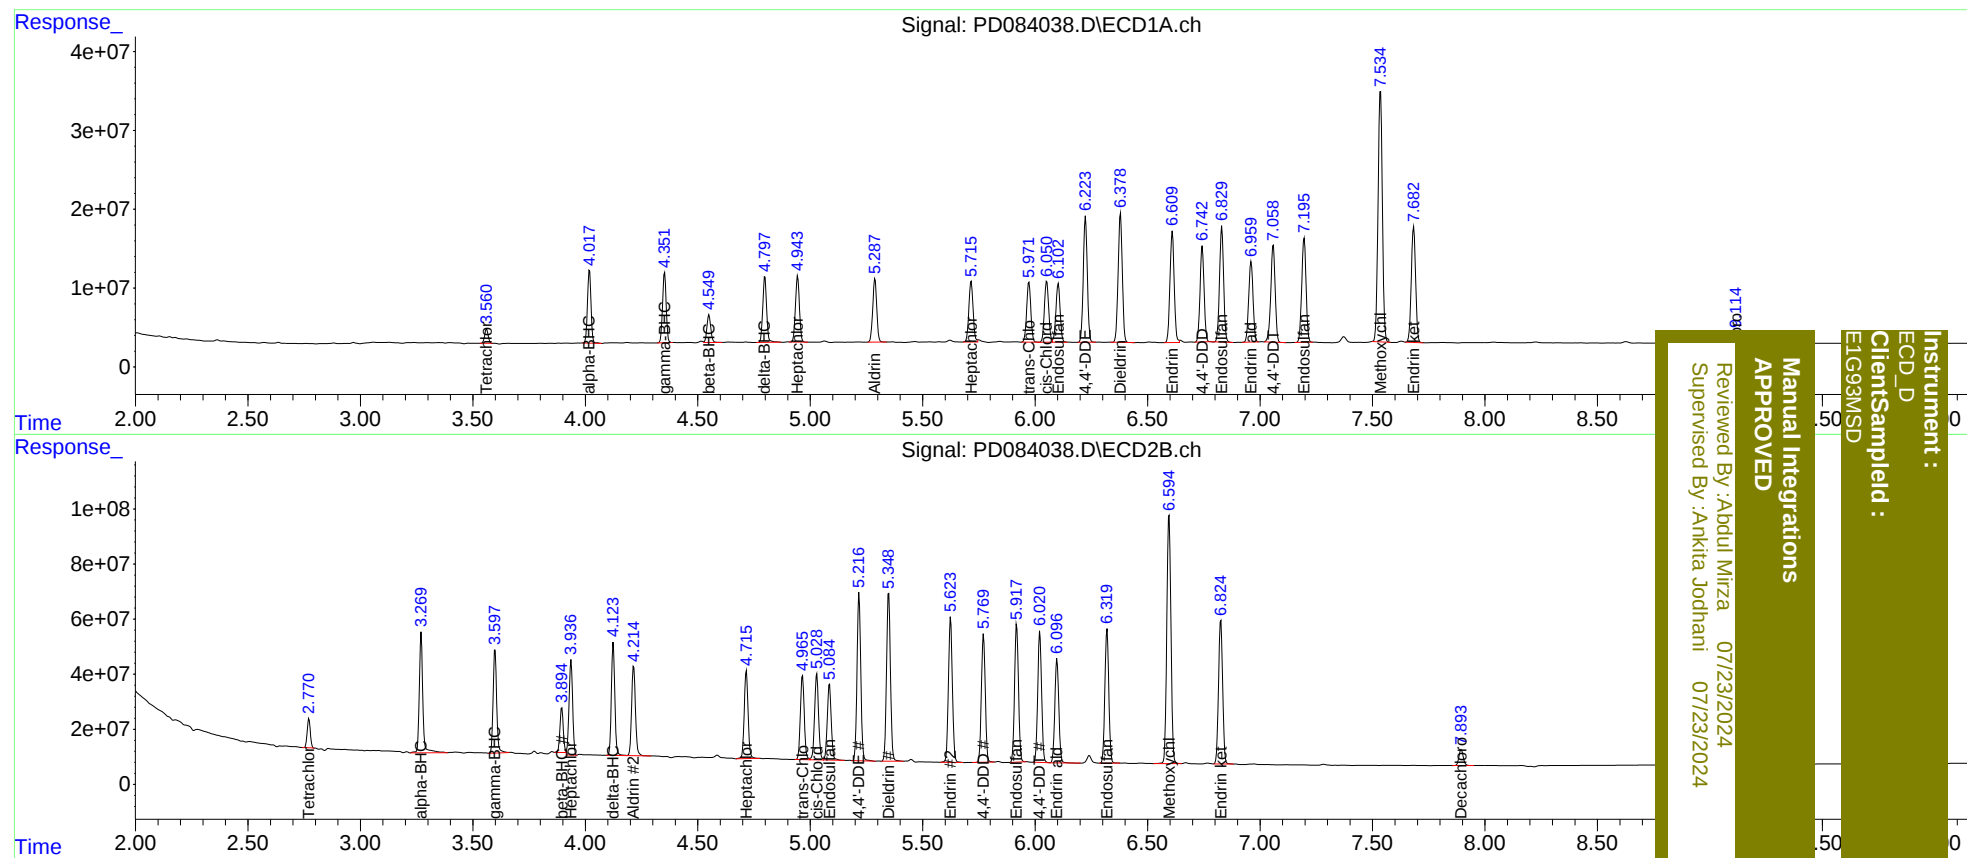

Instrument :
ECD_D
ClientSampled :
E1G93MSD

Manual Integrations
APPROVED

Reviewed By :Abdul Miza 07/23/2024
Supervised By :Ankita Jodhani 07/23/2024