

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072419\
Data File : PD054088.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jul 2019 11:51
Operator : SM\AJ
Sample : K3591-09
Misc : CHLOR MDL 25 PPB
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 07:32:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX071919.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 03:25:06 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	3.313	3.982	13150829	20371670	21.313	21.630
7) SA Decachlor...	8.007	9.024	14028691	19925610	20.562	20.924

Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072419\
Data File : PD054088.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jul 2019 11:51
Operator : SM\AJ
Sample : K3591-09
Misc : CHLOR MDL 25 PPB
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :
MDL-MDL-WATER-03-QT3-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 07:32:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX071919.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 03:25:06 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

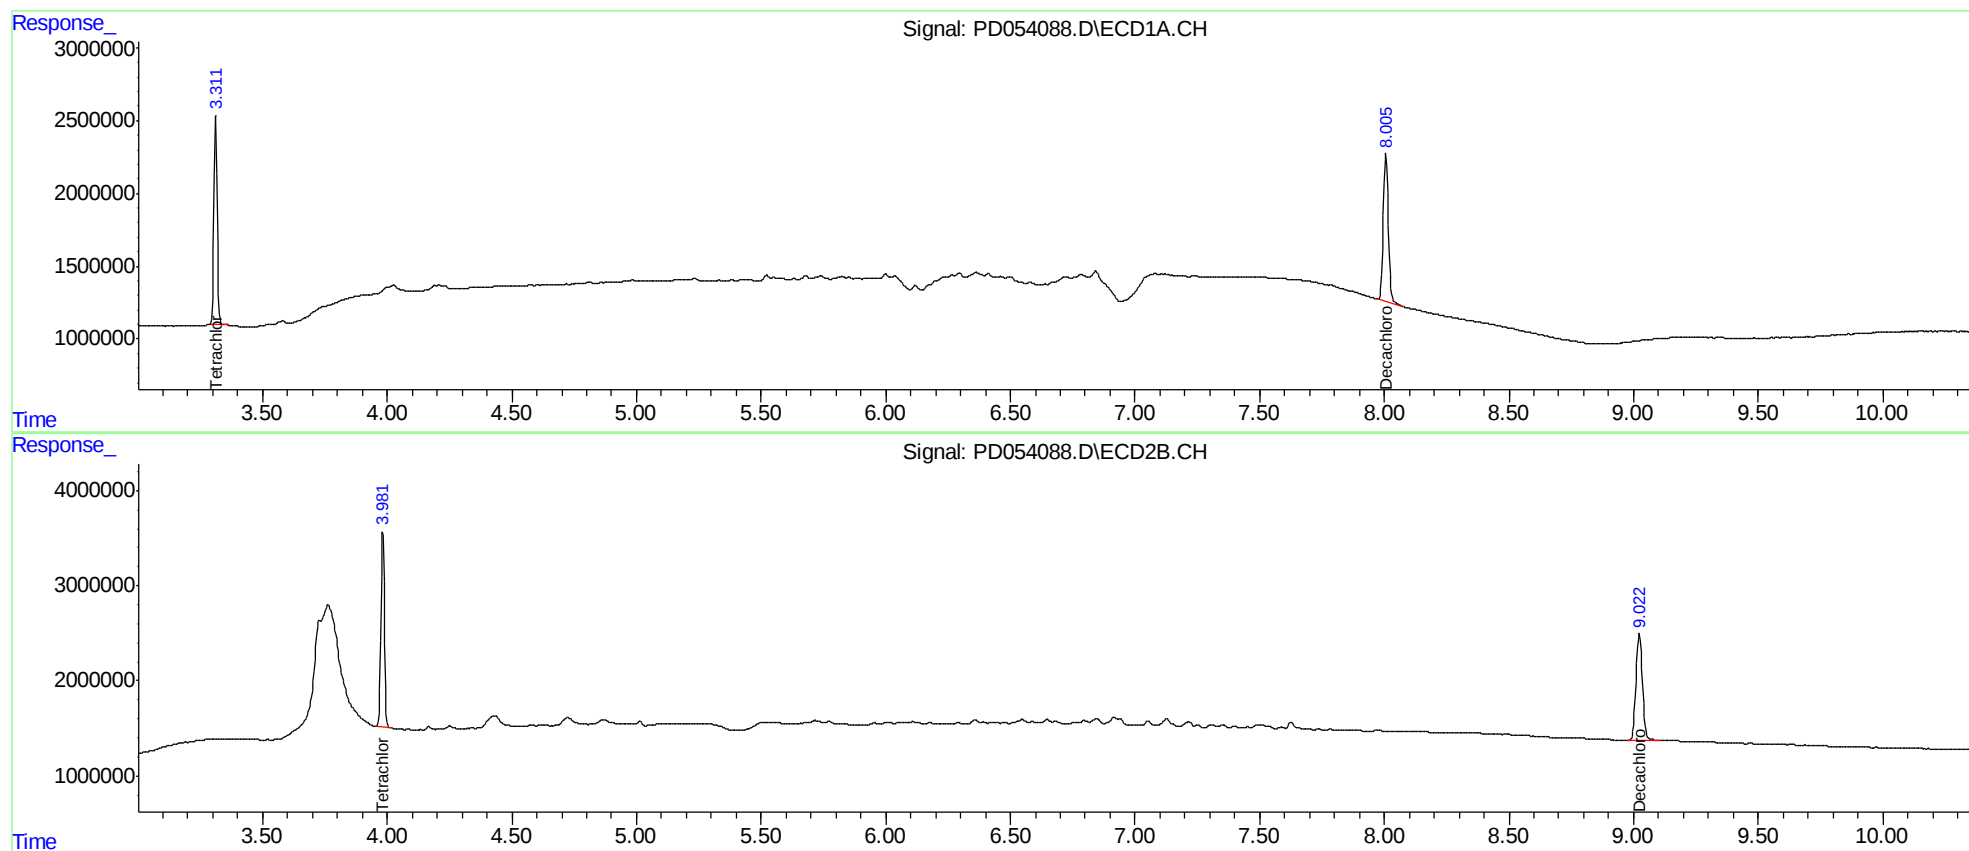


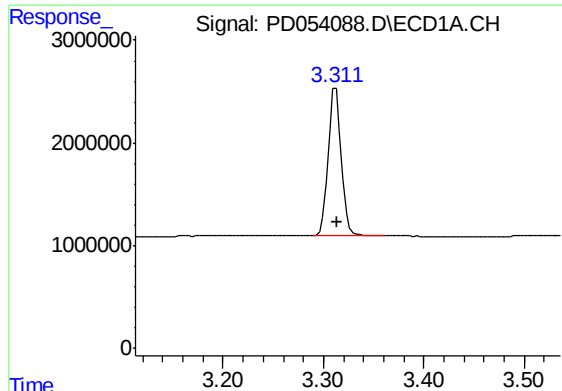

#1 Tetrachloro-m-xylene


R.T.: 3.313 min
Delta R.T.: 0.000 min
Response: 13150829
Conc: 21.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL-MDL-WATER-03-QT3-2019

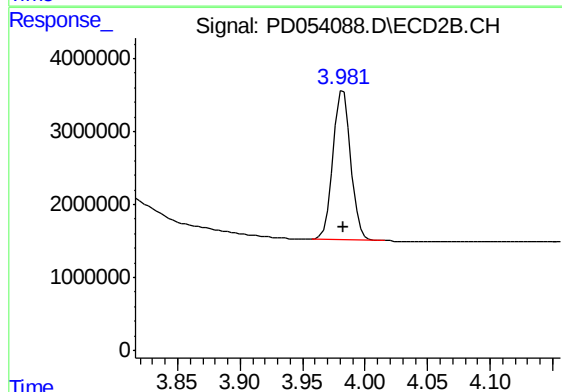


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 20371670
Conc: 21.63 ng/ml

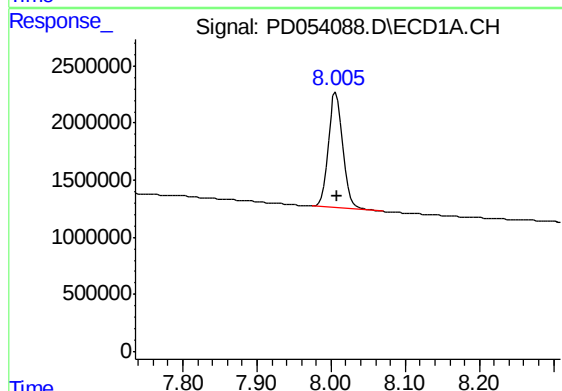

#7 Decachlorobiphenyl

R.T.: 8.007 min
Delta R.T.: -0.001 min
Response: 14028691
Conc: 20.56 ng/ml

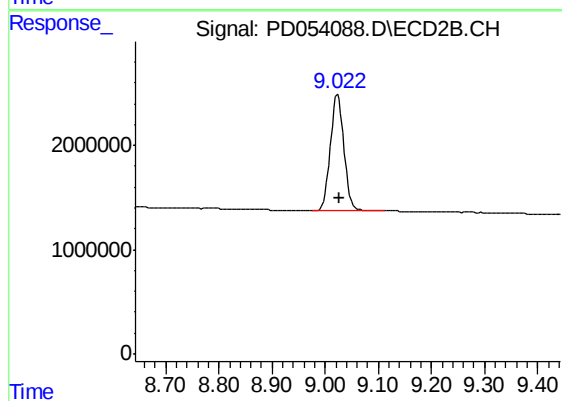

#7 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: -0.003 min
Response: 19925610
Conc: 20.92 ng/ml