

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072424\
 Data File : PD084066.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jul 2024 10:53
 Operator : AR\AJ
 Sample : RESC036
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC040

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 25 10:54:33 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072424CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 25 10:53:26 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.564	2.771	18154721	104.1E6	20.276	19.961
2)	SA Decachlor...	9.119	7.896	77360839	232.7E6	40.305	40.366
Target Compounds							
2)	A alpha-BHC	4.021	3.270	15692786	80876970	9.432	9.461
3)	MA gamma-BHC...	4.355	3.599	15748762	74017932	9.534	9.435
4)	MA Heptachlor	4.947	3.937	17717002	77222641	9.645	9.958
5)	MB Aldrin	5.290	4.216	18567380	77983256	10.056	9.907
6)	B beta-BHC	4.553	3.896	7393551	34095893	9.892	9.542
7)	B delta-BHC	4.802	4.125	18413450	81767319	9.183	9.599
8)	B Heptachlo...	5.719	4.717	19073751	70390085	10.319	9.705
9)	A Endosulfan I	6.106	5.085	17329938	64229331	10.029	9.936
10)	B trans-Chl...	5.975	4.966	17425163	68283240	9.820	9.642
11)	B cis-Chlor...	6.055	5.030	17834723	69275236	9.774	9.583
12)	B 4,4'-DDE	6.228	5.218	35572826	133.8E6	19.342	19.481
13)	MA Dieldrin	6.382	5.350	35700355	139.0E6	19.169	19.609
14)	MA Endrin	6.613	5.626	30792203	122.5E6	19.319	20.094
15)	B Endosulfa...	6.833	5.919	36357615	117.5E6	20.691	19.575
16)	A 4,4'-DDD	6.747	5.772	25252313	103.5E6	19.251	19.784
17)	MA 4,4'-DDT	7.061	6.022	28000224	101.6E6	19.770	19.460
18)	B Endrin al...	6.963	6.099	24829542	89999635	19.798	20.339
19)	B Endosulfa...	7.199	6.321	32119978	115.0E6	19.746	20.040
20)	A Methoxychlor	7.539	6.598	85565034	276.3E6	101.809	107.117
21)	B Endrin ke...	7.686	6.827	36052630	128.6E6	20.009	20.654

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072424\
Data File : PD084066.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2024 10:53
Operator : AR\AJ
Sample : RESC036
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 10:54:33 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072424CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 25 10:53:26 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

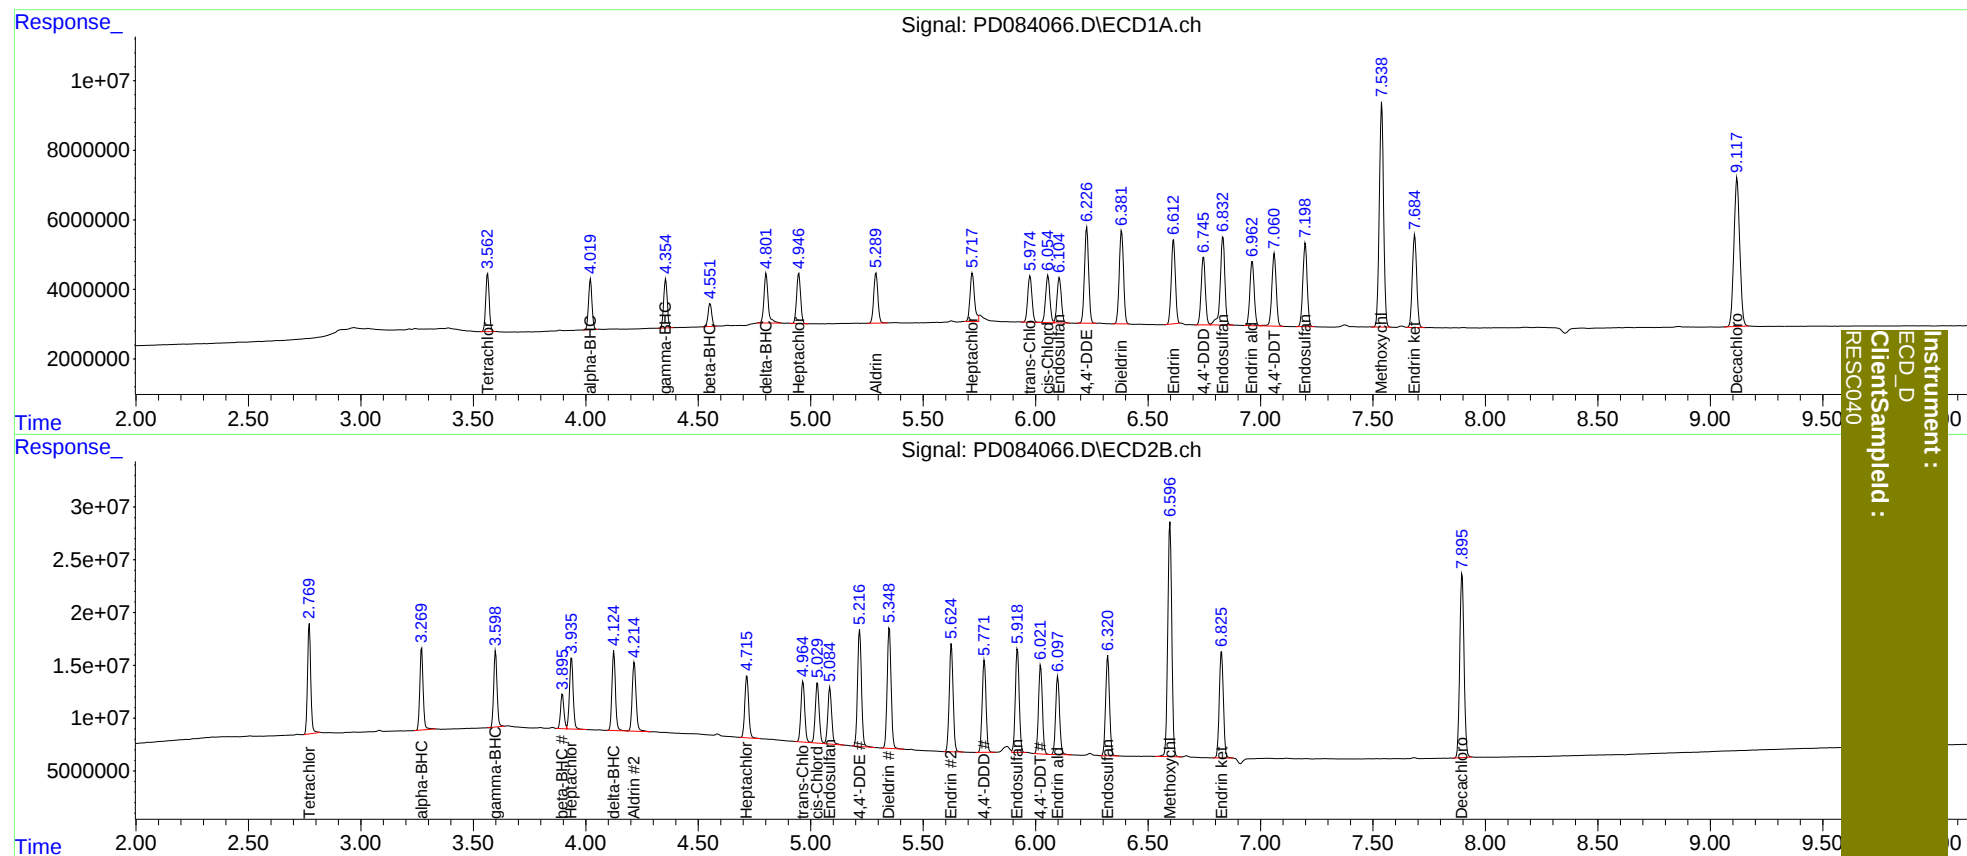

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072424\
Data File : PD084066.D
Acq On : 24 Jul 2024 10:53
Operator : AR\AJ
Sample : RESC036
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC040

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072424CLP.M
Title : GC Extractables
Last Update : Thu Jul 25 10:53:26 2024
Integrator: ChemStation

RT#1	RT#2	Resolution
3.564	4.021	100.00%
4.021	4.355	100.00%
4.355	4.553	100.00%
4.553	4.802	100.00%
4.802	4.947	100.00%
4.947	5.290	100.00%
5.290	5.719	100.00%
5.719	5.975	100.00%
5.975	6.055	100.00%
6.055	6.106	97.23%
6.106	6.228	100.00%
6.228	6.382	100.00%
6.382	6.613	100.00%
6.613	6.747	100.00%
6.747	6.833	97.78%
6.833	6.963	100.00%
6.963	7.061	99.06%
7.061	7.199	100.00%
7.199	7.539	100.00%
7.539	7.686	100.00%
7.686	9.119	100.00%

Signal #2


2.771	3.270	100.00%
3.270	3.599	100.00%
3.599	3.896	100.00%
3.896	3.937	94.00%
3.937	4.125	100.00%
4.125	4.216	100.00%
4.216	4.717	100.00%
4.717	4.966	100.00%
4.966	5.030	100.00%
5.030	5.085	99.52%
5.085	5.218	100.00%
5.218	5.350	100.00%
5.350	5.626	100.00%
5.626	5.772	100.00%
5.772	5.919	100.00%
5.919	6.022	100.00%
6.022	6.099	100.00%
6.099	6.321	100.00%
6.321	6.598	100.00%
6.598	6.827	100.00%
6.827	7.896	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072424\
Data File : PD084066.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2024 10:53
Operator : AR\AJ
Sample : RESC036
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC040

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 10:54:33 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072424CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 25 10:53:26 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

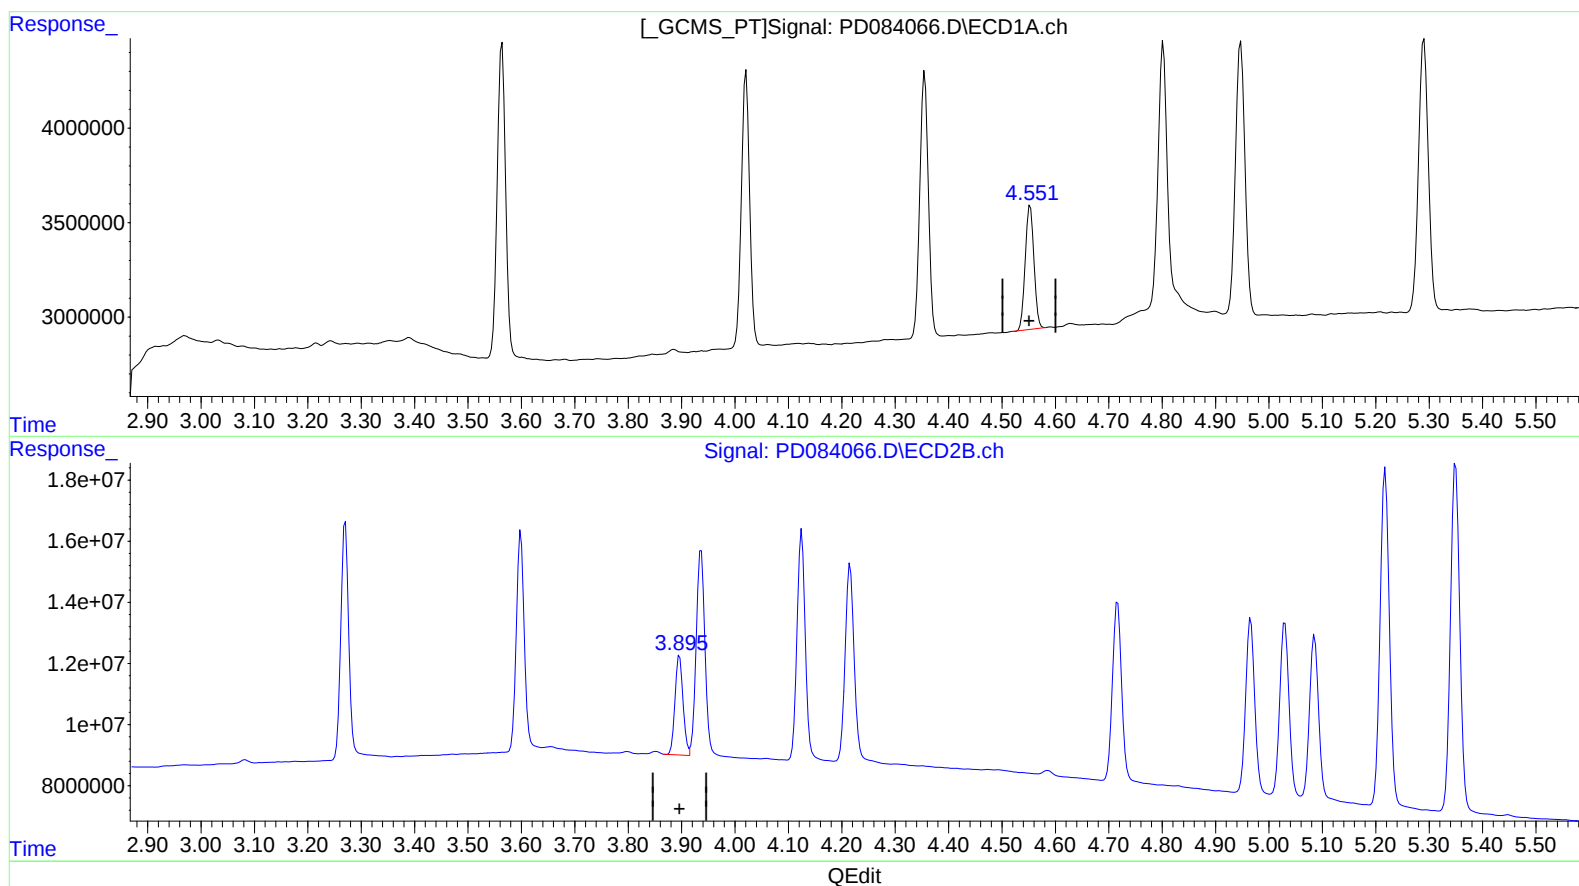

(6) beta-BHC (B)
4.553min 9.892 ng/ml
response 7393551


(6) beta-BHC #2 (B)
3.896min 9.542 ng/ml
response 34095893

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072424\
Data File : PD084066.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2024 10:53
Operator : AR\AJ
Sample : RESC036
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC040

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 10:54:33 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072424CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 25 10:53:26 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

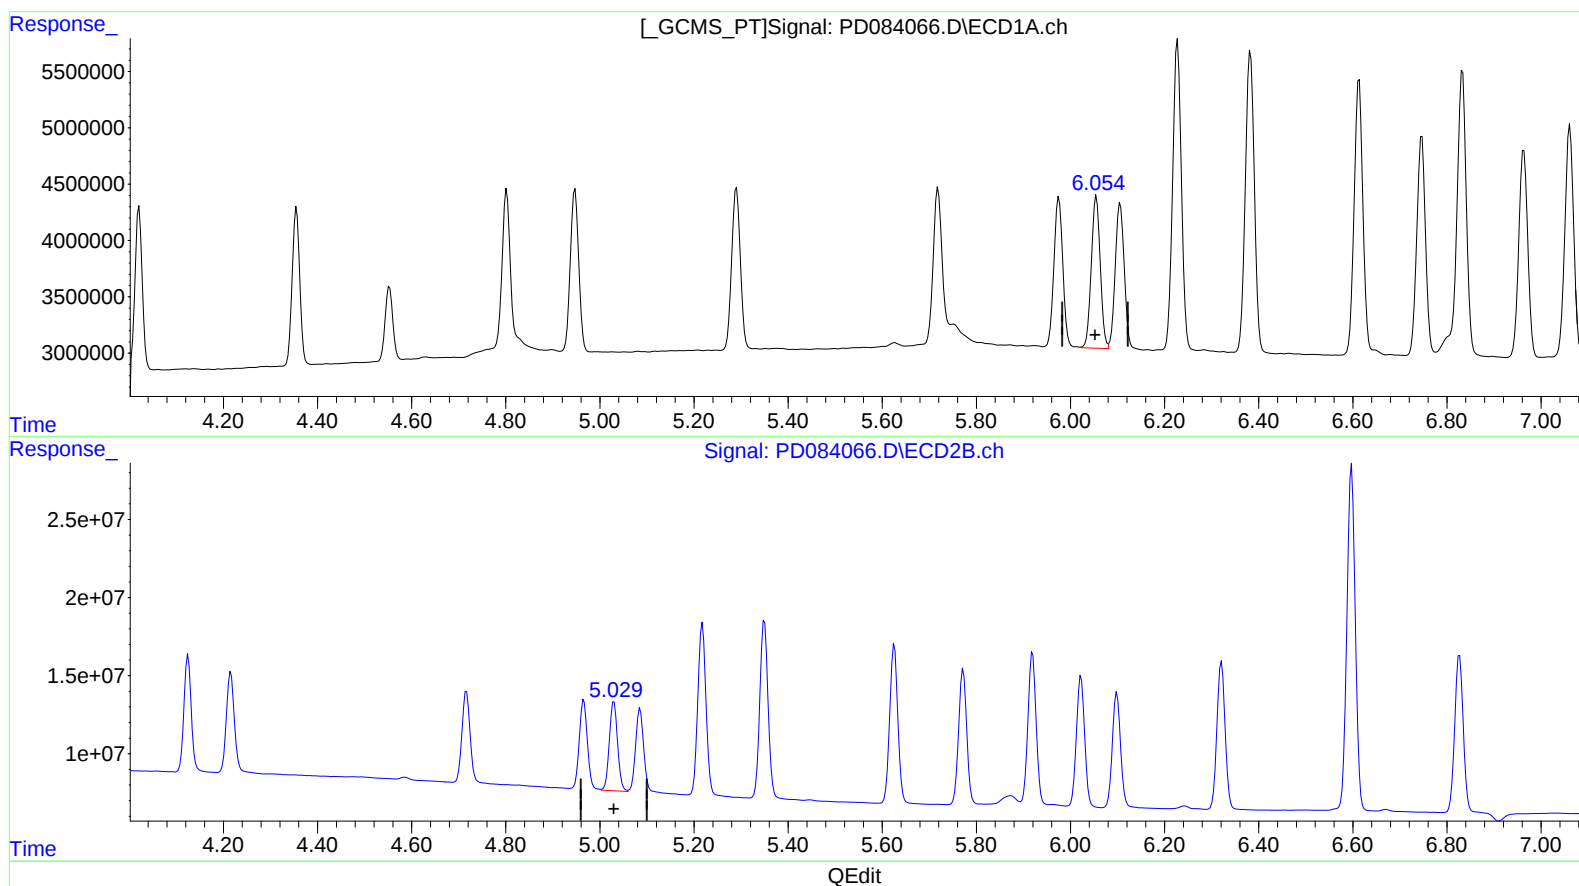

(11) cis-Chlordane (B)

6.055min 9.774 ng/ml

response 17834723

(11) cis-Chlordane #2 (B)

5.030min 9.583 ng/ml


response 69275236

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072424\
Data File : PD084066.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2024 10:53
Operator : AR\AJ
Sample : RESC036
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC040

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 10:54:33 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072424CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 25 10:53:26 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

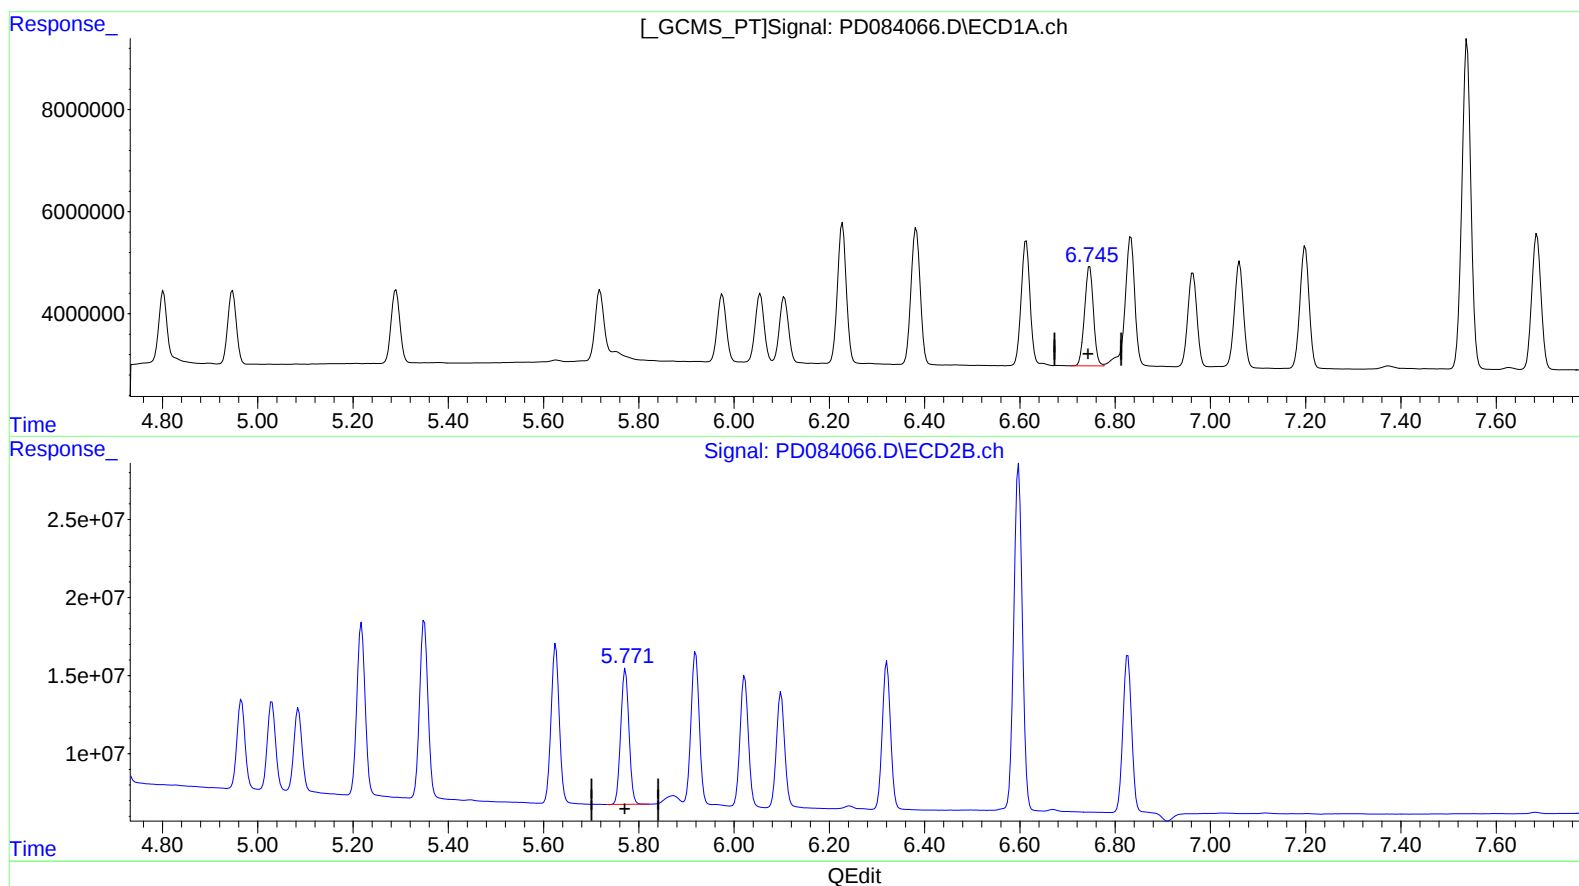

(16) 4,4'-DDD (A)
6.747min 19.251 ng/ml
response 25252313


(16) 4,4'-DDD #2 (A)
5.772min 19.784 ng/ml
response 103520381

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072424\
Data File : PD084066.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2024 10:53
Operator : AR\AJ
Sample : RESC036
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC040

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 10:54:33 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072424CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 25 10:53:26 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

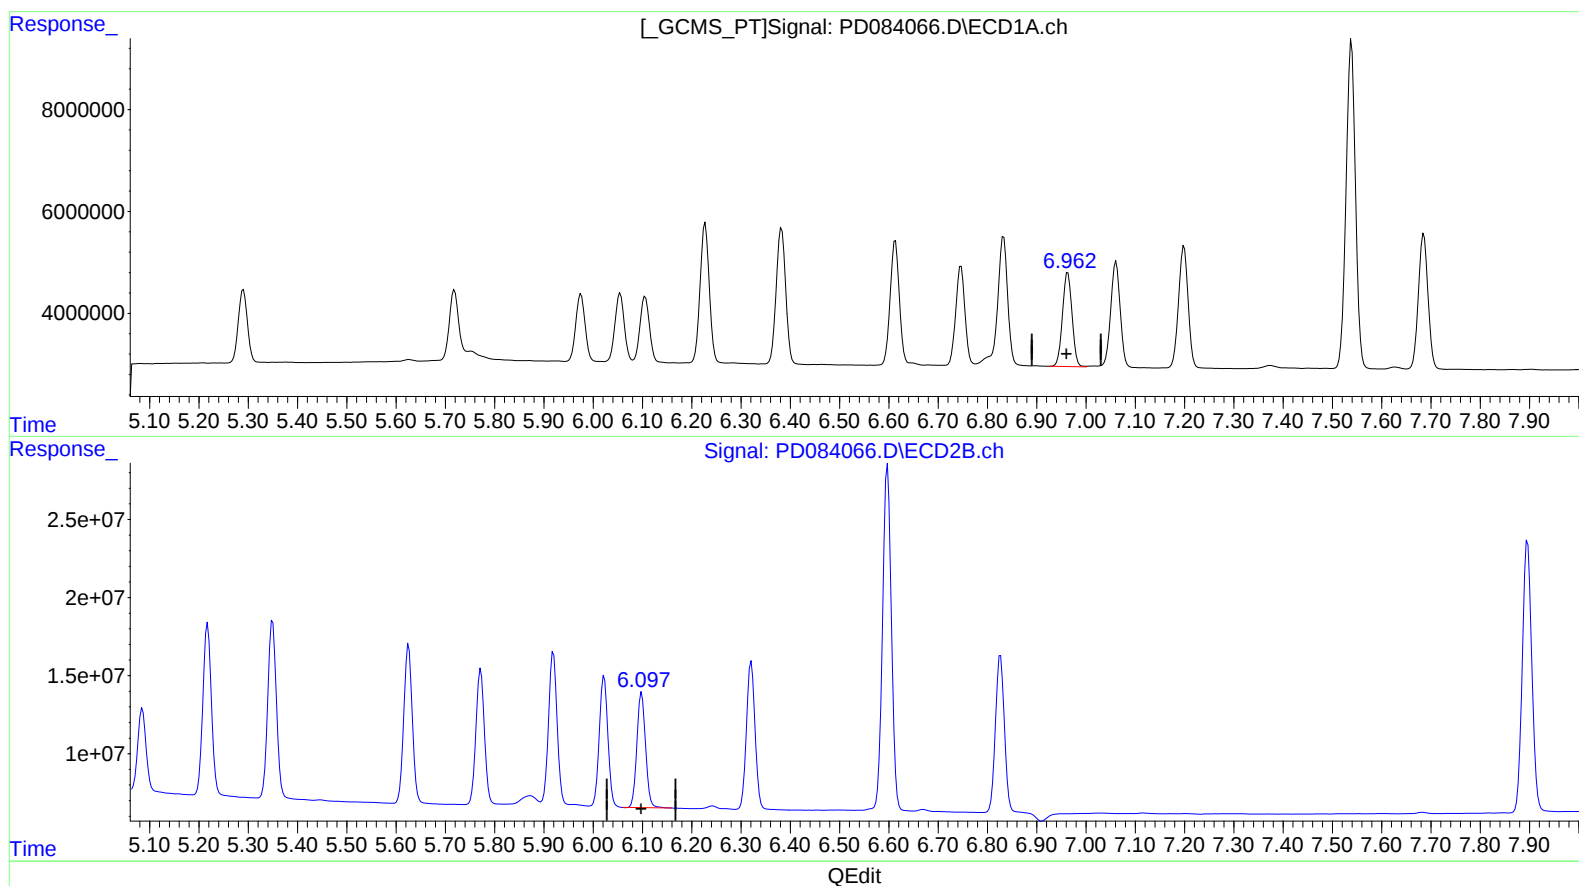

(18) Endrin aldehyde (B)

6.963min 19.798 ng/ml

response 24829542

(18) Endrin aldehyde #2 (B)

6.099min 20.339 ng/ml

response 89999635