

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072425\
 Data File : PD089598.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 15:32
 Operator : AR\AJ
 Sample : PB168928BS
 Misc : (Sig #1); BS / CHLOR (Sig #2)
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB168928BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 02:10:46 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072125.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 22 04:39:29 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	2.877	48268875	475.8E6	16.752	24.315 #
28)	SA Decachlor...	9.068	8.067	82579624	496.2E6	20.107	20.195
Target Compounds							
23)	Chlordane-1	4.712	3.902	40146186	213.3E6	205.140	229.735
24)	Chlordane-2	5.239	4.484	43812987	225.7E6	217.880	230.245
25)	Chlordane-3	5.944	5.121	160.9E6	658.5E6	206.448	228.091
26)	Chlordane-4	6.029	5.186	201.4E6	571.1E6	212.174	236.759
27)	Chlordane-5	6.868	6.085	35226411	266.7E6	213.597	228.231



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072425\
Data File : PD089598.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jul 2025 15:32
Operator : AR\AJ
Sample : PB168928BS
Misc : (Sig #1); BS / CHLOR (Sig #2)
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PB168928BS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 02:10:46 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072125.M
Quant Title : GC Extractables
QLast Update : Tue Jul 22 04:39:29 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

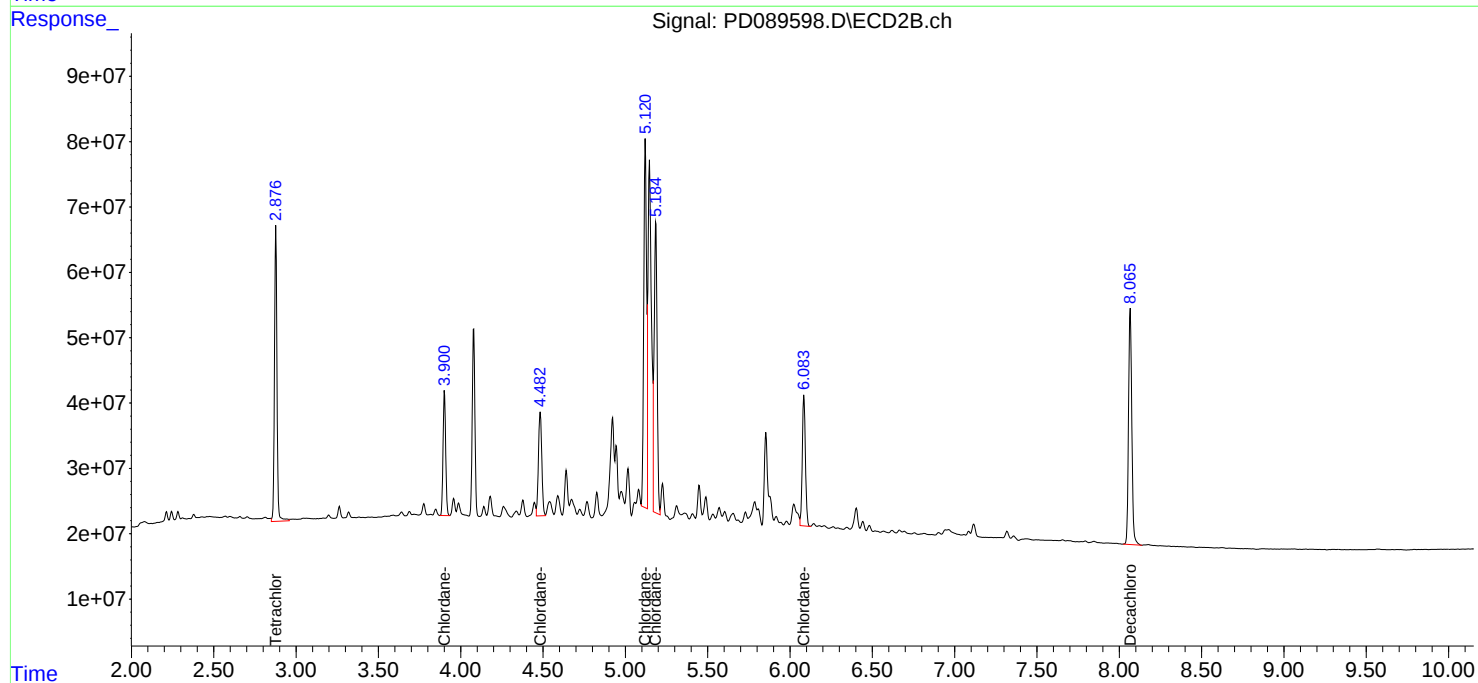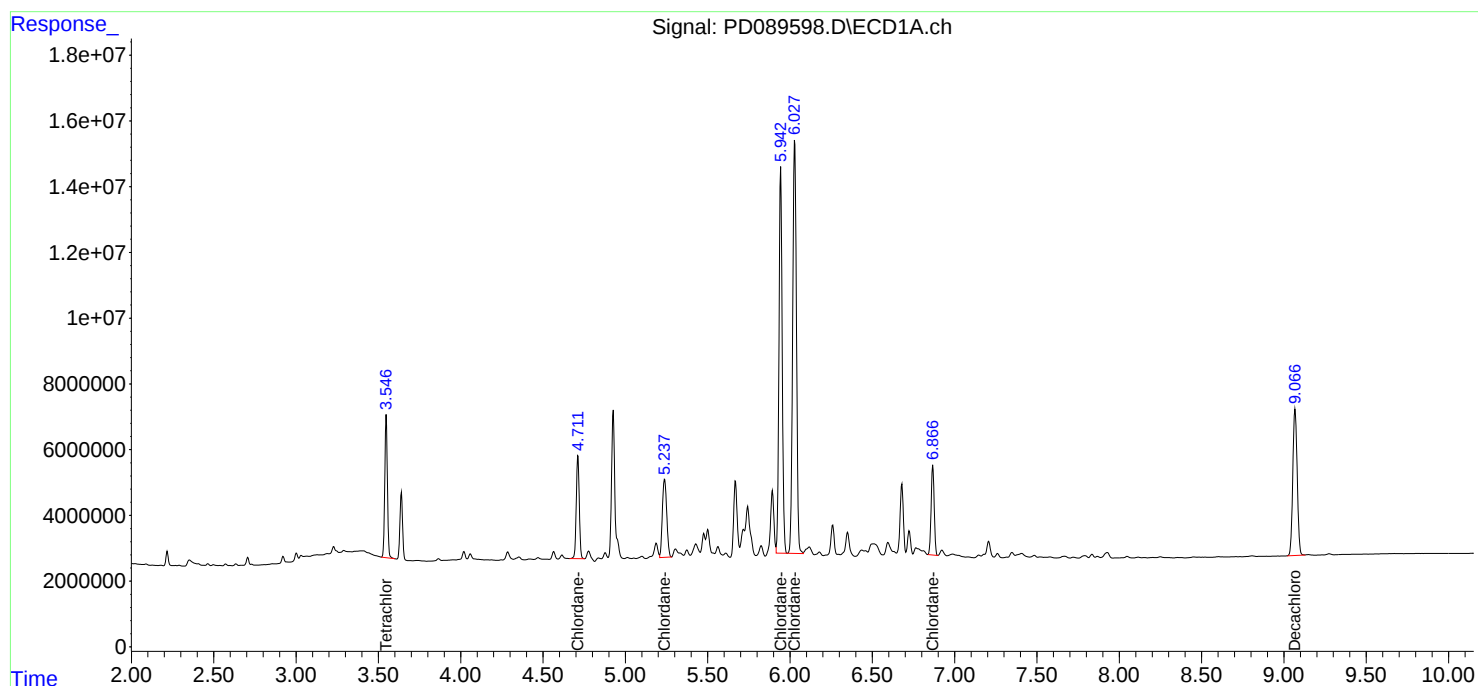


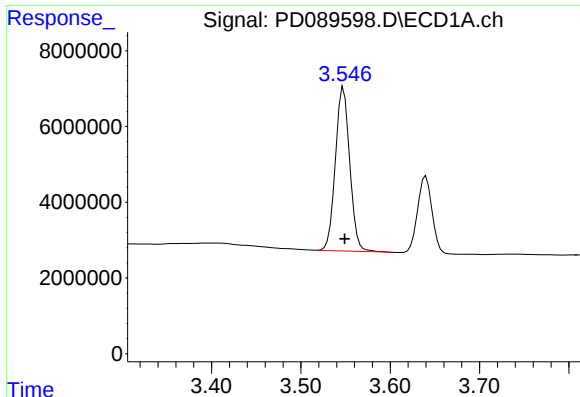

#1 Tetrachloro-m-xylene


R.T.: 3.548 min
Delta R.T.: -0.001 min
Response: 48268875
Conc: 16.75 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB168928BS

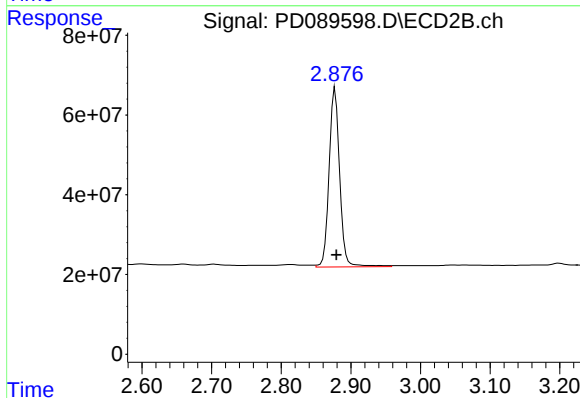


#1 Tetrachloro-m-xylene

R.T.: 2.877 min
Delta R.T.: -0.002 min
Response: 475751109
Conc: 24.32 ng/ml

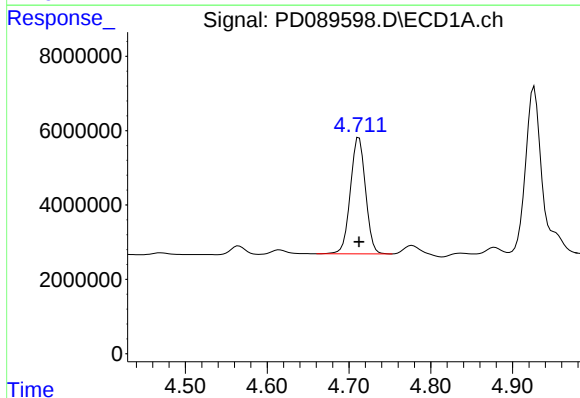


#23 Chlordane-1

R.T.: 4.712 min
Delta R.T.: 0.000 min
Response: 40146186
Conc: 205.14 ng/ml

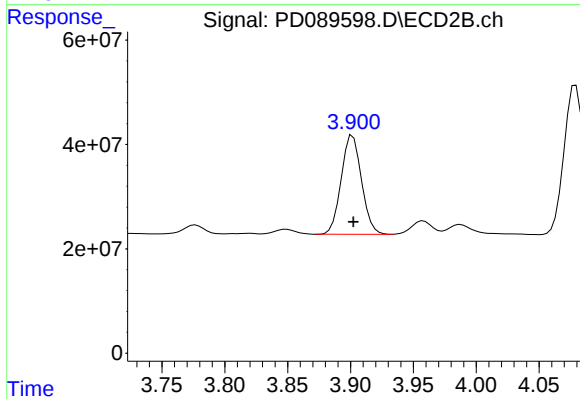

#23 Chlordane-1


R.T.: 3.902 min
Delta R.T.: 0.000 min
Response: 213348279
Conc: 229.73 ng/ml

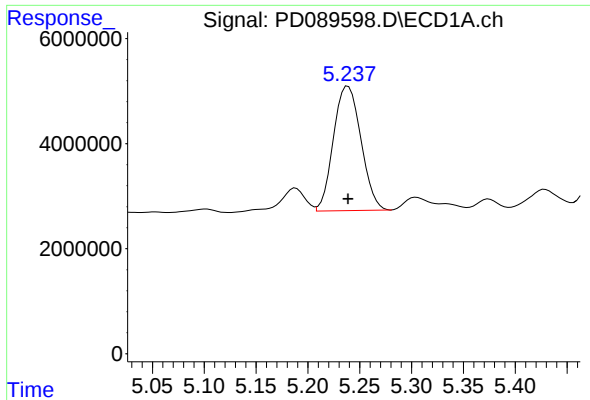

#24 Chlordane-2


R.T.: 5.239 min
Delta R.T.: 0.000 min
Response: 43812987
Conc: 217.88 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB168928BS

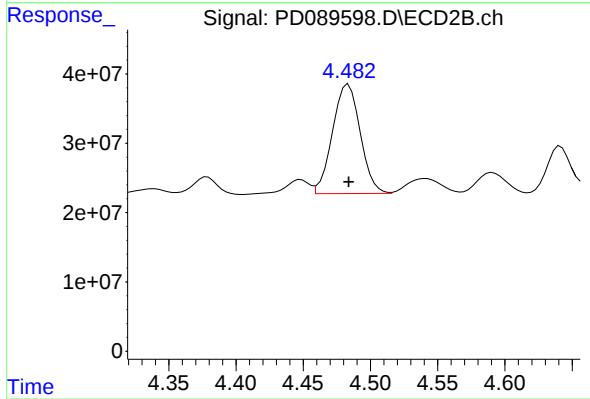


#24 Chlordane-2

R.T.: 4.484 min
Delta R.T.: 0.000 min
Response: 225698156
Conc: 230.24 ng/ml

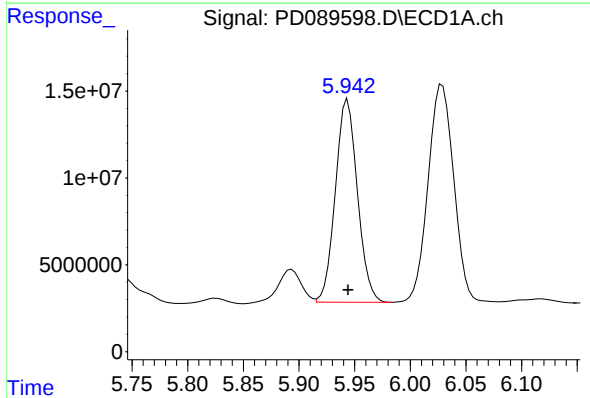


#25 Chlordane-3

R.T.: 5.944 min
Delta R.T.: 0.000 min
Response: 160867860
Conc: 206.45 ng/ml

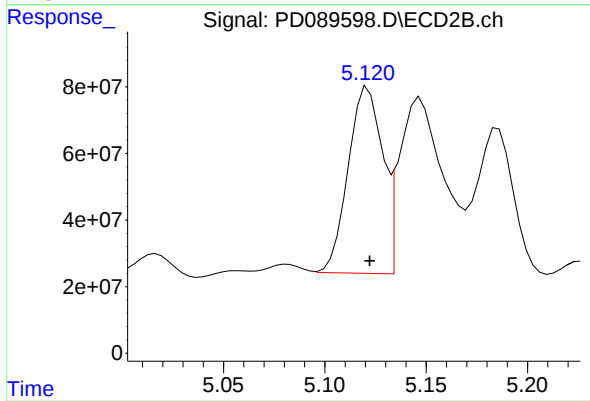

#25 Chlordane-3


R.T.: 5.121 min
Delta R.T.: 0.000 min
Response: 658500244
Conc: 228.09 ng/ml

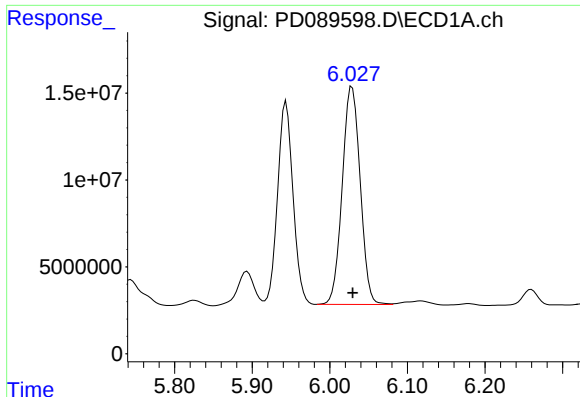

#26 Chlordane-4


R.T.: 6.029 min
Delta R.T.: 0.000 min
Response: 201403856
Conc: 212.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB168928BS

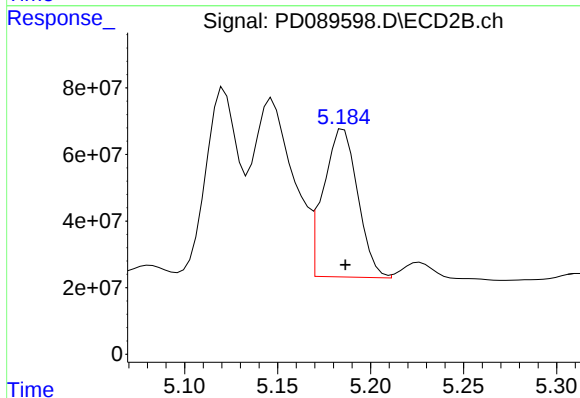


#26 Chlordane-4

R.T.: 5.186 min
Delta R.T.: 0.000 min
Response: 571107370
Conc: 236.76 ng/ml

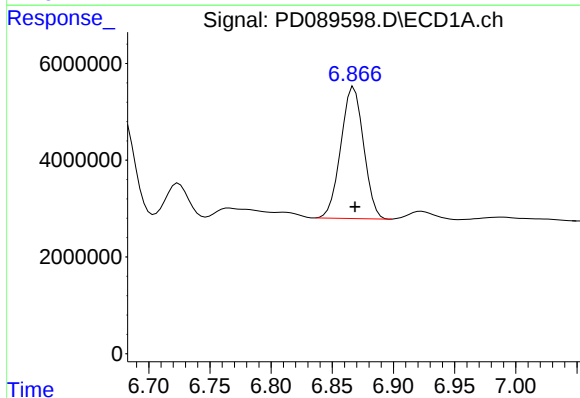


#27 Chlordane-5

R.T.: 6.868 min
Delta R.T.: 0.000 min
Response: 35226411
Conc: 213.60 ng/ml

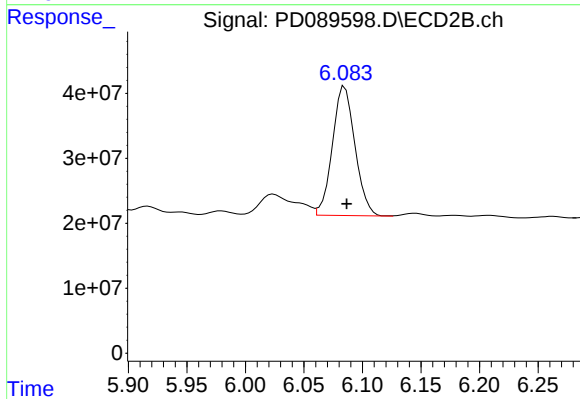

#27 Chlordane-5


R.T.: 6.085 min
Delta R.T.: -0.002 min
Response: 266676549
Conc: 228.23 ng/ml

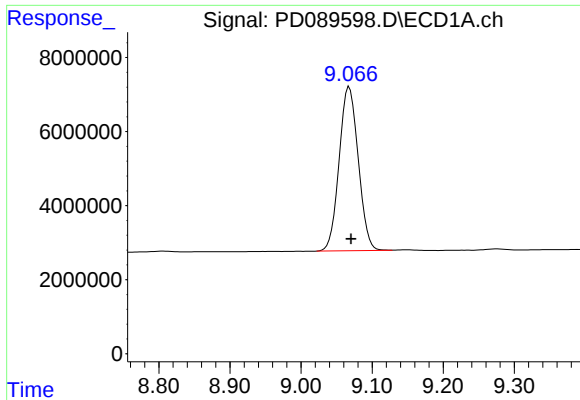

#28 Decachlorobiphenyl

R.T.: 9.068 min
Delta R.T.: -0.003 min
Response: 82579624
Conc: 20.11 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB168928BS

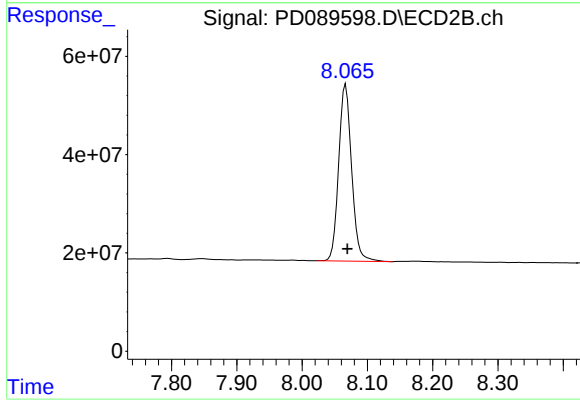

#28 Decachlorobiphenyl

R.T.: 8.067 min
Delta R.T.: -0.003 min
Response: 496165833
Conc: 20.20 ng/ml