

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072520\
 Data File : PD058698.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jul 2020 21:31
 Operator : AJ\MA
 Sample : L3419-02
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AA0

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 25 00:10:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070220CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 02 16:12:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.208	3.866	28389822	40741846	16.891	17.879
27) SA Decachlor...	7.844	8.860	45255151	56245479	25.598	26.473
Target Compounds						
6) B beta-BHC	0.000	4.665f	0	249627	N.D.	0.181
8) B Heptachlo...	4.897f	0.000	2171210	0	1.231	N.D. #
19) B Endosulfa...	6.254f	0.000	2055182	0	1.354	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072520\
Data File : PD058698.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2020 21:31
Operator : AJ\MA
Sample : L3419-02
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
C0AA0

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 00:10:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070220CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 02 16:12:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

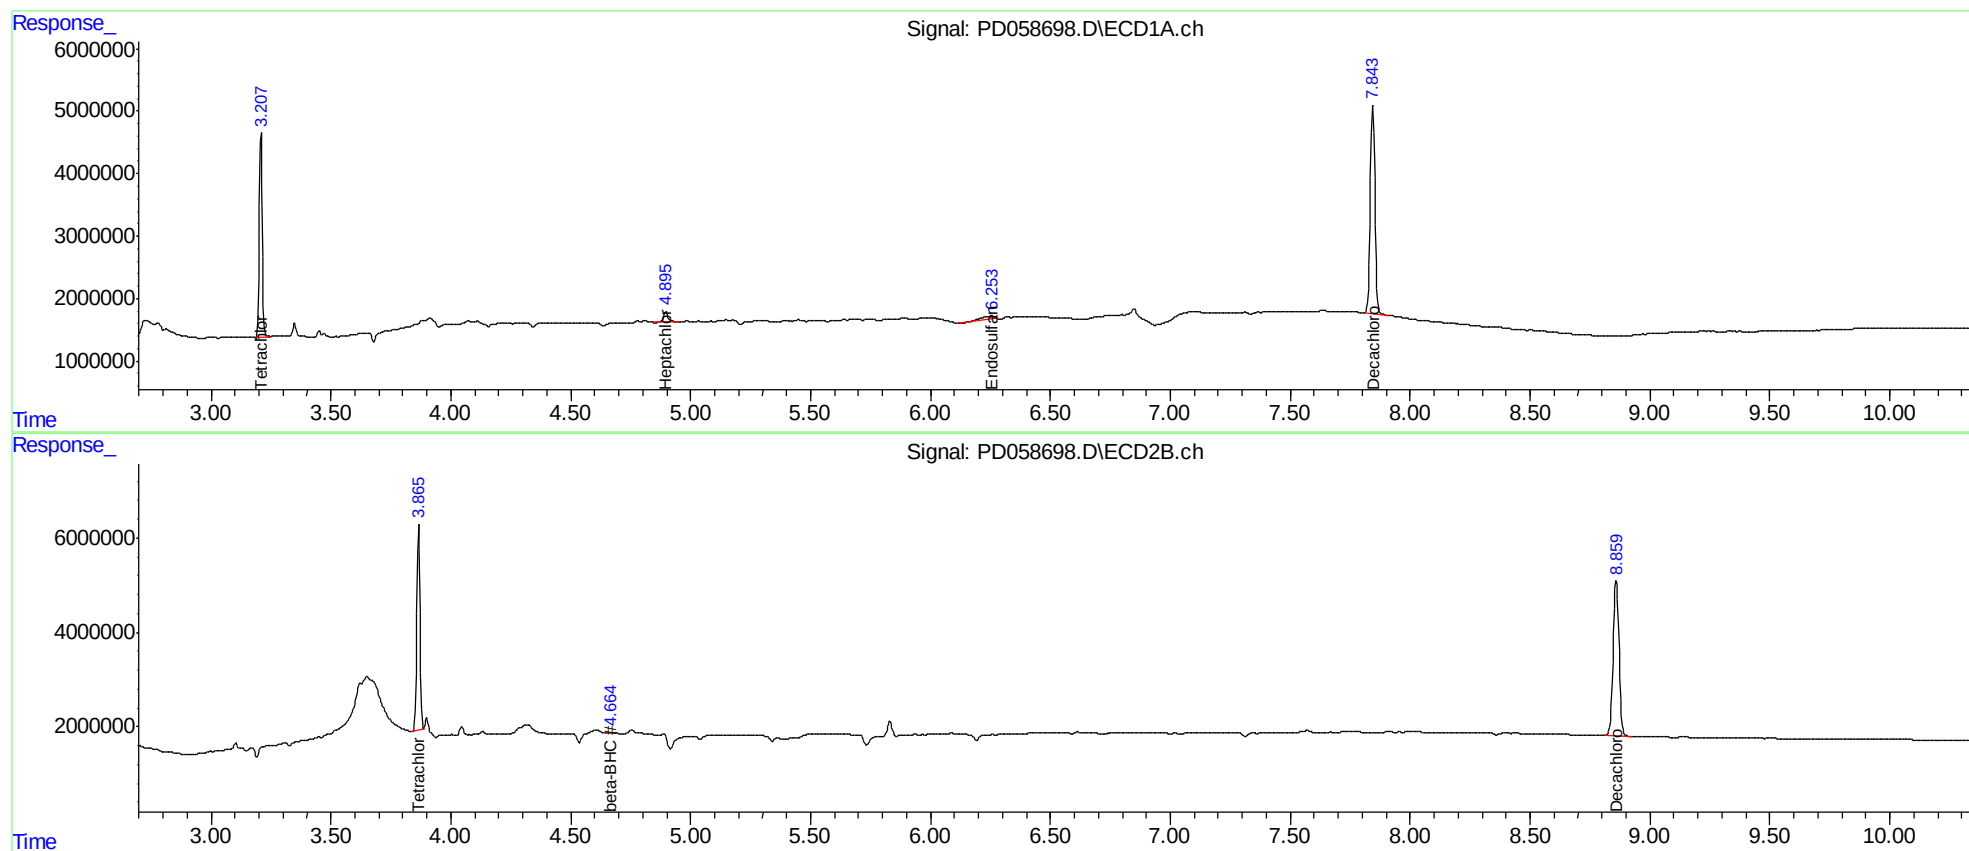


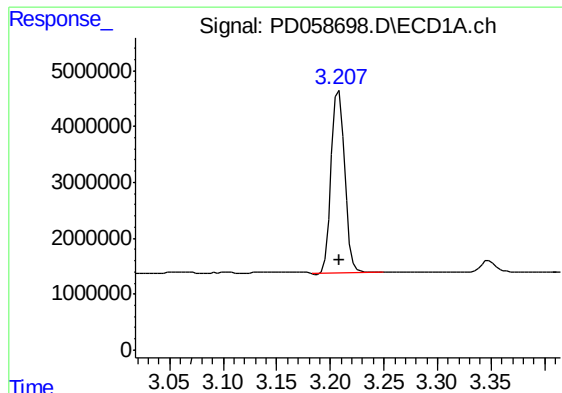

#1 Tetrachloro-m-xylene


R.T.: 3.208 min
Delta R.T.: 0.000 min
Response: 28389822
Conc: 16.89 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AA0

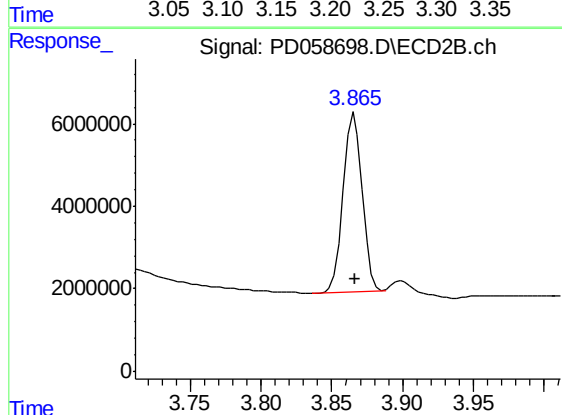


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.000 min
Response: 40741846
Conc: 17.88 ng/ml

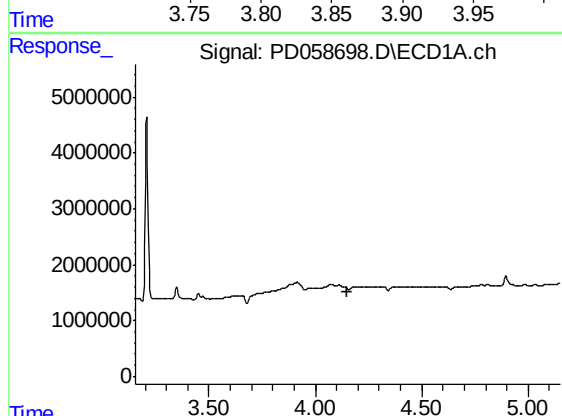


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.152 min
Response: 0
Conc: N.D.

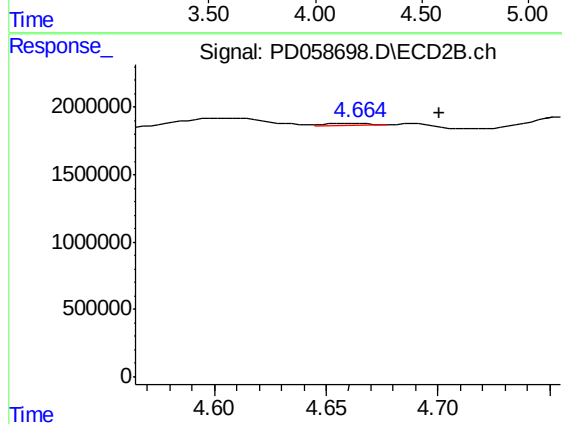

#6 beta-BHC


R.T.: 4.665 min
Delta R.T.: -0.036 min
Response: 249627
Conc: 0.18 ng/ml

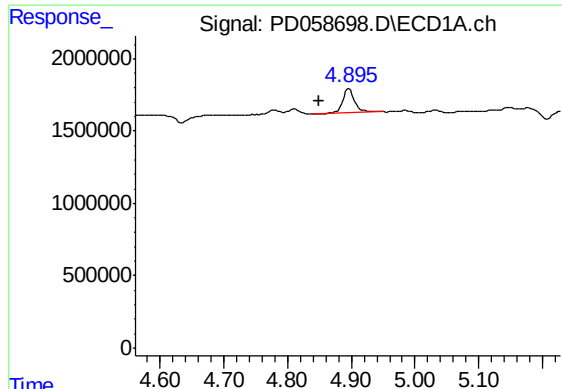

#8 Heptachlor epoxide


R.T.: 4.897 min
Delta R.T.: 0.047 min
Response: 2171210
Conc: 1.23 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AA0

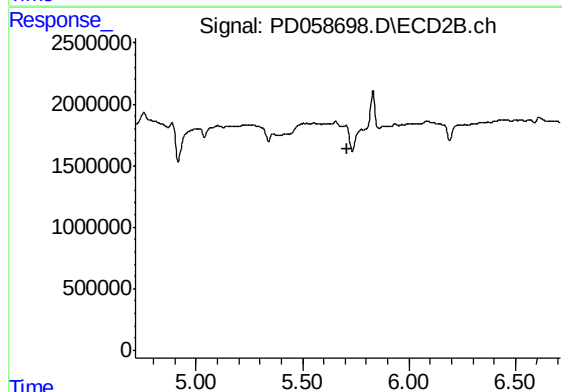


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.712 min
Response: 0
Conc: N.D.

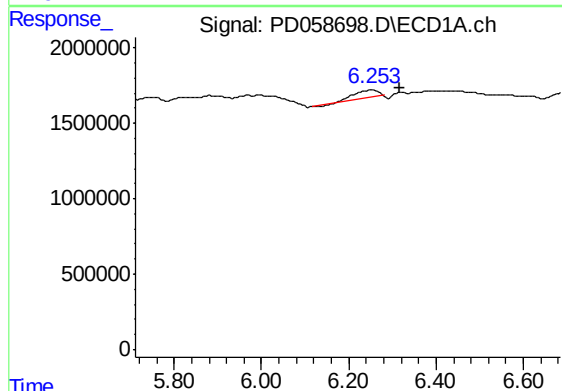


#19 Endosulfan Sulfate

R.T.: 6.254 min
Delta R.T.: -0.062 min
Response: 2055182
Conc: 1.35 ng/ml

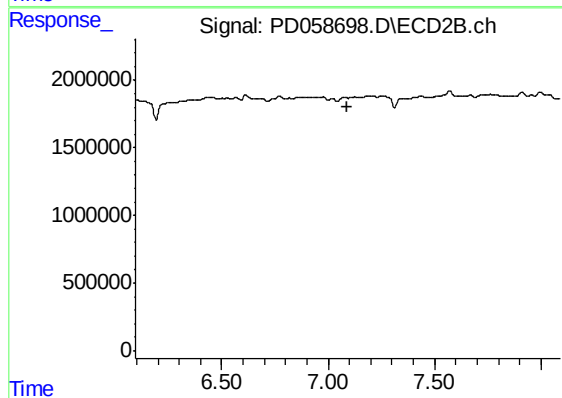

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.092 min
Response: 0
Conc: N.D.

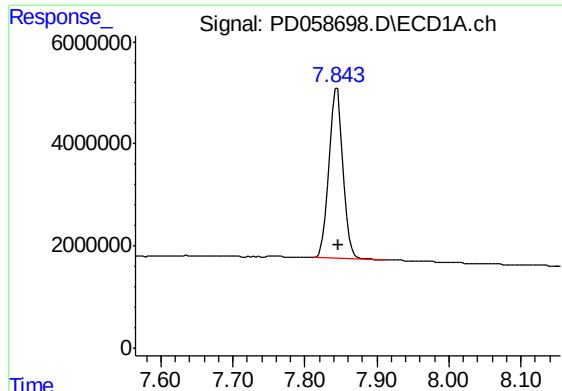

#27 Decachlorobiphenyl

R.T.: 7.844 min
Delta R.T.: -0.002 min
Response: 45255151
Conc: 25.60 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AA0

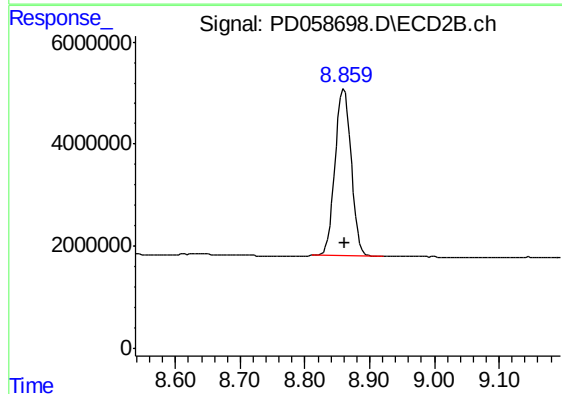

#27 Decachlorobiphenyl

R.T.: 8.860 min
Delta R.T.: -0.001 min
Response: 56245479
Conc: 26.47 ng/ml