

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072520\
 Data File : PD058701.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jul 2020 22:14
 Operator : AJ\MA
 Sample : L3419-07
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AA5

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 25 00:11:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070220CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 02 16:12:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.866	27279397	38663025	16.230	16.967
27)	SA Decachlor...	7.844	8.860	49173671	61026785	27.815	28.724
Target Compounds							
8)	B Heptachlo...	4.897f	0.000	2034007	0	1.153	N.D. #
19)	B Endosulfa...	6.254f	0.000	611691	0	0.403	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072520\
Data File : PD058701.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2020 22:14
Operator : AJ\MA
Sample : L3419-07
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
C0AA5

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 00:11:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070220CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 02 16:12:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

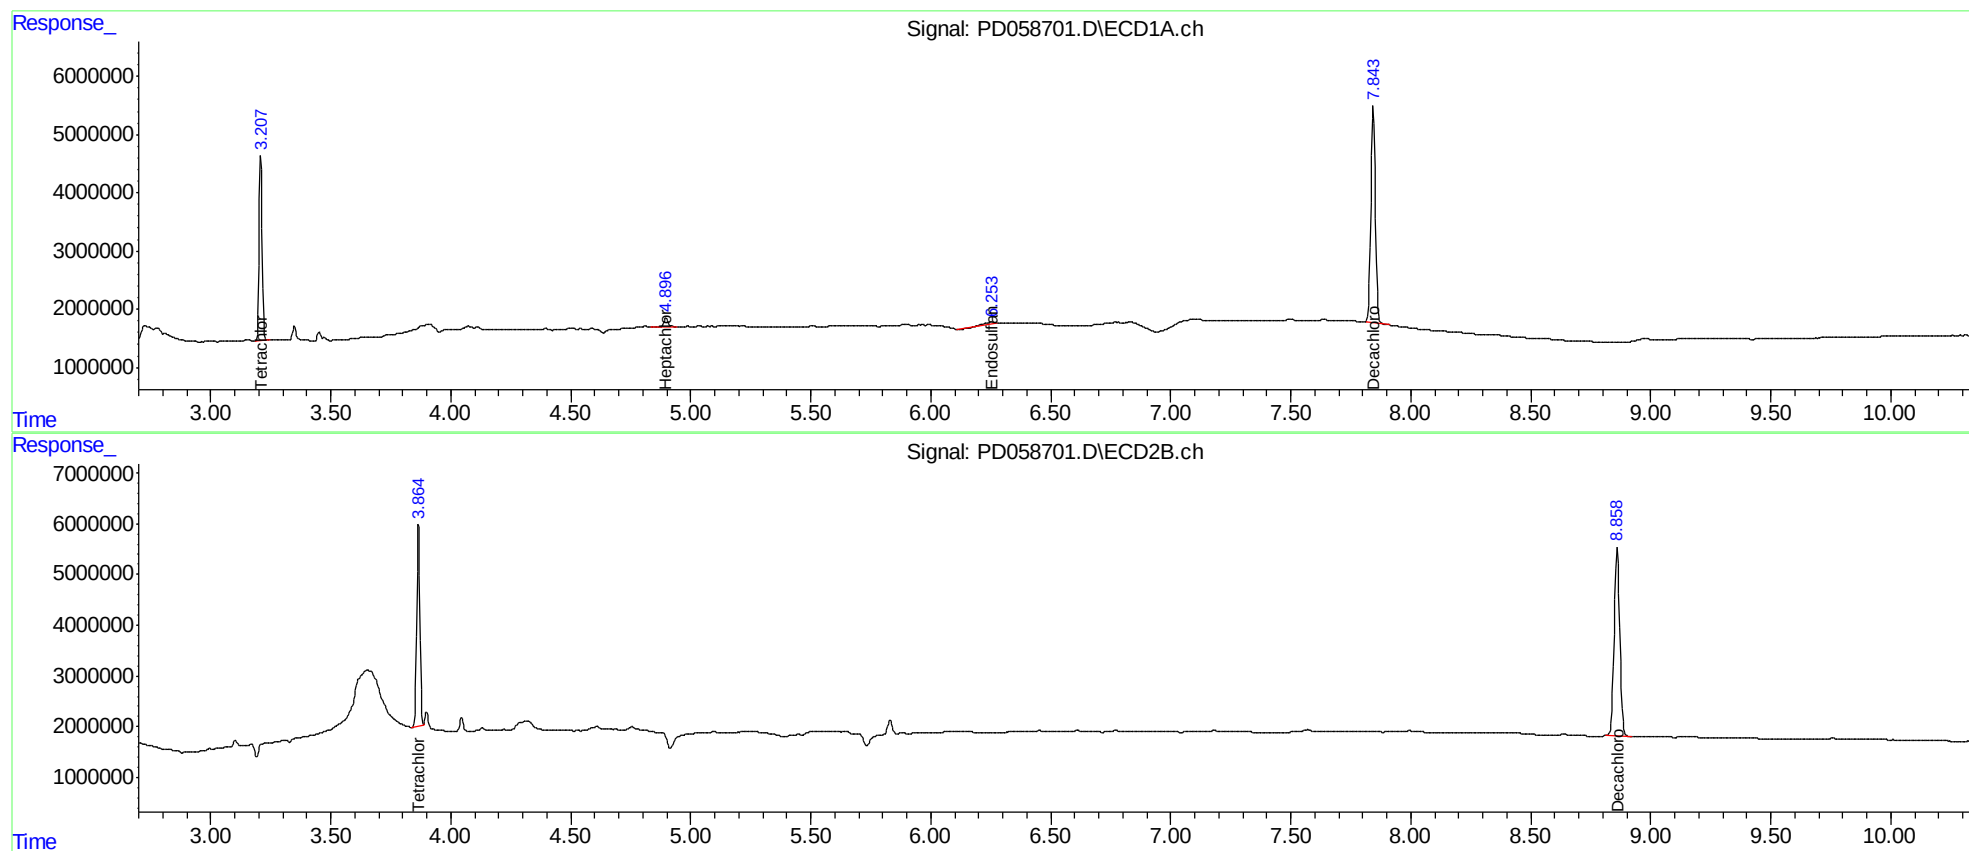


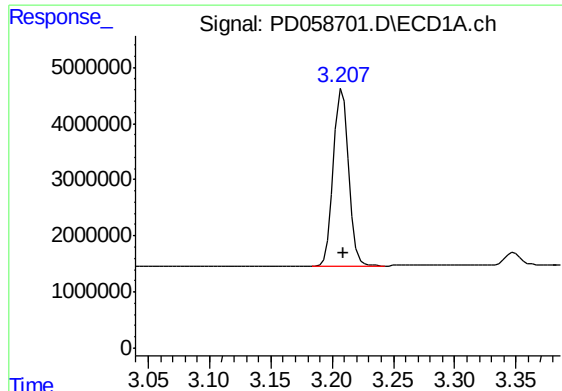

#1 Tetrachloro-m-xylene


R.T.: 3.209 min
Delta R.T.: 0.000 min
Response: 27279397
Conc: 16.23 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AA5

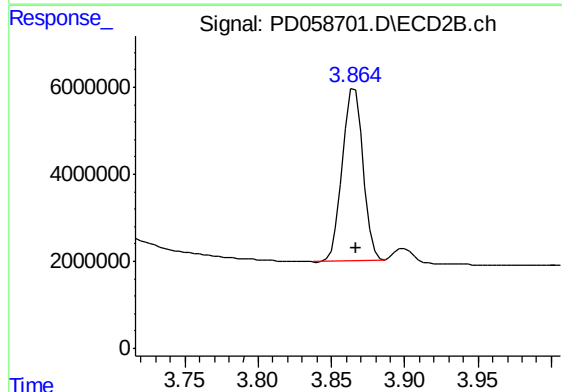


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.000 min
Response: 38663025
Conc: 16.97 ng/ml

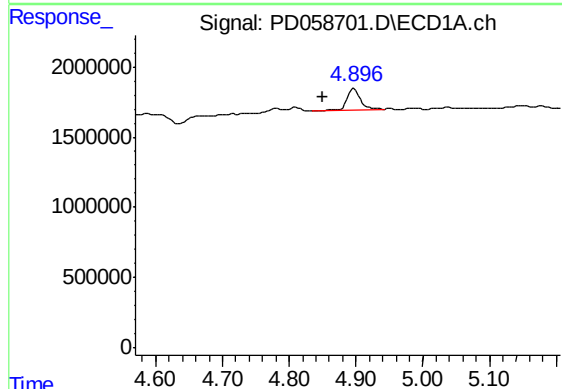


#8 Heptachlor epoxide

R.T.: 4.897 min
Delta R.T.: 0.047 min
Response: 2034007
Conc: 1.15 ng/ml

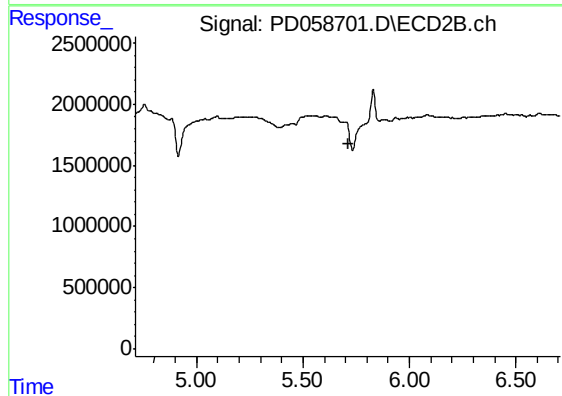

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.712 min
Response: 0
Conc: N.D.

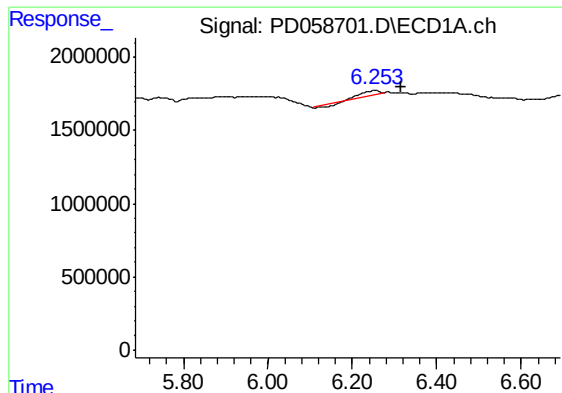

#19 Endosulfan Sulfate


R.T.: 6.254 min
Delta R.T.: -0.063 min
Response: 611691
Conc: 0.40 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AA5

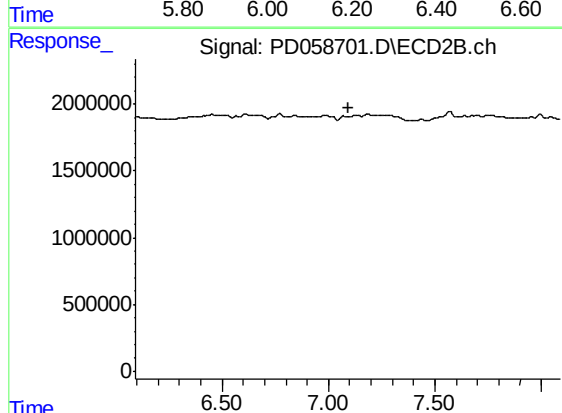


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.092 min
Response: 0
Conc: N.D.

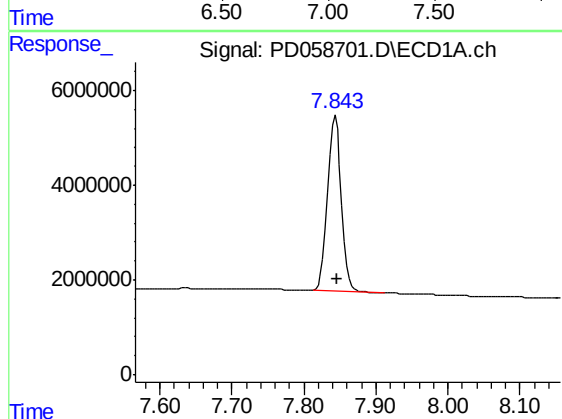

#27 Decachlorobiphenyl

R.T.: 7.844 min
Delta R.T.: -0.003 min
Response: 49173671
Conc: 27.81 ng/ml

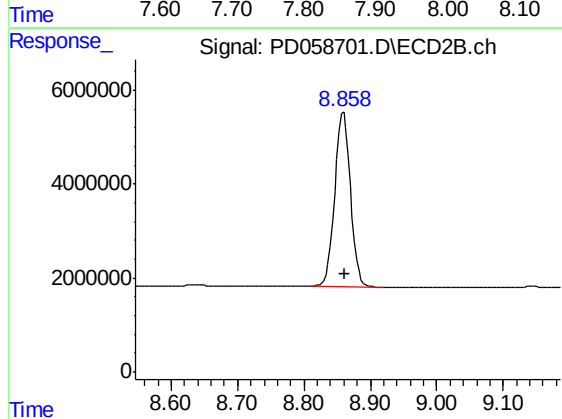

#27 Decachlorobiphenyl

R.T.: 8.860 min
Delta R.T.: -0.002 min
Response: 61026785
Conc: 28.72 ng/ml