

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072520\
 Data File : PD058677.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jul 2020 16:33
 Operator : AJ\MA
 Sample : L3388-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AD0

Manual Integrations
 APPROVED

Ankita
 7/27/2020 12:22:58 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 25 00:02:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070220CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 02 16:12:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.208	3.866	26079110	34730119	15.516	15.241
27)	SA Decachlor...	7.845	8.858	39672979	44660566	22.441	21.021m
Target Compounds							
11)	B cis-Chlor...	5.121	6.019	3722036	5079151	1.879m	1.936m
12)	B 4,4'-DDE	5.285	6.168	1021603	4179152	0.508m	1.628 #
13)	MA Dieldrin	5.402	6.318	25354713	10161296	14.703m	3.732m#
17)	MA 4,4'-DDT	6.029	6.962	2494802	2222338	1.758	0.986m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072520\
Data File : PD058677.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2020 16:33
Operator : AJ\MA
Sample : L3388-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 00:02:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070220CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 02 16:12:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

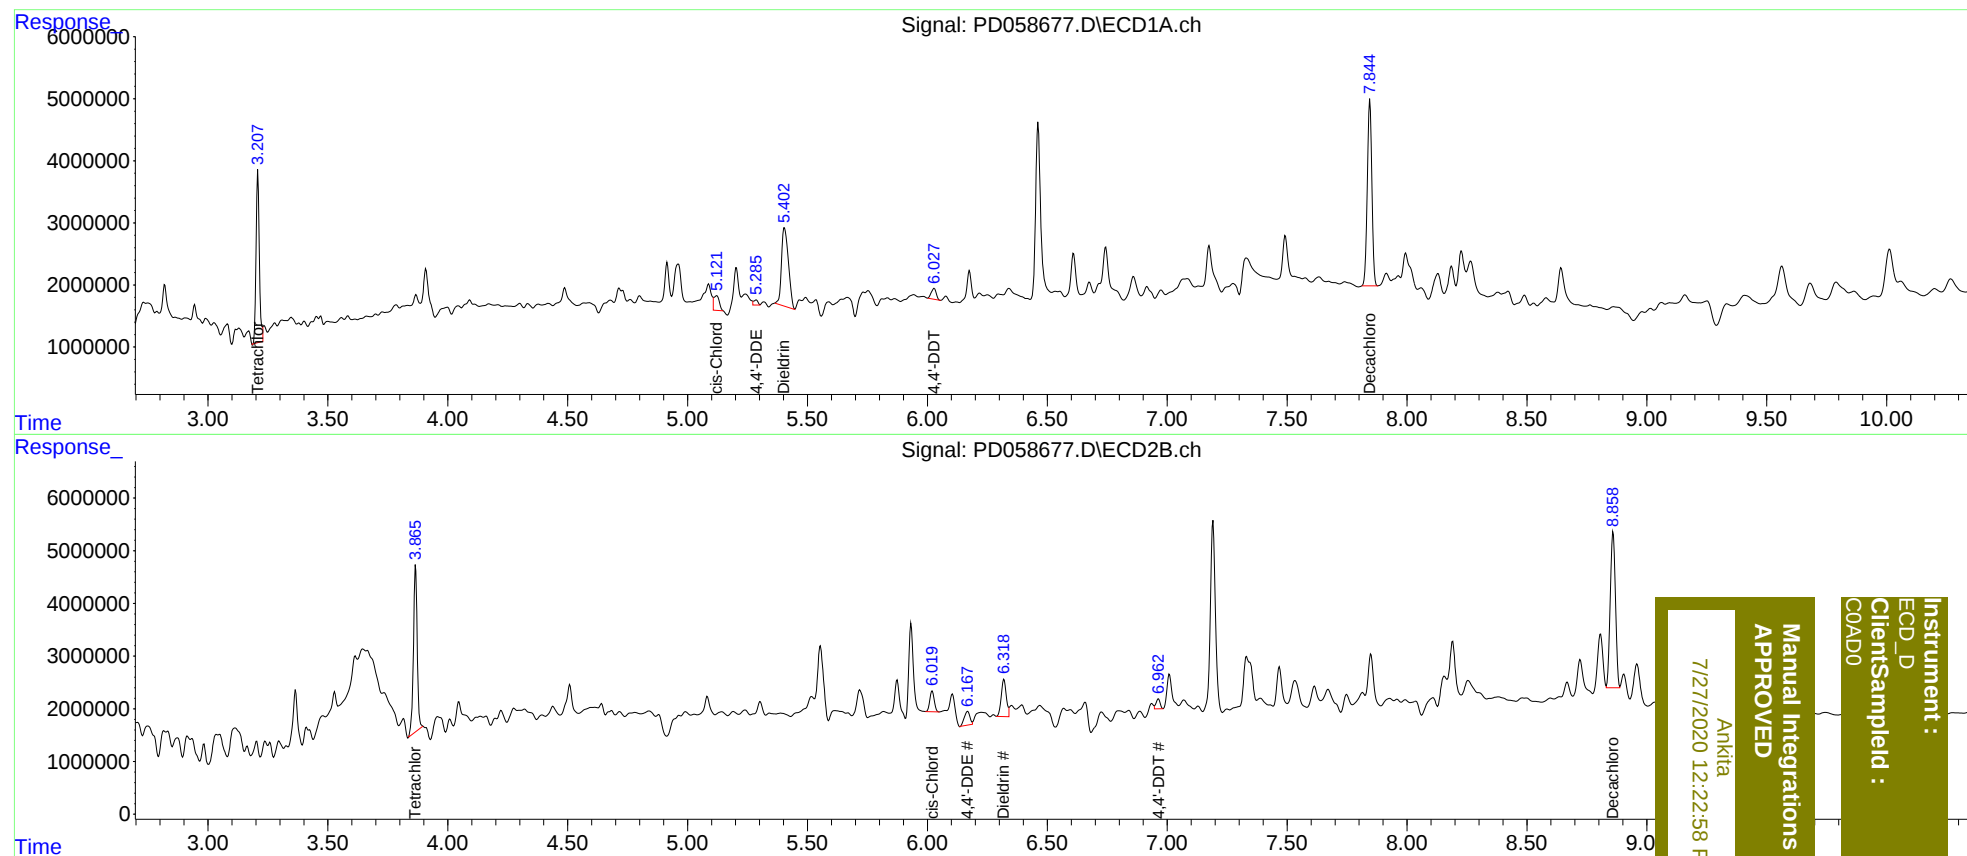

Manual Integrations
APPROVED

Ankita
7/27/2020 12:22:58 PM

Instrument :
ECD_D
Client Sample :
C0AD0