

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072524\
 Data File : PD084094.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jul 2024 17:42
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 25 04:58:19 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072524CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 25 04:52:51 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.561	2.771	4350718	27546105	4.689	5.090
27)	SA Decachlor...	9.112	7.894	19882834	63644069	10.265	10.764
Target Compounds							
2)	A alpha-BHC	4.018	3.270	7699933	41959616	4.613	4.851
3)	MA gamma-BHC...	4.351	3.598	7963032	39015137	4.775	4.751
4)	MA Heptachlor	4.944	3.936	8927042	39054221	4.834	4.889
9)	A Endosulfan I	6.102	5.084	8597567	33183886	4.937	5.004
13)	MA Dieldrin	6.377	5.348	17848073	71319836	9.511	9.766
14)	MA Endrin	6.609	5.624	15093930	61486907	9.598	9.925
16)	A 4,4'-DDD	6.742	5.770	12397935	52701852	9.358	9.676
17)	MA 4,4'-DDT	7.057	6.021	12624373	48323025	9.118	8.984
20)	A Methoxychlor	7.533	6.595	41623034	140.8E6	49.723	52.583


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072524\
Data File : PD084094.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2024 17:42
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 04:58:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072524CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 25 04:52:51 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

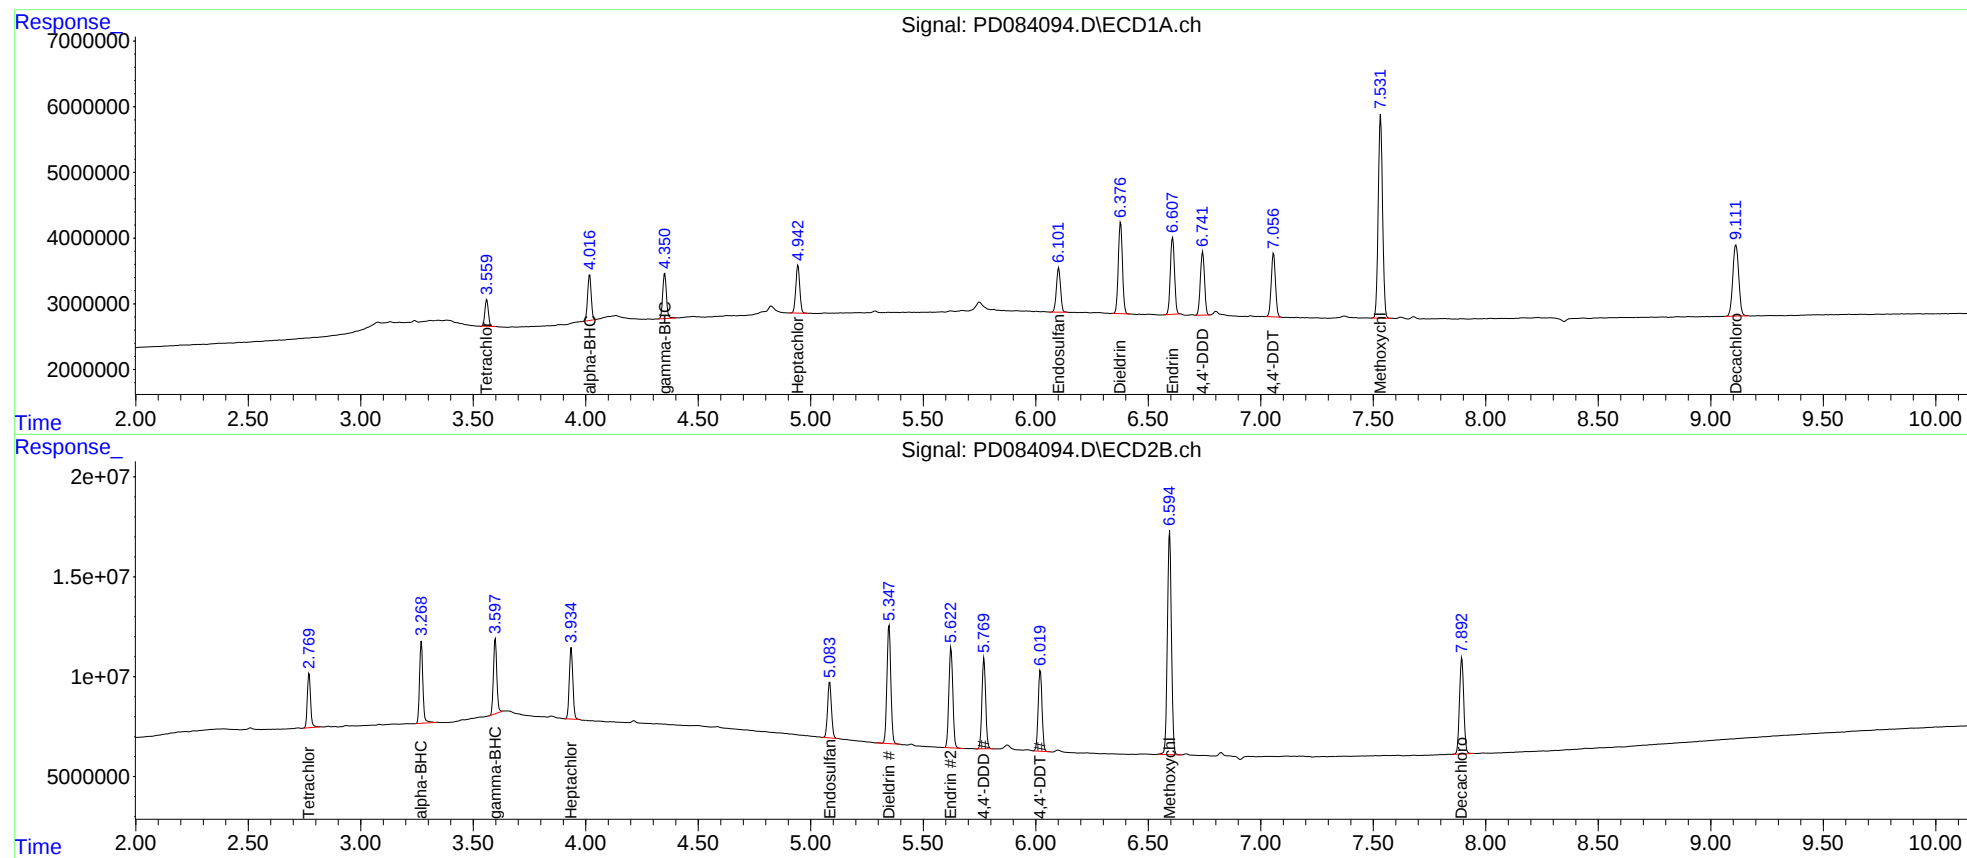

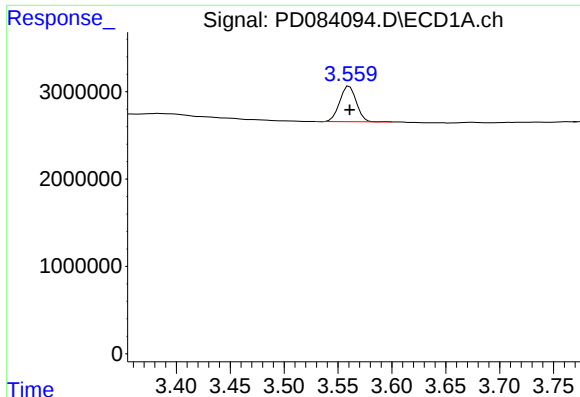


#1 Tetrachloro-m-xylene

R.T.: 3.561 min
Delta R.T.: 0.000 min
Response: 4350718
Conc: 4.69 ng/ml

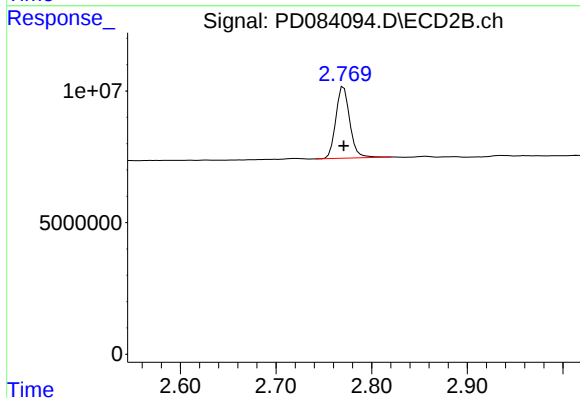


#1 Tetrachloro-m-xylene

R.T.: 2.771 min
Delta R.T.: 0.000 min
Response: 27546105
Conc: 5.09 ng/ml

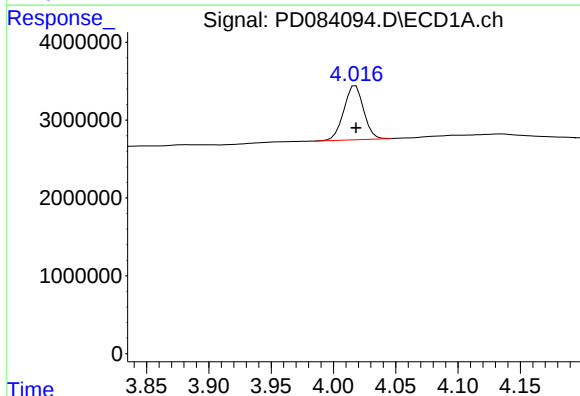


#2 alpha-BHC

R.T.: 4.018 min
Delta R.T.: 0.000 min
Response: 7699933
Conc: 4.61 ng/ml

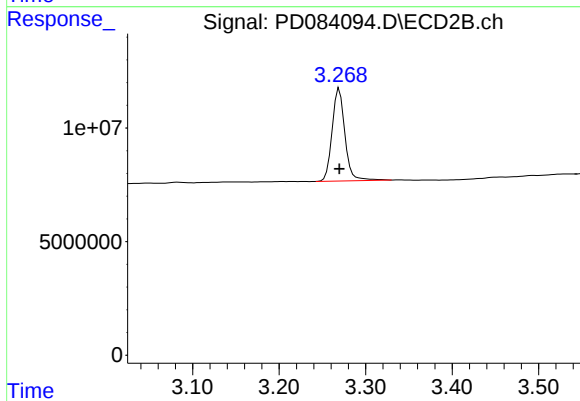


#2 alpha-BHC

R.T.: 3.270 min
Delta R.T.: 0.000 min
Response: 41959616
Conc: 4.85 ng/ml

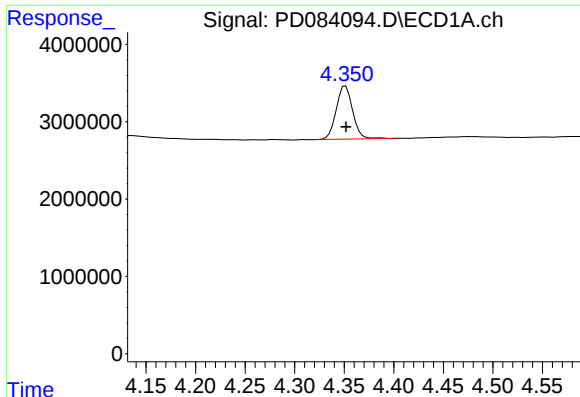


#3 gamma-BHC (Lindane)

R.T.: 4.351 min
Delta R.T.: 0.000 min
Response: 7963032
Conc: 4.78 ng/ml

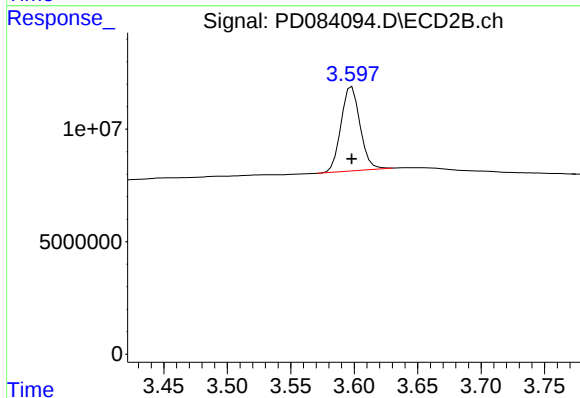


#3 gamma-BHC (Lindane)

R.T.: 3.598 min
Delta R.T.: 0.000 min
Response: 39015137
Conc: 4.75 ng/ml

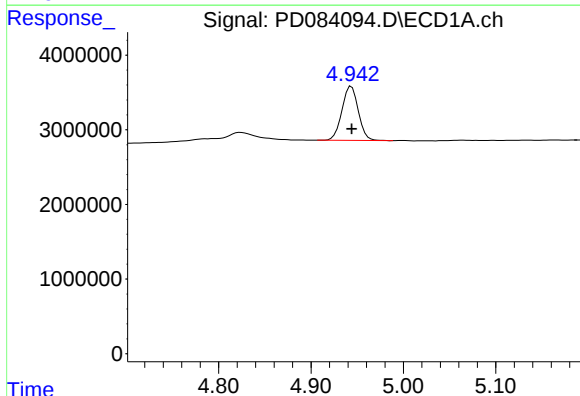


#4 Heptachlor

R.T.: 4.944 min
Delta R.T.: 0.000 min
Response: 8927042
Conc: 4.83 ng/ml

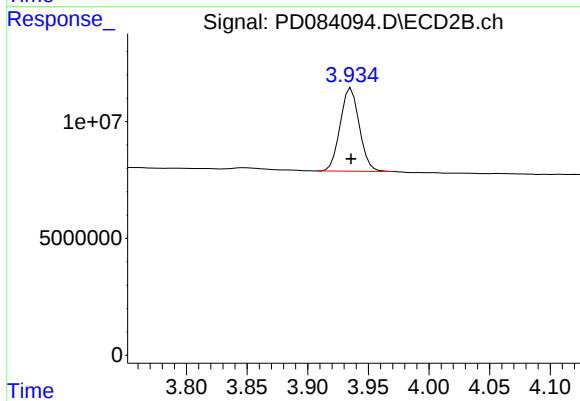


#4 Heptachlor

R.T.: 3.936 min
Delta R.T.: 0.000 min
Response: 39054221
Conc: 4.89 ng/ml

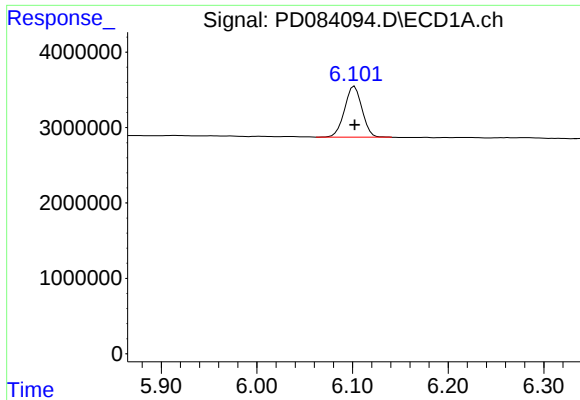


#9 Endosulfan I

R.T.: 6.102 min
Delta R.T.: 0.000 min
Response: 8597567
Conc: 4.94 ng/ml

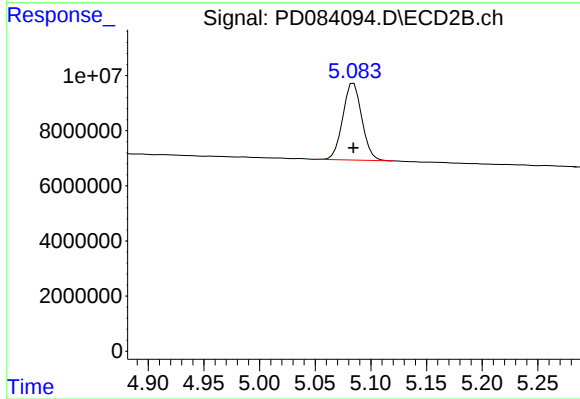


#9 Endosulfan I

R.T.: 5.084 min
Delta R.T.: 0.000 min
Response: 33183886
Conc: 5.00 ng/ml

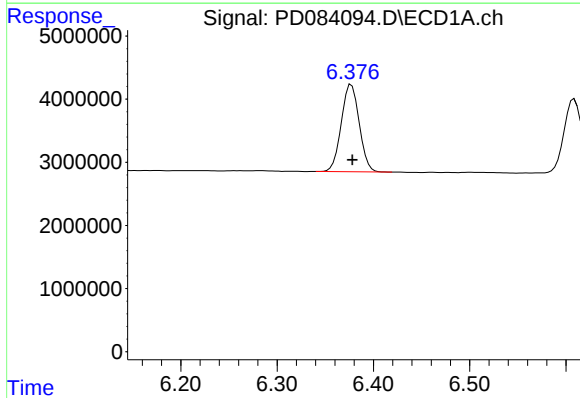


#13 Dieldrin

R.T.: 6.377 min
Delta R.T.: -0.001 min
Response: 17848073
Conc: 9.51 ng/ml

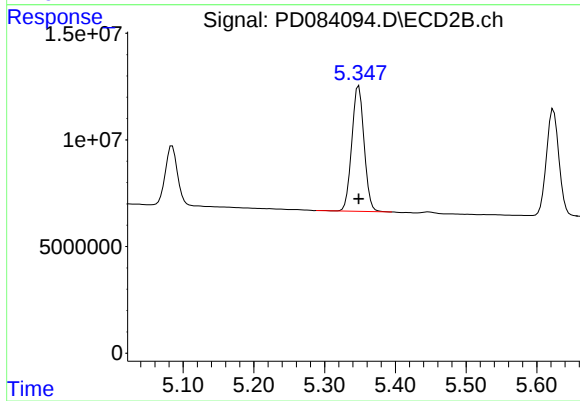


#13 Dieldrin

R.T.: 5.348 min
Delta R.T.: 0.000 min
Response: 71319836
Conc: 9.77 ng/ml

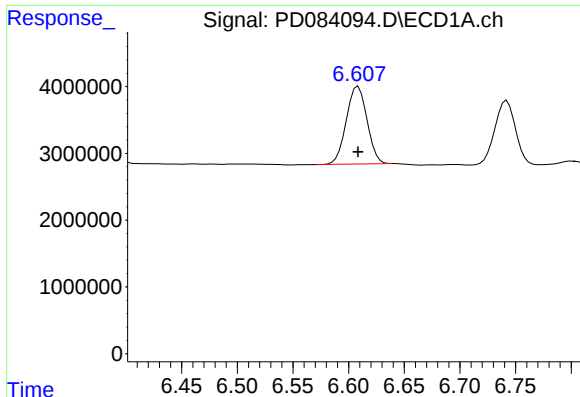


#14 Endrin

R.T.: 6.609 min
Delta R.T.: 0.000 min
Response: 15093930
Conc: 9.60 ng/ml

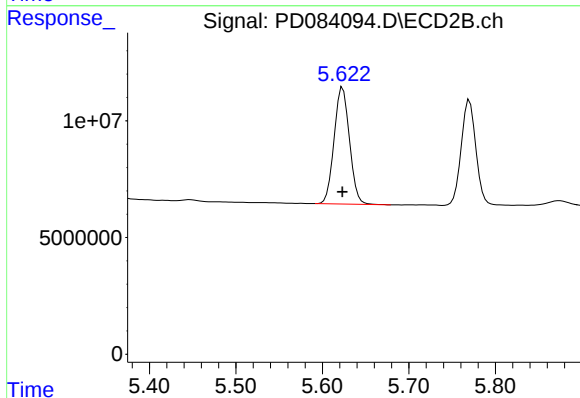


#14 Endrin

R.T.: 5.624 min
Delta R.T.: 0.000 min
Response: 61486907
Conc: 9.92 ng/ml

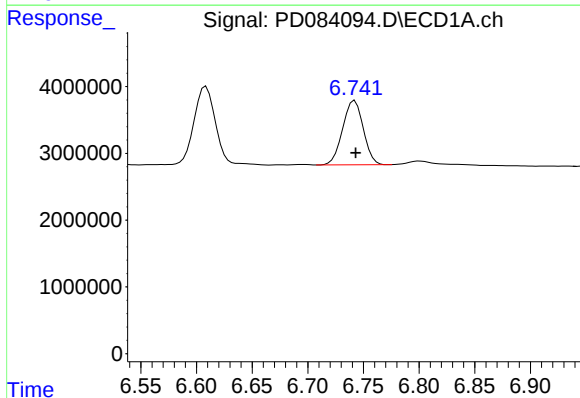


#16 4,4'-DDD

R.T.: 6.742 min
Delta R.T.: 0.000 min
Response: 12397935
Conc: 9.36 ng/ml

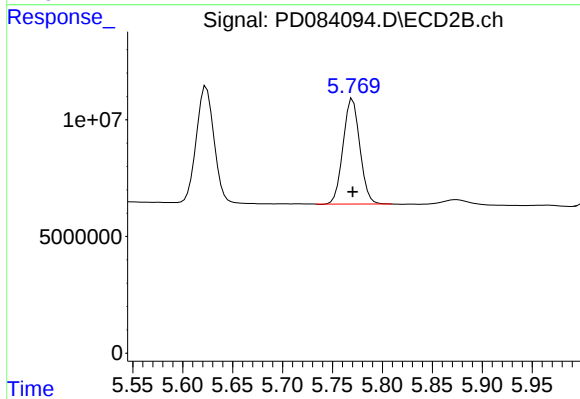


#16 4,4'-DDD

R.T.: 5.770 min
Delta R.T.: 0.000 min
Response: 52701852
Conc: 9.68 ng/ml

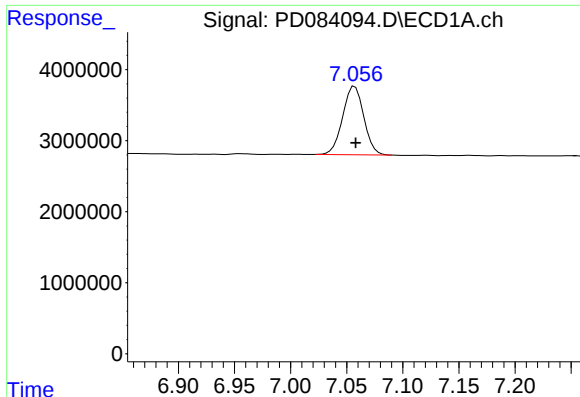


#17 4,4'-DDT

R.T.: 7.057 min
Delta R.T.: 0.000 min
Response: 12624373
Conc: 9.12 ng/ml

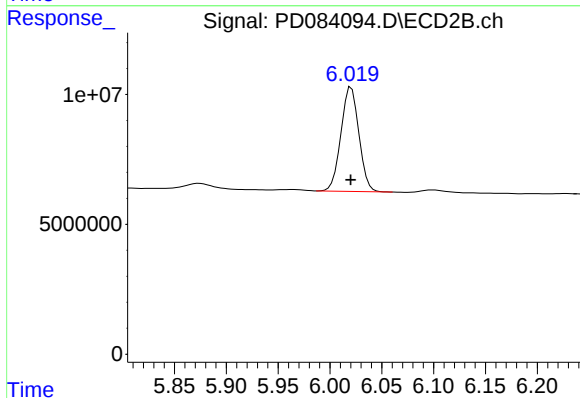


#17 4,4'-DDT

R.T.: 6.021 min
Delta R.T.: 0.000 min
Response: 48323025
Conc: 8.98 ng/ml

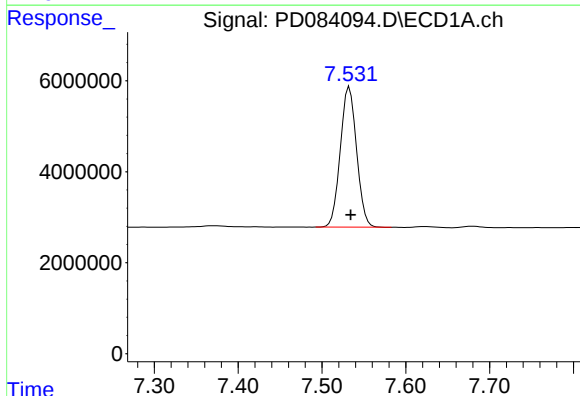


#20 Methoxychlor

R.T.: 7.533 min
Delta R.T.: -0.002 min
Response: 41623034
Conc: 49.72 ng/ml

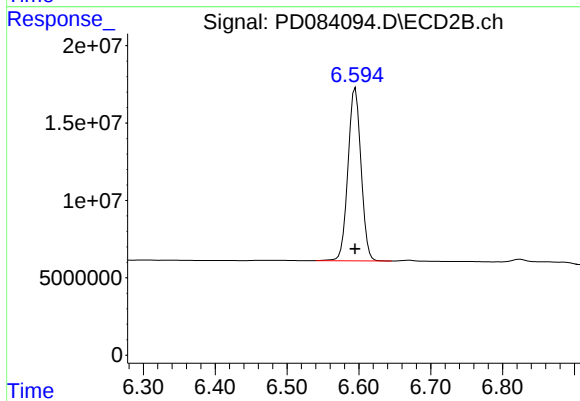


#20 Methoxychlor

R.T.: 6.595 min
Delta R.T.: 0.000 min
Response: 140781227
Conc: 52.58 ng/ml

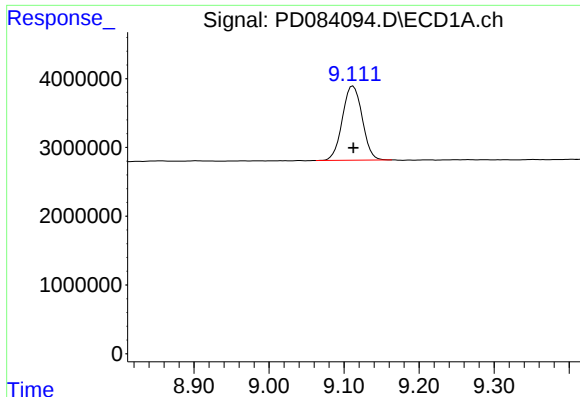

#27 Decachlorobiphenyl

R.T.: 9.112 min
Delta R.T.: 0.000 min
Response: 19882834
Conc: 10.27 ng/ml

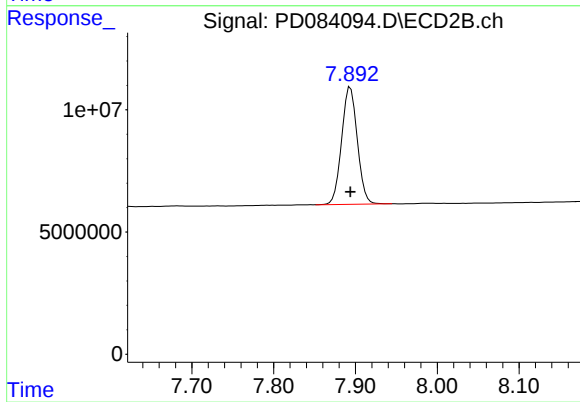

#27 Decachlorobiphenyl

R.T.: 7.894 min
Delta R.T.: 0.000 min
Response: 63644069
Conc: 10.76 ng/ml