

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072524\
 Data File : PD084096.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jul 2024 18:09
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 25 04:58:36 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072524CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 25 04:52:51 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.561	2.771	9195806	54690370	9.911	10.106
27)	SA Decachlor...	9.112	7.893	39289525	122.7E6	20.285	20.756
Target Compounds							
2)	A alpha-BHC	4.018	3.270	16156062	85316633	9.678	9.863
3)	MA gamma-BHC...	4.352	3.598	16294347	80948203	9.771	9.858
4)	MA Heptachlor	4.943	3.936	18243522	79112034	9.879	9.904
9)	A Endosulfan I	6.102	5.085	17484256	66516004	10.040	10.031
13)	MA Dieldrin	6.377	5.348	36618296	146.2E6	19.513	20.018
14)	MA Endrin	6.608	5.623	30879355	124.5E6	19.635	20.101
16)	A 4,4'-DDD	6.742	5.770	25643027	107.7E6	19.356	19.782
17)	MA 4,4'-DDT	7.057	6.020	26268939	102.5E6	18.973	19.057
20)	A Methoxychlor	7.533	6.595	83741454	277.8E6	100.038	103.747


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072524\
Data File : PD084096.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2024 18:09
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 04:58:36 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072524CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 25 04:52:51 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

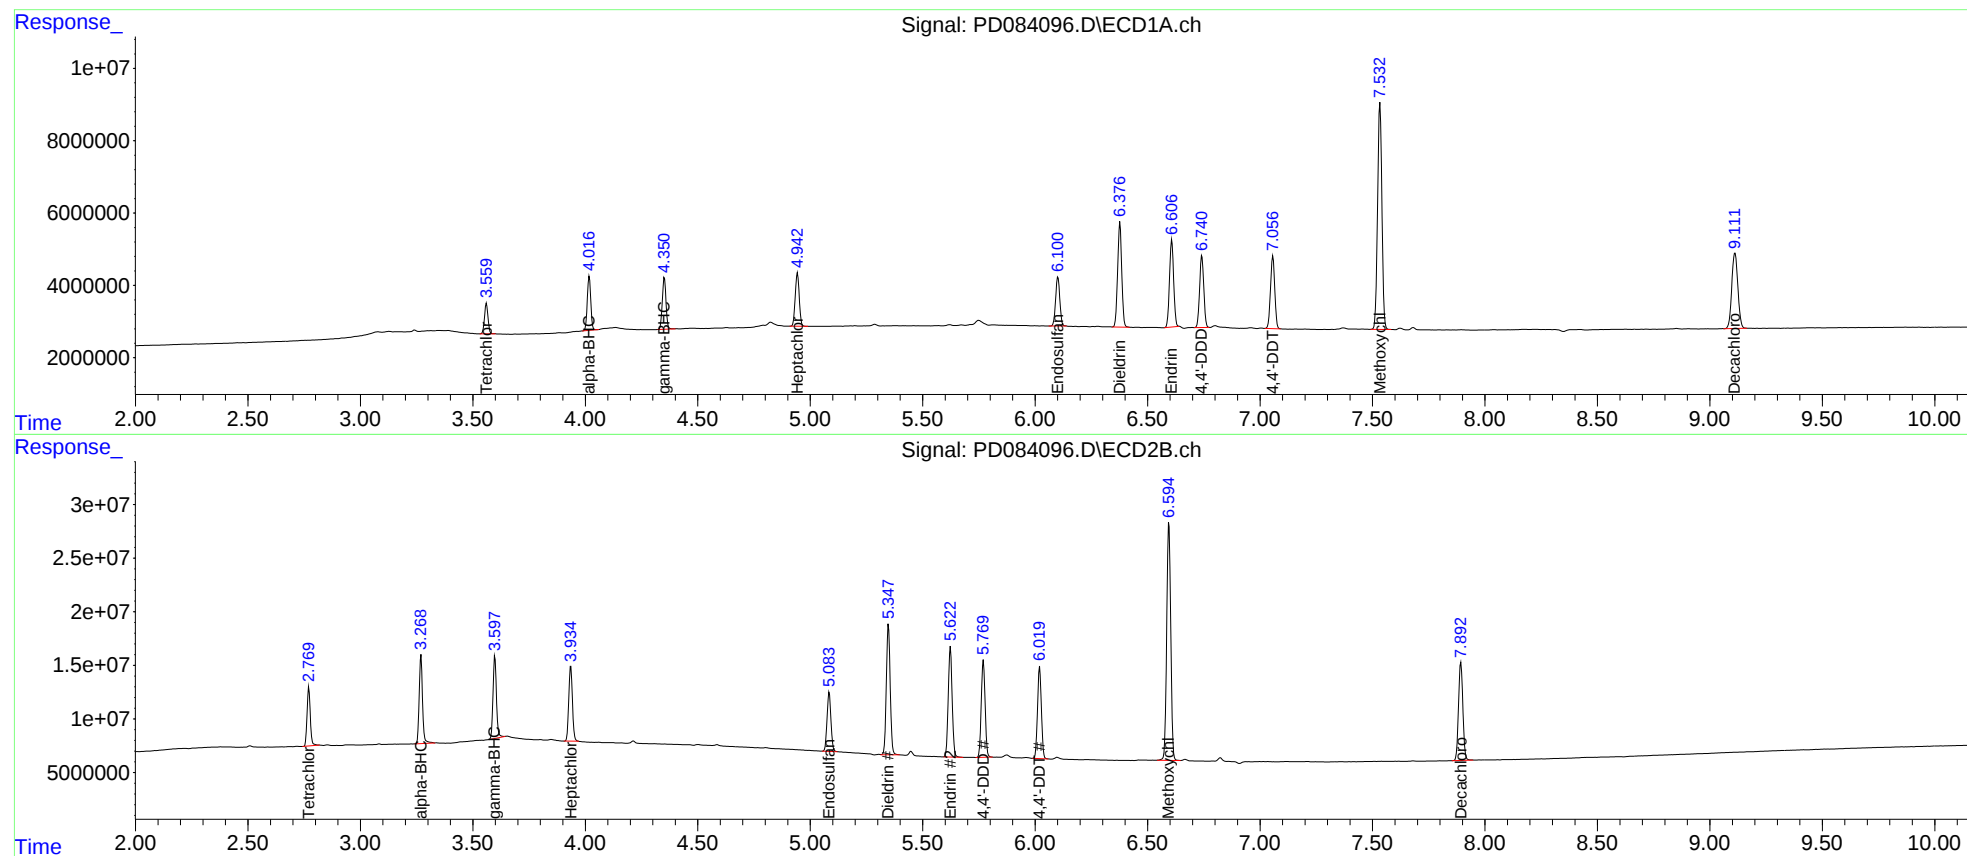

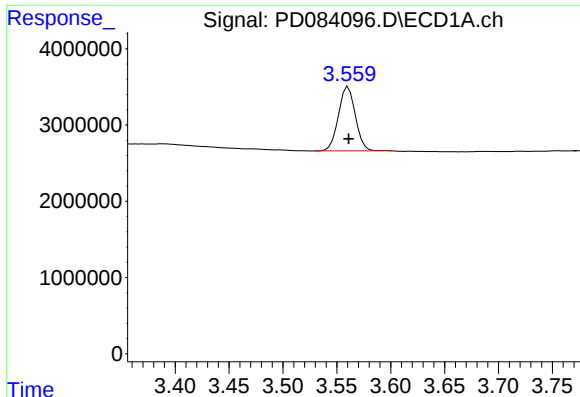


#1 Tetrachloro-m-xylene

R.T.: 3.561 min
Delta R.T.: 0.000 min
Response: 9195806
Conc: 9.91 ng/ml

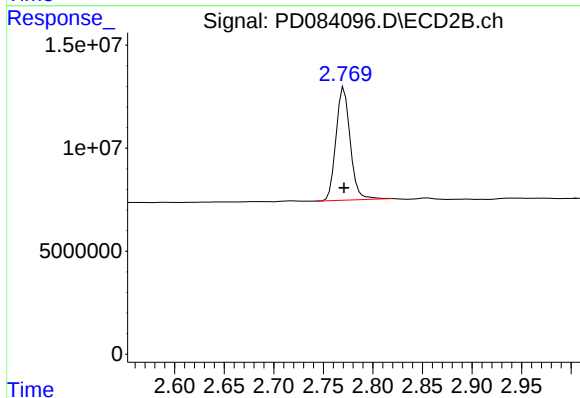


#1 Tetrachloro-m-xylene

R.T.: 2.771 min
Delta R.T.: 0.000 min
Response: 54690370
Conc: 10.11 ng/ml

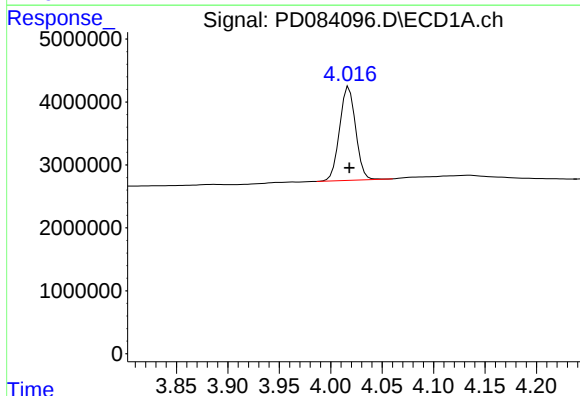


#2 alpha-BHC

R.T.: 4.018 min
Delta R.T.: 0.000 min
Response: 16156062
Conc: 9.68 ng/ml

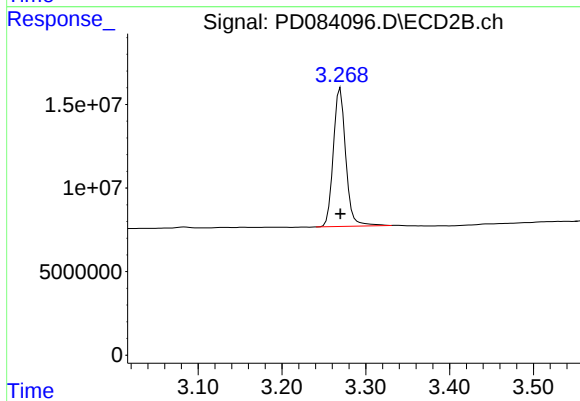


#2 alpha-BHC

R.T.: 3.270 min
Delta R.T.: 0.000 min
Response: 85316633
Conc: 9.86 ng/ml

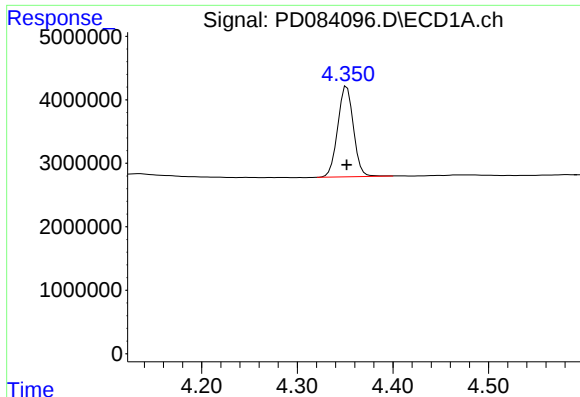


#3 gamma-BHC (Lindane)

R.T.: 4.352 min
Delta R.T.: 0.000 min
Response: 16294347
Conc: 9.77 ng/ml

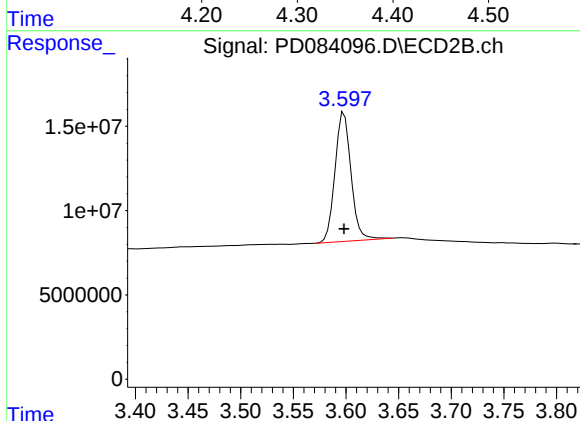


#3 gamma-BHC (Lindane)

R.T.: 3.598 min
Delta R.T.: 0.000 min
Response: 80948203
Conc: 9.86 ng/ml

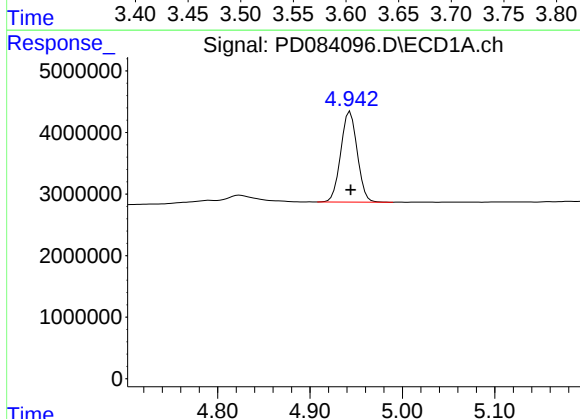


#4 Heptachlor

R.T.: 4.943 min
Delta R.T.: 0.000 min
Response: 18243522
Conc: 9.88 ng/ml

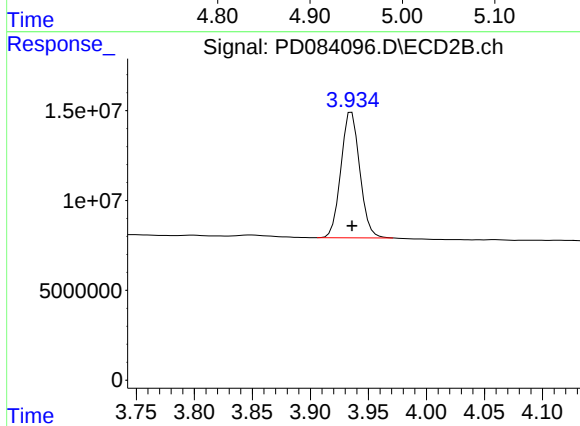


#4 Heptachlor

R.T.: 3.936 min
Delta R.T.: 0.000 min
Response: 79112034
Conc: 9.90 ng/ml

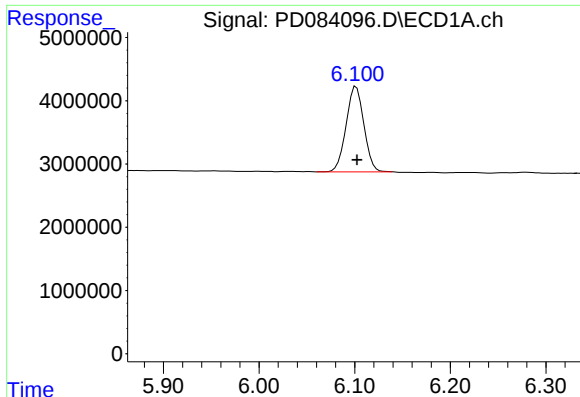


#9 Endosulfan I

R.T.: 6.102 min
Delta R.T.: 0.000 min
Response: 17484256
Conc: 10.04 ng/ml

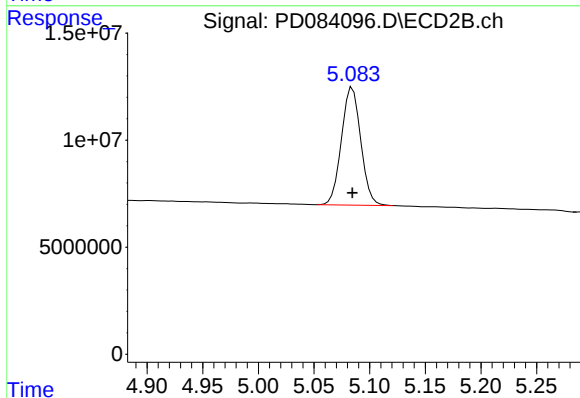


#9 Endosulfan I

R.T.: 5.085 min
Delta R.T.: 0.000 min
Response: 66516004
Conc: 10.03 ng/ml

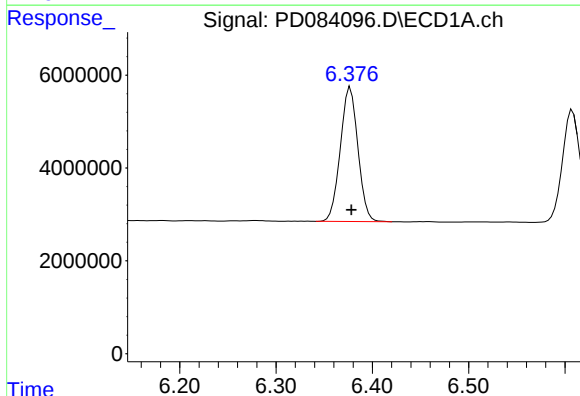


#13 Dieldrin

R.T.: 6.377 min
Delta R.T.: -0.001 min
Response: 36618296
Conc: 19.51 ng/ml

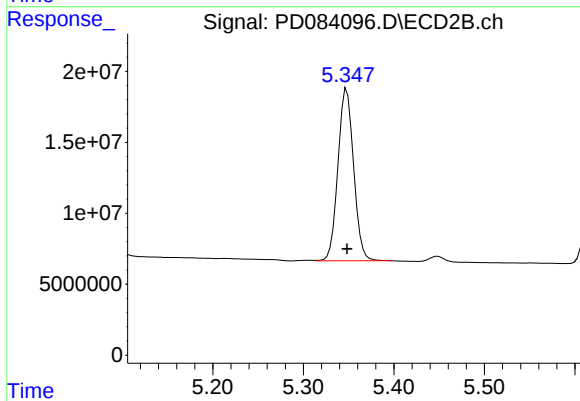


#13 Dieldrin

R.T.: 5.348 min
Delta R.T.: 0.000 min
Response: 146185323
Conc: 20.02 ng/ml

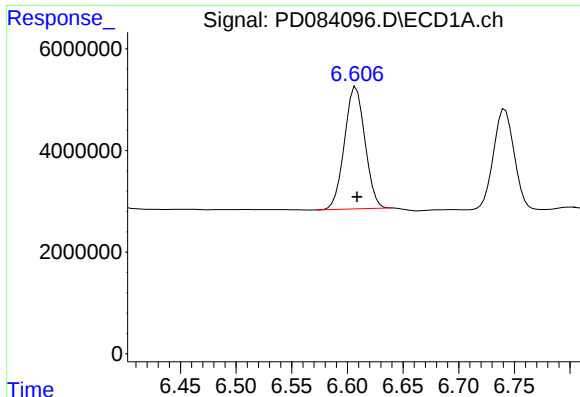


#14 Endrin

R.T.: 6.608 min
Delta R.T.: 0.000 min
Response: 30879355
Conc: 19.64 ng/ml

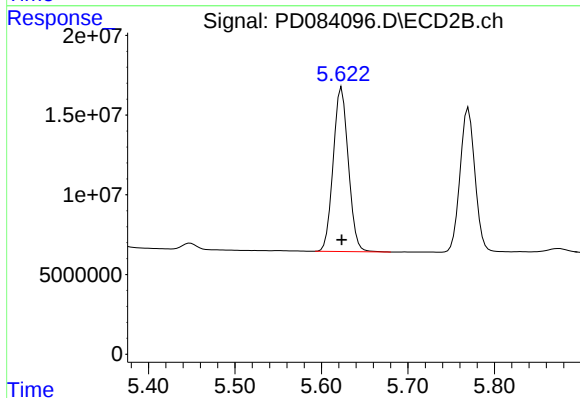


#14 Endrin

R.T.: 5.623 min
Delta R.T.: 0.000 min
Response: 124532865
Conc: 20.10 ng/ml

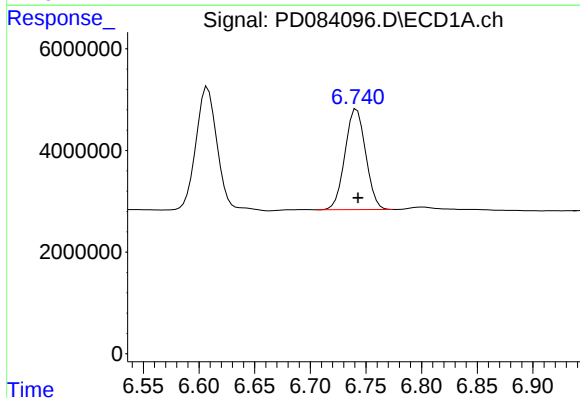


#16 4,4'-DDD

R.T.: 6.742 min
Delta R.T.: -0.001 min
Response: 25643027
Conc: 19.36 ng/ml

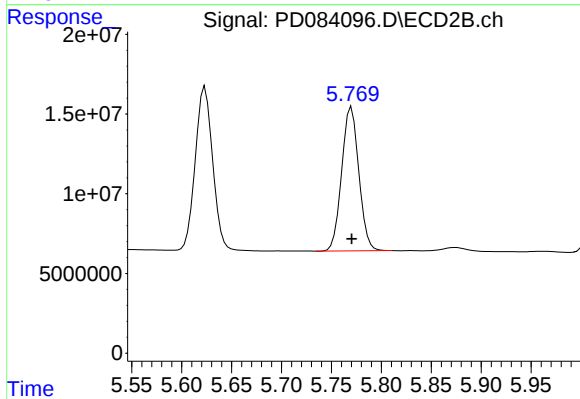


#16 4,4'-DDD

R.T.: 5.770 min
Delta R.T.: 0.000 min
Response: 107746184
Conc: 19.78 ng/ml

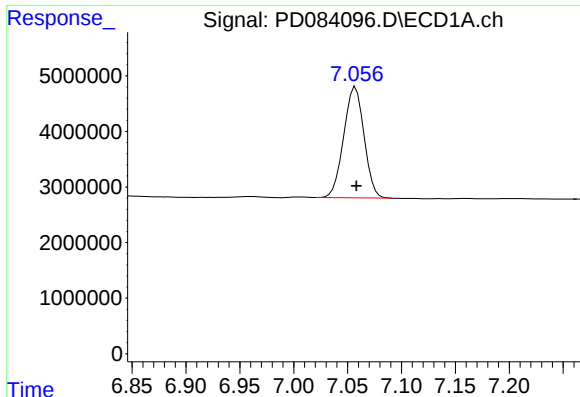


#17 4,4'-DDT

R.T.: 7.057 min
Delta R.T.: 0.000 min
Response: 26268939
Conc: 18.97 ng/ml

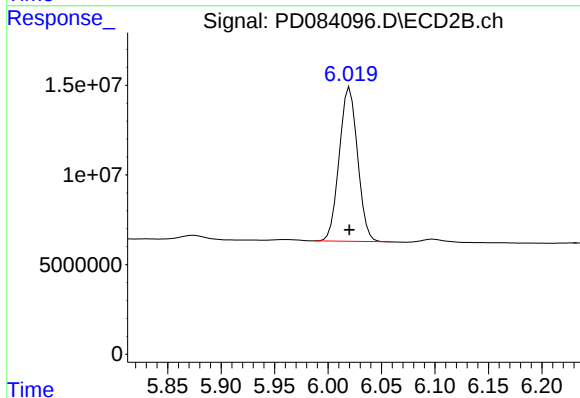


#17 4,4'-DDT

R.T.: 6.020 min
Delta R.T.: 0.000 min
Response: 102509576
Conc: 19.06 ng/ml

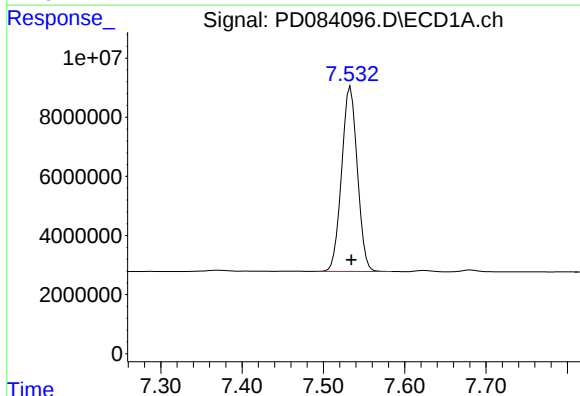


#20 Methoxychlor

R.T.: 7.533 min
Delta R.T.: 0.000 min
Response: 83741454
Conc: 100.04 ng/ml

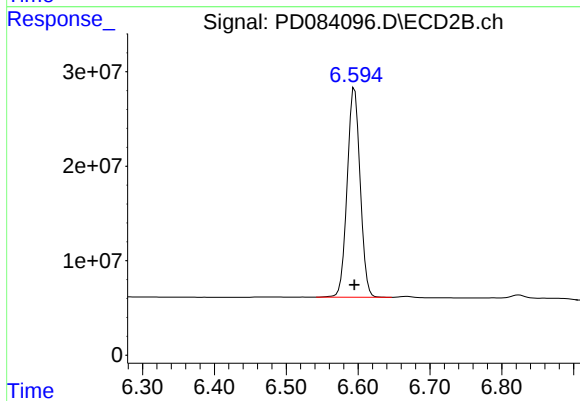

#20 Methoxychlor

R.T.: 6.595 min
Delta R.T.: 0.000 min
Response: 277765662
Conc: 103.75 ng/ml

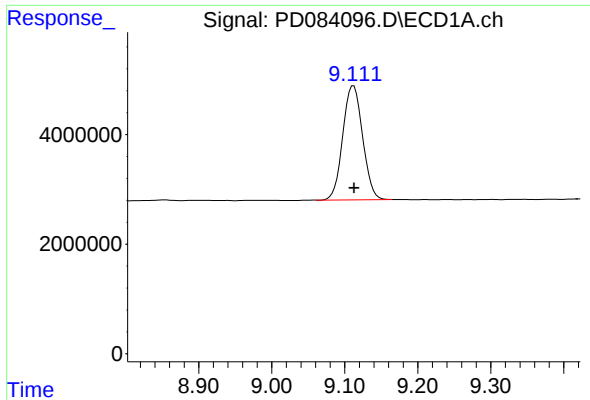


#27 Decachlorobiphenyl

R.T.: 9.112 min

Delta R.T.: 0.000 min

Response: 39289525

Conc: 20.28 ng/ml

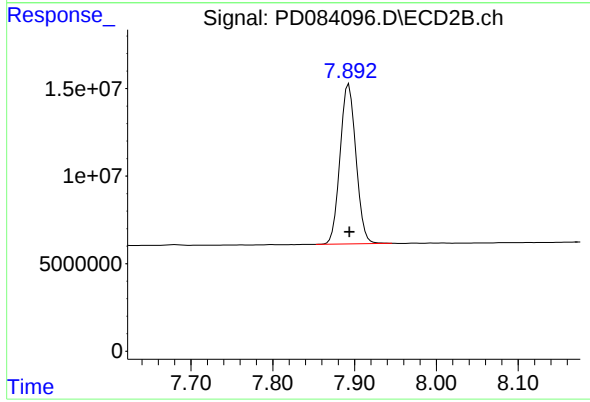

#27 Decachlorobiphenyl

R.T.: 7.893 min

Delta R.T.: 0.000 min

Response: 122724534

Conc: 20.76 ng/ml