

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072524\
 Data File : PD084098.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jul 2024 18:35
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 25 04:58:52 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072524CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 25 04:52:51 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.561	2.771	18556820	108.2E6	20.000	20.000
27)	SA Decachlor...	9.113	7.894	77476538	236.5E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	4.018	3.270	33385478	173.0E6	20.000	20.000
3)	MA gamma-BHC...	4.352	3.598	33351862	164.2E6	20.000	20.000
4)	MA Heptachlor	4.944	3.936	36932168	159.8E6	20.000	20.000
9)	A Endosulfan I	6.102	5.084	34830893	132.6E6	20.000	20.000
13)	MA Dieldrin	6.378	5.348	75065930	292.1E6	40.000	40.000
14)	MA Endrin	6.609	5.623	62906117	247.8E6	40.000	40.000
16)	A 4,4'-DDD	6.743	5.770	52992626	217.9E6	40.000	40.000
17)	MA 4,4'-DDT	7.058	6.020	55382517	215.2E6	40.000	40.000
20)	A Methoxychlor	7.534	6.595	167.4E6	535.5E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072524\
Data File : PD084098.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2024 18:35
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 04:58:52 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072524CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 25 04:52:51 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

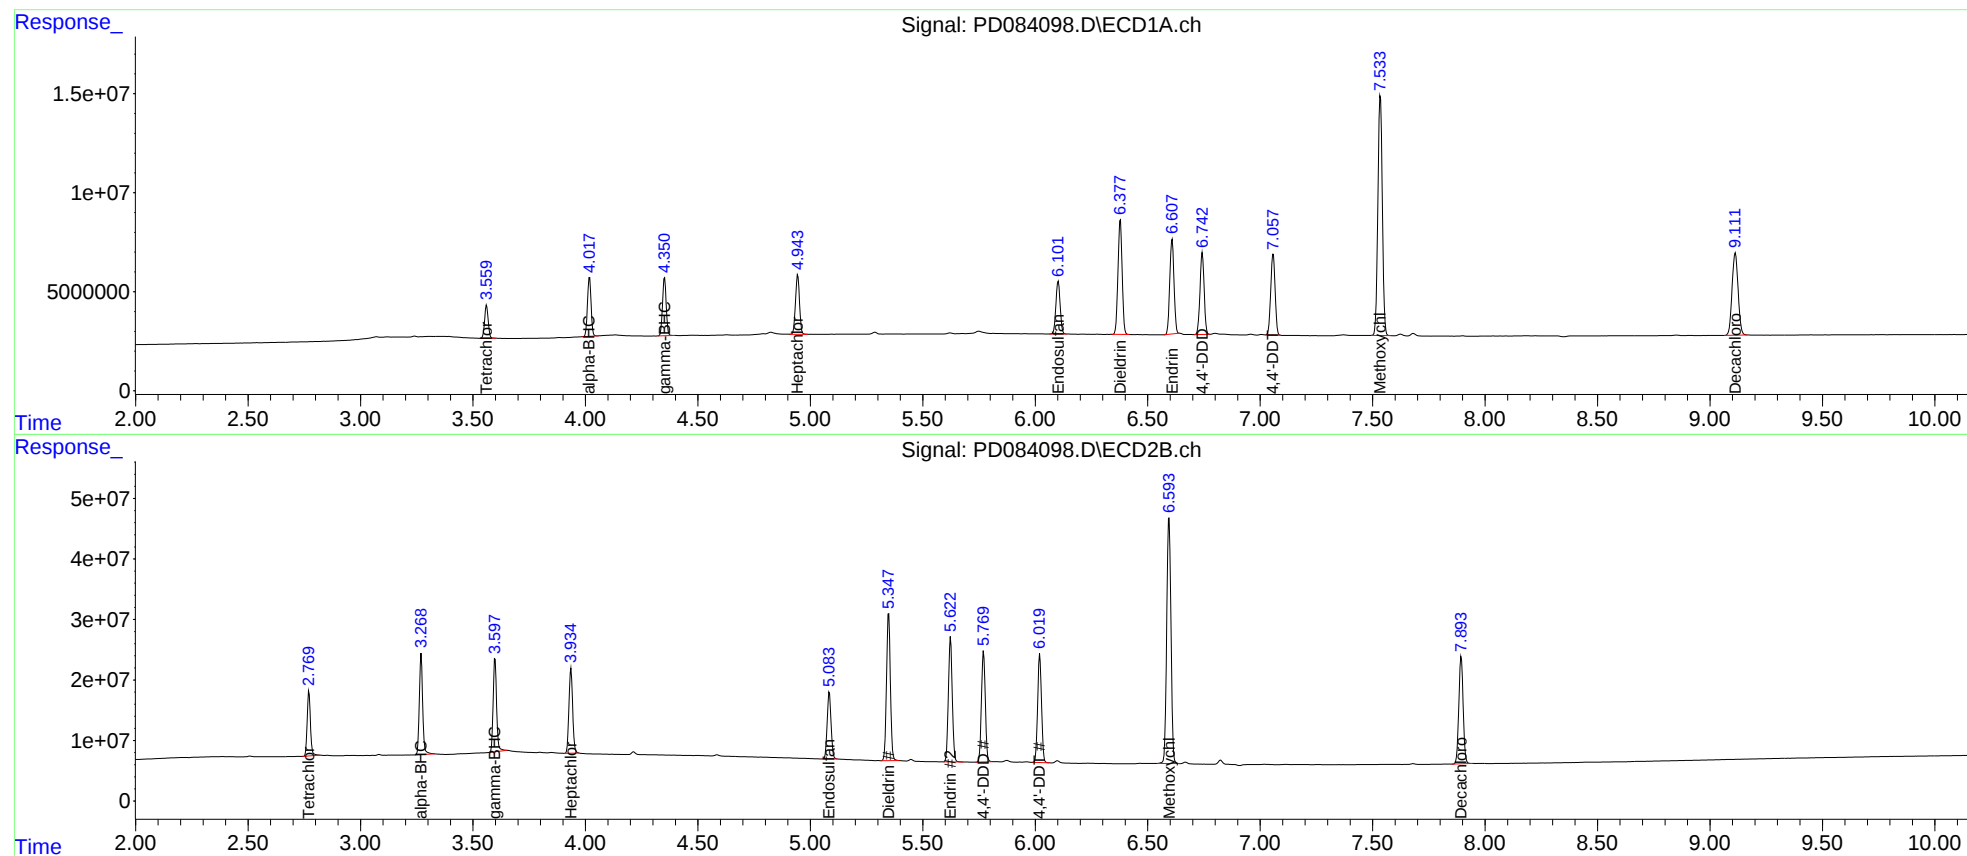

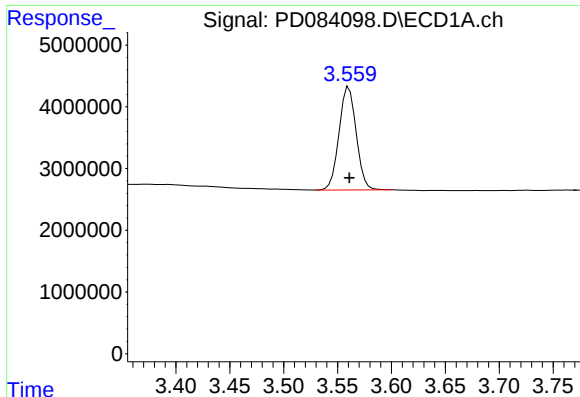


#1 Tetrachloro-m-xylene

R.T.: 3.561 min
Delta R.T.: 0.000 min
Response: 18556820
Conc: 20.00 ng/ml

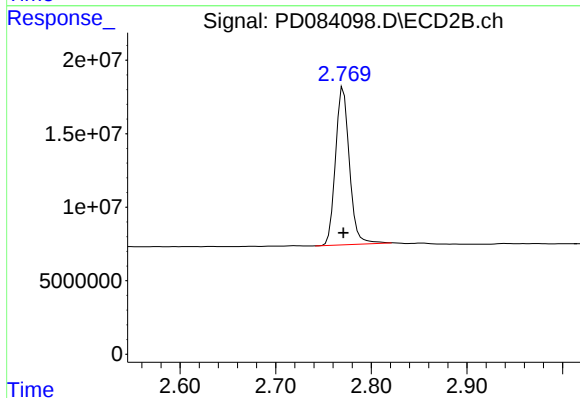


#1 Tetrachloro-m-xylene

R.T.: 2.771 min
Delta R.T.: 0.000 min
Response: 108234868
Conc: 20.00 ng/ml

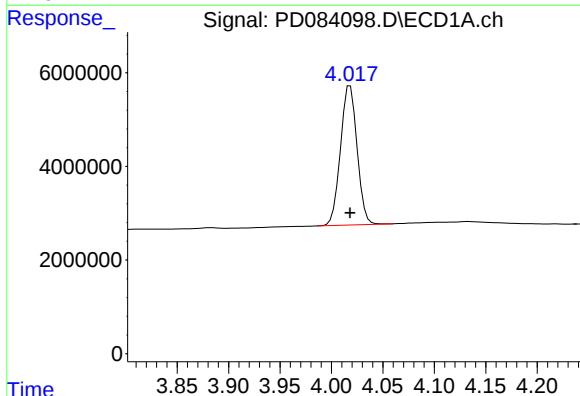


#2 alpha-BHC

R.T.: 4.018 min
Delta R.T.: 0.000 min
Response: 33385478
Conc: 20.00 ng/ml

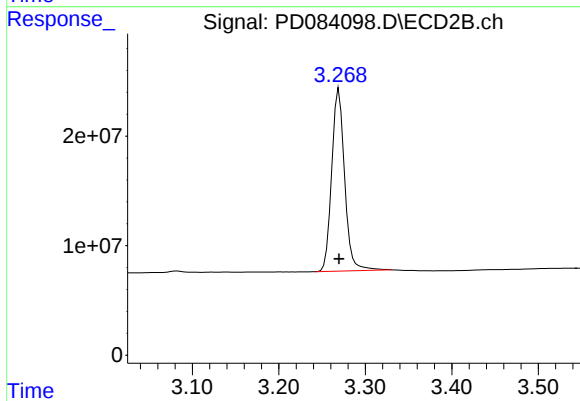


#2 alpha-BHC

R.T.: 3.270 min
Delta R.T.: 0.000 min
Response: 173001848
Conc: 20.00 ng/ml

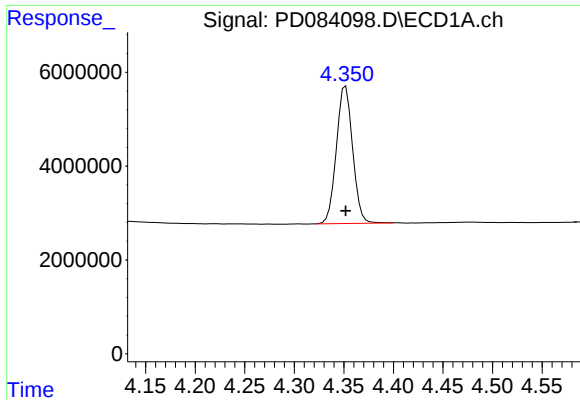


#3 gamma-BHC (Lindane)

R.T.: 4.352 min
Delta R.T.: 0.000 min
Response: 33351862
Conc: 20.00 ng/ml

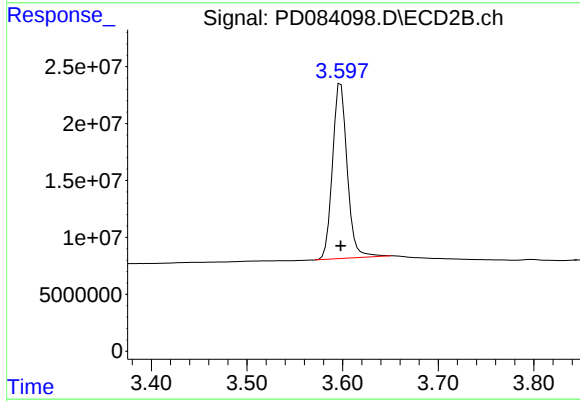


#3 gamma-BHC (Lindane)

R.T.: 3.598 min
Delta R.T.: 0.000 min
Response: 164227006
Conc: 20.00 ng/ml

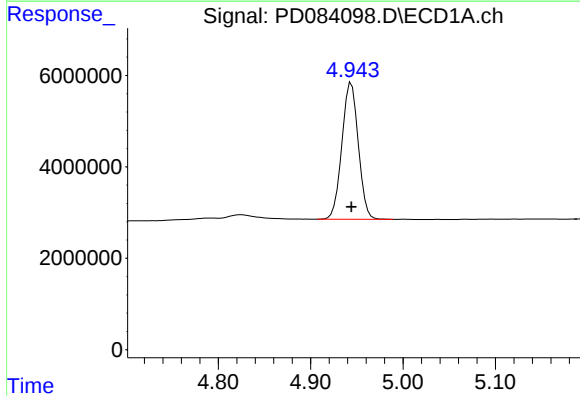


#4 Heptachlor

R.T.: 4.944 min
Delta R.T.: 0.000 min
Response: 36932168
Conc: 20.00 ng/ml

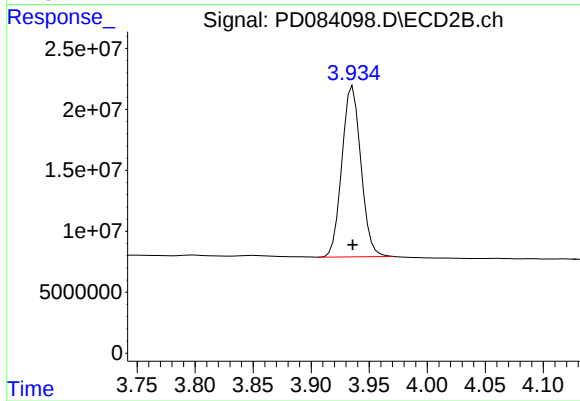


#4 Heptachlor

R.T.: 3.936 min
Delta R.T.: 0.000 min
Response: 159765788
Conc: 20.00 ng/ml

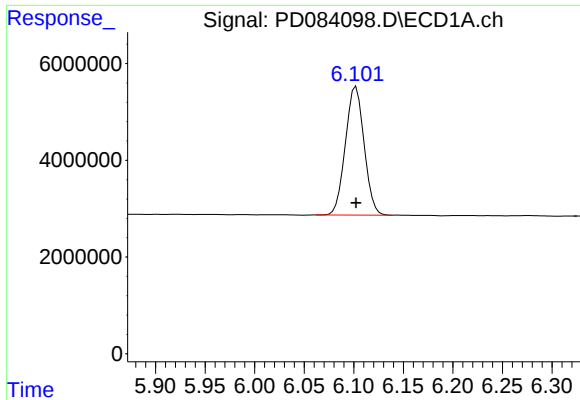


#9 Endosulfan I

R.T.: 6.102 min
Delta R.T.: 0.000 min
Response: 34830893
Conc: 20.00 ng/ml

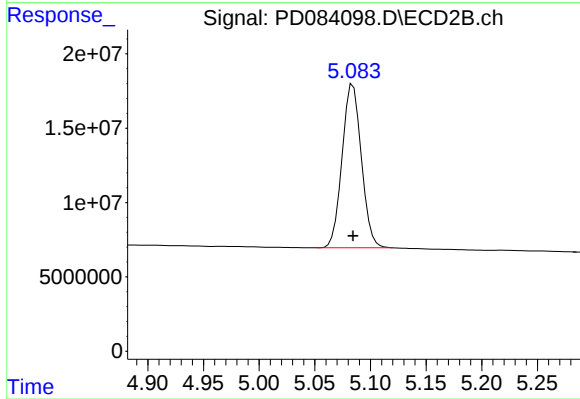


#9 Endosulfan I

R.T.: 5.084 min
Delta R.T.: 0.000 min
Response: 132616604
Conc: 20.00 ng/ml

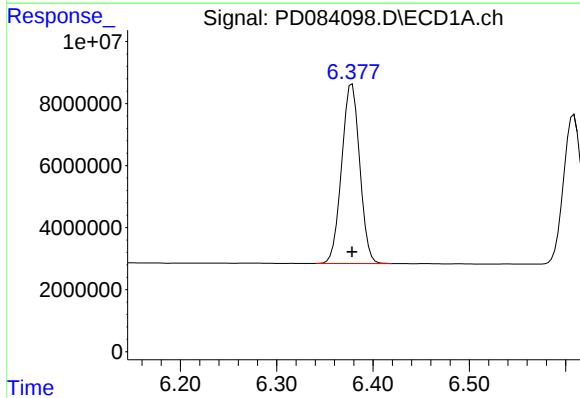


#13 Dieldrin

R.T.: 6.378 min
Delta R.T.: 0.000 min
Response: 75065930
Conc: 40.00 ng/ml

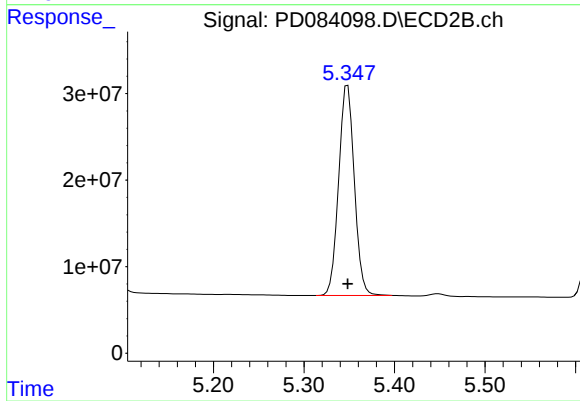


#13 Dieldrin

R.T.: 5.348 min
Delta R.T.: 0.000 min
Response: 292105926
Conc: 40.00 ng/ml

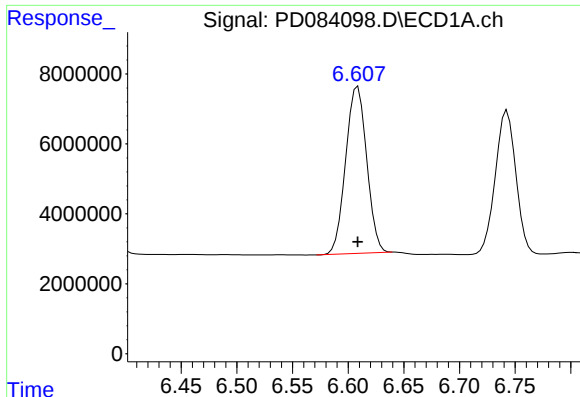


#14 Endrin

R.T.: 6.609 min
Delta R.T.: 0.000 min
Response: 62906117
Conc: 40.00 ng/ml

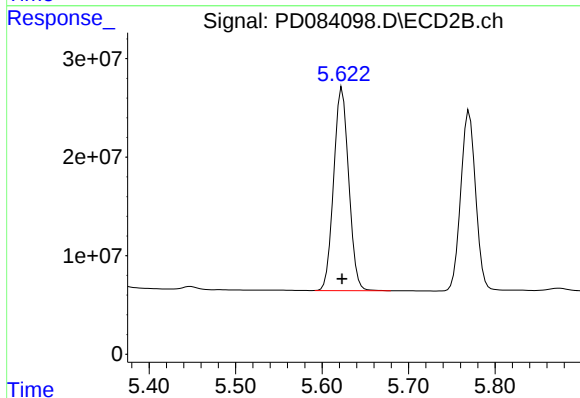


#14 Endrin

R.T.: 5.623 min
Delta R.T.: 0.000 min
Response: 247813519
Conc: 40.00 ng/ml

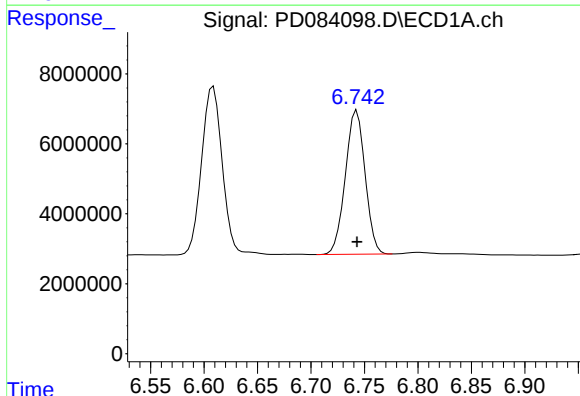


#16 4,4'-DDD

R.T.: 6.743 min
Delta R.T.: 0.000 min
Response: 52992626
Conc: 40.00 ng/ml

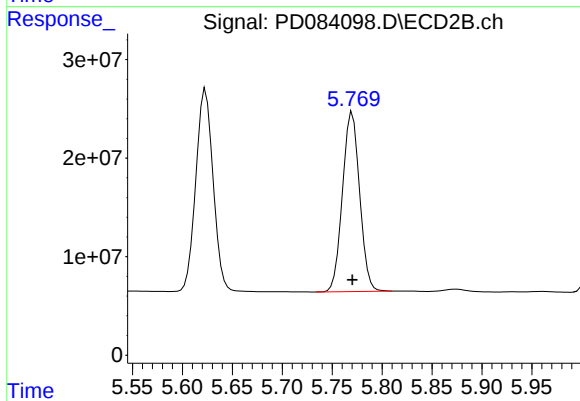


#16 4,4'-DDD

R.T.: 5.770 min
Delta R.T.: 0.000 min
Response: 217870044
Conc: 40.00 ng/ml

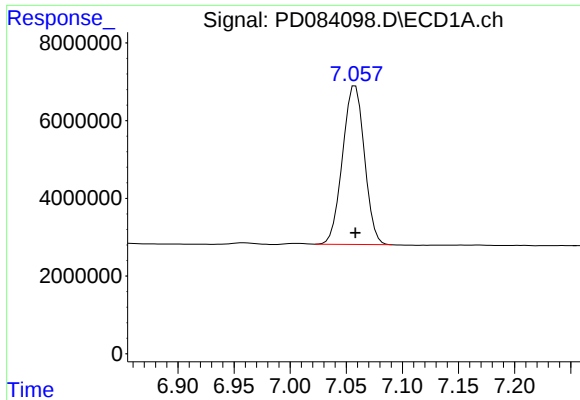


#17 4,4'-DDT

R.T.: 7.058 min
Delta R.T.: 0.000 min
Response: 55382517
Conc: 40.00 ng/ml

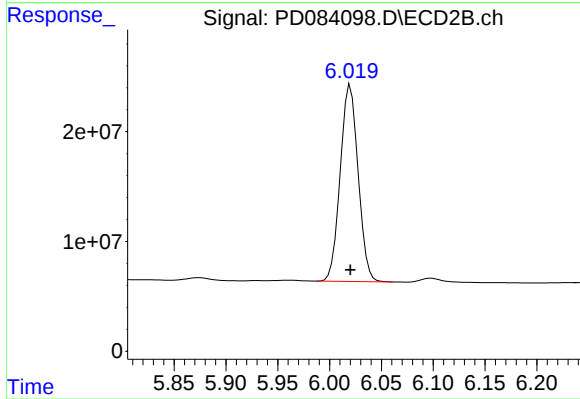


#17 4,4'-DDT

R.T.: 6.020 min
Delta R.T.: 0.000 min
Response: 215158968
Conc: 40.00 ng/ml

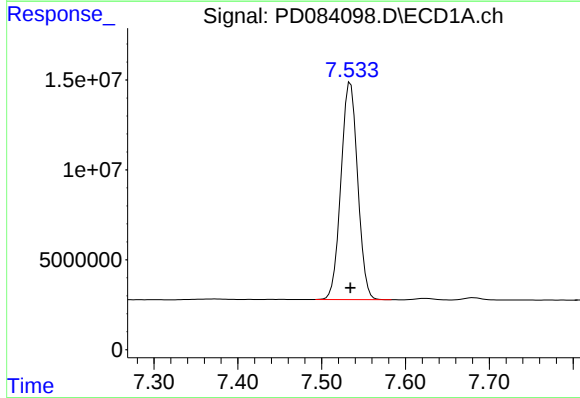


#20 Methoxychlor

R.T.: 7.534 min
Delta R.T.: 0.000 min
Response: 167418792
Conc: 200.00 ng/ml

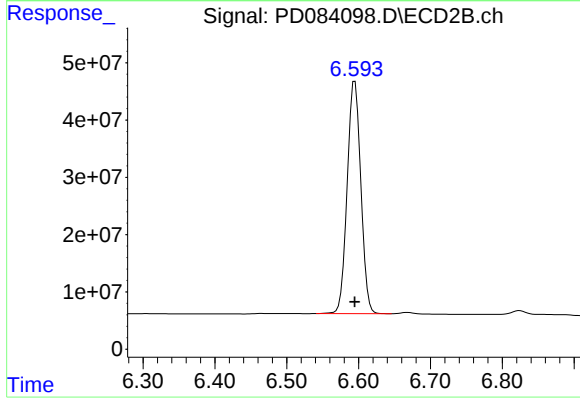


#20 Methoxychlor

R.T.: 6.595 min
Delta R.T.: 0.000 min
Response: 535465157
Conc: 200.00 ng/ml

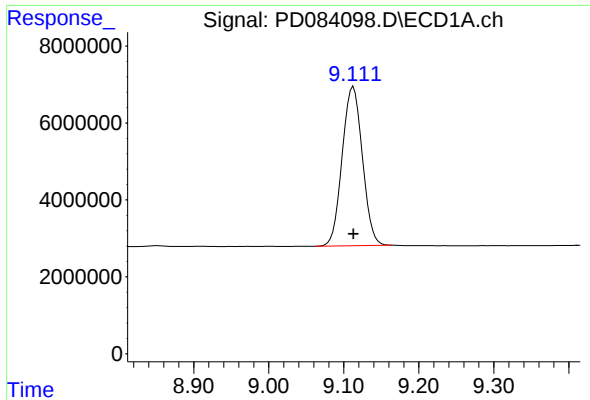

#27 Decachlorobiphenyl

R.T.: 9.113 min
Delta R.T.: 0.000 min
Response: 77476538
Conc: 40.00 ng/ml

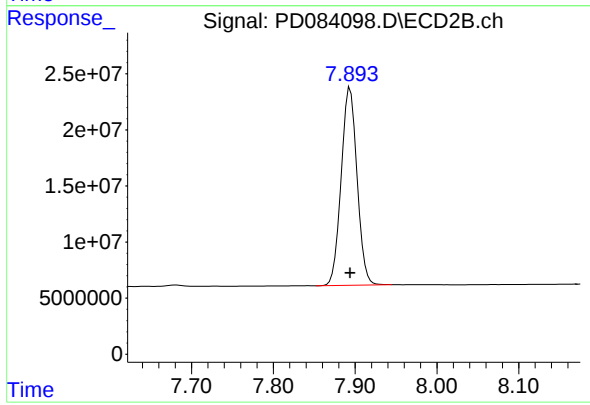

#27 Decachlorobiphenyl

R.T.: 7.894 min
Delta R.T.: 0.000 min
Response: 236509980
Conc: 40.00 ng/ml