

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072524\
 Data File : PD084100.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jul 2024 19:02
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 25 04:59:09 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072524CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 25 04:52:51 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.561	2.771	36335703	209.5E6	39.162	38.711
27)	SA Decachlor...	9.112	7.894	151.1E6	448.0E6	78.032	75.771
Target Compounds							
2)	A alpha-BHC	4.018	3.270	70558425	346.1E6	42.269	40.013
3)	MA gamma-BHC...	4.352	3.599	69192944	325.4E6	41.493	39.631
4)	MA Heptachlor	4.944	3.936	74726279	314.2E6	40.467	39.335
9)	A Endosulfan I	6.102	5.085	69555580	259.6E6	39.939	39.146
13)	MA Dieldrin	6.378	5.349	154.5E6	572.7E6	82.302	78.425
14)	MA Endrin	6.609	5.624	128.7E6	485.4E6	81.826	78.342
16)	A 4,4'-DDD	6.741	5.771	109.7E6	431.6E6	82.791	79.237
17)	MA 4,4'-DDT	7.058	6.021	116.6E6	438.3E6	84.204	81.482
20)	A Methoxychlor	7.534	6.595	332.0E6	987.7E6	396.622	368.923


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072524\
Data File : PD084100.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2024 19:02
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 04:59:09 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072524CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 25 04:52:51 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

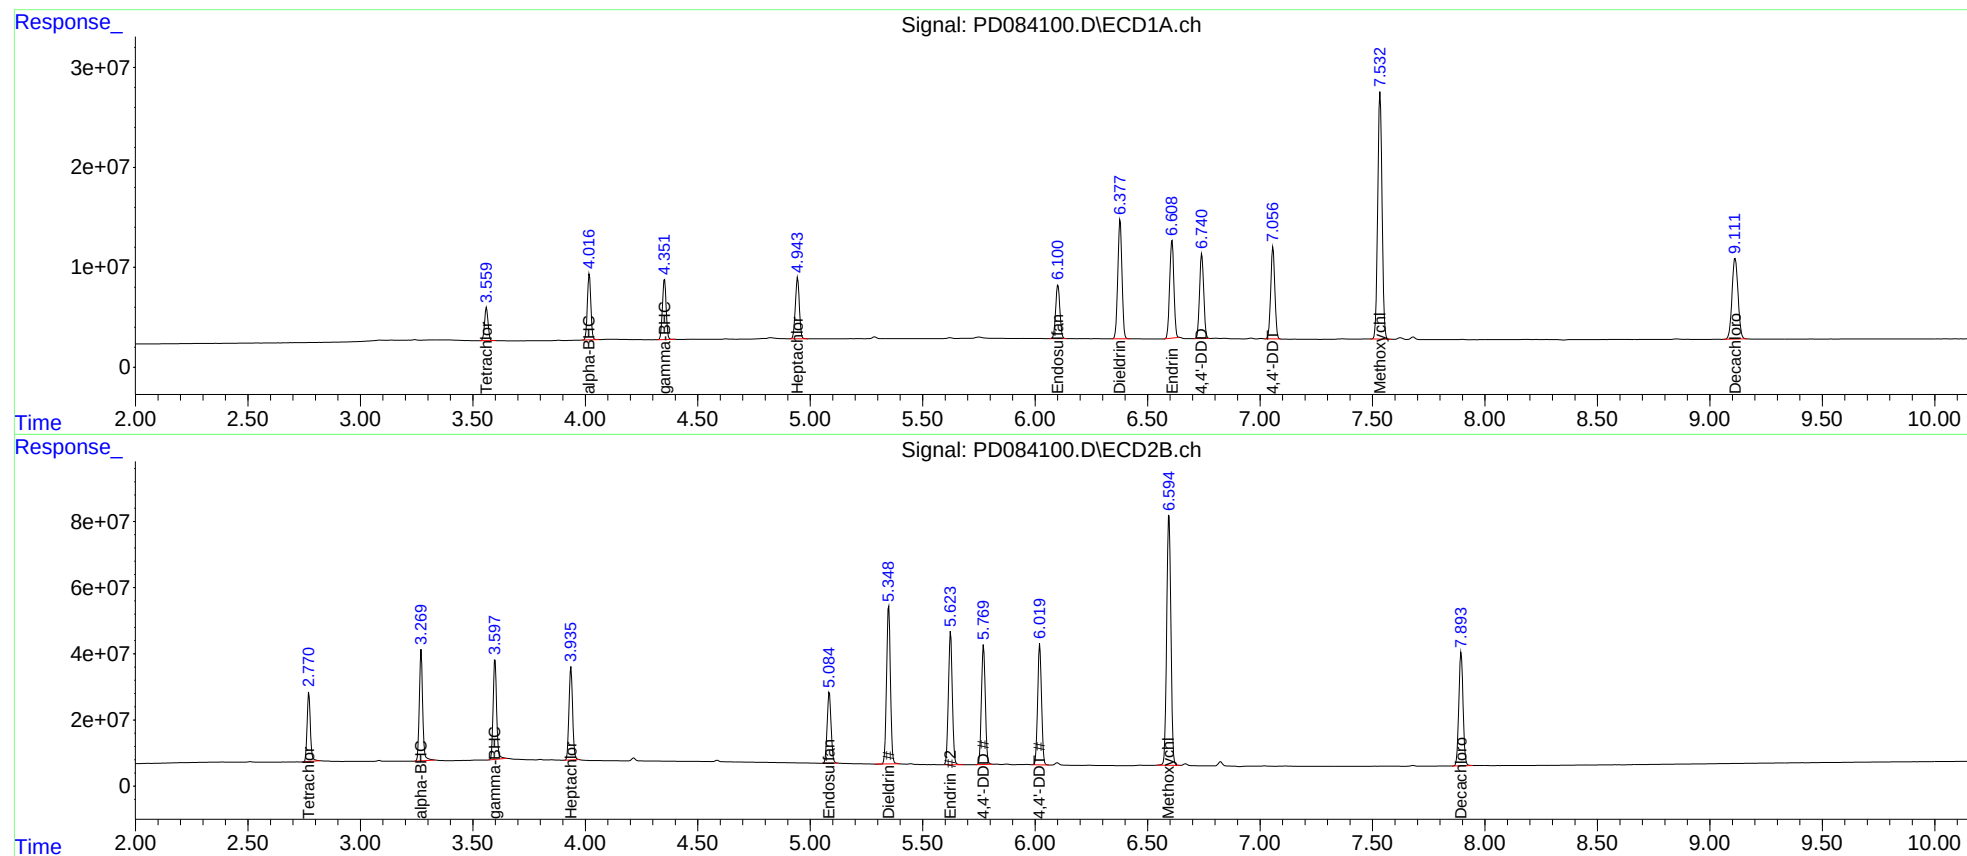

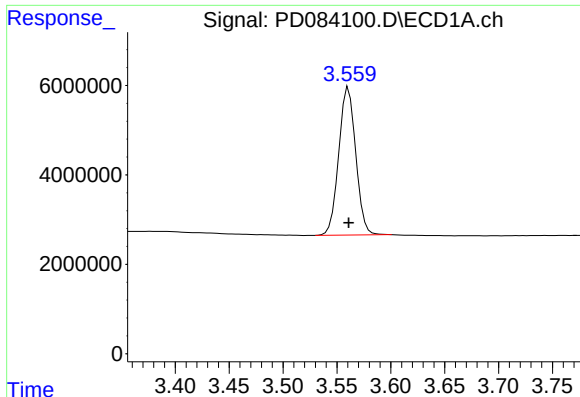


#1 Tetrachloro-m-xylene

R.T.: 3.561 min
Delta R.T.: 0.000 min
Response: 36335703
Conc: 39.16 ng/ml

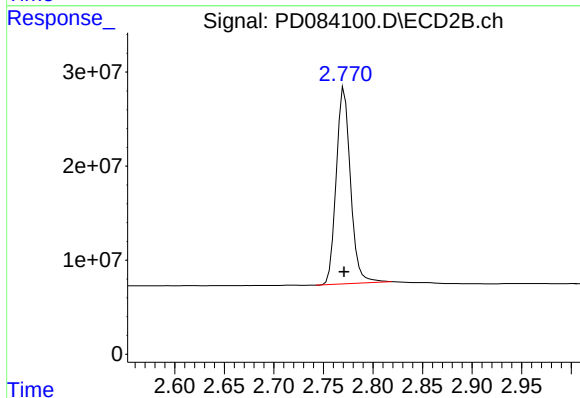


#1 Tetrachloro-m-xylene

R.T.: 2.771 min
Delta R.T.: 0.000 min
Response: 209496174
Conc: 38.71 ng/ml

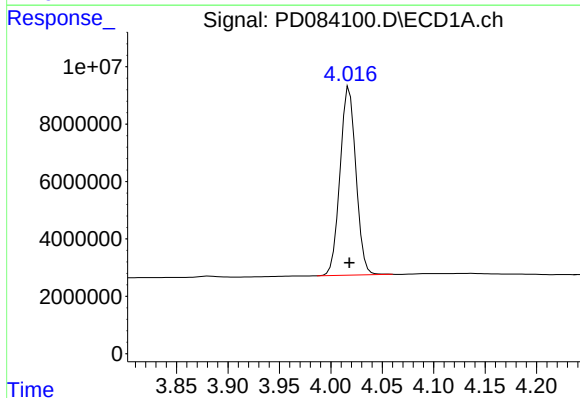


#2 alpha-BHC

R.T.: 4.018 min
Delta R.T.: 0.000 min
Response: 70558425
Conc: 42.27 ng/ml

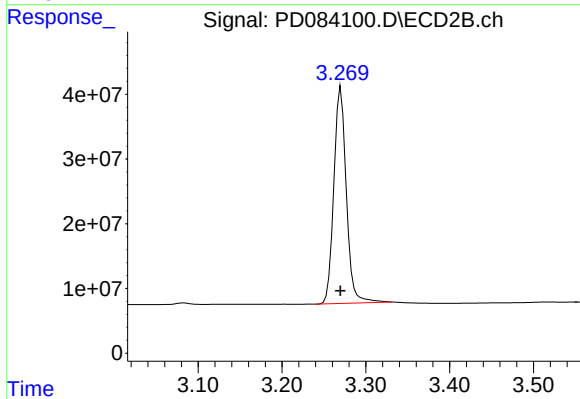


#2 alpha-BHC

R.T.: 3.270 min
Delta R.T.: 0.000 min
Response: 346115794
Conc: 40.01 ng/ml

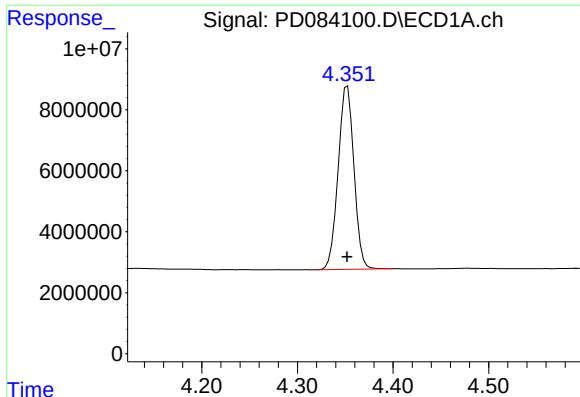


#3 gamma-BHC (Lindane)

R.T.: 4.352 min
Delta R.T.: 0.000 min
Response: 69192944
Conc: 41.49 ng/ml

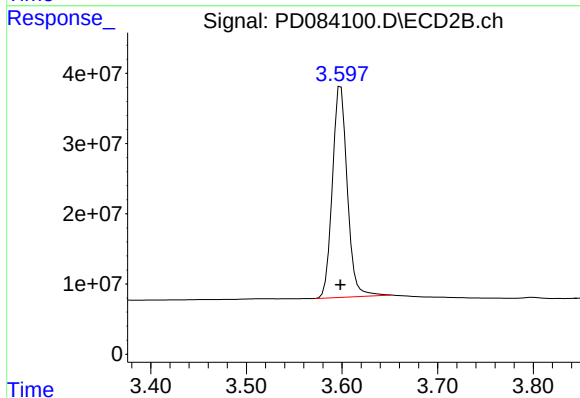


#3 gamma-BHC (Lindane)

R.T.: 3.599 min
Delta R.T.: 0.000 min
Response: 325422343
Conc: 39.63 ng/ml

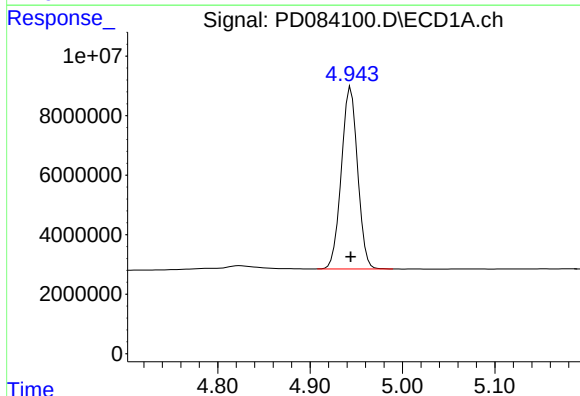


#4 Heptachlor

R.T.: 4.944 min
Delta R.T.: 0.000 min
Response: 74726279
Conc: 40.47 ng/ml

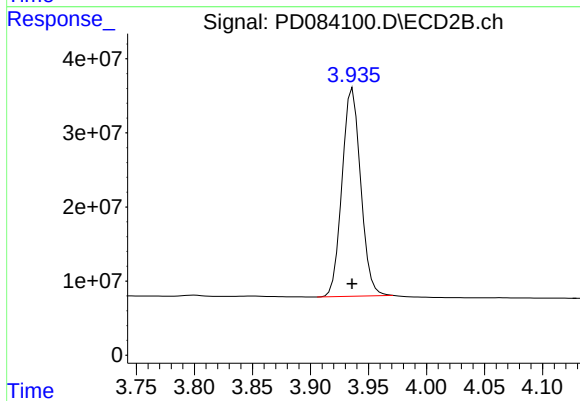


#4 Heptachlor

R.T.: 3.936 min
Delta R.T.: 0.000 min
Response: 314220025
Conc: 39.34 ng/ml

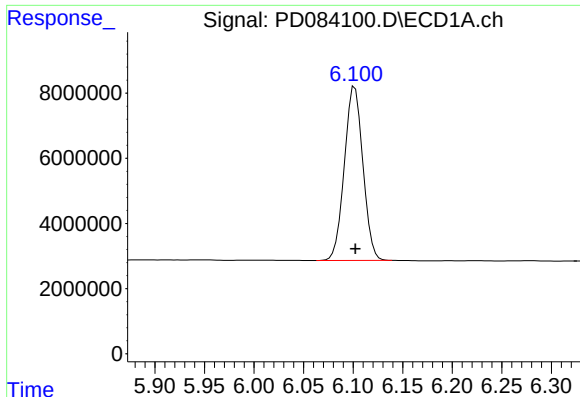


#9 Endosulfan I

R.T.: 6.102 min
Delta R.T.: 0.000 min
Response: 69555580
Conc: 39.94 ng/ml

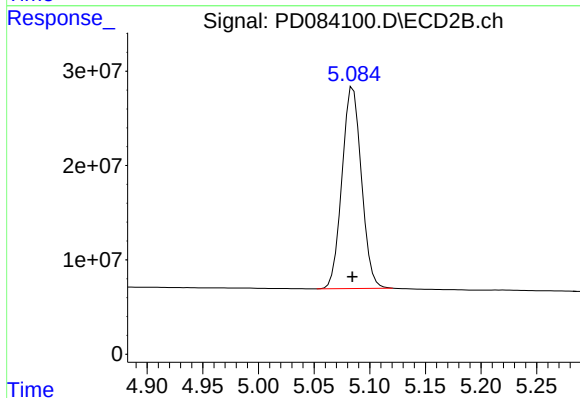


#9 Endosulfan I

R.T.: 5.085 min
Delta R.T.: 0.000 min
Response: 259570189
Conc: 39.15 ng/ml

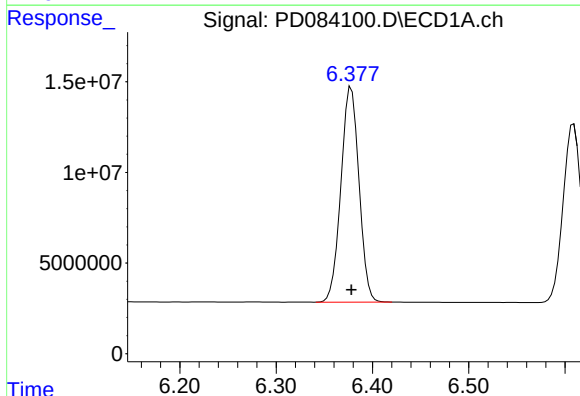


#13 Dieldrin

R.T.: 6.378 min
Delta R.T.: 0.000 min
Response: 154451163
Conc: 82.30 ng/ml

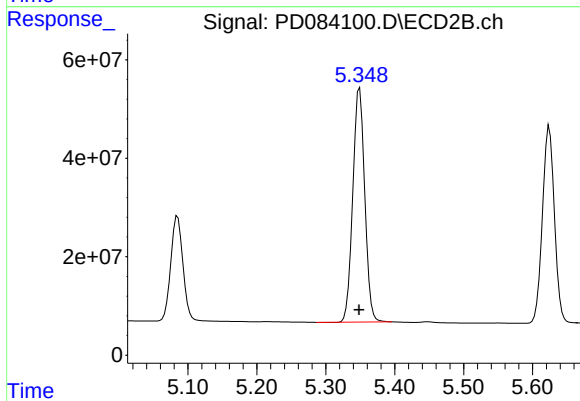


#13 Dieldrin

R.T.: 5.349 min
Delta R.T.: 0.000 min
Response: 572709305
Conc: 78.42 ng/ml

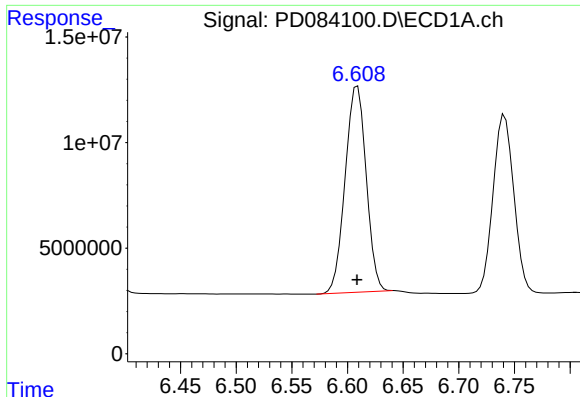


#14 Endrin

R.T.: 6.609 min
Delta R.T.: 0.000 min
Response: 128683318
Conc: 81.83 ng/ml

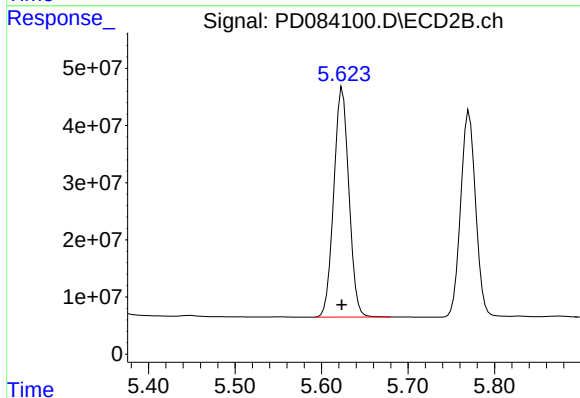


#14 Endrin

R.T.: 5.624 min
Delta R.T.: 0.000 min
Response: 485356246
Conc: 78.34 ng/ml

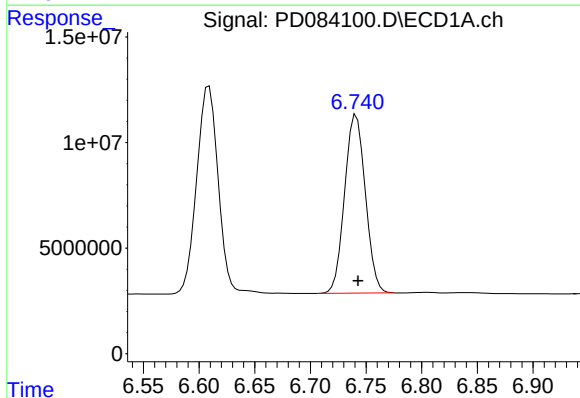


#16 4,4'-DDD

R.T.: 6.741 min
Delta R.T.: -0.002 min
Response: 109683354
Conc: 82.79 ng/ml

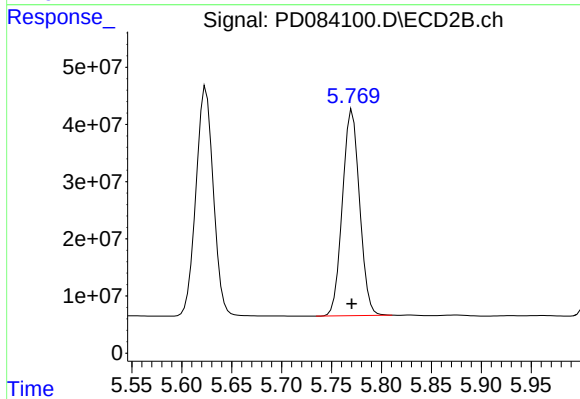


#16 4,4'-DDD

R.T.: 5.771 min
Delta R.T.: 0.000 min
Response: 431585033
Conc: 79.24 ng/ml

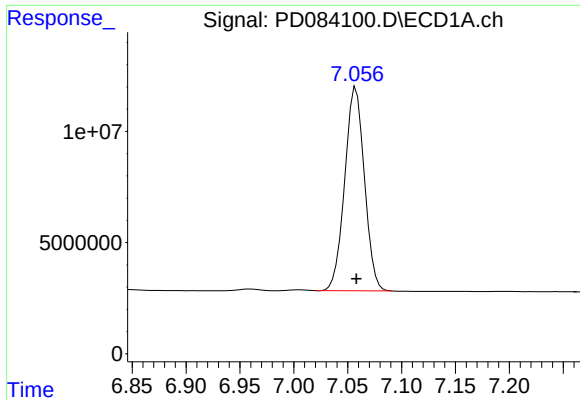


#17 4,4'-DDT

R.T.: 7.058 min
Delta R.T.: 0.000 min
Response: 116585601
Conc: 84.20 ng/ml

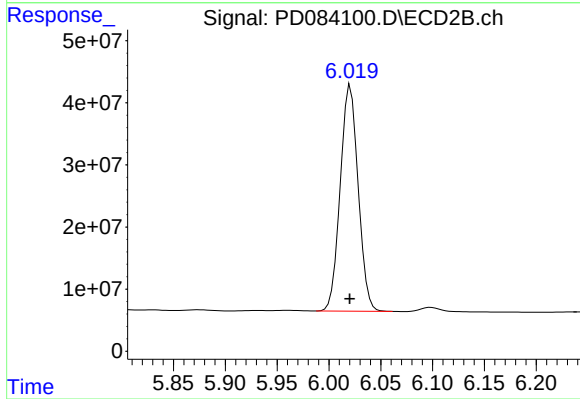


#17 4,4'-DDT

R.T.: 6.021 min
Delta R.T.: 0.000 min
Response: 438287993
Conc: 81.48 ng/ml

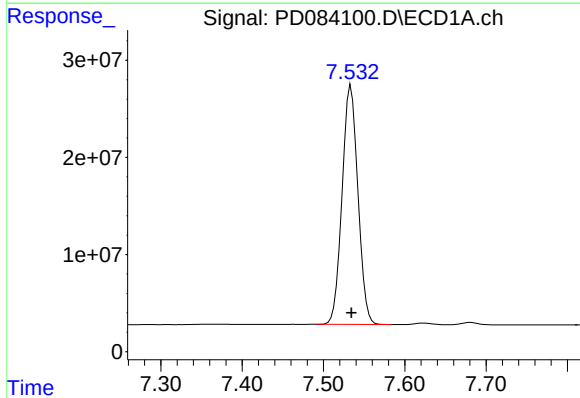


#20 Methoxychlor

R.T.: 7.534 min
Delta R.T.: 0.000 min
Response: 332009489
Conc: 396.62 ng/ml

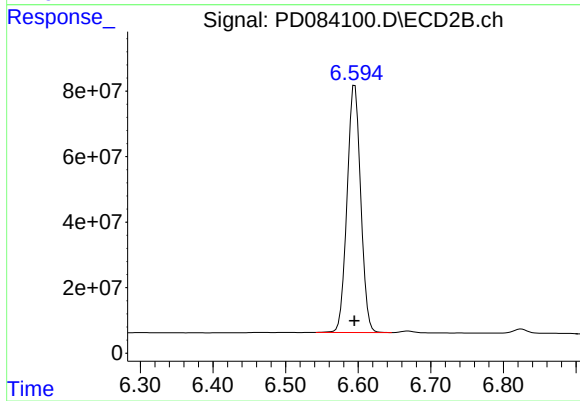


#20 Methoxychlor

R.T.: 6.595 min
Delta R.T.: 0.000 min
Response: 987728072
Conc: 368.92 ng/ml

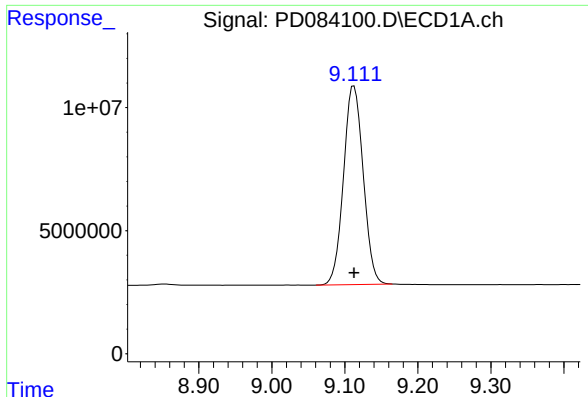

#27 Decachlorobiphenyl

R.T.: 9.112 min
Delta R.T.: 0.000 min
Response: 151141525
Conc: 78.03 ng/ml

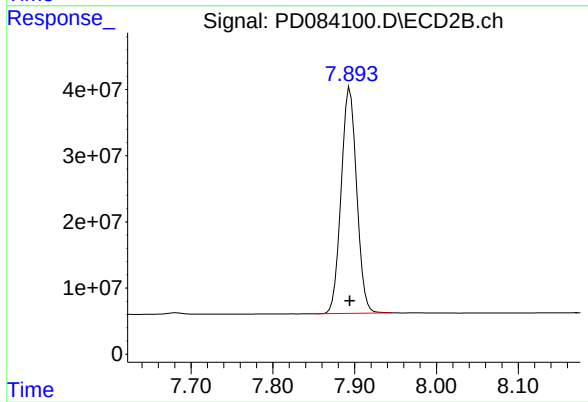

#27 Decachlorobiphenyl

R.T.: 7.894 min
Delta R.T.: 0.000 min
Response: 448015311
Conc: 75.77 ng/ml