

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072524\
 Data File : PD084101.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jul 2024 19:15
 Operator : AR\AJ
 Sample : INDB401
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 25 03:51:00 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072524CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 25 03:48:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.561	2.771	37670383	213.8E6	39.664	38.477
27)	SA Decachlor...	9.112	7.893	156.1E6	468.8E6	78.658	77.056
Target Compounds							
5)	MB Aldrin	5.287	4.215	76434429	324.6E6	41.060	40.129
6)	B beta-BHC	4.550	3.895	30584847	145.4E6	39.660	38.988
7)	B delta-BHC	4.798	4.124	78064096	353.4E6	41.634	40.511
8)	B Heptachlo...	5.715	4.715	69711270	295.9E6	40.464	39.540
10)	B trans-Chl...	5.971	4.965	72380487	291.7E6	40.290	39.954
11)	B cis-Chlor...	6.051	5.029	74112504	295.8E6	40.321	39.825
12)	B 4,4'-DDE	6.223	5.216	150.6E6	565.2E6	81.728	79.970
15)	B Endosulfa...	6.828	5.917	139.6E6	484.7E6	80.575	78.720
18)	B Endrin al...	6.959	6.097	101.8E6	358.2E6	79.695	78.071
19)	B Endosulfa...	7.195	6.319	132.8E6	465.4E6	80.776	78.644
21)	B Endrin ke...	7.681	6.825	147.5E6	506.3E6	81.546	78.861


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072524\
Data File : PD084101.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2024 19:15
Operator : AR\AJ
Sample : INDB401
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 03:51:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072524CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 25 03:48:48 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

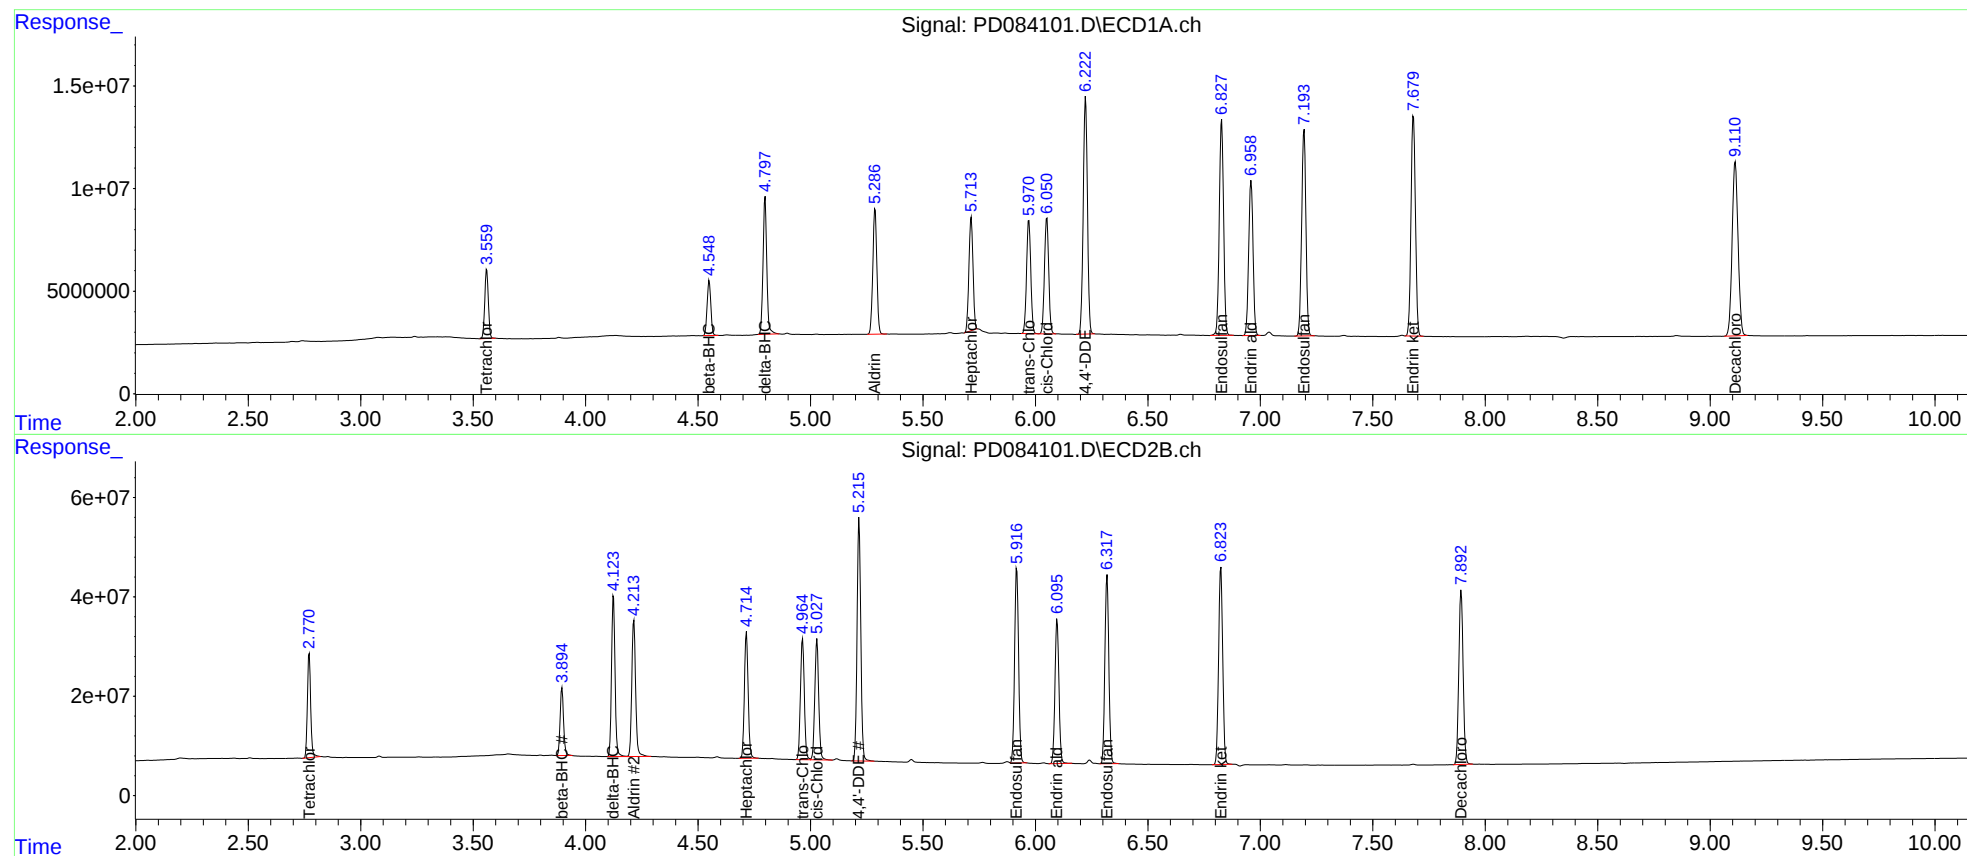

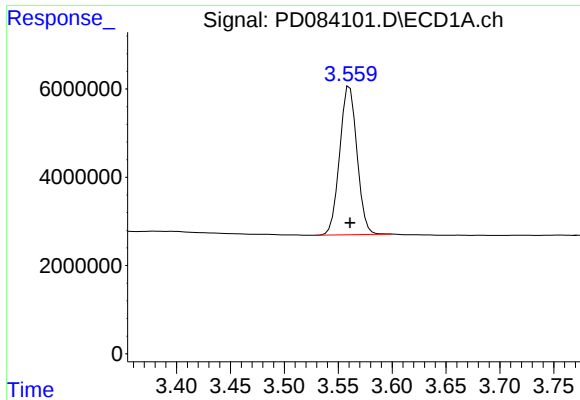


#1 Tetrachloro-m-xylene

R.T.: 3.561 min
Delta R.T.: 0.000 min
Response: 37670383
Conc: 39.66 ng/ml

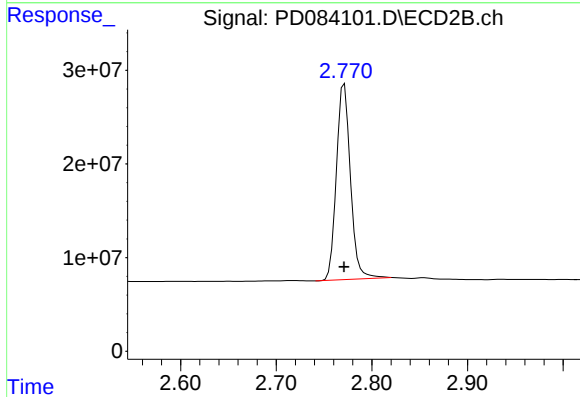


#1 Tetrachloro-m-xylene

R.T.: 2.771 min
Delta R.T.: 0.000 min
Response: 213786101
Conc: 38.48 ng/ml

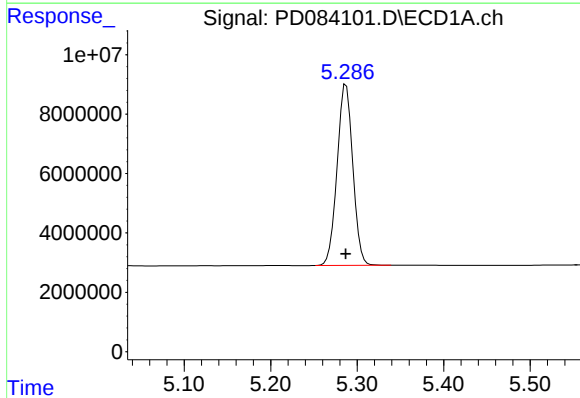


#5 Aldrin

R.T.: 5.287 min
Delta R.T.: 0.000 min
Response: 76434429
Conc: 41.06 ng/ml

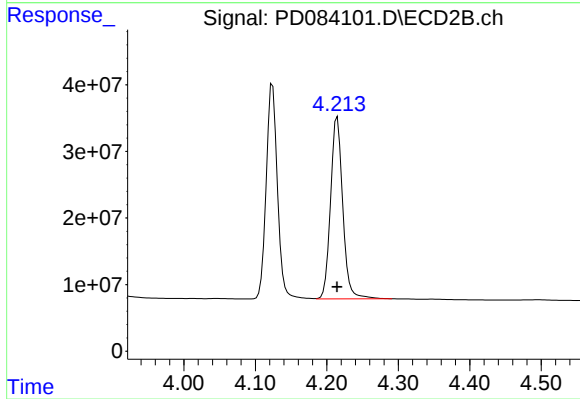


#5 Aldrin

R.T.: 4.215 min
Delta R.T.: 0.000 min
Response: 324566067
Conc: 40.13 ng/ml

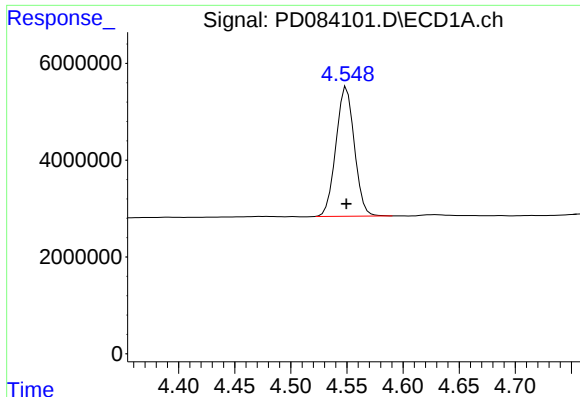


#6 beta-BHC

R.T.: 4.550 min
Delta R.T.: 0.000 min
Response: 30584847
Conc: 39.66 ng/ml

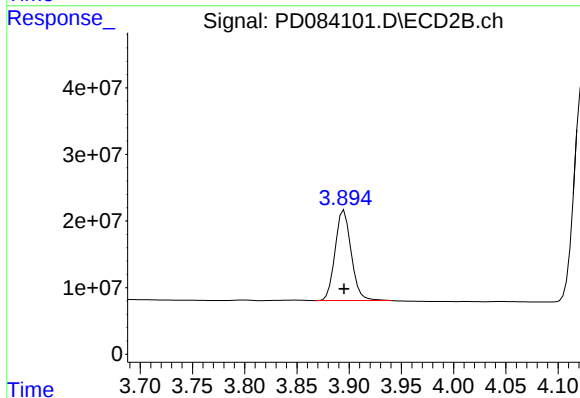


#6 beta-BHC

R.T.: 3.895 min
Delta R.T.: 0.000 min
Response: 145365073
Conc: 38.99 ng/ml

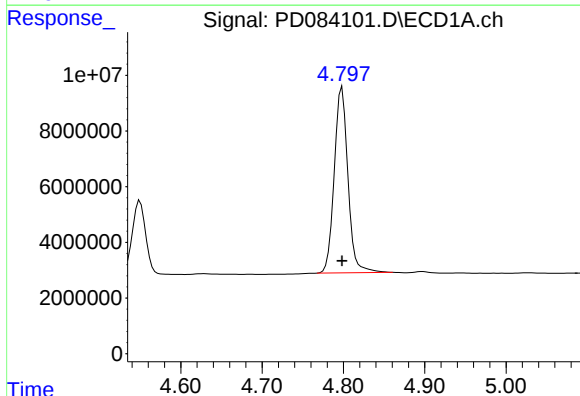


#7 delta-BHC

R.T.: 4.798 min
Delta R.T.: 0.000 min
Response: 78064096
Conc: 41.63 ng/ml

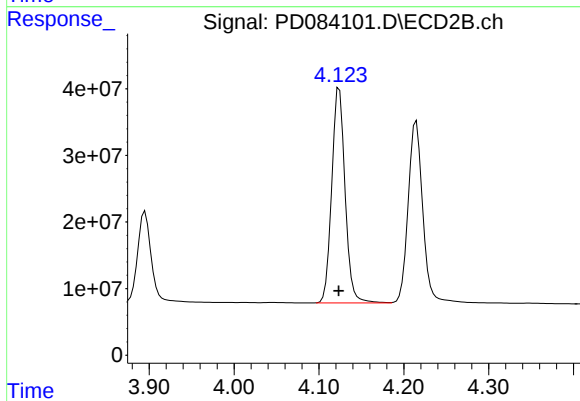


#7 delta-BHC

R.T.: 4.124 min
Delta R.T.: 0.000 min
Response: 353403511
Conc: 40.51 ng/ml

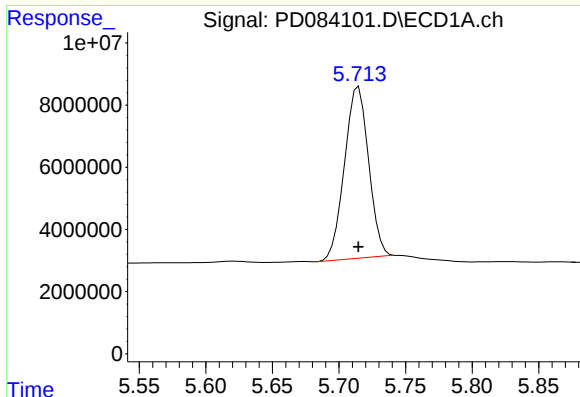


#8 Heptachlor epoxide

R.T.: 5.715 min
Delta R.T.: 0.000 min
Response: 69711270
Conc: 40.46 ng/ml

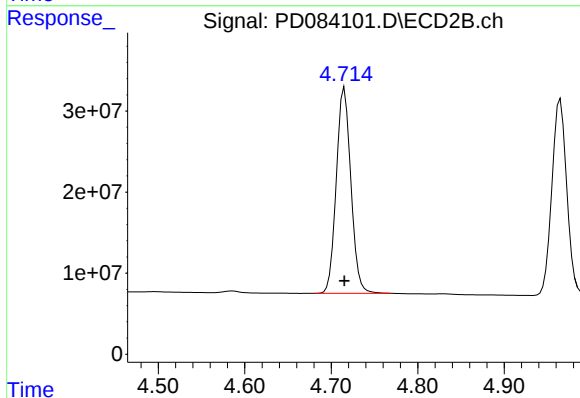


#8 Heptachlor epoxide

R.T.: 4.715 min
Delta R.T.: 0.000 min
Response: 295861474
Conc: 39.54 ng/ml

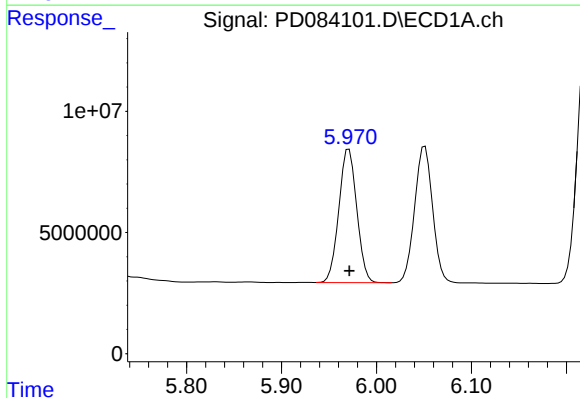


#10 trans-Chlordane

R.T.: 5.971 min
Delta R.T.: 0.000 min
Response: 72380487
Conc: 40.29 ng/ml

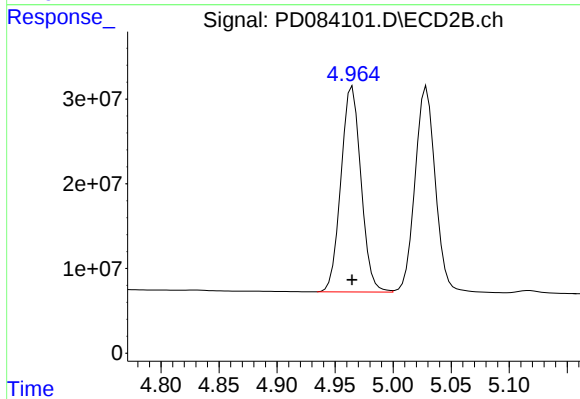


#10 trans-Chlordane

R.T.: 4.965 min
Delta R.T.: 0.000 min
Response: 291731262
Conc: 39.95 ng/ml

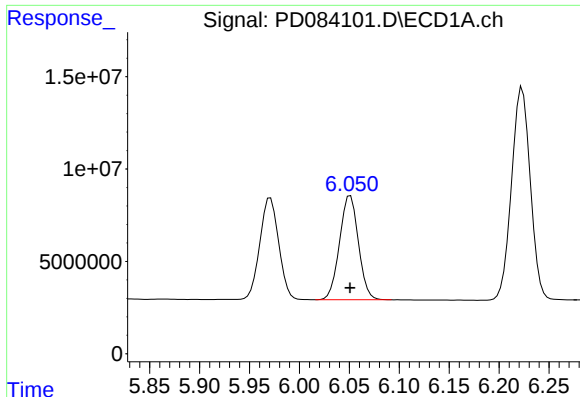


#11 cis-Chlordane

R.T.: 6.051 min
Delta R.T.: 0.000 min
Response: 74112504
Conc: 40.32 ng/ml

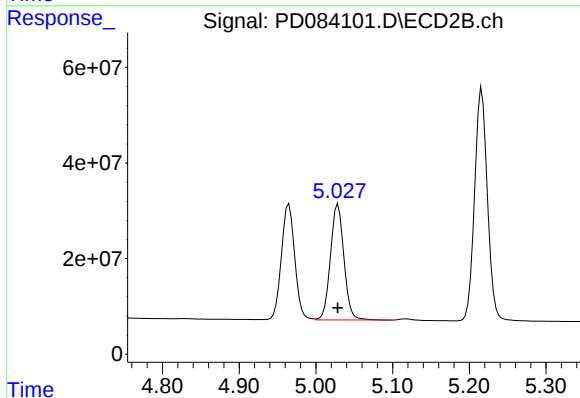


#11 cis-Chlordane

R.T.: 5.029 min
Delta R.T.: 0.000 min
Response: 295784809
Conc: 39.83 ng/ml

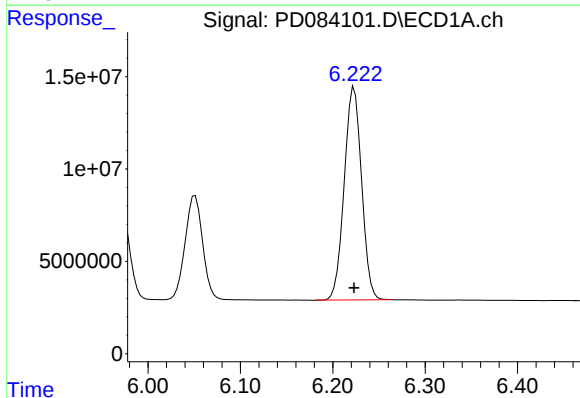


#12 4,4'-DDE

R.T.: 6.223 min
Delta R.T.: 0.000 min
Response: 150588159
Conc: 81.73 ng/ml

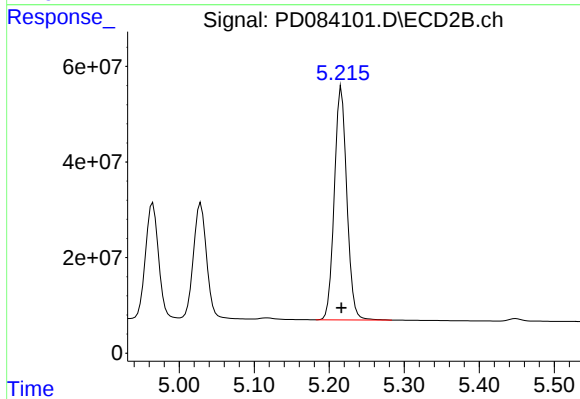


#12 4,4'-DDE

R.T.: 5.216 min
Delta R.T.: 0.000 min
Response: 565174167
Conc: 79.97 ng/ml

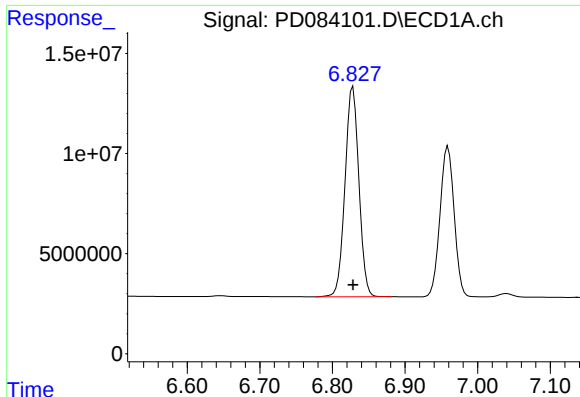


#15 Endosulfan II

R.T.: 6.828 min
Delta R.T.: 0.000 min
Response: 139620485
Conc: 80.57 ng/ml

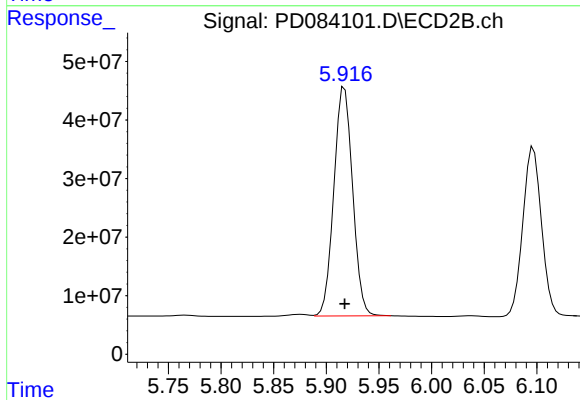


#15 Endosulfan II

R.T.: 5.917 min
Delta R.T.: 0.000 min
Response: 484673067
Conc: 78.72 ng/ml

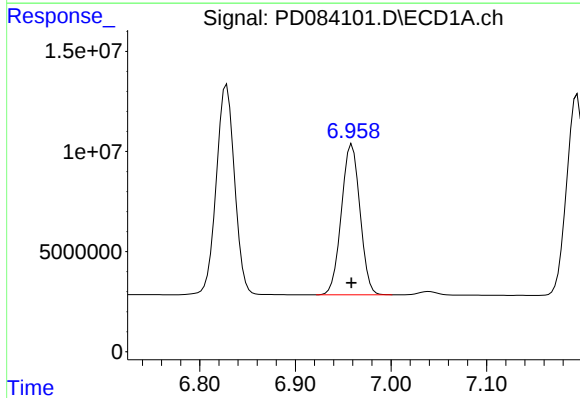


#18 Endrin aldehyde

R.T.: 6.959 min
Delta R.T.: 0.000 min
Response: 101817981
Conc: 79.69 ng/ml

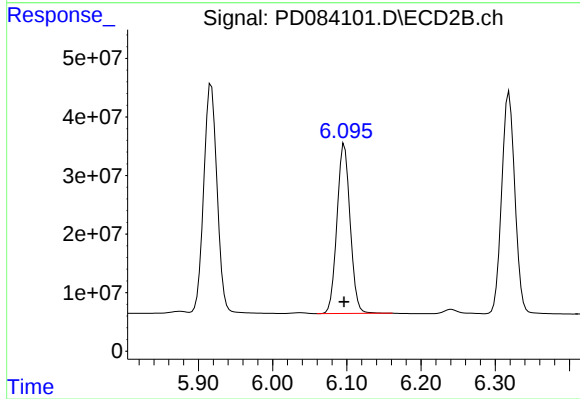


#18 Endrin aldehyde

R.T.: 6.097 min
Delta R.T.: 0.000 min
Response: 358239427
Conc: 78.07 ng/ml

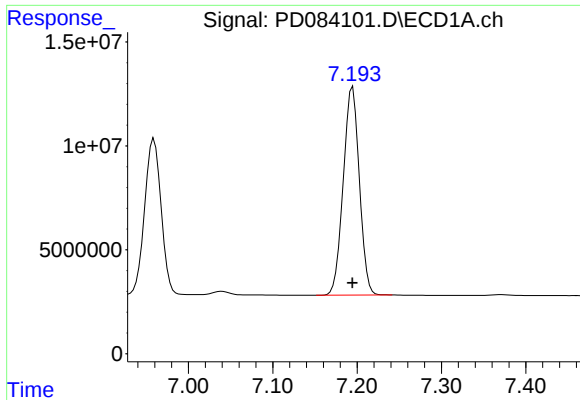


#19 Endosulfan Sulfate

R.T.: 7.195 min
Delta R.T.: 0.000 min
Response: 132817347
Conc: 80.78 ng/ml

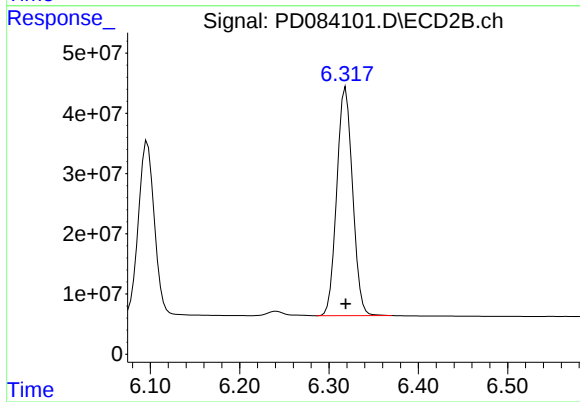


#19 Endosulfan Sulfate

R.T.: 6.319 min
Delta R.T.: 0.000 min
Response: 465440456
Conc: 78.64 ng/ml

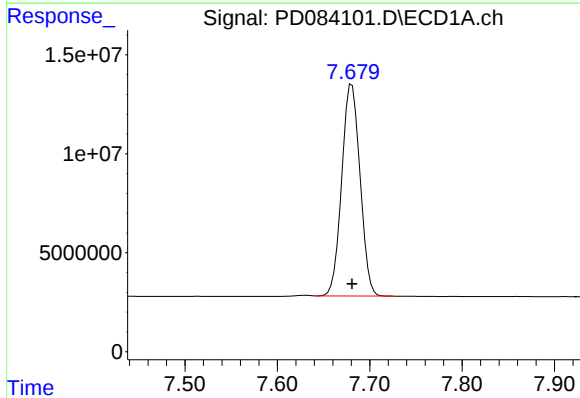


#21 Endrin ketone

R.T.: 7.681 min
Delta R.T.: 0.000 min
Response: 147472806
Conc: 81.55 ng/ml

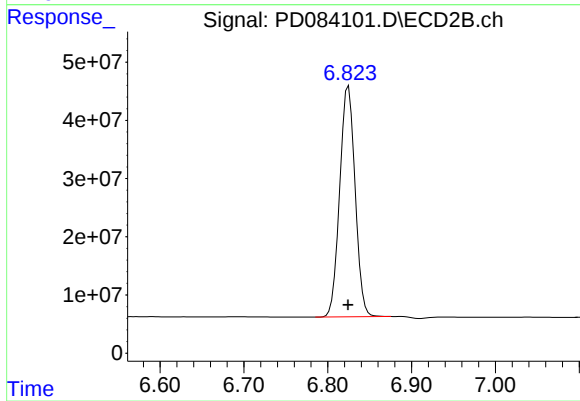


#21 Endrin ketone

R.T.: 6.825 min
Delta R.T.: 0.000 min
Response: 506339273
Conc: 78.86 ng/ml

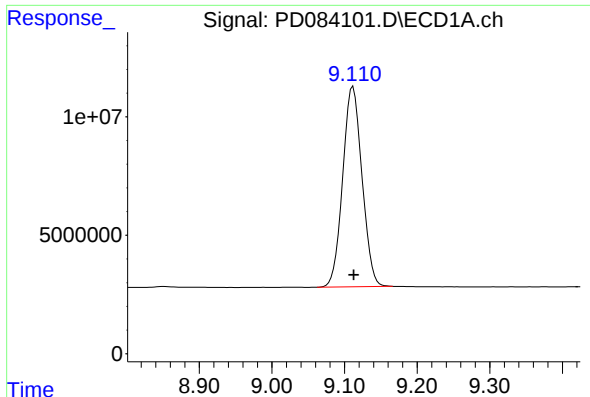

#27 Decachlorobiphenyl

R.T.: 9.112 min
Delta R.T.: -0.001 min
Response: 156129454
Conc: 78.66 ng/ml

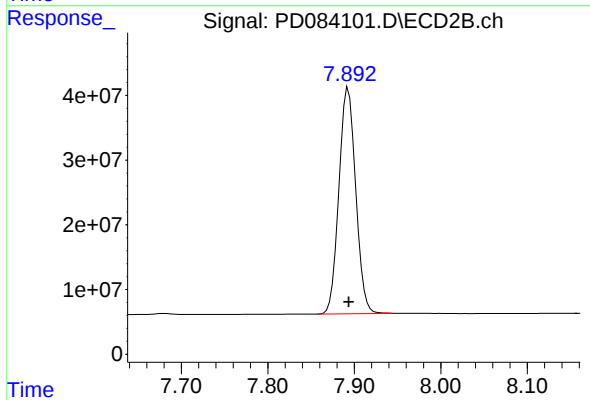

#27 Decachlorobiphenyl

R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 468752676
Conc: 77.06 ng/ml