

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072524\
 Data File : PD084102.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jul 2024 19:29
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 25 04:59:24 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072524CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 25 04:52:51 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.561	2.771	71717818	405.6E6	77.295	74.955
27)	SA Decachlor...	9.112	7.894	294.8E6	857.3E6	152.223	145.000
Target Compounds							
2)	A alpha-BHC	4.019	3.270	150.4E6	685.8E6	90.117	79.282
3)	MA gamma-BHC...	4.352	3.599	145.7E6	641.9E6	87.371	78.176
4)	MA Heptachlor	4.944	3.936	152.9E6	614.9E6	82.817	76.981
9)	A Endosulfan I	6.103	5.085	139.2E6	503.4E6	79.904	75.922
13)	MA Dieldrin	6.378	5.349	317.9E6	1107.0E6	169.376	151.584
14)	MA Endrin	6.609	5.624	263.6E6	938.1E6	167.628	151.417
16)	A 4,4'-DDD	6.743	5.771	228.0E6	845.7E6	172.069	155.262
17)	MA 4,4'-DDT	7.058	6.021	242.8E6	877.5E6	175.344	163.135
20)	A Methoxychlor	7.534	6.595	650.8E6	1771.8E6	777.456	661.798


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072524\
Data File : PD084102.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2024 19:29
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 04:59:24 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072524CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 25 04:52:51 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

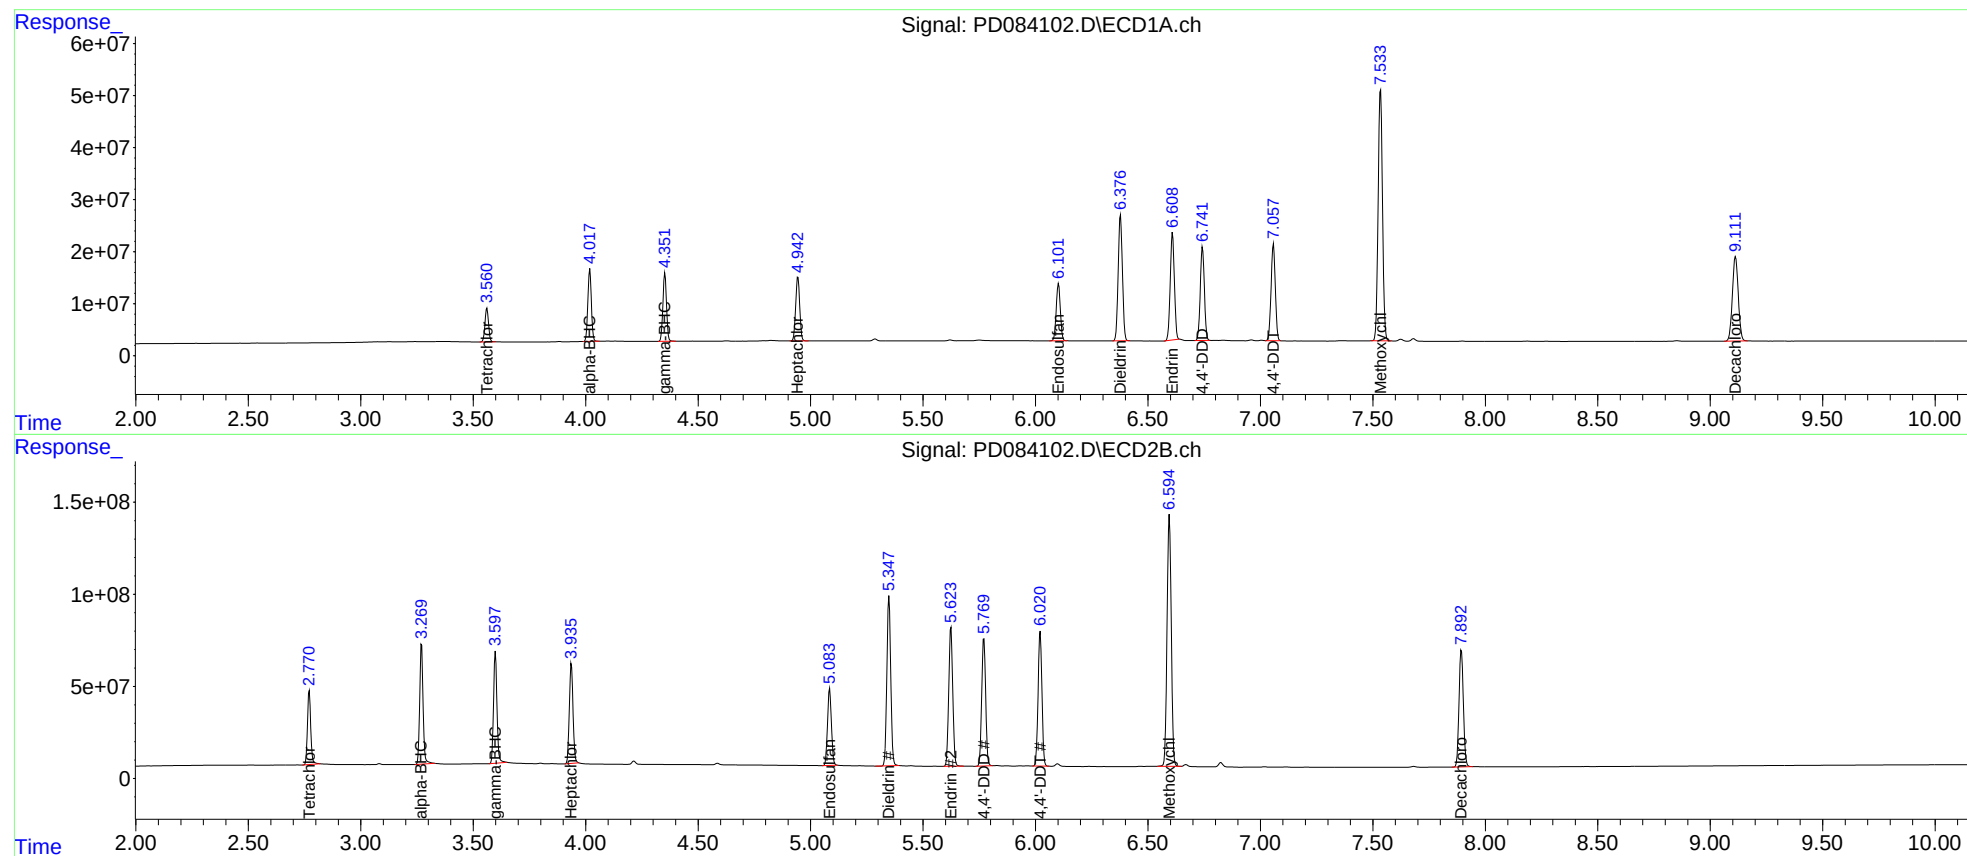

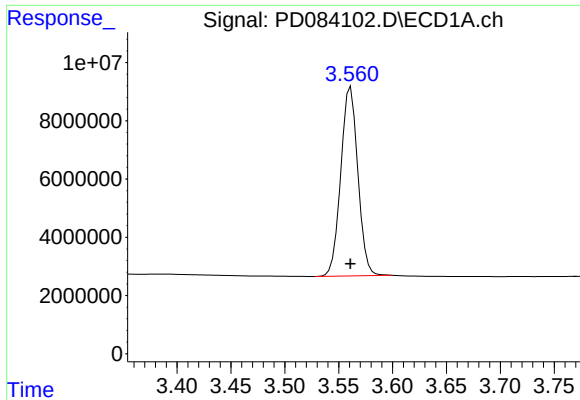


#1 Tetrachloro-m-xylene

R.T.: 3.561 min
Delta R.T.: 0.000 min
Response: 71717818
Conc: 77.30 ng/ml

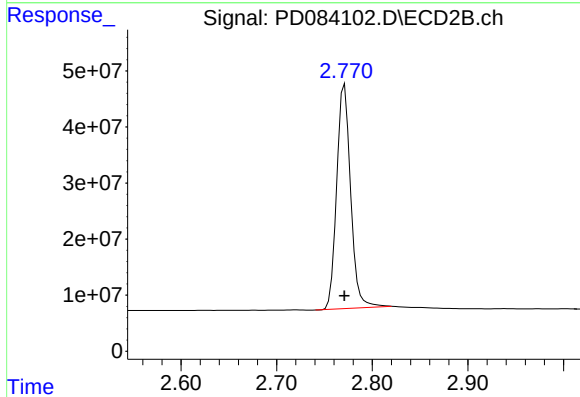


#1 Tetrachloro-m-xylene

R.T.: 2.771 min
Delta R.T.: 0.000 min
Response: 405635397
Conc: 74.95 ng/ml

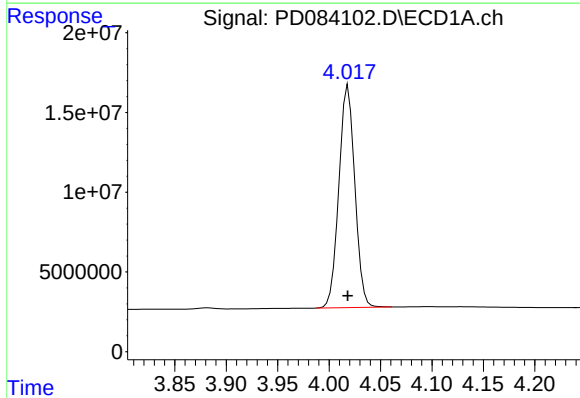


#2 alpha-BHC

R.T.: 4.019 min
Delta R.T.: 0.000 min
Response: 150430041
Conc: 90.12 ng/ml

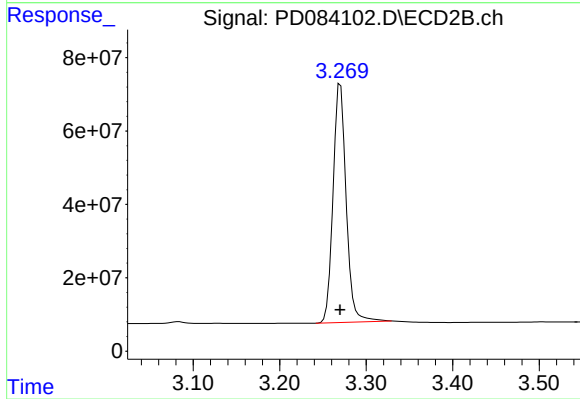


#2 alpha-BHC

R.T.: 3.270 min
Delta R.T.: 0.000 min
Response: 685795385
Conc: 79.28 ng/ml

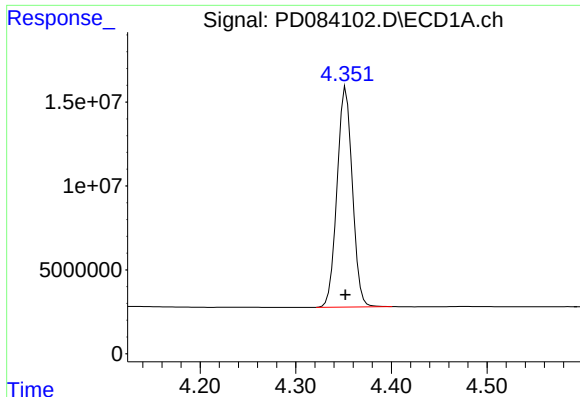


#3 gamma-BHC (Lindane)

R.T.: 4.352 min
Delta R.T.: 0.000 min
Response: 145699958
Conc: 87.37 ng/ml

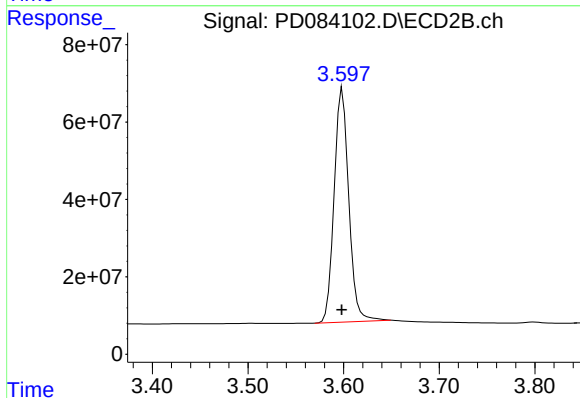


#3 gamma-BHC (Lindane)

R.T.: 3.599 min
Delta R.T.: 0.000 min
Response: 641930904
Conc: 78.18 ng/ml

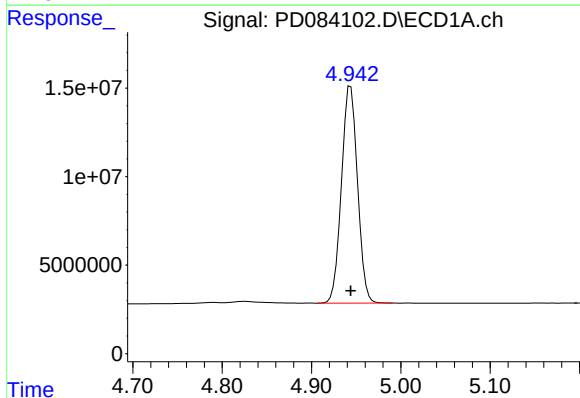


#4 Heptachlor

R.T.: 4.944 min
Delta R.T.: 0.000 min
Response: 152929998
Conc: 82.82 ng/ml

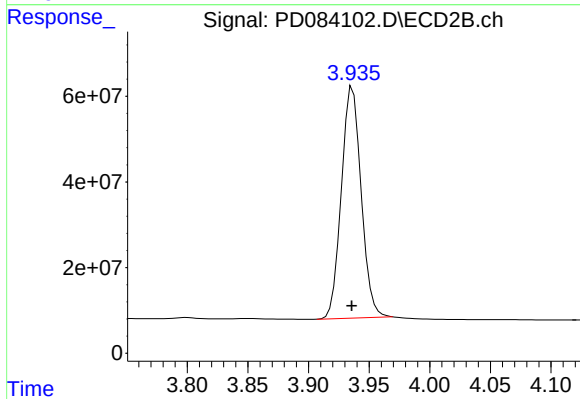


#4 Heptachlor

R.T.: 3.936 min
Delta R.T.: 0.000 min
Response: 614949723
Conc: 76.98 ng/ml

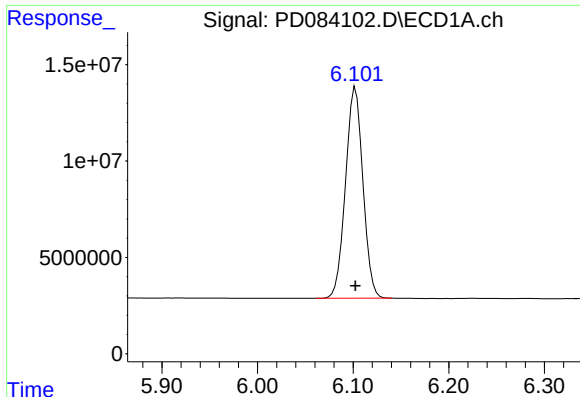


#9 Endosulfan I

R.T.: 6.103 min
Delta R.T.: 0.000 min
Response: 139156000
Conc: 79.90 ng/ml

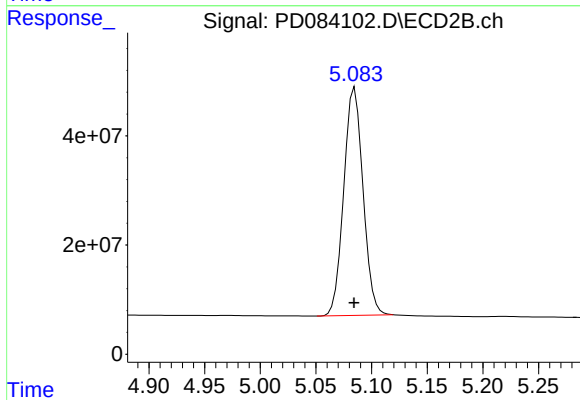


#9 Endosulfan I

R.T.: 5.085 min
Delta R.T.: 0.000 min
Response: 503425727
Conc: 75.92 ng/ml

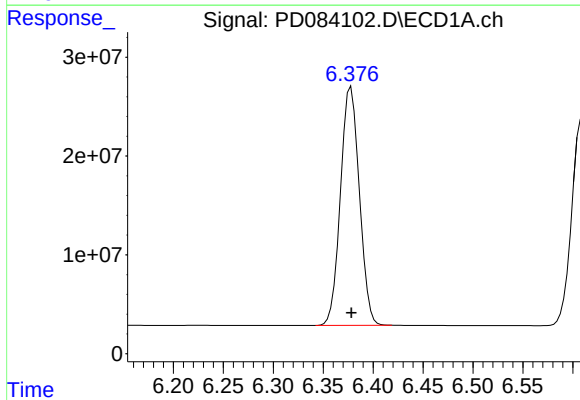


#13 Dieldrin

R.T.: 6.378 min
Delta R.T.: 0.000 min
Response: 317859873
Conc: 169.38 ng/ml

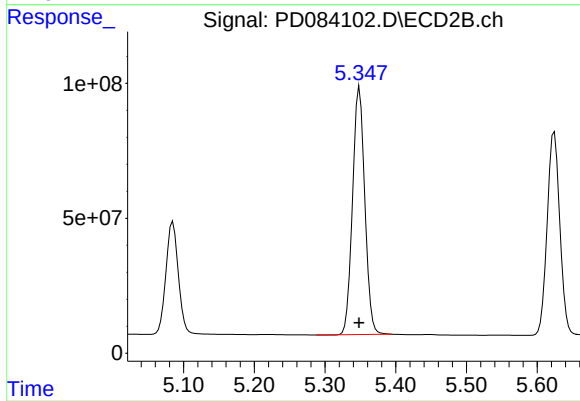


#13 Dieldrin

R.T.: 5.349 min
Delta R.T.: 0.000 min
Response: 1106966520
Conc: 151.58 ng/ml

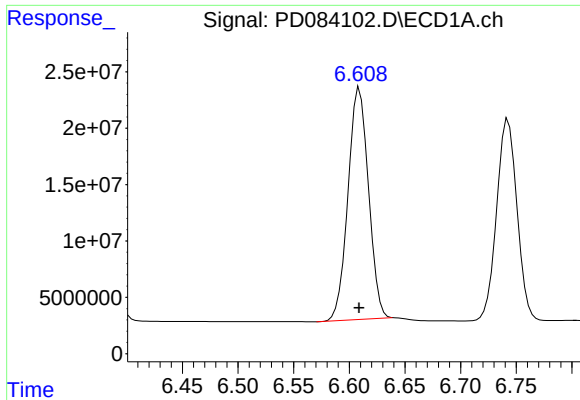


#14 Endrin

R.T.: 6.609 min
Delta R.T.: 0.000 min
Response: 263620082
Conc: 167.63 ng/ml

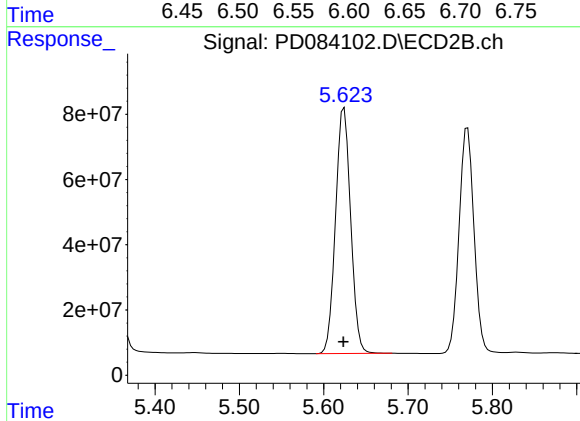


#14 Endrin

R.T.: 5.624 min
Delta R.T.: 0.000 min
Response: 938081728
Conc: 151.42 ng/ml

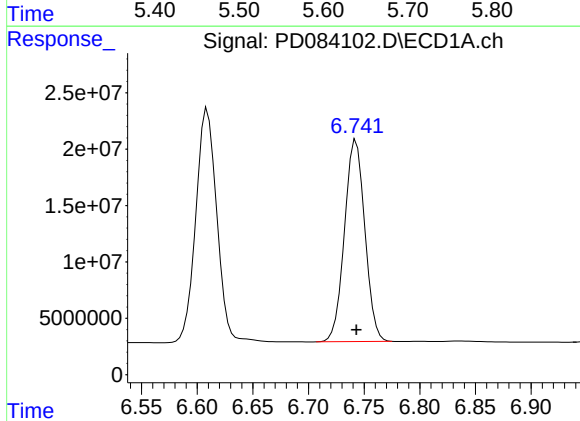


#16 4,4'-DDD

R.T.: 6.743 min
Delta R.T.: 0.000 min
Response: 227959736
Conc: 172.07 ng/ml

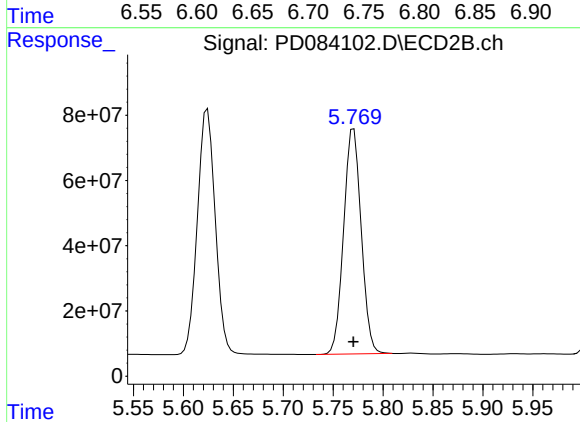


#16 4,4'-DDD

R.T.: 5.771 min
Delta R.T.: 0.000 min
Response: 845673962
Conc: 155.26 ng/ml

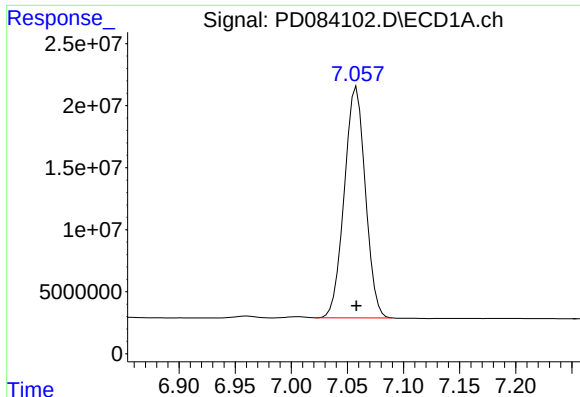


#17 4,4'-DDT

R.T.: 7.058 min
Delta R.T.: 0.000 min
Response: 242774422
Conc: 175.34 ng/ml

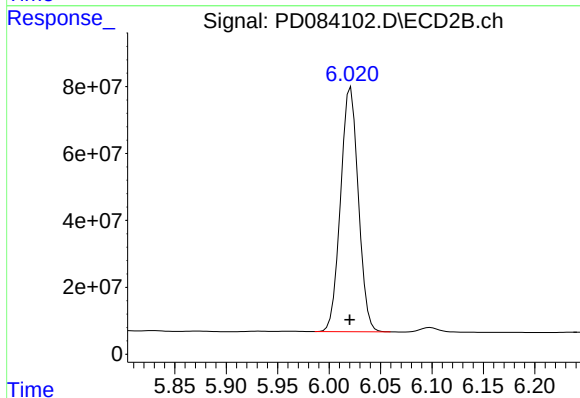


#17 4,4'-DDT

R.T.: 6.021 min
Delta R.T.: 0.000 min
Response: 877496867
Conc: 163.13 ng/ml

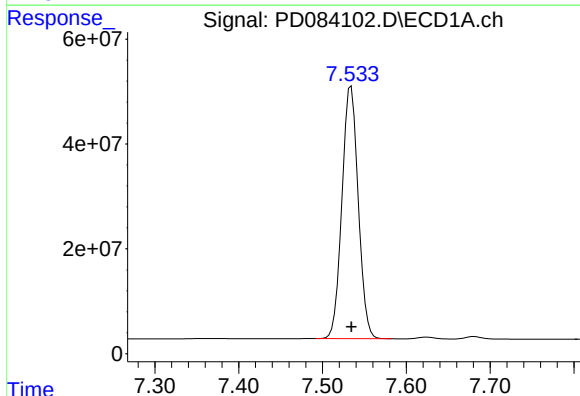


#20 Methoxychlor

R.T.: 7.534 min
Delta R.T.: 0.000 min
Response: 650803828
Conc: 777.46 ng/ml

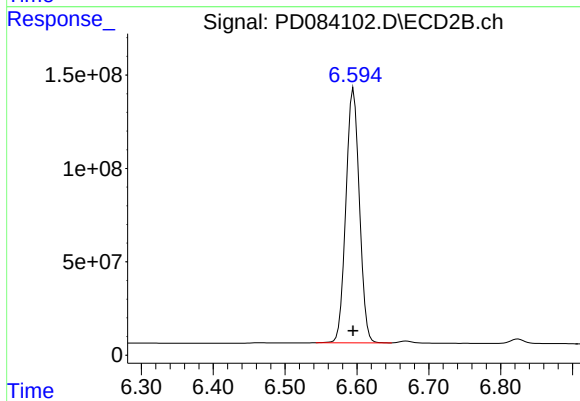


#20 Methoxychlor

R.T.: 6.595 min
Delta R.T.: 0.000 min
Response: 1771849032
Conc: 661.80 ng/ml

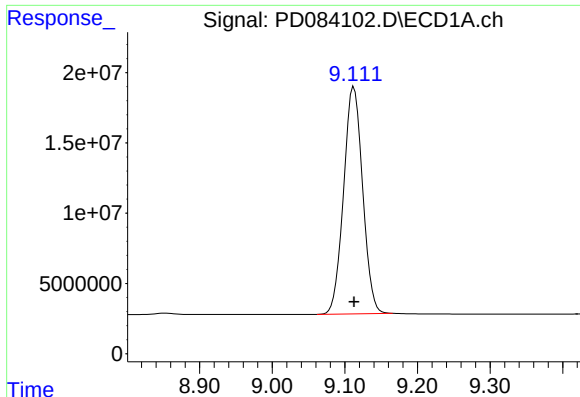

#27 Decachlorobiphenyl

R.T.: 9.112 min
Delta R.T.: 0.000 min
Response: 294843663
Conc: 152.22 ng/ml

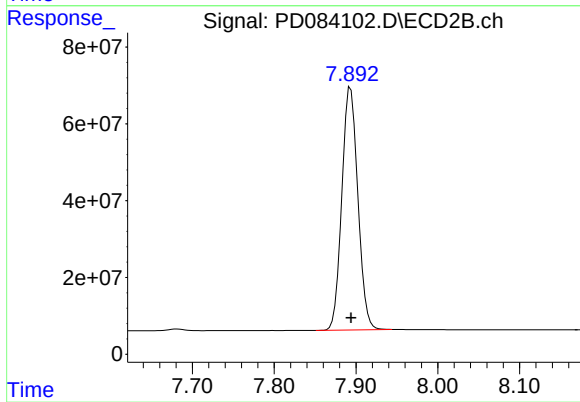

#27 Decachlorobiphenyl

R.T.: 7.894 min
Delta R.T.: 0.000 min
Response: 857346987
Conc: 145.00 ng/ml