

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072524\
 Data File : PD084104.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jul 2024 19:55
 Operator : AR\AJ
 Sample : INDA601
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 25 04:59:42 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072524CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 25 04:52:51 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.561	2.771	144.7E6	786.7E6	155.994	145.363
27)	SA Decachlor...	9.111	7.893	587.9E6	1648.4E6	303.542	278.787
Target Compounds							
2)	A alpha-BHC	4.018	3.270	327.2E6	1359.0E6	196.029	157.104
3)	MA gamma-BHC...	4.353	3.598	312.4E6	1261.6E6	187.350	153.645
4)	MA Heptachlor	4.944	3.936	322.1E6	1189.8E6	174.403	148.941
9)	A Endosulfan I	6.102	5.085	286.7E6	976.8E6	164.646	147.315
13)	MA Dieldrin	6.377	5.348	665.8E6	2110.0E6	354.773	288.937
14)	MA Endrin	6.609	5.624	551.0E6	1774.4E6	350.383	286.409
16)	A 4,4'-DDD	6.741	5.770	484.6E6	1644.3E6	365.771	301.883
17)	MA 4,4'-DDT	7.057	6.020	520.9E6	1733.7E6	376.204	322.303
20)	A Methoxychlor	7.533	6.595	1290.9E6	3114.8E6	1542.088	1163.408


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072524\
Data File : PD084104.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2024 19:55
Operator : AR\AJ
Sample : INDA601
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 04:59:42 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072524CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 25 04:52:51 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

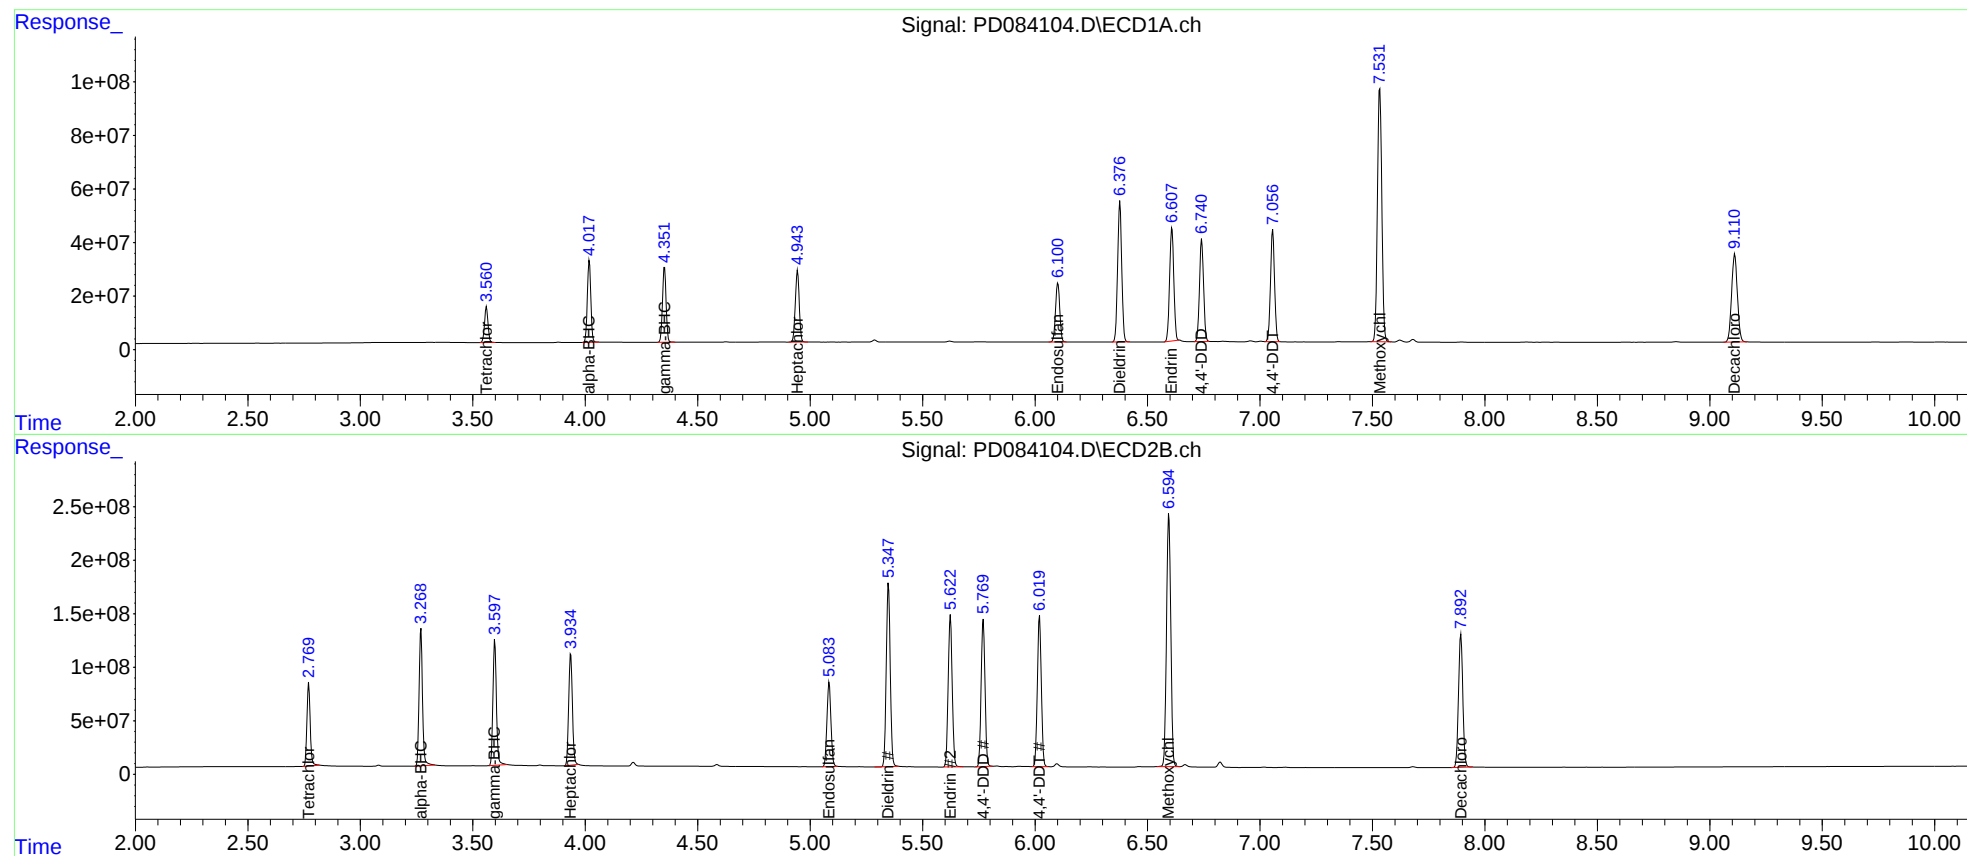

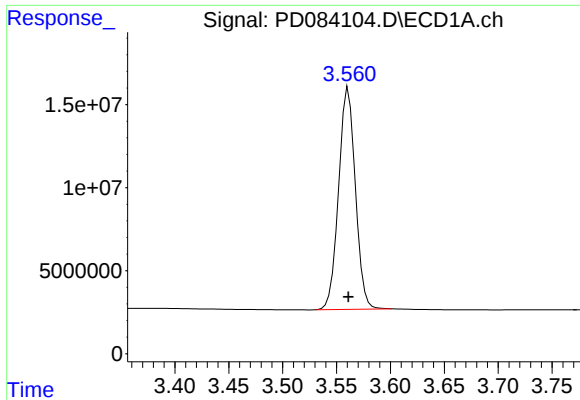


#1 Tetrachloro-m-xylene

R.T.: 3.561 min
Delta R.T.: 0.000 min
Response: 144737747
Conc: 155.99 ng/ml

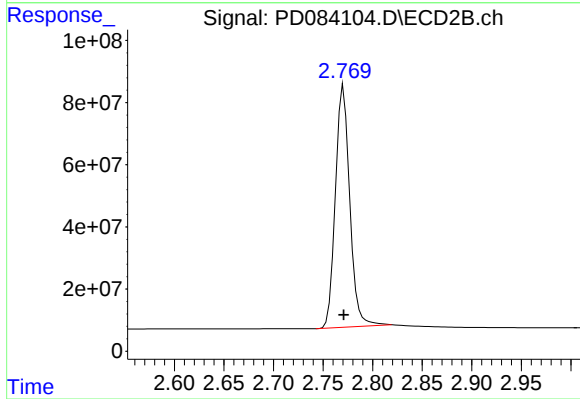


#1 Tetrachloro-m-xylene

R.T.: 2.771 min
Delta R.T.: 0.000 min
Response: 786669748
Conc: 145.36 ng/ml

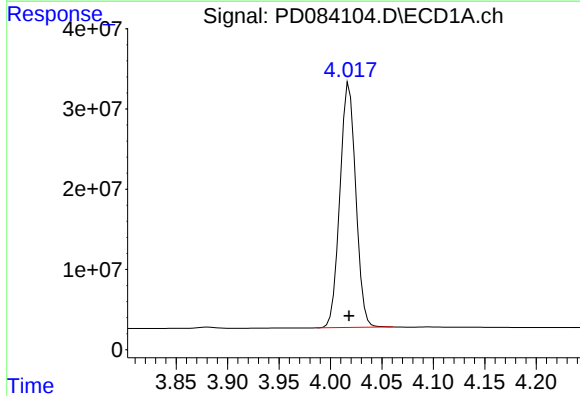


#2 alpha-BHC

R.T.: 4.018 min
Delta R.T.: 0.000 min
Response: 327225878
Conc: 196.03 ng/ml

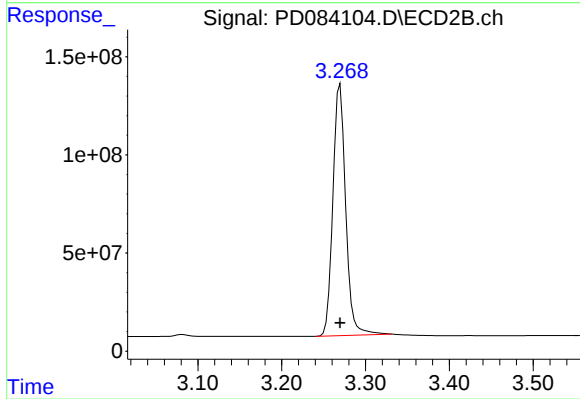


#2 alpha-BHC

R.T.: 3.270 min
Delta R.T.: 0.000 min
Response: 1358964516
Conc: 157.10 ng/ml

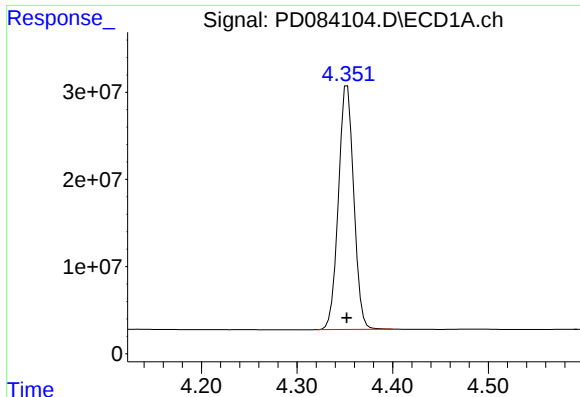


#3 gamma-BHC (Lindane)

R.T.: 4.353 min
Delta R.T.: 0.000 min
Response: 312424334
Conc: 187.35 ng/ml

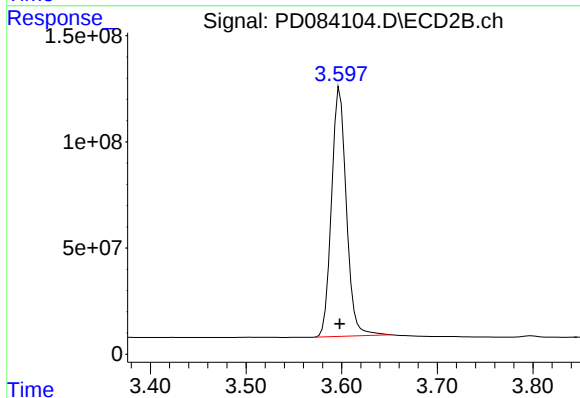


#3 gamma-BHC (Lindane)

R.T.: 3.598 min
Delta R.T.: 0.000 min
Response: 1261635671
Conc: 153.65 ng/ml

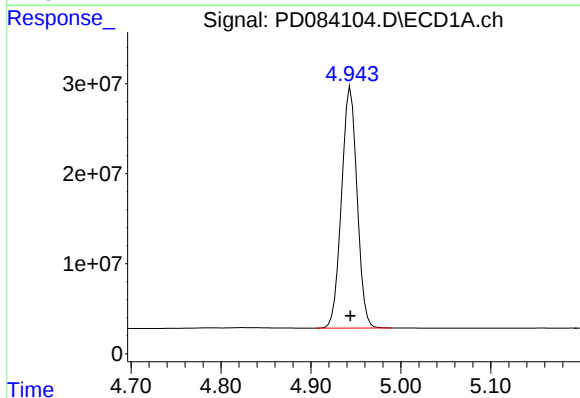


#4 Heptachlor

R.T.: 4.944 min
Delta R.T.: 0.000 min
Response: 322054151
Conc: 174.40 ng/ml

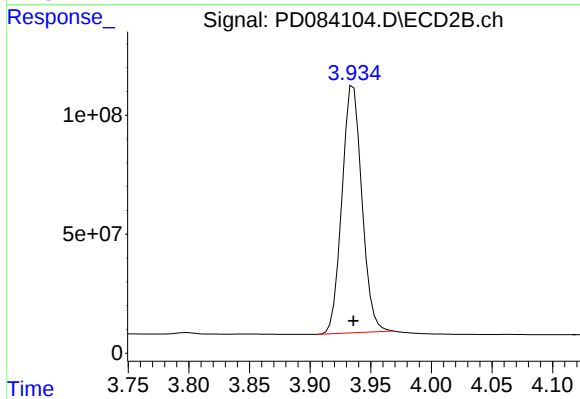


#4 Heptachlor

R.T.: 3.936 min
Delta R.T.: 0.000 min
Response: 1189784610
Conc: 148.94 ng/ml

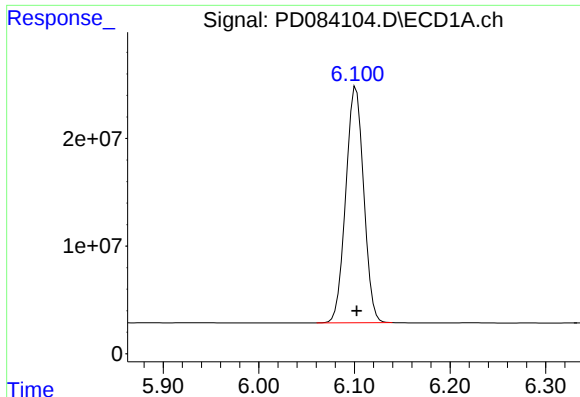


#9 Endosulfan I

R.T.: 6.102 min
Delta R.T.: 0.000 min
Response: 286737715
Conc: 164.65 ng/ml

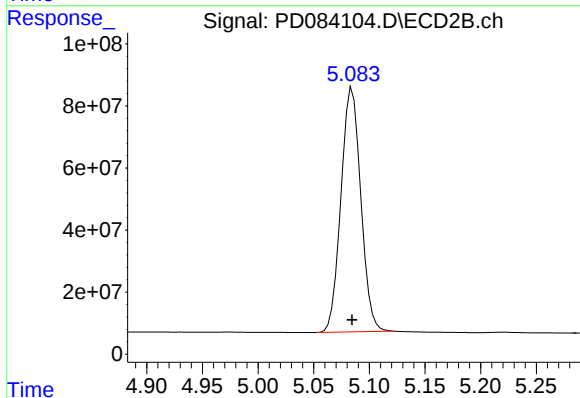


#9 Endosulfan I

R.T.: 5.085 min
Delta R.T.: 0.000 min
Response: 976822276
Conc: 147.32 ng/ml

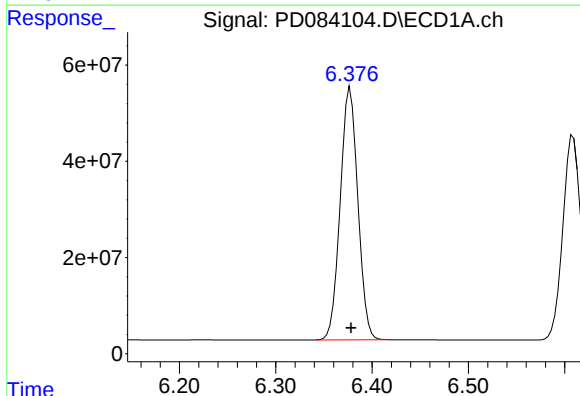


#13 Dieldrin

R.T.: 6.377 min
Delta R.T.: 0.000 min
Response: 665783398
Conc: 354.77 ng/ml

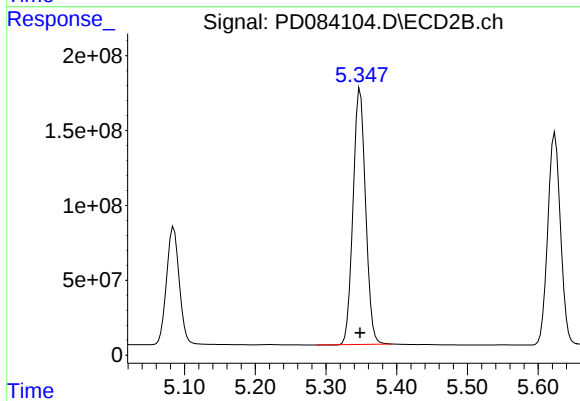


#13 Dieldrin

R.T.: 5.348 min
Delta R.T.: 0.000 min
Response: 2110003378
Conc: 288.94 ng/ml

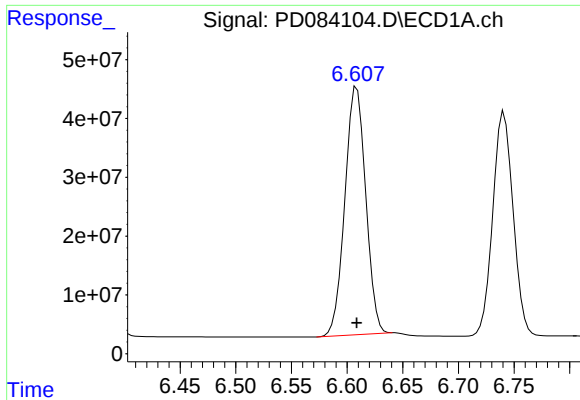


#14 Endrin

R.T.: 6.609 min
Delta R.T.: 0.000 min
Response: 551031043
Conc: 350.38 ng/ml

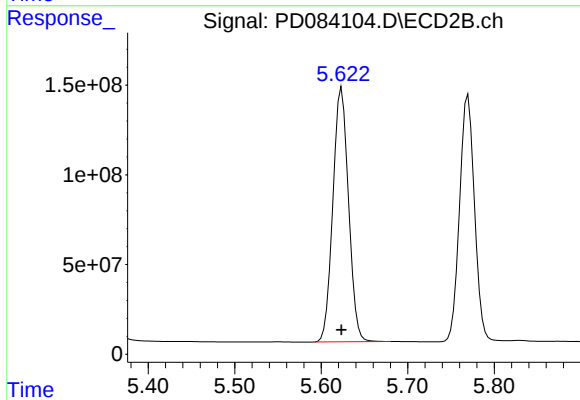


#14 Endrin

R.T.: 5.624 min
Delta R.T.: 0.000 min
Response: 1774403125
Conc: 286.41 ng/ml

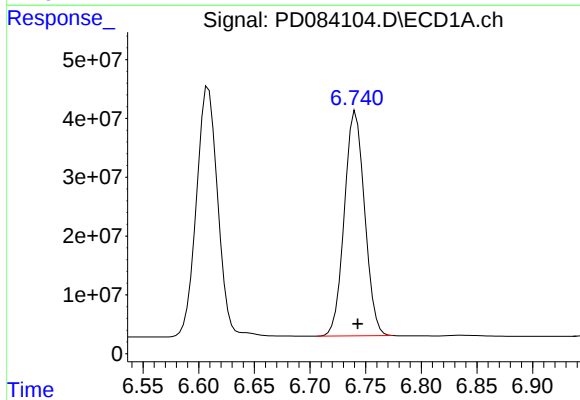


#16 4,4'-DDD

R.T.: 6.741 min
Delta R.T.: -0.002 min
Response: 484578885
Conc: 365.77 ng/ml

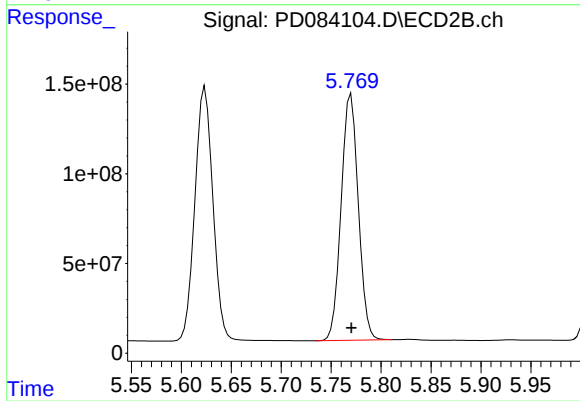


#16 4,4'-DDD

R.T.: 5.770 min
Delta R.T.: 0.000 min
Response: 1644279748
Conc: 301.88 ng/ml

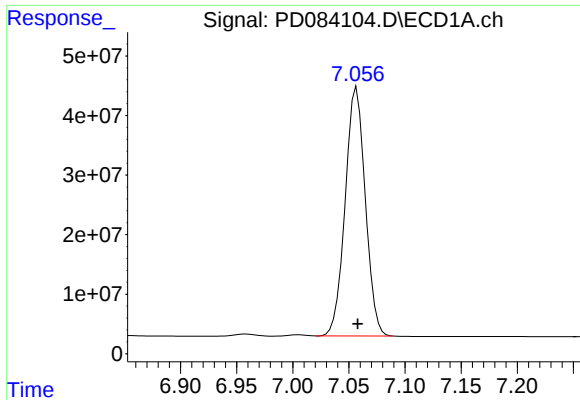


#17 4,4'-DDT

R.T.: 7.057 min
Delta R.T.: -0.001 min
Response: 520878629
Conc: 376.20 ng/ml

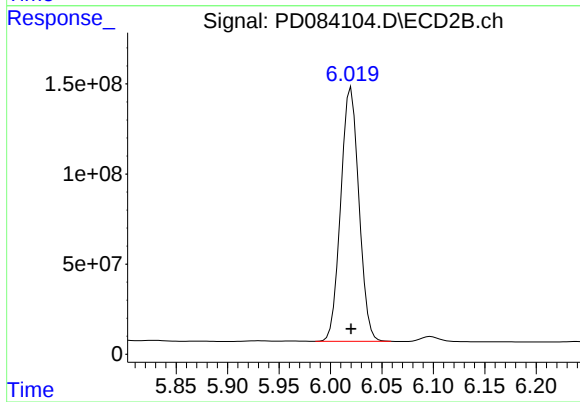


#17 4,4'-DDT

R.T.: 6.020 min
Delta R.T.: 0.000 min
Response: 1733661684
Conc: 322.30 ng/ml

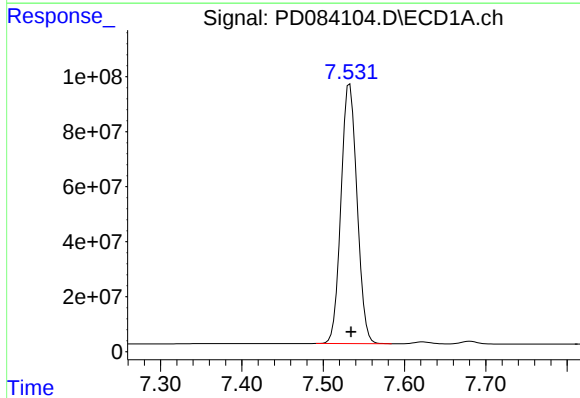


#20 Methoxychlor

R.T.: 7.533 min
Delta R.T.: -0.002 min
Response: 1290872697
Conc: 1542.09 ng/ml

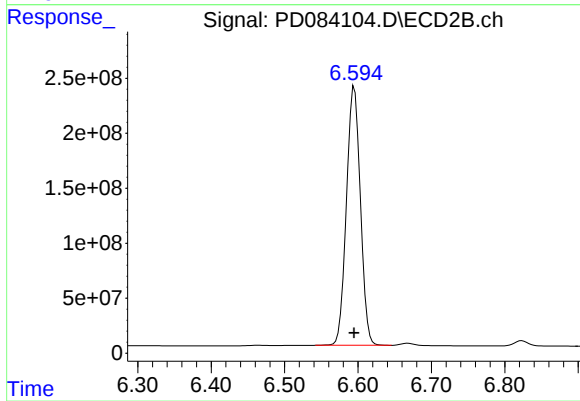


#20 Methoxychlor

R.T.: 6.595 min
Delta R.T.: 0.000 min
Response: 3114822266
Conc: 1163.41 ng/ml

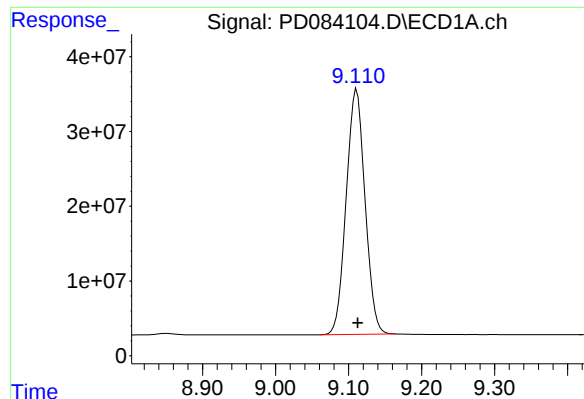

#27 Decachlorobiphenyl

R.T.: 9.111 min
Delta R.T.: -0.002 min
Response: 587935214
Conc: 303.54 ng/ml

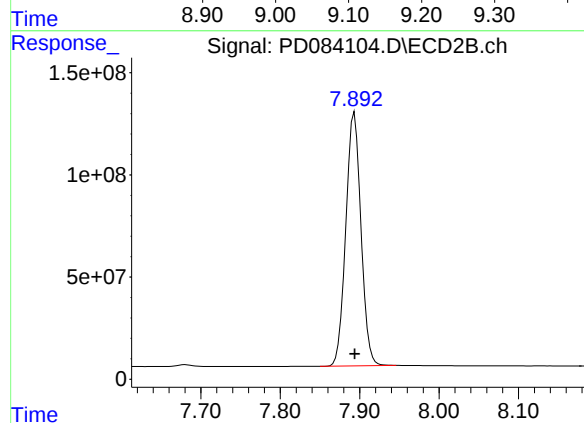

#27 Decachlorobiphenyl

R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 1648399224
Conc: 278.79 ng/ml