

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD072524\  
 Data File : PD084104.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 24 Jul 2024 19:55  
 Operator : AR\AJ  
 Sample : INDA601  
 Misc :  
 ALS Vial : 20 Sample Multiplier: 1

Instrument :  
 ECD\_D  
 ClientSampleId :  
 INDA6066

Manual Integrations  
 APPROVED

Reviewed By :Abdul Mirza 07/26/2024  
 Supervised By :Ankita Jodhani 07/26/2024

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jul 25 05:15:31 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD072524CLP-TCLP.M  
 Quant Title : GC Extractables  
 QLast Update : Thu Jul 25 05:15:23 2024  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm


|                             | Compound        | RT#1  | RT#2  | Resp#1   | Resp#2   | ng/ml    | ng/ml    |
|-----------------------------|-----------------|-------|-------|----------|----------|----------|----------|
| -----                       |                 |       |       |          |          |          |          |
| System Monitoring Compounds |                 |       |       |          |          |          |          |
| 1)                          | SA Tetrachlo... | 3.561 | 2.771 | 144.7E6  | 786.7E6  | 160.018  | 149.299  |
| 2)                          | SA Decachlor... | 9.111 | 7.893 | 587.9E6  | 1648.4E6 | 307.846  | 286.485  |
| Target Compounds            |                 |       |       |          |          |          |          |
| 2)                          | A alpha-BHC     | 4.018 | 3.270 | 327.2E6  | 1359.0E6 | 186.731  | 158.966  |
| 3)                          | MA gamma-BHC... | 4.353 | 3.598 | 312.4E6  | 1261.6E6 | 180.360  | 157.200  |
| 4)                          | MA Heptachlor   | 4.944 | 3.936 | 322.1E6  | 1189.8E6 | 171.778  | 152.900  |
| 9)                          | A Endosulfan I  | 6.102 | 5.085 | 286.7E6  | 976.8E6  | 164.164  | 151.030  |
| 13)                         | MA Dieldrin     | 6.377 | 5.347 | 665.8E6  | 2130.4E6 | 347.661  | 301.362m |
| 14)                         | MA Endrin       | 6.609 | 5.624 | 551.0E6  | 1774.4E6 | 344.245  | 295.359  |
| 16)                         | A 4,4'-DDD      | 6.741 | 5.770 | 484.6E6  | 1644.3E6 | 356.445  | 309.047  |
| 17)                         | MA 4,4'-DDT     | 7.057 | 6.020 | 520.9E6  | 1733.7E6 | 364.980  | 327.958  |
| 20)                         | A Methoxychlor  | 7.533 | 6.595 | 1290.9E6 | 3114.8E6 | 1562.392 | 1254.164 |
| -----                       |                 |       |       |          |          |          |          |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD072524\  
Data File : PD084104.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 24 Jul 2024 19:55  
Operator : AR\AJ  
Sample : INDA601  
Misc :  
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jul 25 05:15:31 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD072524CLP-TCLP.M  
Quant Title : GC Extractables  
QLast Update : Thu Jul 25 05:15:23 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

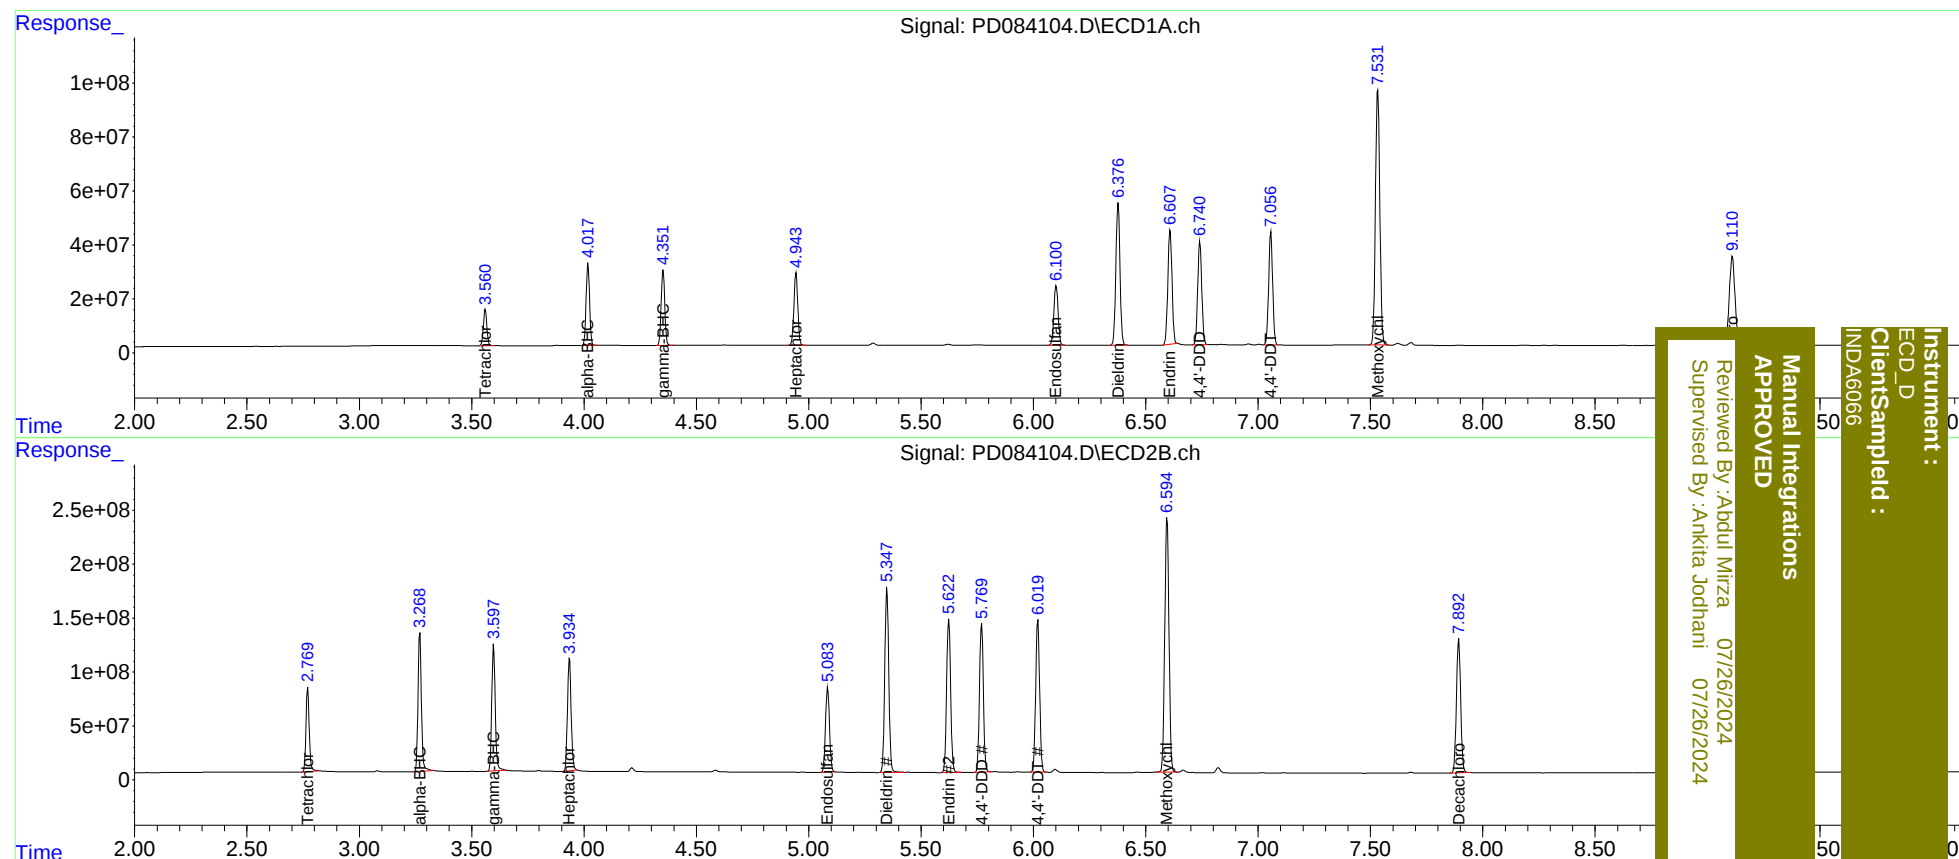

Manual Integrations  
APPROVED  
Reviewed By: Abdul Mirza 07/26/2024  
Supervised By: Ankita Jodhani 07/26/2024

Instrument :  
ECD\_D  
Client Sampled :  
INDA6066