

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD D\Data\PD072618\
 Data File : PD048510.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Jul 2018 18:56
 Operator : AJ\SJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 02:53:08 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072618.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 26 02:53:16 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.361	3.968	139.3E6	1254.2E6	100.944	97.640
28)	SA Decachlor...	8.042	8.988	139.9E6	1539.9E6	99.309	96.316
Target Compounds							
23)	Chlordane-1	4.207	4.954	56088368	628.3E6	945.562	973.299
24)	Chlordane-2	4.699	5.417	59008218	604.5E6	998.604	975.968
25)	Chlordane-3	5.255	6.057	330.3E6	2057.8E6	1679.728	969.446 #
26)	Chlordane-4	5.312	6.133	173.8E6	2344.5E6	1006.966	966.804
27)	Chlordane-5	6.137	6.926	63685993	540.8E6	1009.012	976.710



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD D\Data\PD072618\
Data File : PD048510.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jul 2018 18:56
Operator : AJ\SJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 02:53:08 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072618.M
Quant Title : GC Extractables
QLast Update : Thu Jul 26 02:53:16 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

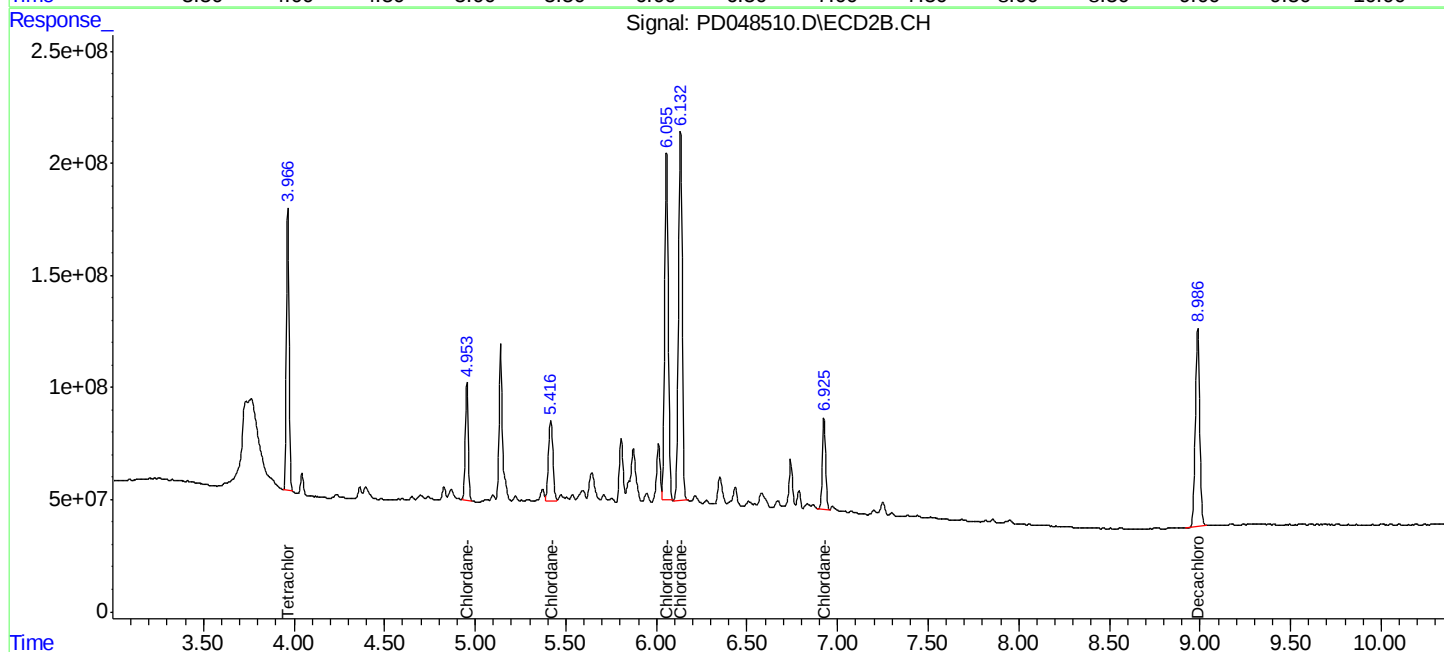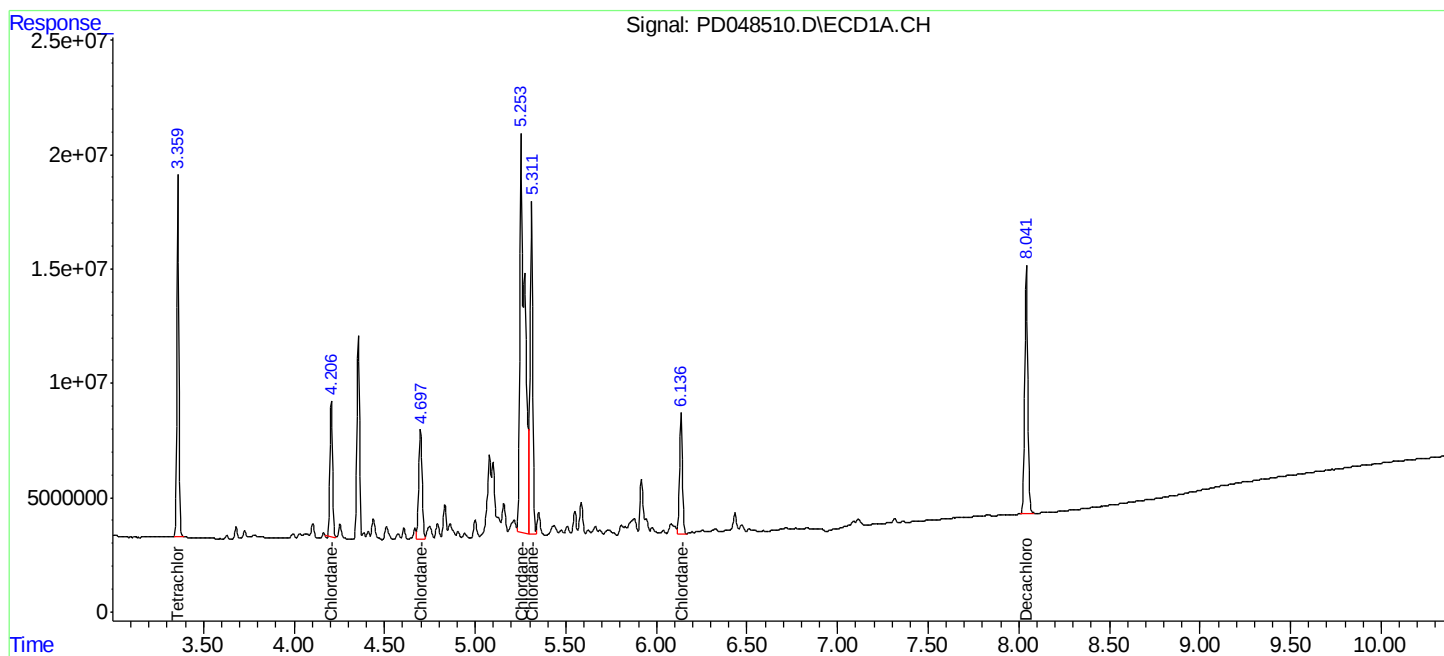


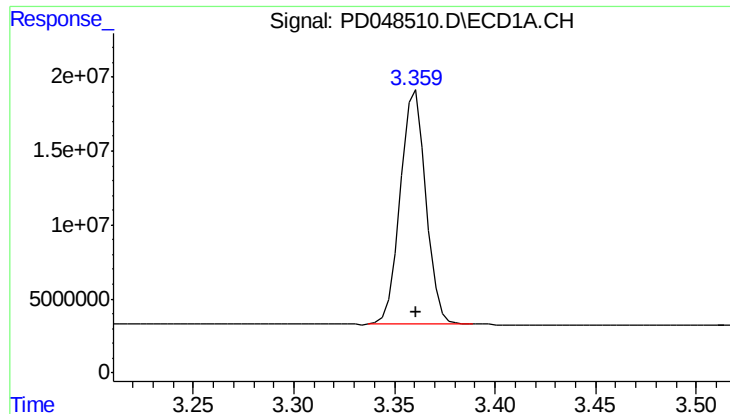

#1 Tetrachloro-m-xylene


R.T.: 3.361 min
Delta R.T.: 0.000 min
Response: 139292531
Conc: 100.94 ng/ml

Instrument :
ECD_D
ClientSampleId :

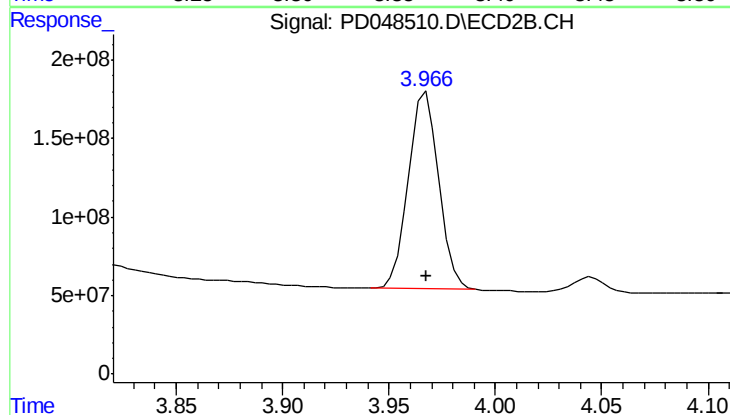


#1 Tetrachloro-m-xylene

R.T.: 3.968 min
Delta R.T.: 0.000 min
Response: 1254220063
Conc: 97.64 ng/ml

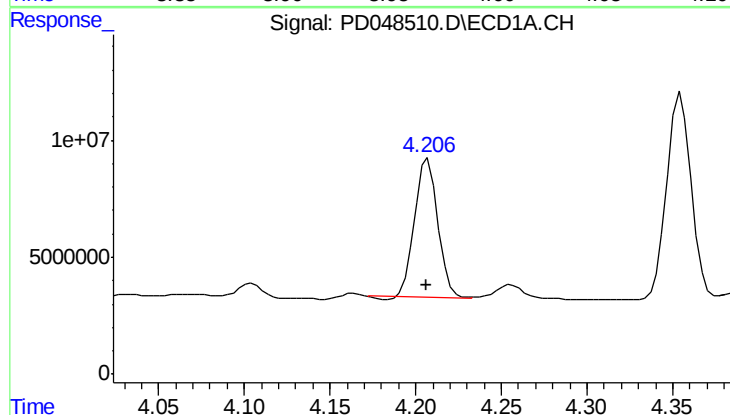


#23 Chlordane-1

R.T.: 4.207 min
Delta R.T.: 0.001 min
Response: 56088368
Conc: 945.56 ng/ml

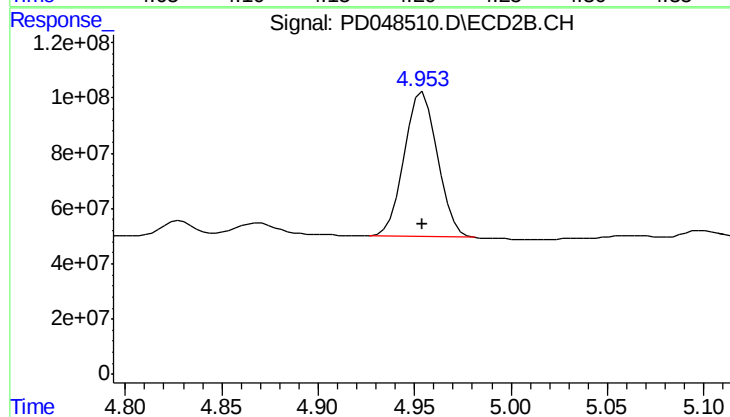

#23 Chlordane-1


R.T.: 4.954 min
Delta R.T.: 0.000 min
Response: 628325450
Conc: 973.30 ng/ml

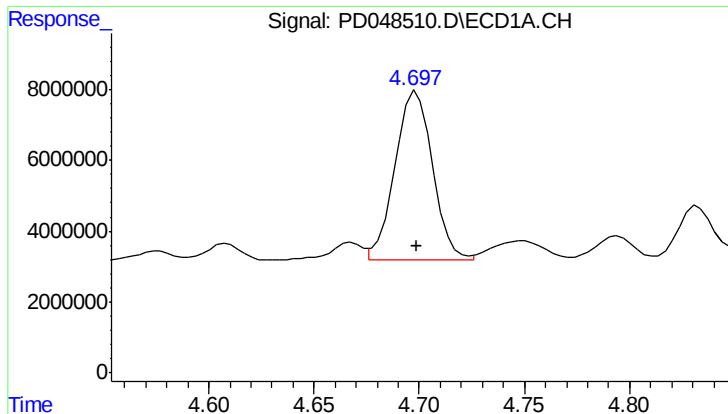

#24 Chlordane-2


R.T.: 4.699 min
Delta R.T.: 0.000 min
Response: 59008218
Conc: 998.60 ng/ml

Instrument :
ECD_D
ClientSampleId :

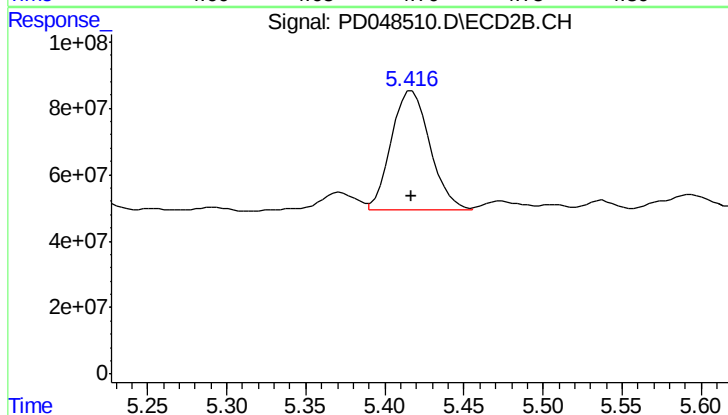


#24 Chlordane-2

R.T.: 5.417 min
Delta R.T.: 0.000 min
Response: 604452856
Conc: 975.97 ng/ml

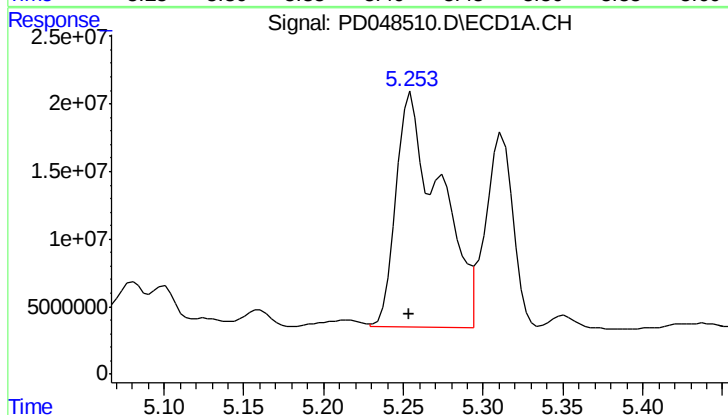


#25 Chlordane-3

R.T.: 5.255 min
Delta R.T.: 0.002 min
Response: 330294773
Conc: 1679.73 ng/ml

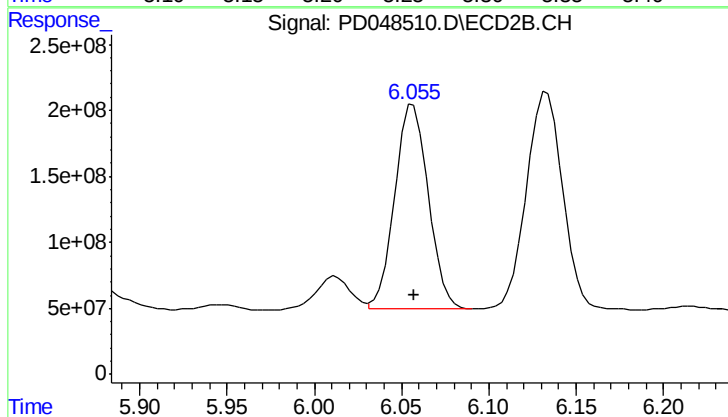

#25 Chlordane-3


R.T.: 6.057 min
Delta R.T.: 0.000 min
Response: 2057764814
Conc: 969.45 ng/ml

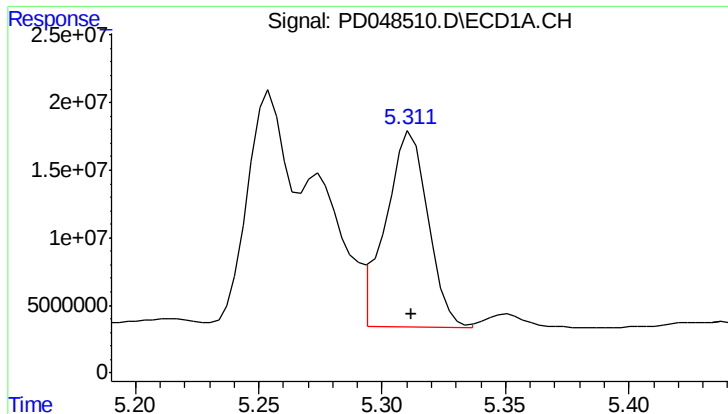

#26 Chlordane-4


R.T.: 5.312 min
Delta R.T.: 0.000 min
Response: 173788283
Conc: 1006.97 ng/ml

Instrument :
ECD_D
ClientSampleId :

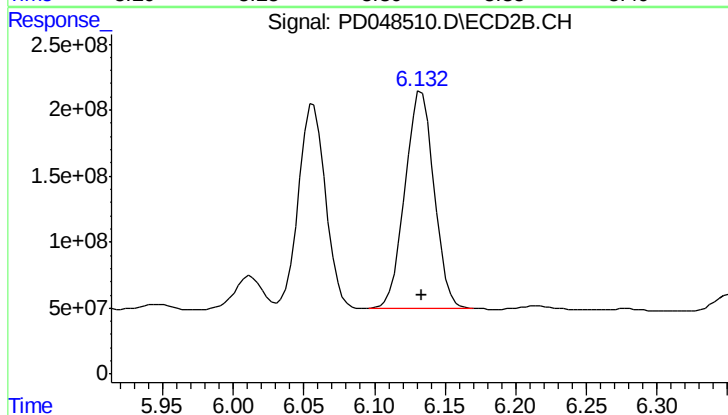


#26 Chlordane-4

R.T.: 6.133 min
Delta R.T.: 0.000 min
Response: 2344482398
Conc: 966.80 ng/ml

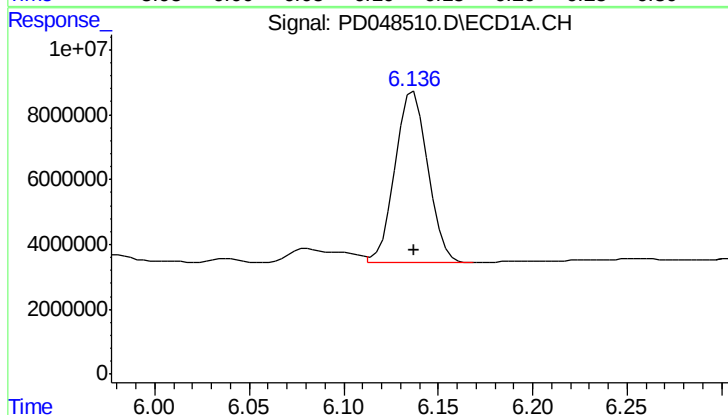


#27 Chlordane-5

R.T.: 6.137 min
Delta R.T.: 0.000 min
Response: 63685993
Conc: 1009.01 ng/ml

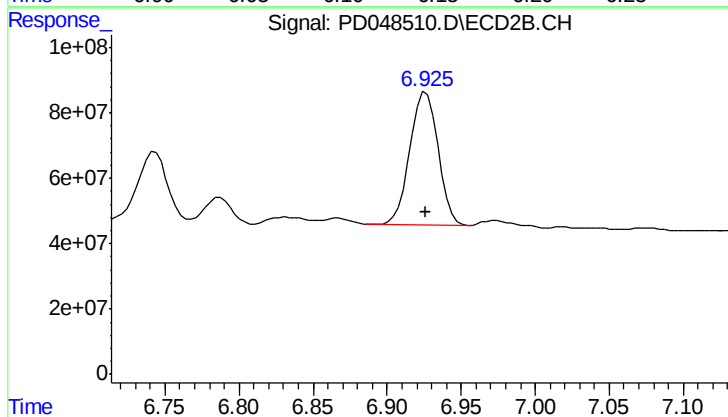

#27 Chlordane-5


R.T.: 6.926 min
Delta R.T.: 0.000 min
Response: 540775326
Conc: 976.71 ng/ml

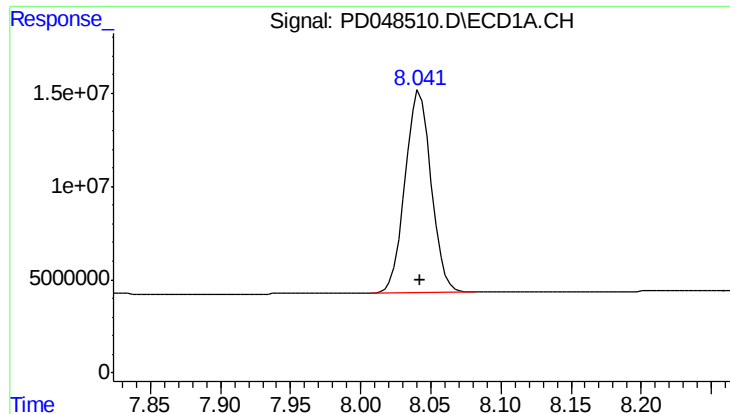

#28 Decachlorobiphenyl

R.T.: 8.042 min
Delta R.T.: 0.000 min
Response: 139885914
Conc: 99.31 ng/ml

Instrument :
ECD_D
ClientSampleId :

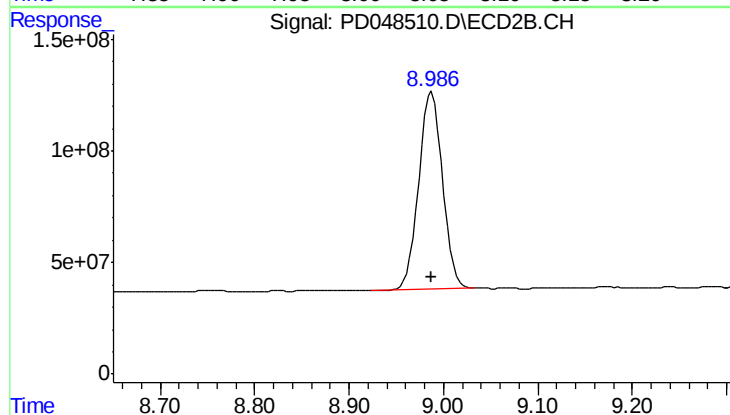

#28 Decachlorobiphenyl

R.T.: 8.988 min
Delta R.T.: 0.000 min
Response: 1539949182
Conc: 96.32 ng/ml