

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072622\
 Data File : PD071148.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jul 2022 19:24
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 03:44:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 26 03:39:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.815	3.574	61765647	650.0E6	21.779	23.089
28)	SA Decachlor...	8.019	9.106	57643743	220.9E6	20.784	21.339
Target Compounds							
9)	A Endosulfan I	5.174	6.117	36754027	161.9E6	10.730	11.779
10)	B gamma-Chl...	5.053	5.984	41533838	170.5E6	10.931	11.607
12)	B 4,4'-DDE	5.309	6.234	73676155	320.6E6	21.526	22.427
13)	MA Dieldrin	5.441	6.394	79693353	338.9E6	22.003	23.064
19)	B Endosulfa...	6.420	7.216	58090819	250.6E6	20.200	21.010
20)	A Methoxychlor	6.703	7.545	169.8E6	663.2E6	102.957	96.219
21)	B Endrin ke...	6.931	7.709	69713201	301.2E6	21.400	22.440



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072622\
Data File : PD071148.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jul 2022 19:24
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 03:44:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072622.M
Quant Title : GC Extractables
QLast Update : Tue Jul 26 03:39:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

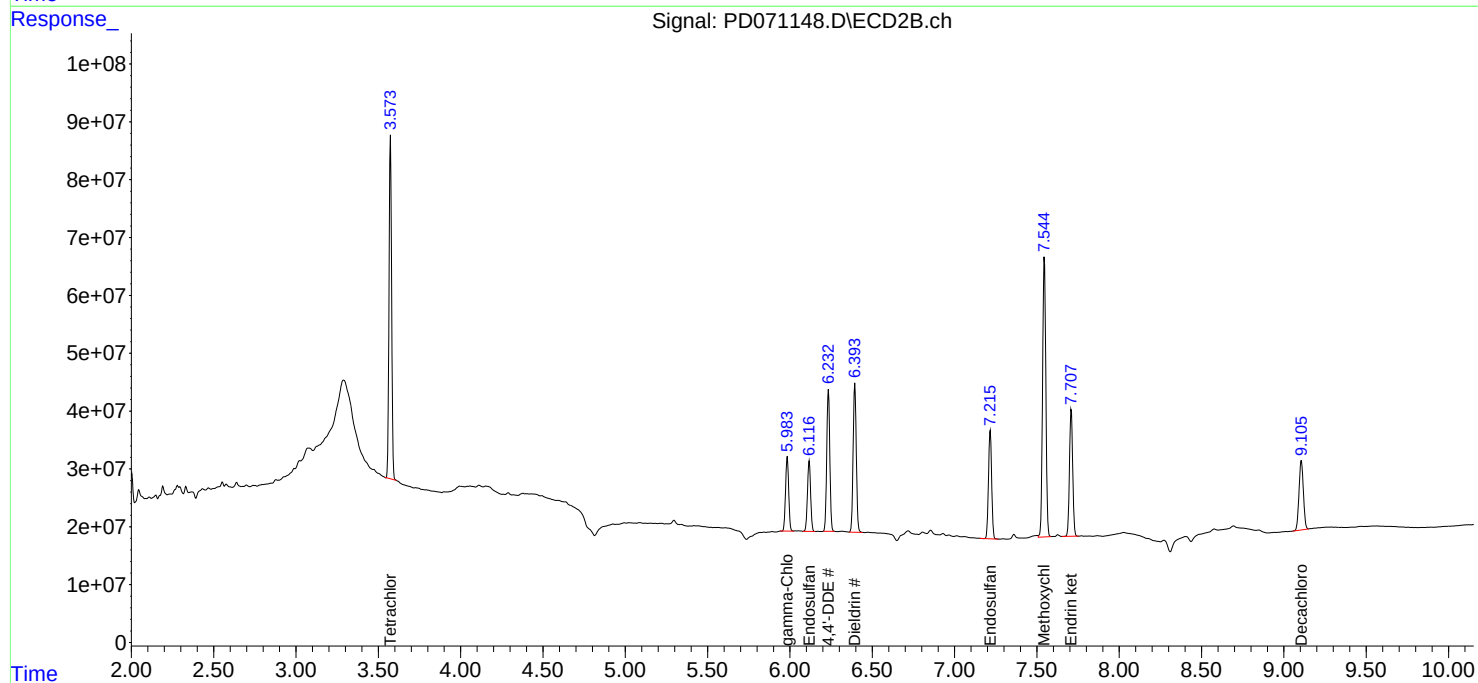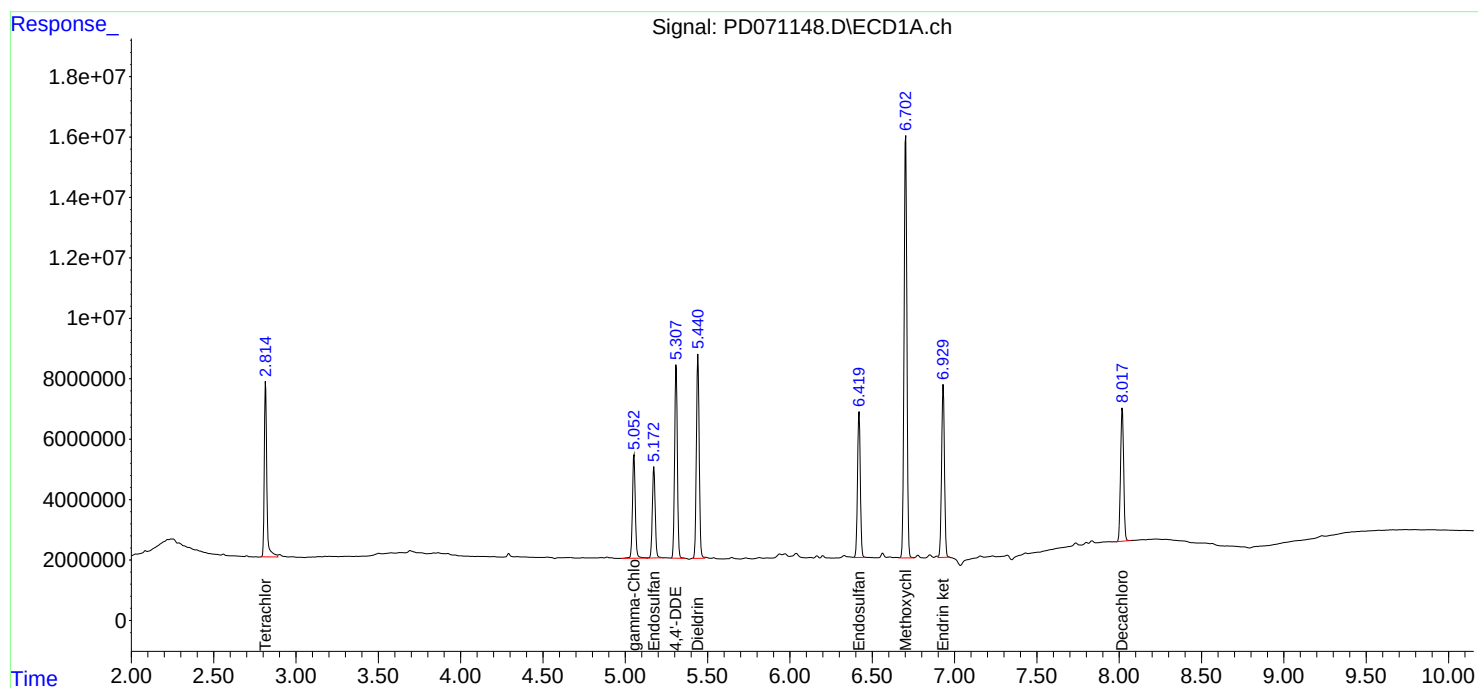


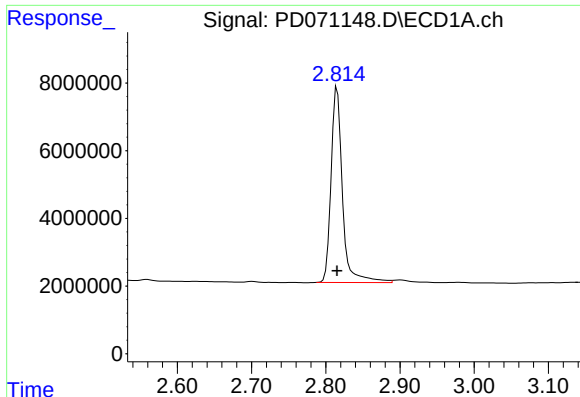

#1 Tetrachloro-m-xylene


R.T.: 2.815 min
Delta R.T.: 0.000 min
Response: 61765647
Conc: 21.78 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

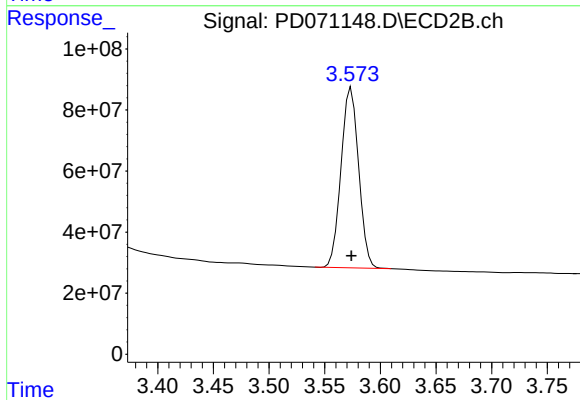


#1 Tetrachloro-m-xylene

R.T.: 3.574 min
Delta R.T.: 0.000 min
Response: 649956443
Conc: 23.09 ng/ml

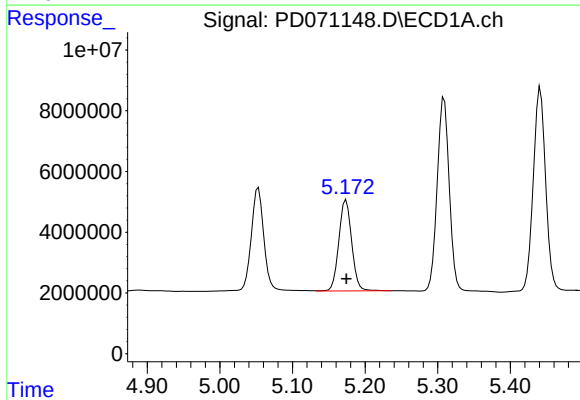


#9 Endosulfan I

R.T.: 5.174 min
Delta R.T.: 0.000 min
Response: 36754027
Conc: 10.73 ng/ml

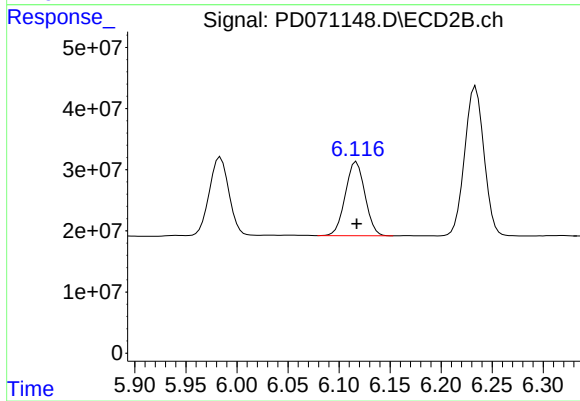

#9 Endosulfan I


R.T.: 6.117 min
Delta R.T.: 0.000 min
Response: 161944439
Conc: 11.78 ng/ml

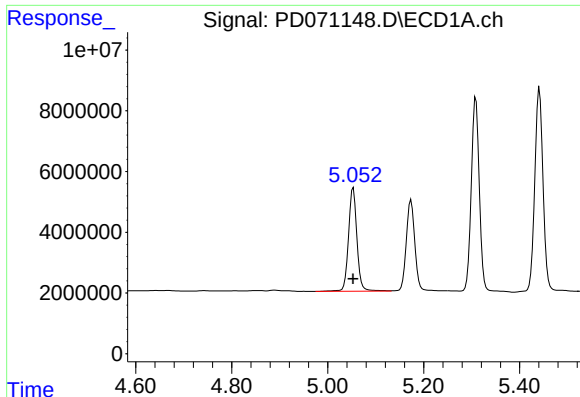

#10 gamma-Chlordane


R.T.: 5.053 min
Delta R.T.: 0.000 min
Response: 41533838
Conc: 10.93 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

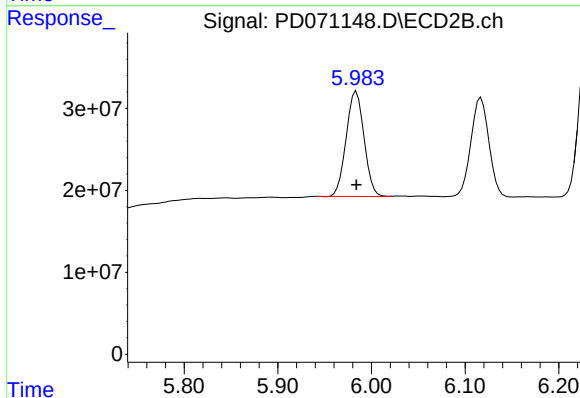


#10 gamma-Chlordane

R.T.: 5.984 min
Delta R.T.: 0.000 min
Response: 170455487
Conc: 11.61 ng/ml

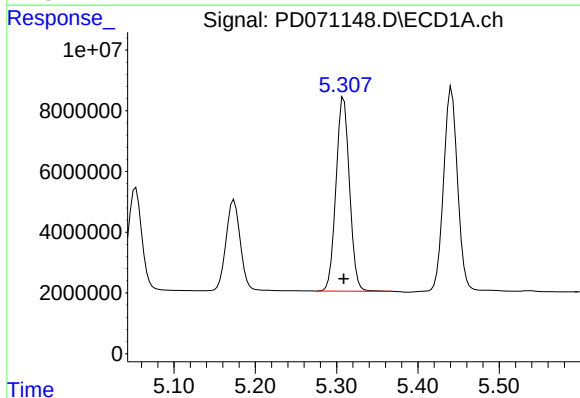


#12 4,4'-DDE

R.T.: 5.309 min
Delta R.T.: 0.000 min
Response: 73676155
Conc: 21.53 ng/ml

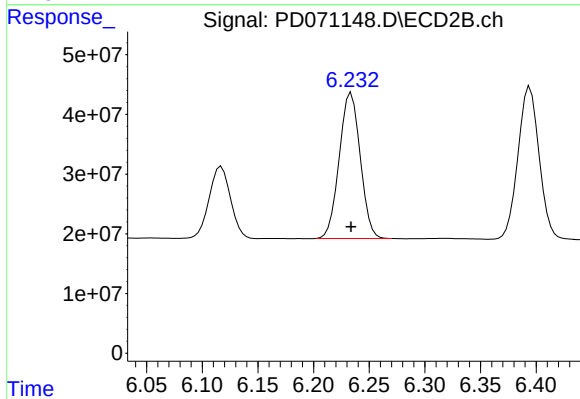

#12 4,4'-DDE


R.T.: 6.234 min
Delta R.T.: 0.000 min
Response: 320590801
Conc: 22.43 ng/ml

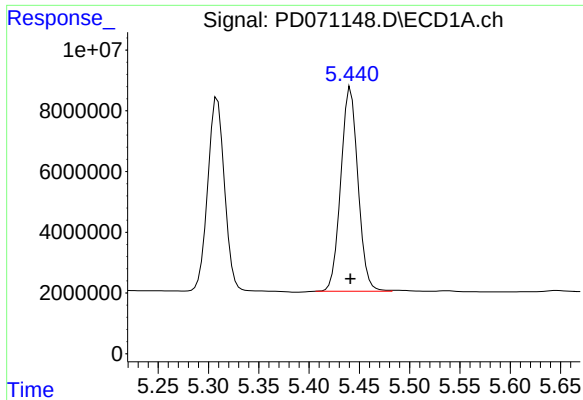

#13 Dieldrin


R.T.: 5.441 min
Delta R.T.: 0.000 min
Response: 79693353
Conc: 22.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

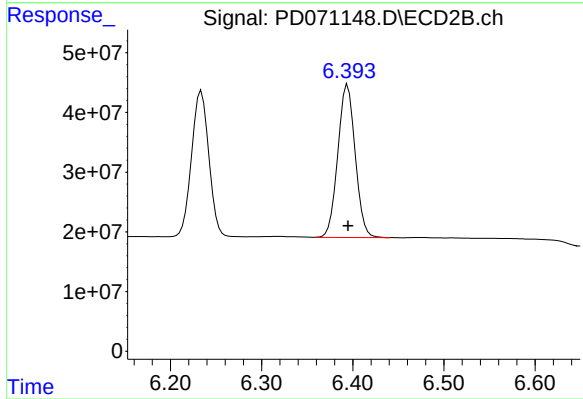


#13 Dieldrin

R.T.: 6.394 min
Delta R.T.: 0.000 min
Response: 338916396
Conc: 23.06 ng/ml

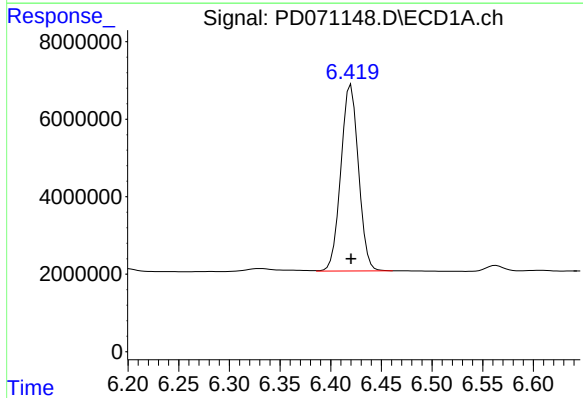


#19 Endosulfan Sulfate

R.T.: 6.420 min
Delta R.T.: 0.000 min
Response: 58090819
Conc: 20.20 ng/ml

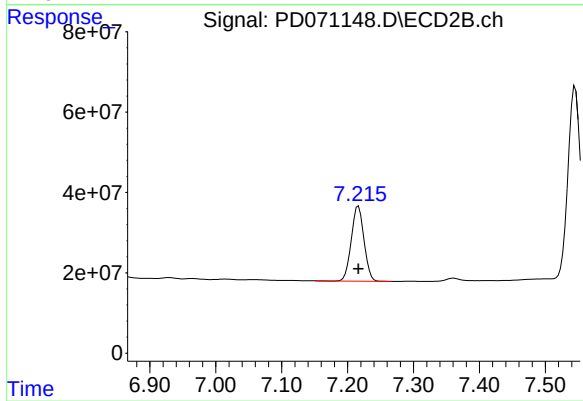

#19 Endosulfan Sulfate


R.T.: 7.216 min
Delta R.T.: 0.000 min
Response: 250585508
Conc: 21.01 ng/ml

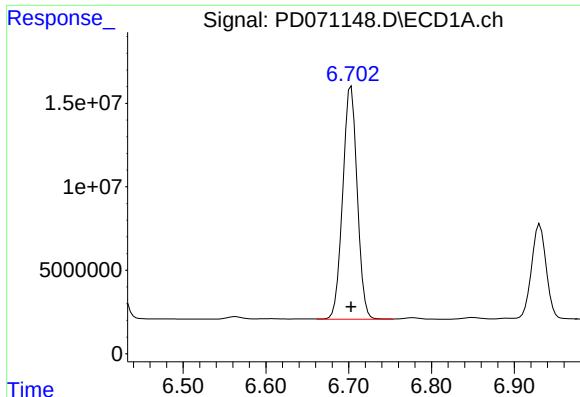

#20 Methoxychlor


R.T.: 6.703 min
Delta R.T.: 0.000 min
Response: 169829600
Conc: 102.96 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

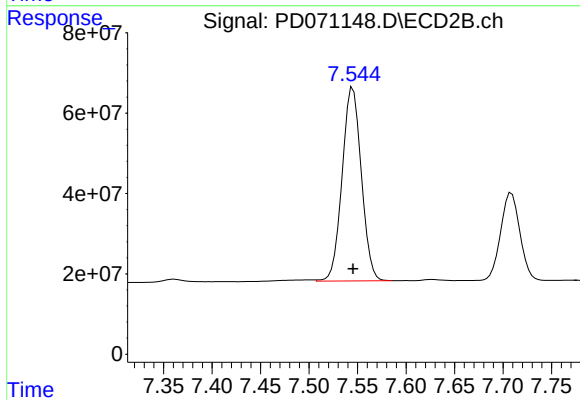


#20 Methoxychlor

R.T.: 7.545 min
Delta R.T.: 0.000 min
Response: 663212121
Conc: 96.22 ng/ml

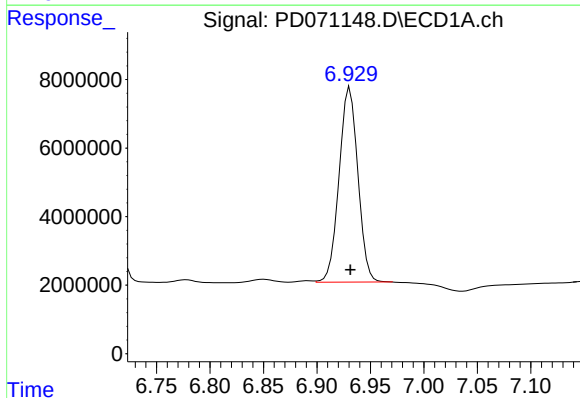


#21 Endrin ketone

R.T.: 6.931 min
Delta R.T.: 0.000 min
Response: 69713201
Conc: 21.40 ng/ml

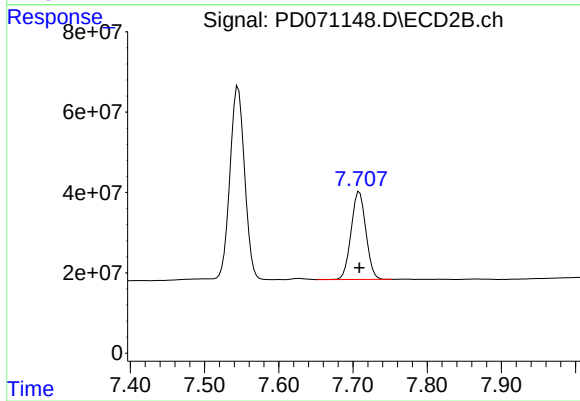

#21 Endrin ketone


R.T.: 7.709 min
Delta R.T.: 0.000 min
Response: 301241048
Conc: 22.44 ng/ml

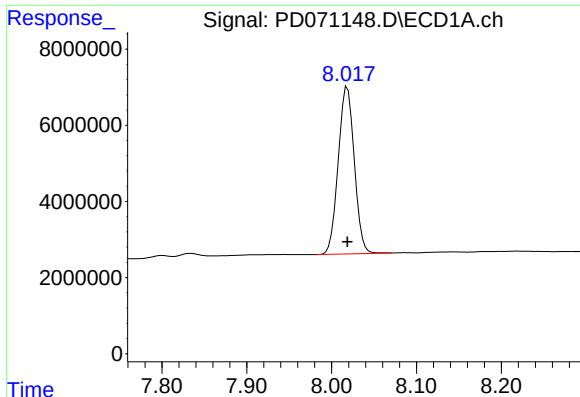

#28 Decachlorobiphenyl

R.T.: 8.019 min
Delta R.T.: 0.000 min
Response: 57643743
Conc: 20.78 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

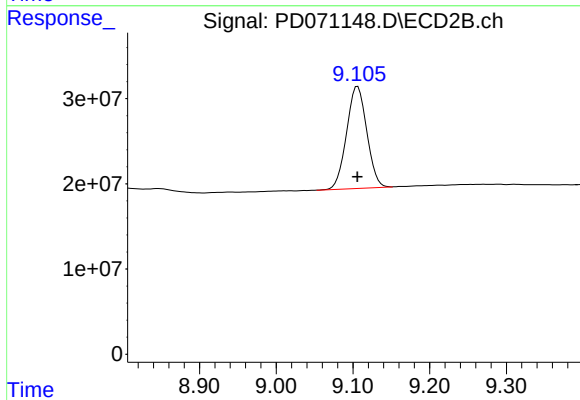

#28 Decachlorobiphenyl

R.T.: 9.106 min
Delta R.T.: 0.000 min
Response: 220917292
Conc: 21.34 ng/ml