

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072622\
 Data File : PD071154.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jul 2022 20:45
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 01:50:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 26 01:43:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.815	3.574	317.8E6	2496.1E6	98.695	97.801
28)	SA Decachlor...	8.019	9.106	244.3E6	864.8E6	97.036	95.030
Target Compounds							
23)	Chlordane-1	3.831	4.738	99933586	664.4E6	963.589	942.122
24)	Chlordane-2	4.415	5.271	108.5E6	529.2E6	955.257	935.499
25)	Chlordane-3	5.054	5.983	342.8E6	1710.3E6	976.199	956.171
26)	Chlordane-4	5.117	6.062	317.3E6	1988.3E6	985.343	953.578
27)	Chlordane-5	6.021	6.924	115.0E6	418.0E6	981.117	949.735



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072622\
Data File : PD071154.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jul 2022 20:45
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 01:50:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072622.M
Quant Title : GC Extractables
QLast Update : Tue Jul 26 01:43:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

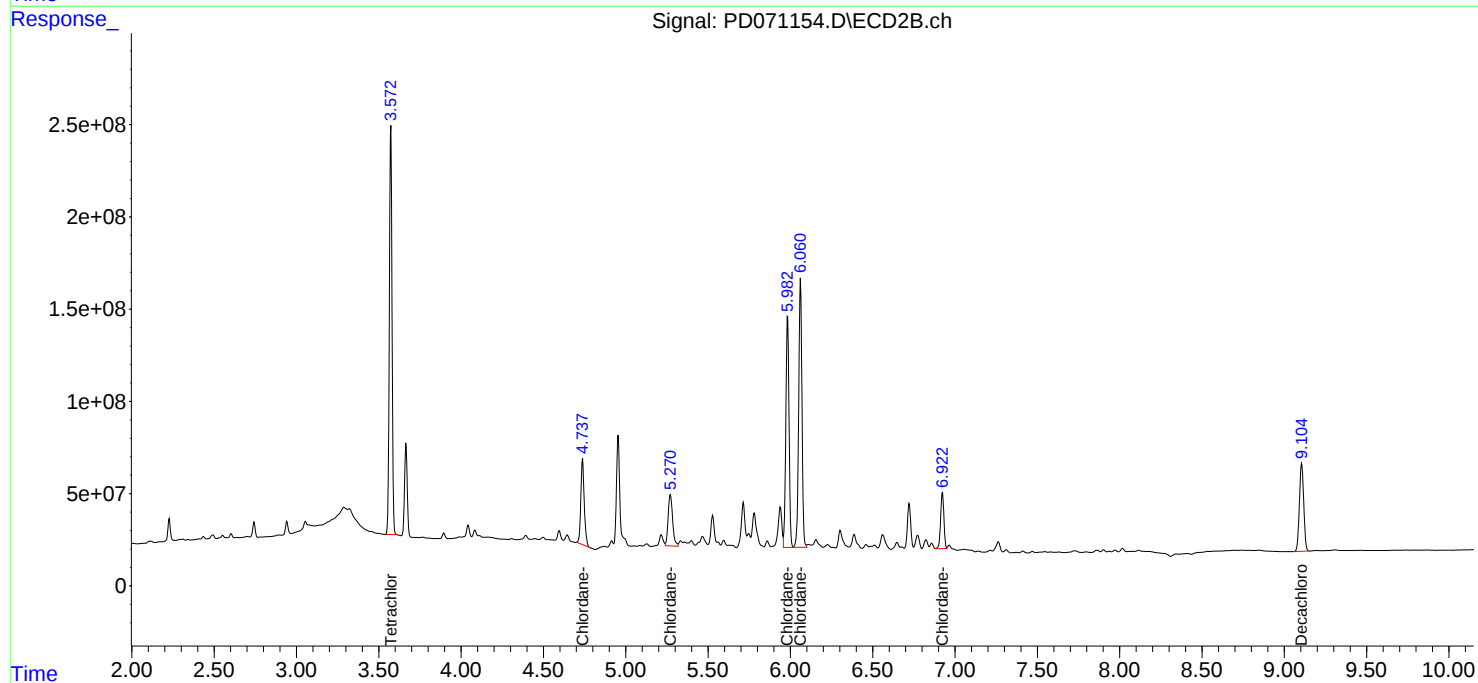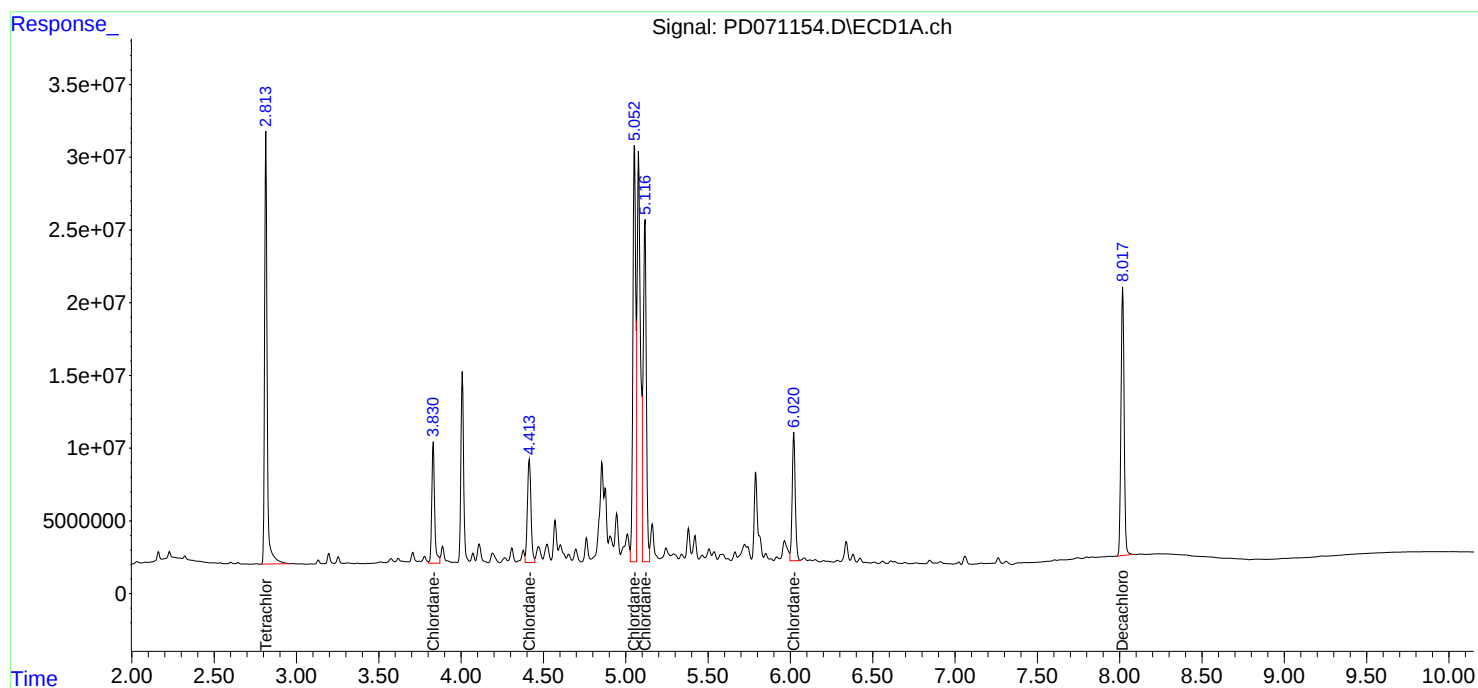


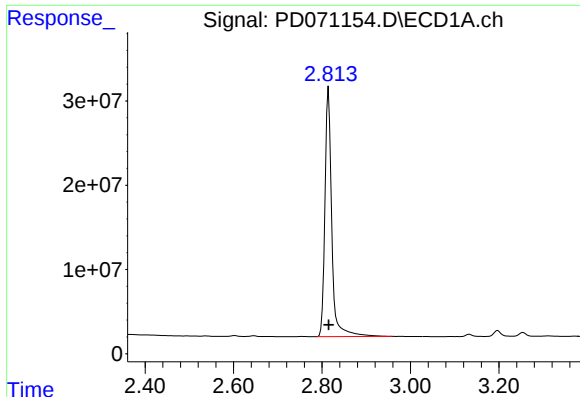

#1 Tetrachloro-m-xylene


R.T.: 2.815 min
Delta R.T.: 0.000 min
Response: 317793076
Conc: 98.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

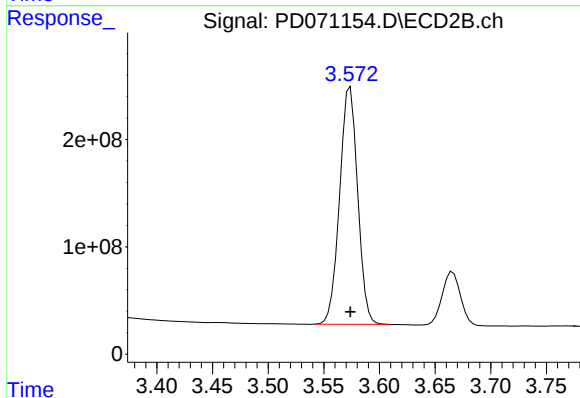


#1 Tetrachloro-m-xylene

R.T.: 3.574 min
Delta R.T.: 0.000 min
Response: 2496067969
Conc: 97.80 ng/ml

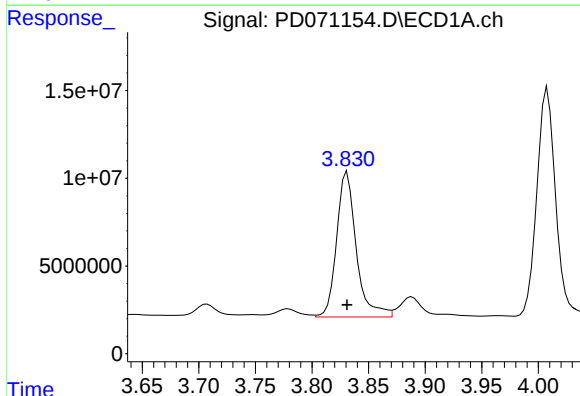


#23 Chlordane-1

R.T.: 3.831 min
Delta R.T.: 0.000 min
Response: 99933586
Conc: 963.59 ng/ml

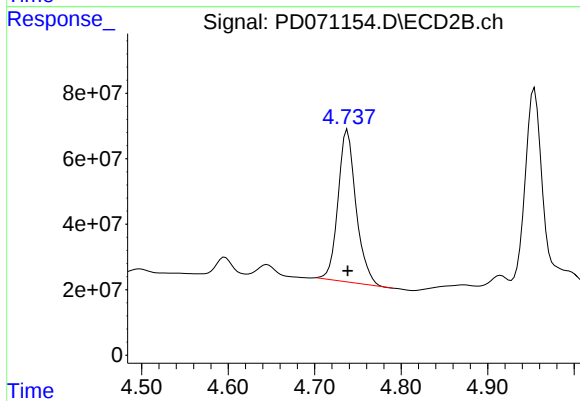

#23 Chlordane-1


R.T.: 4.738 min
Delta R.T.: 0.000 min
Response: 664413880
Conc: 942.12 ng/ml

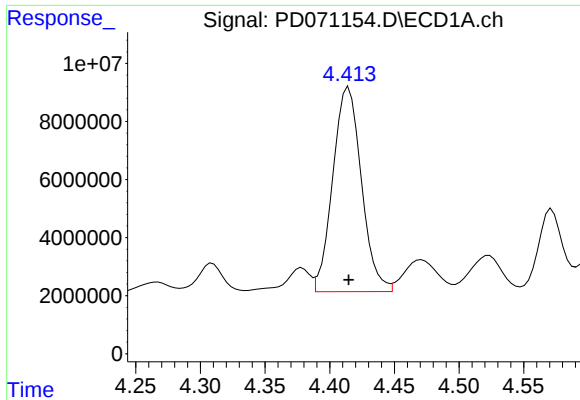

#24 Chlordane-2


R.T.: 4.415 min
Delta R.T.: 0.000 min
Response: 108502038
Conc: 955.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

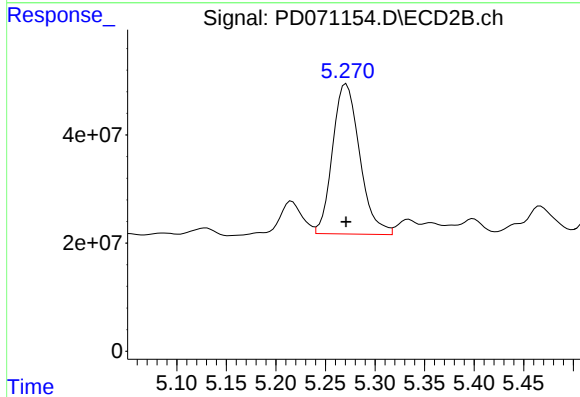


#24 Chlordane-2

R.T.: 5.271 min
Delta R.T.: 0.000 min
Response: 529215926
Conc: 935.50 ng/ml

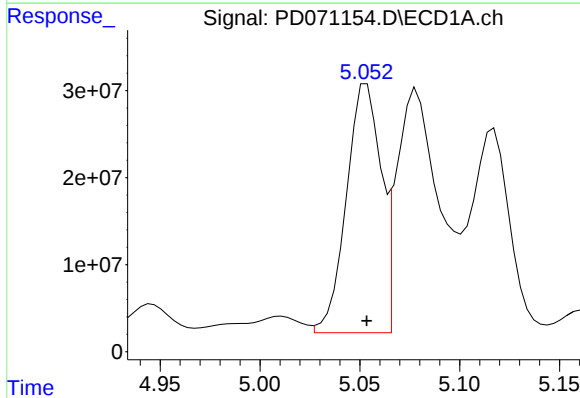


#25 Chlordane-3

R.T.: 5.054 min
Delta R.T.: 0.000 min
Response: 342752020
Conc: 976.20 ng/ml

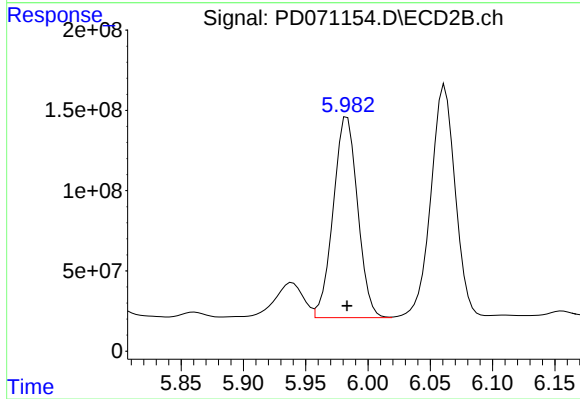

#25 Chlordane-3


R.T.: 5.983 min
Delta R.T.: 0.000 min
Response: 1710296293
Conc: 956.17 ng/ml

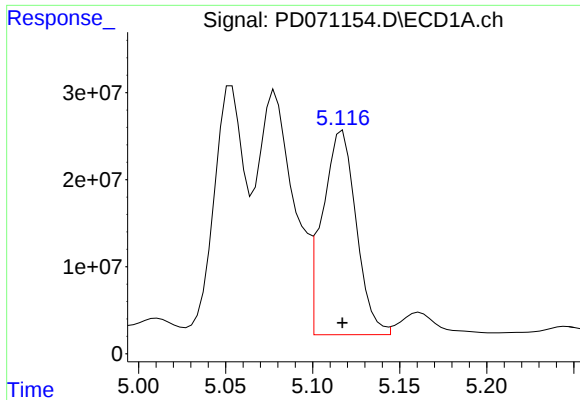

#26 Chlordane-4


R.T.: 5.117 min
Delta R.T.: 0.000 min
Response: 317257088
Conc: 985.34 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

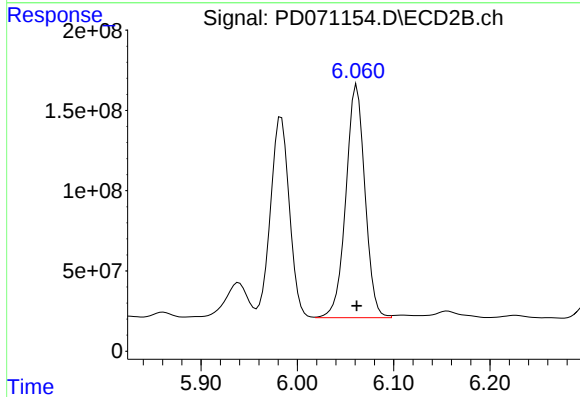


#26 Chlordane-4

R.T.: 6.062 min
Delta R.T.: 0.000 min
Response: 1988291359
Conc: 953.58 ng/ml

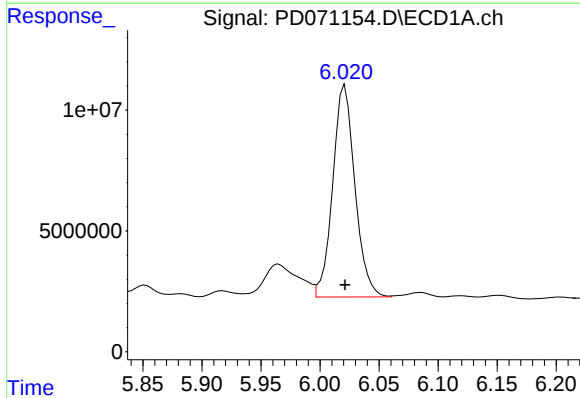


#27 Chlordane-5

R.T.: 6.021 min
Delta R.T.: 0.000 min
Response: 114977963
Conc: 981.12 ng/ml

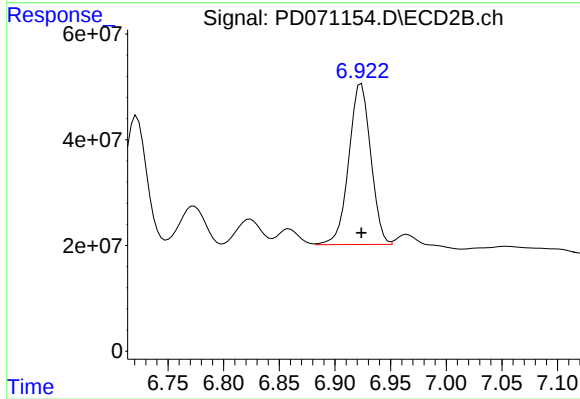

#27 Chlordane-5


R.T.: 6.924 min
Delta R.T.: 0.000 min
Response: 417992338
Conc: 949.74 ng/ml

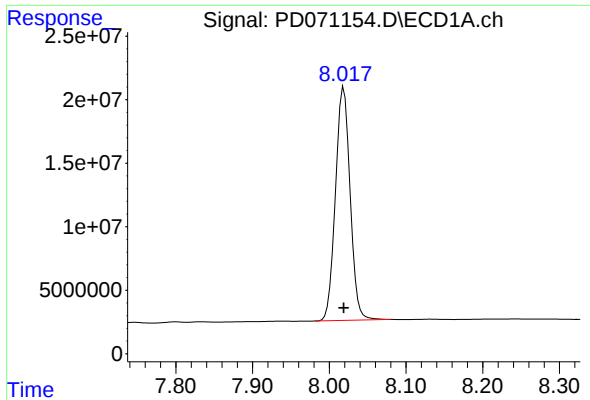

#28 Decachlorobiphenyl

R.T.: 8.019 min
Delta R.T.: 0.000 min
Response: 244291498
Conc: 97.04 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

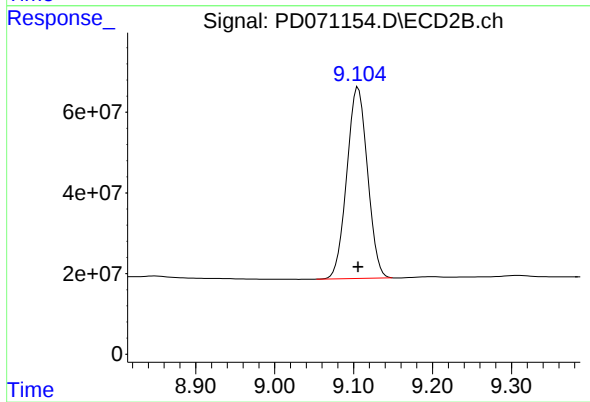

#28 Decachlorobiphenyl

R.T.: 9.106 min
Delta R.T.: 0.000 min
Response: 864840174
Conc: 95.03 ng/ml