

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072622\
 Data File : PD071155.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jul 2022 20:59
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 01:52:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 26 01:43:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.815	3.574	235.5E6	1859.8E6	73.740	73.567
28)	SA Decachlor...	8.018	9.106	183.5E6	660.6E6	73.580	73.374
Target Compounds							
23)	Chlordane-1	3.831	4.738	75148590	507.4E6	732.877	729.412
24)	Chlordane-2	4.415	5.271	82356466	410.3E6	733.194	733.381
25)	Chlordane-3	5.054	5.983	255.1E6	1296.6E6	734.256	733.081
26)	Chlordane-4	5.118	6.062	237.3E6	1515.5E6	741.262	734.390
27)	Chlordane-5	6.021	6.923	86002824	320.9E6	739.169	735.997



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072622\
Data File : PD071155.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jul 2022 20:59
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 01:52:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072622.M
Quant Title : GC Extractables
QLast Update : Tue Jul 26 01:43:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

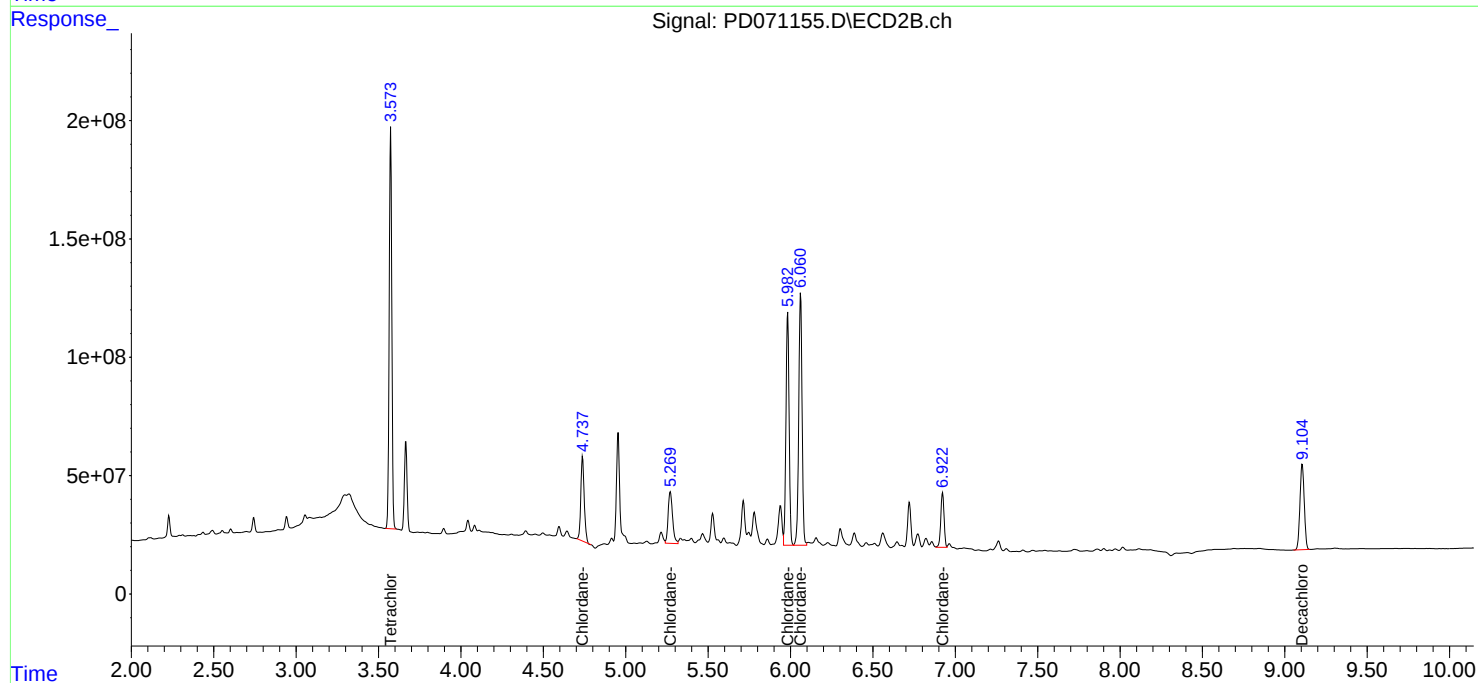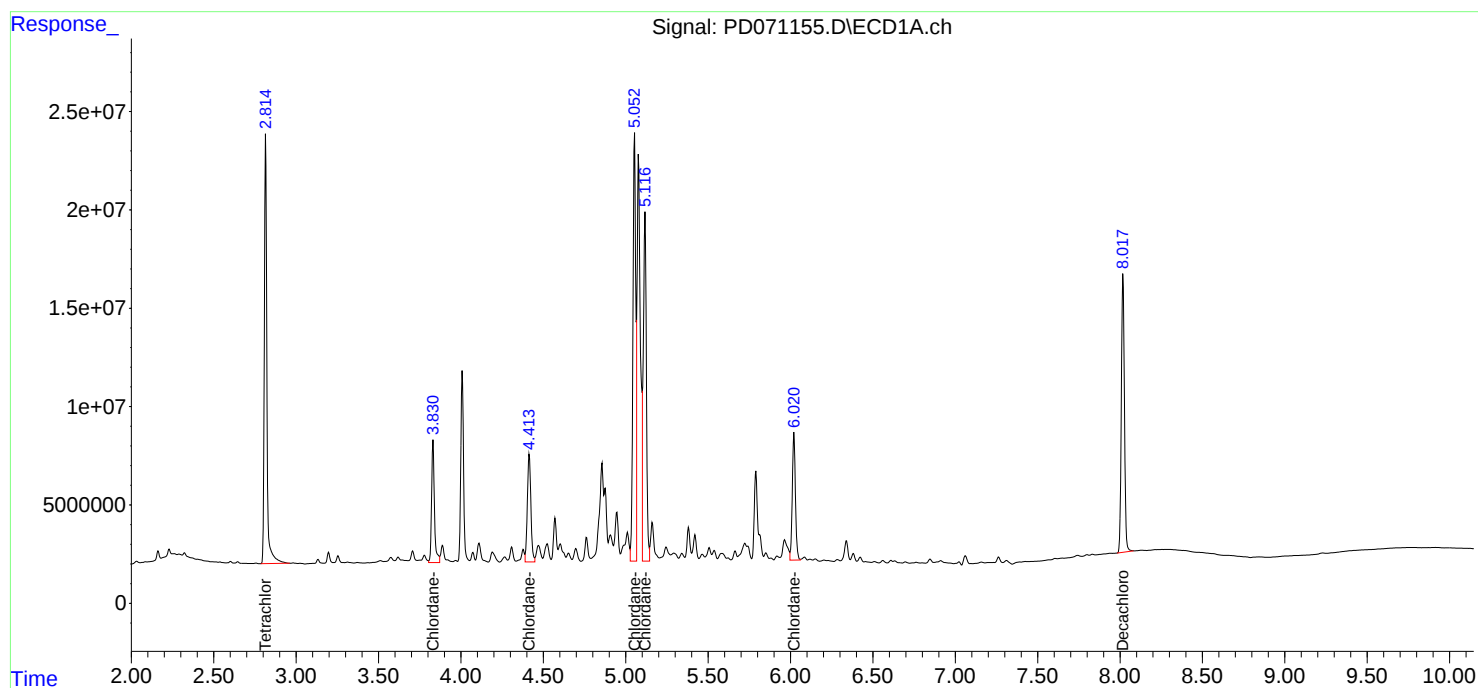


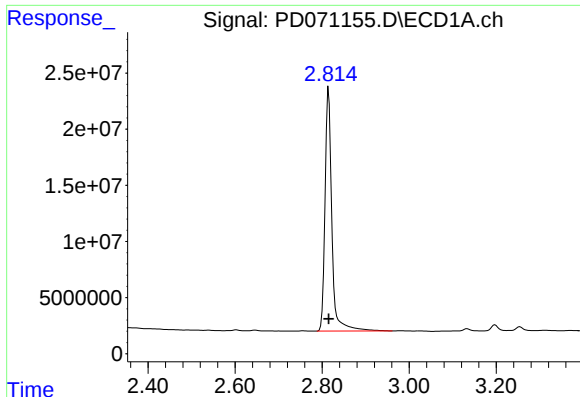

#1 Tetrachloro-m-xylene


R.T.: 2.815 min
Delta R.T.: 0.000 min
Response: 235461909
Conc: 73.74 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

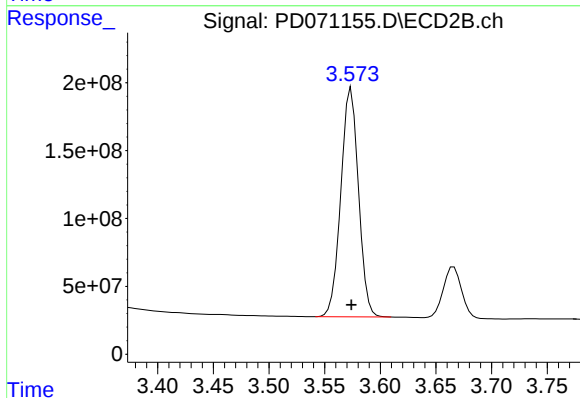


#1 Tetrachloro-m-xylene

R.T.: 3.574 min
Delta R.T.: 0.000 min
Response: 1859827571
Conc: 73.57 ng/ml

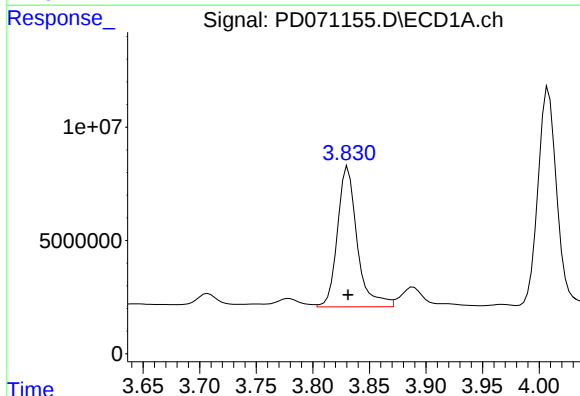


#23 Chlordane-1

R.T.: 3.831 min
Delta R.T.: 0.000 min
Response: 75148590
Conc: 732.88 ng/ml

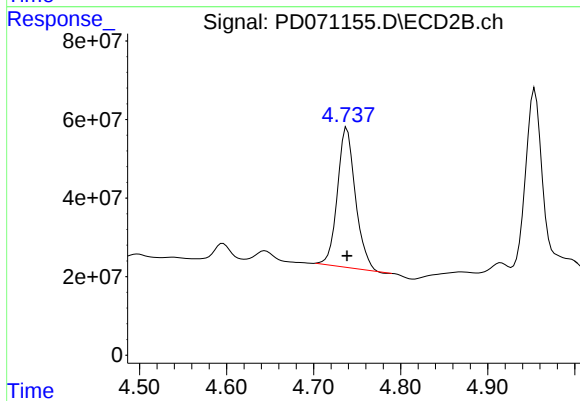

#23 Chlordane-1


R.T.: 4.738 min
Delta R.T.: 0.000 min
Response: 507439463
Conc: 729.41 ng/ml

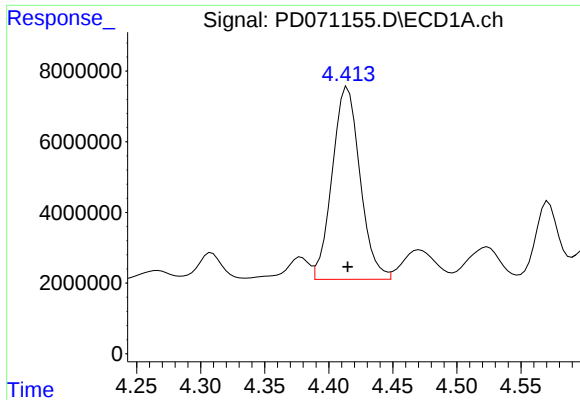

#24 Chlordane-2


R.T.: 4.415 min
Delta R.T.: 0.000 min
Response: 82356466
Conc: 733.19 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

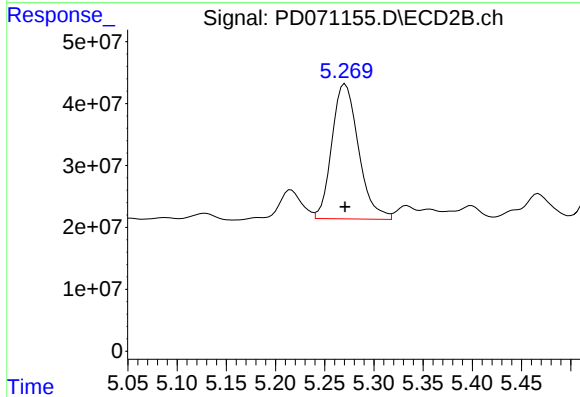


#24 Chlordane-2

R.T.: 5.271 min
Delta R.T.: 0.000 min
Response: 410330412
Conc: 733.38 ng/ml

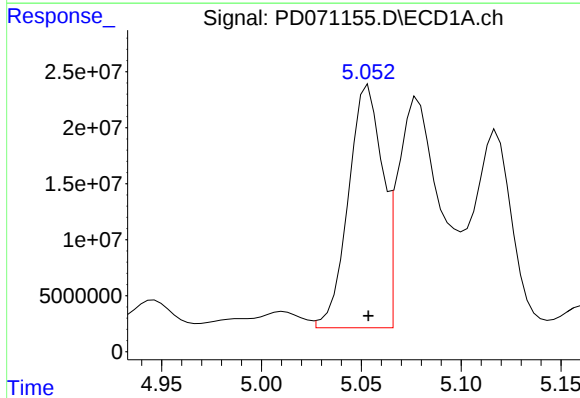


#25 Chlordane-3

R.T.: 5.054 min
Delta R.T.: 0.000 min
Response: 255126044
Conc: 734.26 ng/ml

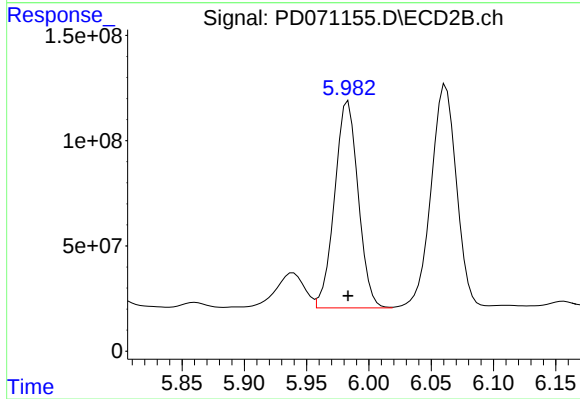

#25 Chlordane-3


R.T.: 5.983 min
Delta R.T.: 0.000 min
Response: 1296632693
Conc: 733.08 ng/ml

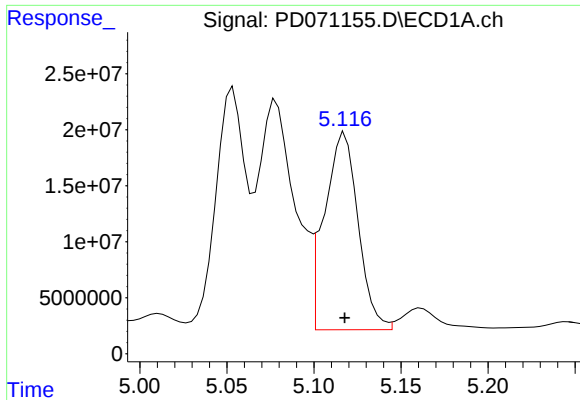

#26 Chlordane-4


R.T.: 5.118 min
Delta R.T.: 0.000 min
Response: 237286344
Conc: 741.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

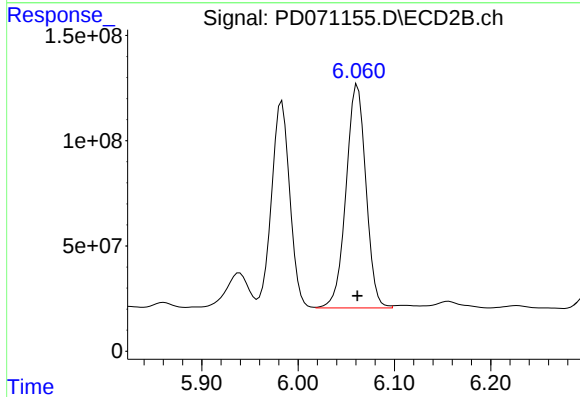


#26 Chlordane-4

R.T.: 6.062 min
Delta R.T.: 0.000 min
Response: 1515495166
Conc: 734.39 ng/ml

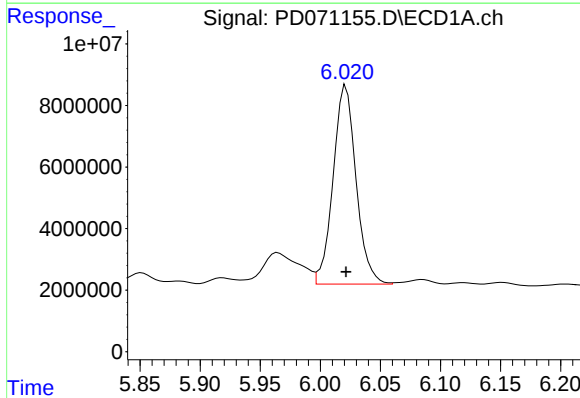


#27 Chlordane-5

R.T.: 6.021 min
Delta R.T.: 0.000 min
Response: 86002824
Conc: 739.17 ng/ml

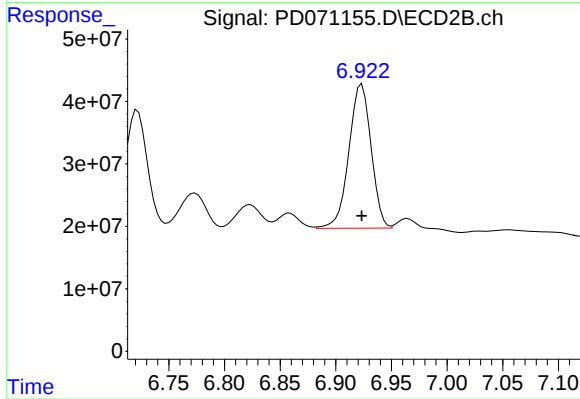

#27 Chlordane-5


R.T.: 6.923 min
Delta R.T.: 0.000 min
Response: 320927280
Conc: 736.00 ng/ml

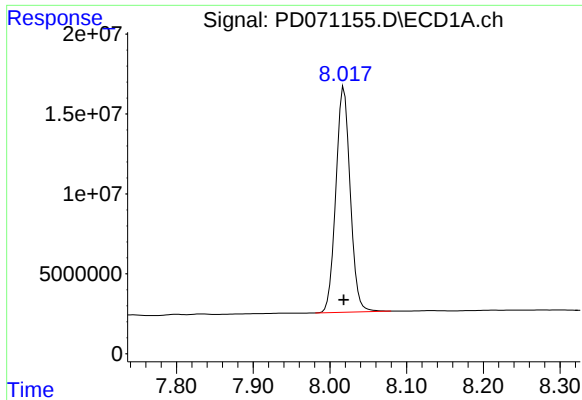

#28 Decachlorobiphenyl

R.T.: 8.018 min
Delta R.T.: 0.000 min
Response: 183503608
Conc: 73.58 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

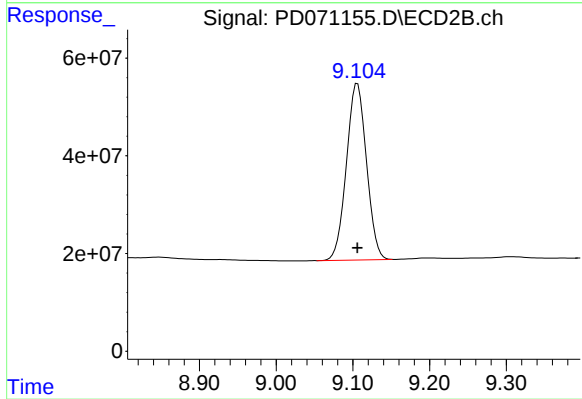

#28 Decachlorobiphenyl

R.T.: 9.106 min
Delta R.T.: 0.000 min
Response: 660589288
Conc: 73.37 ng/ml