

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072622\
 Data File : PD071156.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jul 2022 21:13
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 01:45:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 26 01:43:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.815	3.574	163.1E6	1304.2E6	50.000	50.000
28)	SA Decachlor...	8.019	9.105	129.6E6	477.6E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	3.831	4.738	53742951	373.0E6	500.000	500.000
24)	Chlordane-2	4.415	5.272	59333161	301.1E6	500.000	500.000
25)	Chlordane-3	5.054	5.984	179.7E6	933.5E6	500.000	500.000
26)	Chlordane-4	5.117	6.062	163.3E6	1090.9E6	500.000	500.000
27)	Chlordane-5	6.021	6.924	59701921	231.1E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072622\
Data File : PD071156.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jul 2022 21:13
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 01:45:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072622.M
Quant Title : GC Extractables
QLast Update : Tue Jul 26 01:43:16 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

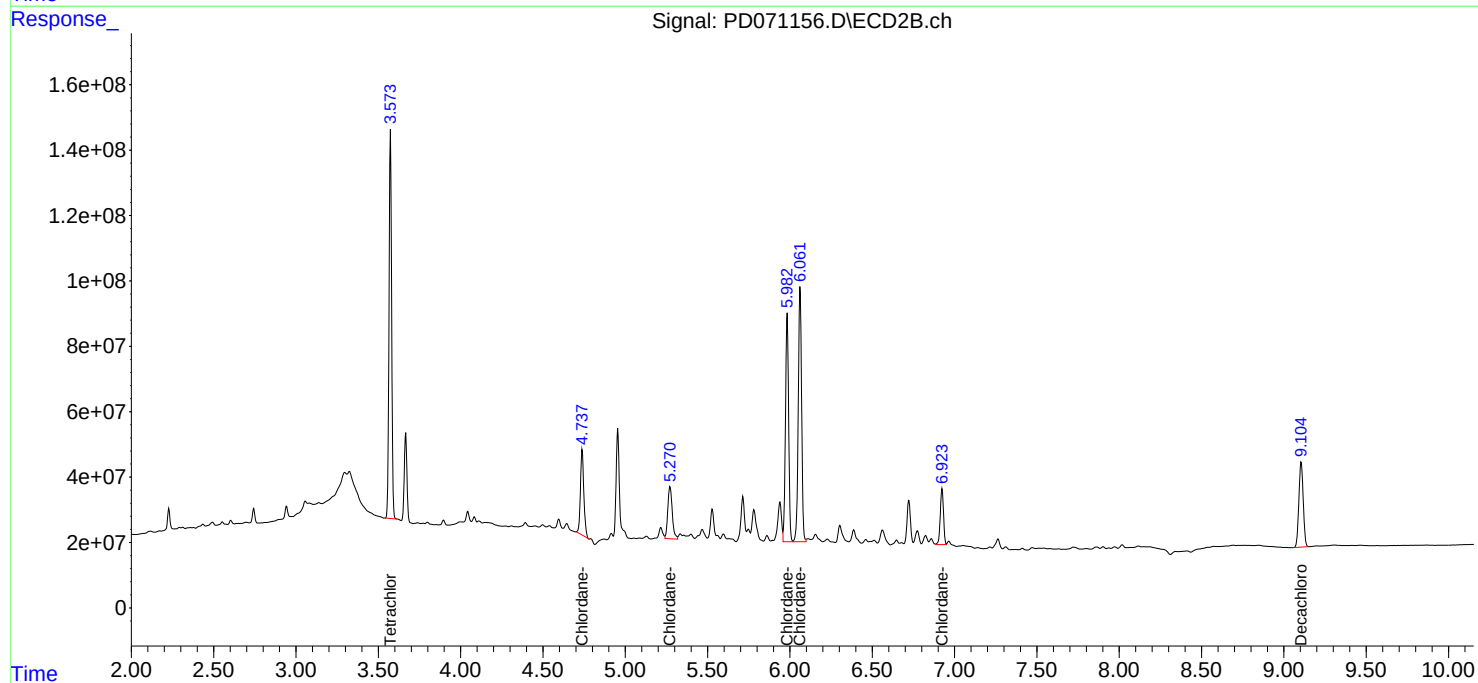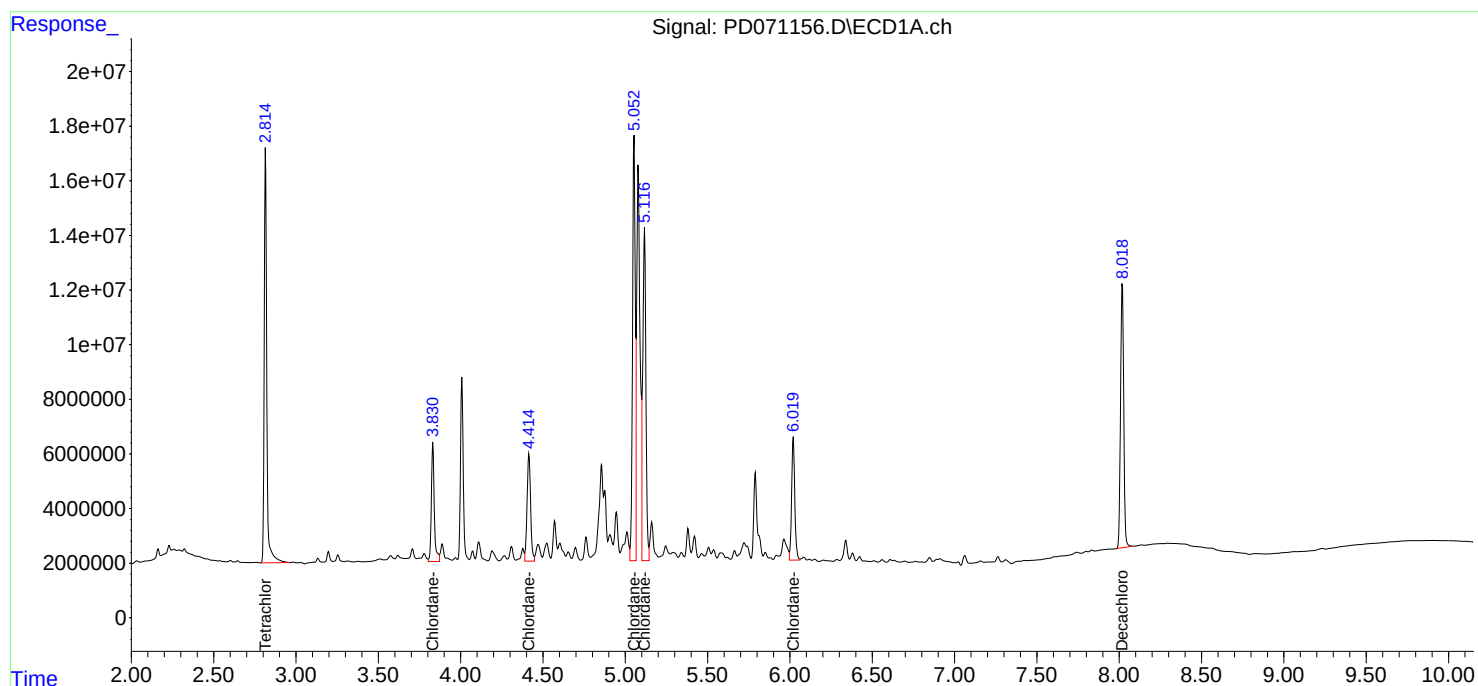


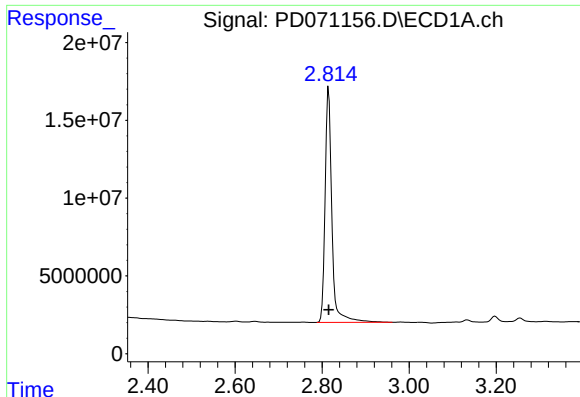

#1 Tetrachloro-m-xylene


R.T.: 2.815 min
Delta R.T.: 0.000 min
Response: 163098769
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

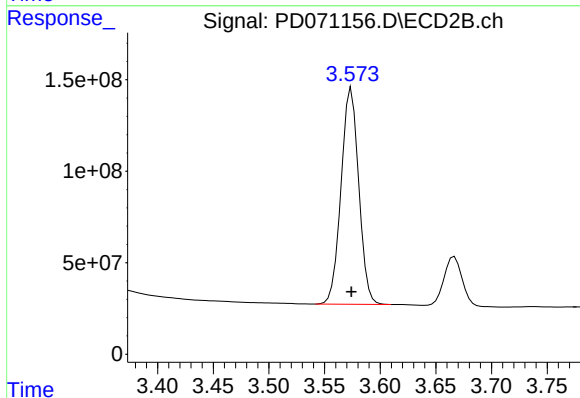


#1 Tetrachloro-m-xylene

R.T.: 3.574 min
Delta R.T.: 0.000 min
Response: 1304167010
Conc: 50.00 ng/ml

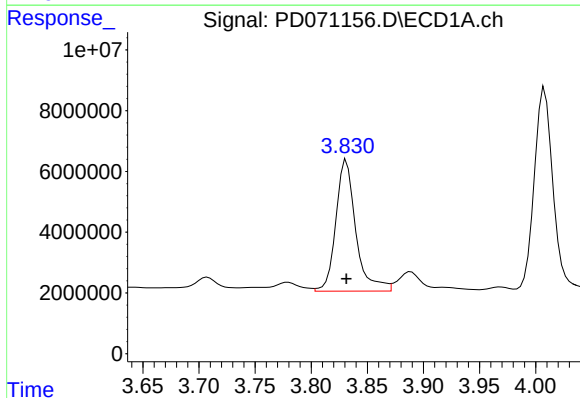


#23 Chlordane-1

R.T.: 3.831 min
Delta R.T.: 0.000 min
Response: 53742951
Conc: 500.00 ng/ml

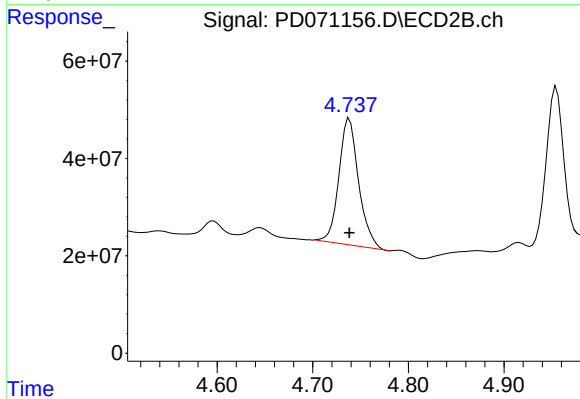

#23 Chlordane-1


R.T.: 4.738 min
Delta R.T.: 0.000 min
Response: 373024080
Conc: 500.00 ng/ml

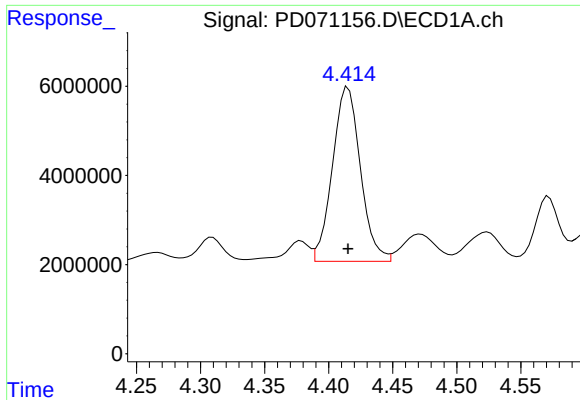

#24 Chlordane-2


R.T.: 4.415 min
Delta R.T.: 0.000 min
Response: 59333161
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

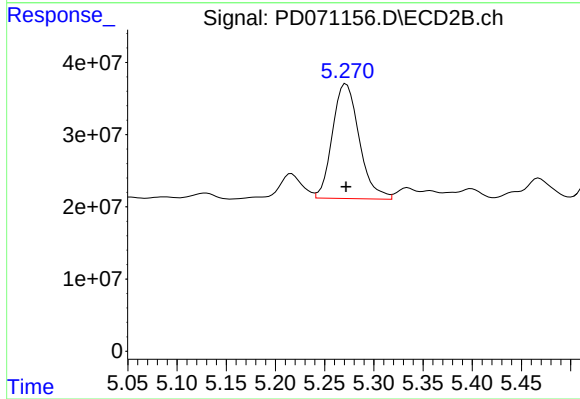


#24 Chlordane-2

R.T.: 5.272 min
Delta R.T.: 0.000 min
Response: 301096646
Conc: 500.00 ng/ml

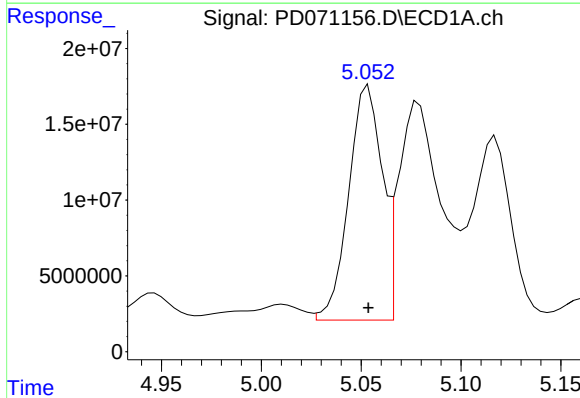


#25 Chlordane-3

R.T.: 5.054 min
Delta R.T.: 0.000 min
Response: 179732906
Conc: 500.00 ng/ml

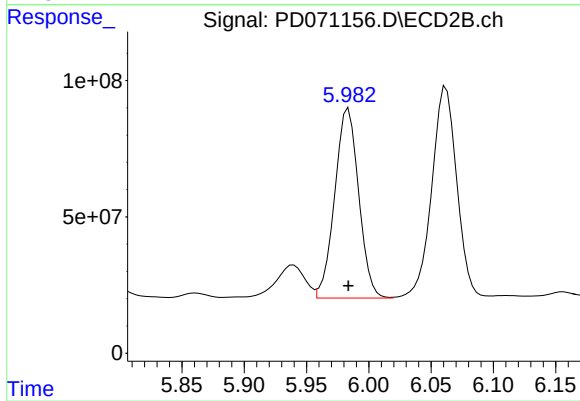

#25 Chlordane-3


R.T.: 5.984 min
Delta R.T.: 0.000 min
Response: 933545093
Conc: 500.00 ng/ml

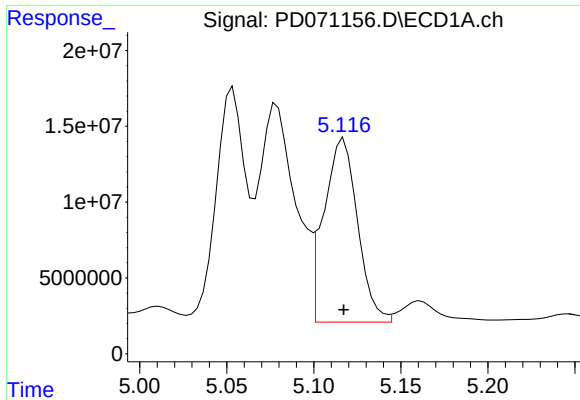

#26 Chlordane-4


R.T.: 5.117 min
Delta R.T.: 0.000 min
Response: 163347625
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

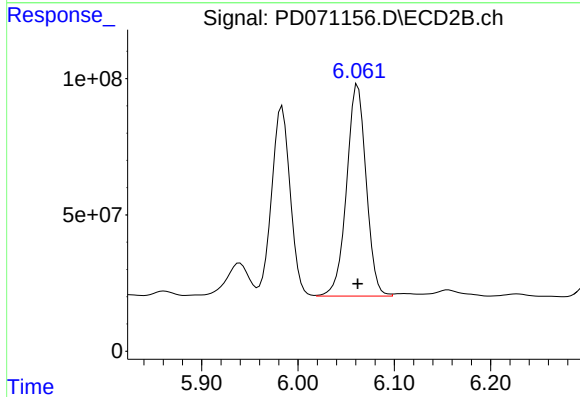


#26 Chlordane-4

R.T.: 6.062 min
Delta R.T.: 0.000 min
Response: 1090938555
Conc: 500.00 ng/ml

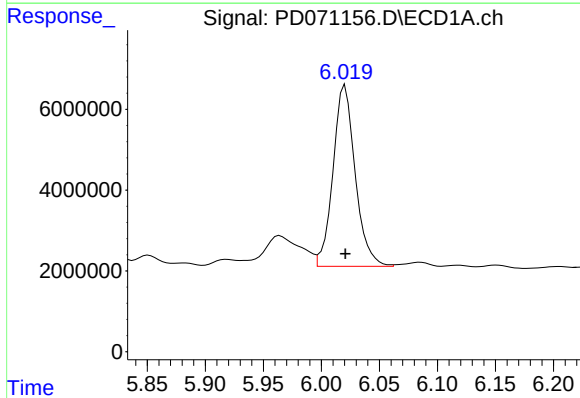


#27 Chlordane-5

R.T.: 6.021 min
Delta R.T.: 0.000 min
Response: 59701921
Conc: 500.00 ng/ml

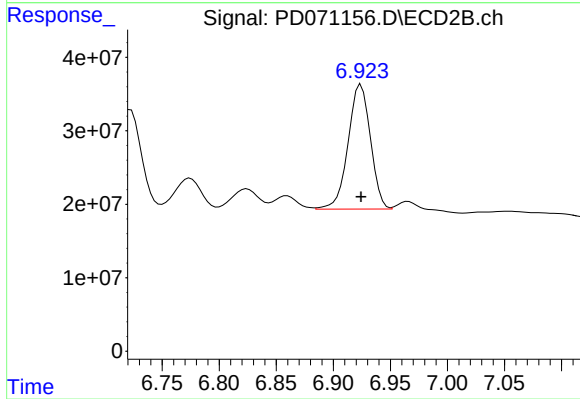

#27 Chlordane-5


R.T.: 6.924 min
Delta R.T.: 0.000 min
Response: 231118309
Conc: 500.00 ng/ml

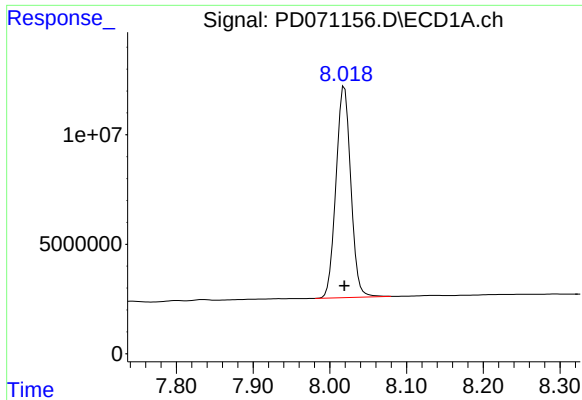

#28 Decachlorobiphenyl

R.T.: 8.019 min
Delta R.T.: 0.000 min
Response: 129606772
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

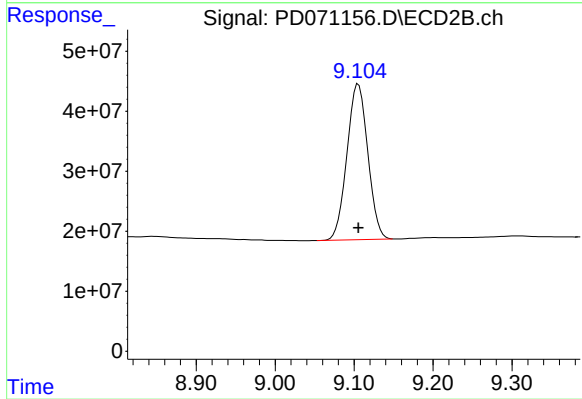

#28 Decachlorobiphenyl

R.T.: 9.105 min
Delta R.T.: 0.000 min
Response: 477647284
Conc: 50.00 ng/ml