

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072622\
 Data File : PD071165.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jul 2022 23:15
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD072622CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 02:31:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 26 02:29:58 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.815	3.574	161.1E6	1305.1E6	52.243	50.480
28)	SA Decachlor...	8.018	9.105	130.2E6	469.9E6	51.700	50.794
Target Compounds							
23)	Chlordane-1	3.831	4.738	51305285	378.8E6	477.844	500.604
24)	Chlordane-2	4.415	5.272	58557501	301.5E6	499.598	503.399
25)	Chlordane-3	5.053	5.984	175.1E6	936.6E6	512.758	505.195
26)	Chlordane-4	5.117	6.062	162.3E6	1093.7E6	511.572	501.780
27)	Chlordane-5	6.021	6.924	60368280	231.9E6	499.292	512.741


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072622\
Data File : PD071165.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jul 2022 23:15
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD072622CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 02:31:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072622.M
Quant Title : GC Extractables
QLast Update : Tue Jul 26 02:29:58 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

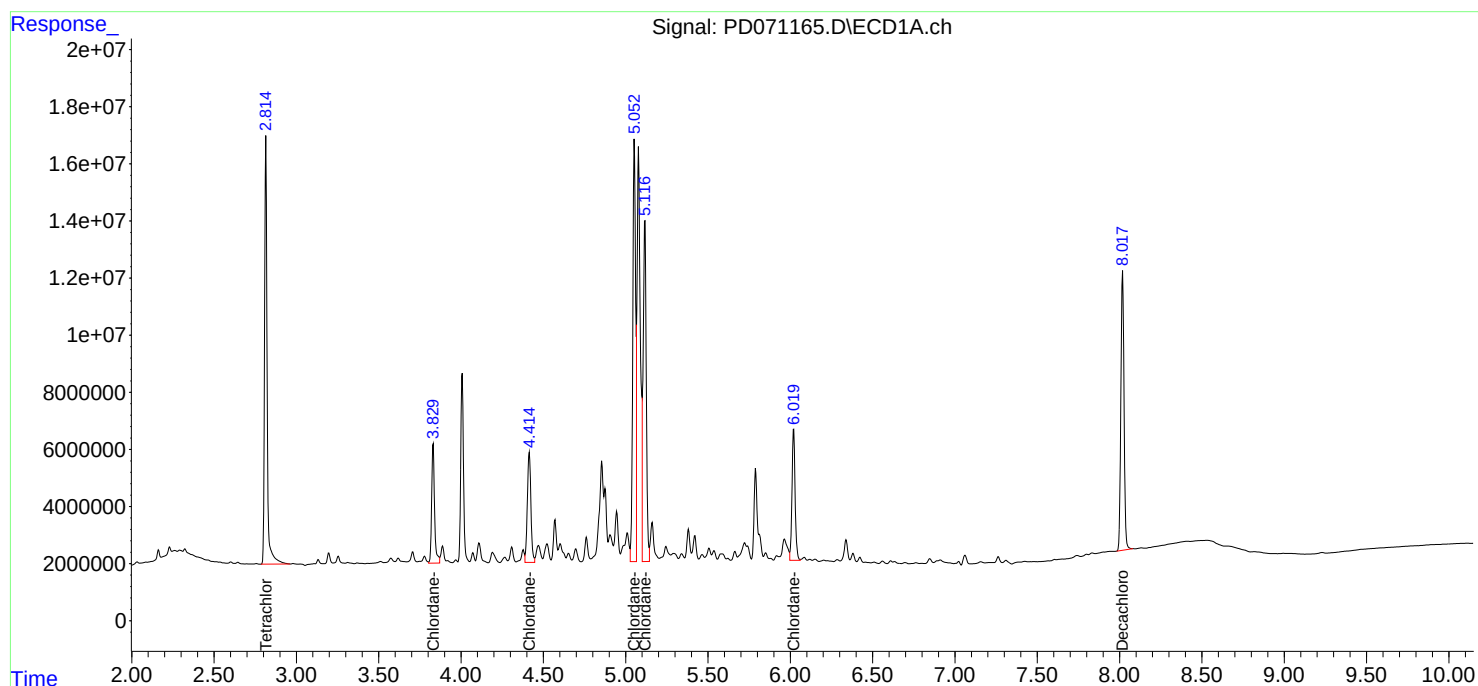


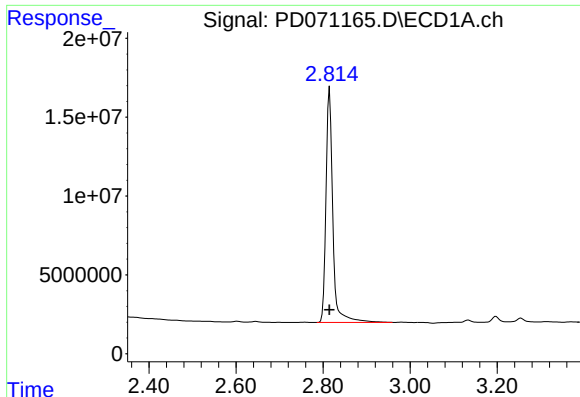

#1 Tetrachloro-m-xylene


R.T.: 2.815 min
Delta R.T.: 0.000 min
Response: 161098649
Conc: 52.24 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD072622CHLOR

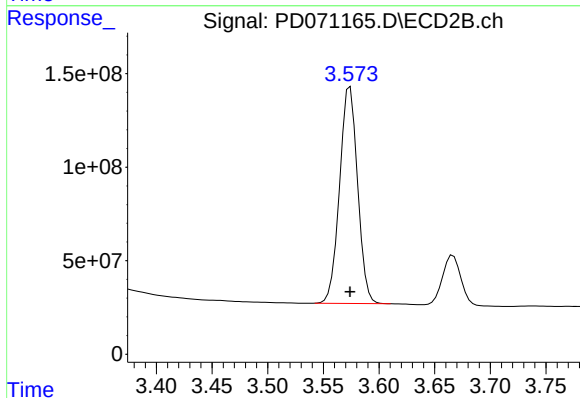


#1 Tetrachloro-m-xylene

R.T.: 3.574 min
Delta R.T.: 0.000 min
Response: 1305134068
Conc: 50.48 ng/ml

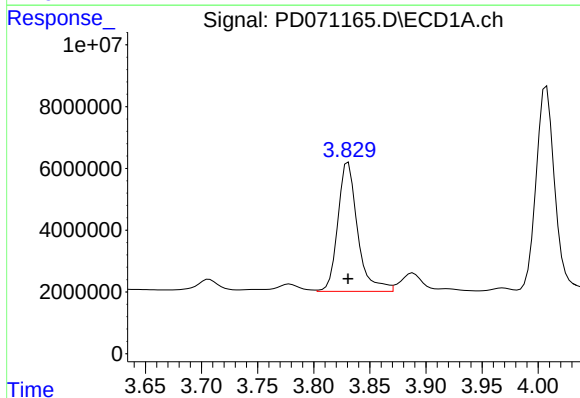


#23 Chlordane-1

R.T.: 3.831 min
Delta R.T.: 0.000 min
Response: 51305285
Conc: 477.84 ng/ml

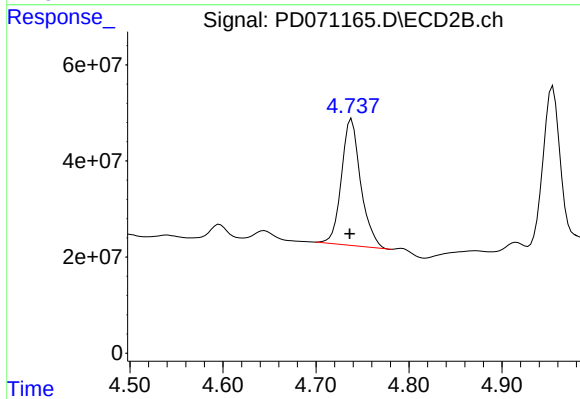

#23 Chlordane-1


R.T.: 4.738 min
Delta R.T.: 0.002 min
Response: 378820516
Conc: 500.60 ng/ml

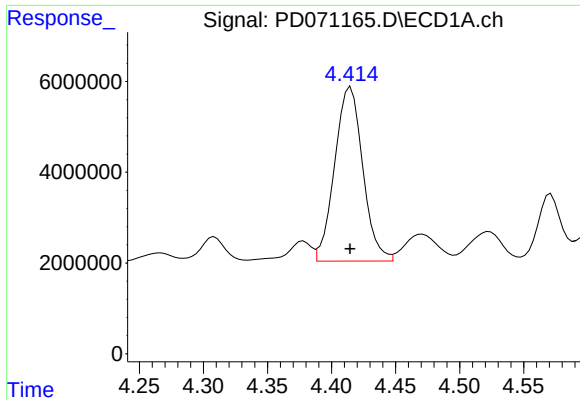

#24 Chlordane-2


R.T.: 4.415 min
Delta R.T.: 0.000 min
Response: 58557501
Conc: 499.60 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD072622CHLOR

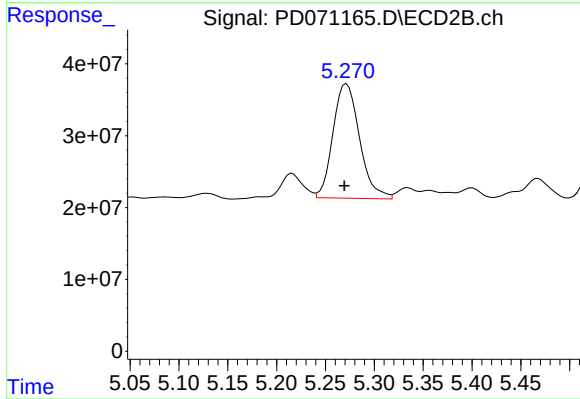


#24 Chlordane-2

R.T.: 5.272 min
Delta R.T.: 0.002 min
Response: 301539668
Conc: 503.40 ng/ml

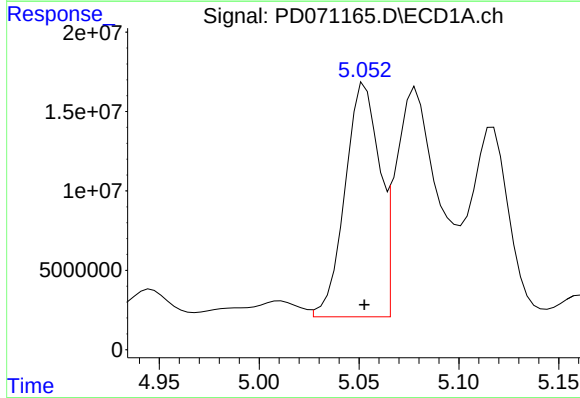


#25 Chlordane-3

R.T.: 5.053 min
Delta R.T.: 0.000 min
Response: 175084805
Conc: 512.76 ng/ml

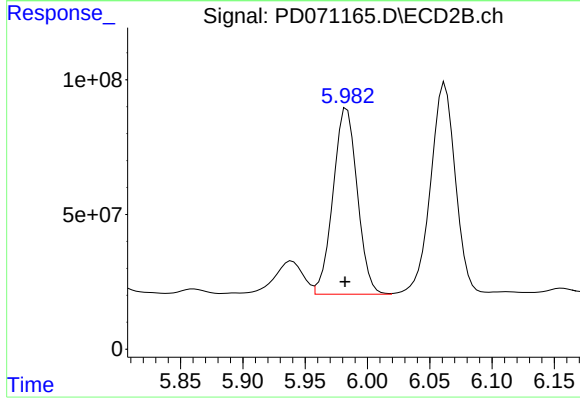

#25 Chlordane-3


R.T.: 5.984 min
Delta R.T.: 0.001 min
Response: 936593298
Conc: 505.20 ng/ml

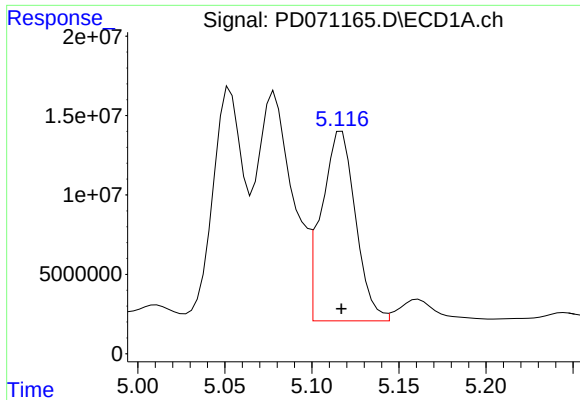

#26 Chlordane-4


R.T.: 5.117 min
Delta R.T.: 0.000 min
Response: 162298793
Conc: 511.57 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD072622CHLOR

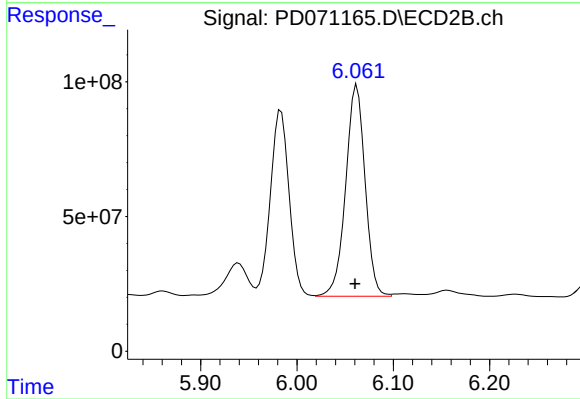


#26 Chlordane-4

R.T.: 6.062 min
Delta R.T.: 0.002 min
Response: 1093690348
Conc: 501.78 ng/ml

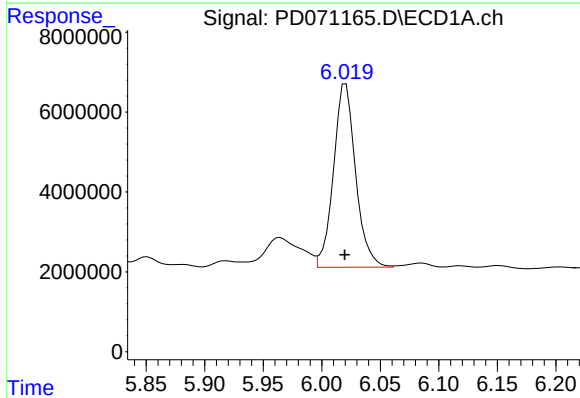


#27 Chlordane-5

R.T.: 6.021 min
Delta R.T.: 0.001 min
Response: 60368280
Conc: 499.29 ng/ml

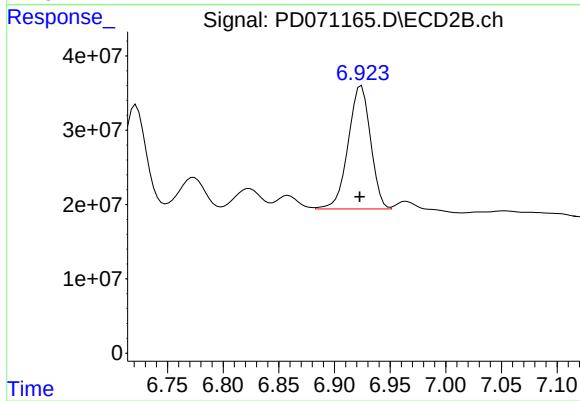

#27 Chlordane-5


R.T.: 6.924 min
Delta R.T.: 0.002 min
Response: 231911227
Conc: 512.74 ng/ml

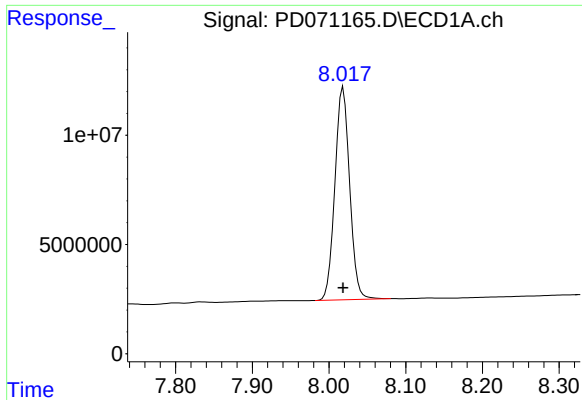

#28 Decachlorobiphenyl

R.T.: 8.018 min
Delta R.T.: 0.000 min
Response: 130177037
Conc: 51.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD072622CHLOR

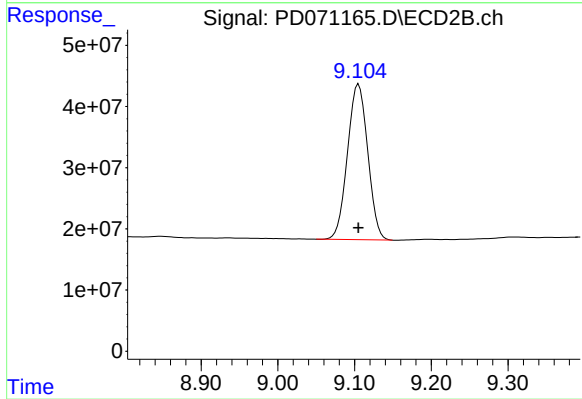

#28 Decachlorobiphenyl

R.T.: 9.105 min
Delta R.T.: 0.000 min
Response: 469904141
Conc: 50.79 ng/ml