

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072720\
 Data File : PD058719.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2020 16:29
 Operator : AJ\MA
 Sample : L3443-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 28 00:59:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070220CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 02 16:12:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.208	3.866	33684048	48644221	20.040	21.347
27)	SA Decachlor...	7.846	8.861	50910724	59918411	28.797	28.202
Target Compounds							
2)	A alpha-BHC	3.620	4.285f	919817	4067536	0.370	1.202 #
4)	MA Heptachlor	0.000	5.018	0	2508861	N.D.	0.863
6)	B beta-BHC	4.119f	0.000	1331464	0	1.405	N.D. #
7)	B delta-BHC	4.330	0.000	1597159	0	0.694	N.D. #
8)	B Heptachlo...	4.813f	5.689	552207	4082118	0.313	1.578 #
19)	B Endosulfa...	6.258f	0.000	654855	0	0.431	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072720\
Data File : PD058719.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2020 16:29
Operator : AJ\MA
Sample : L3443-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 00:59:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070220CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 02 16:12:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

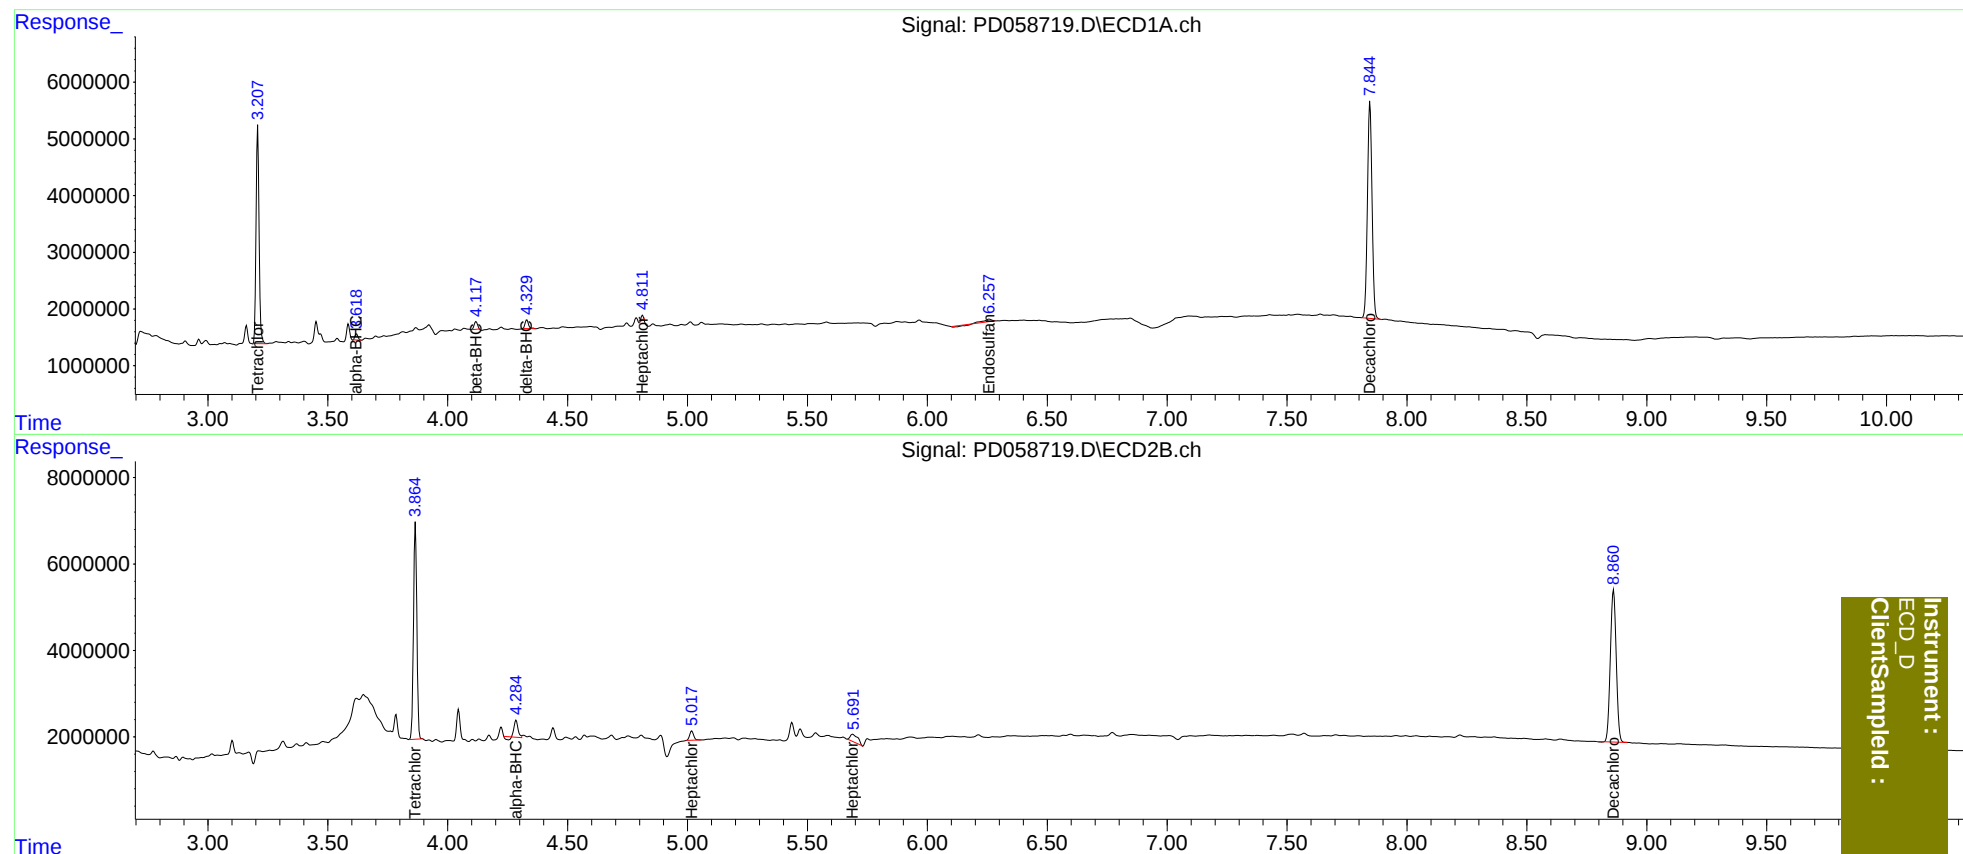


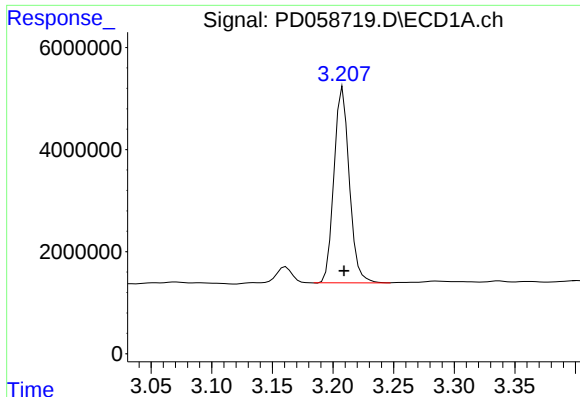

#1 Tetrachloro-m-xylene


R.T.: 3.208 min
Delta R.T.: 0.000 min
Response: 33684048
Conc: 20.04 ng/ml

Instrument :
ECD_D
ClientSampleId :

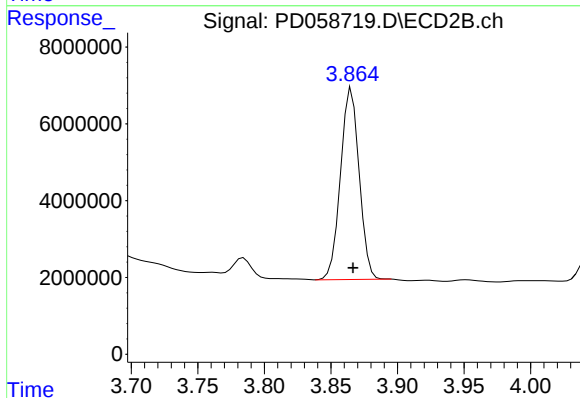


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: -0.001 min
Response: 48644221
Conc: 21.35 ng/ml

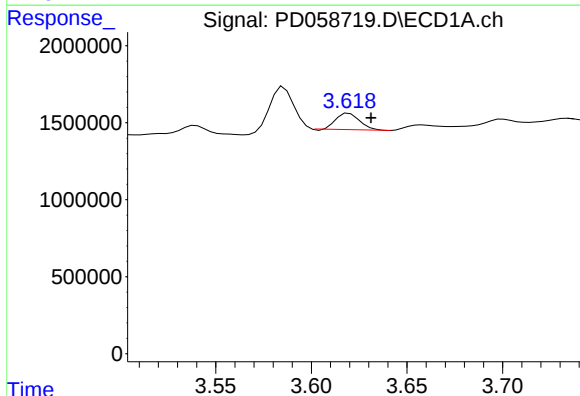


#2 alpha-BHC

R.T.: 3.620 min
Delta R.T.: -0.011 min
Response: 919817
Conc: 0.37 ng/ml

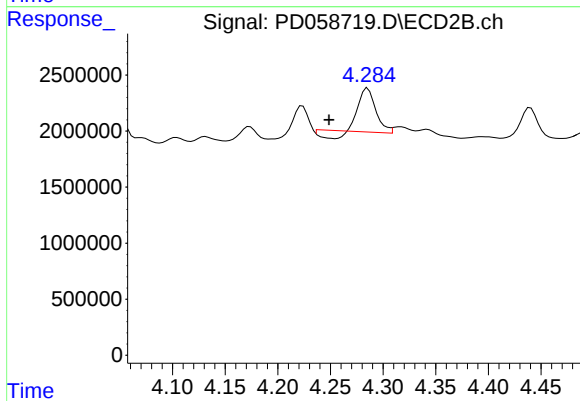

#2 alpha-BHC


R.T.: 4.285 min
Delta R.T.: 0.037 min
Response: 4067536
Conc: 1.20 ng/ml

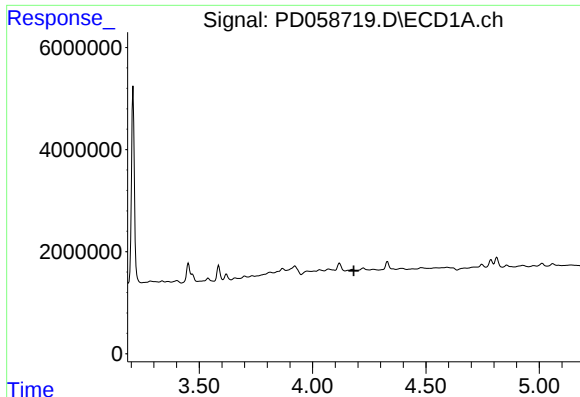

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.182 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

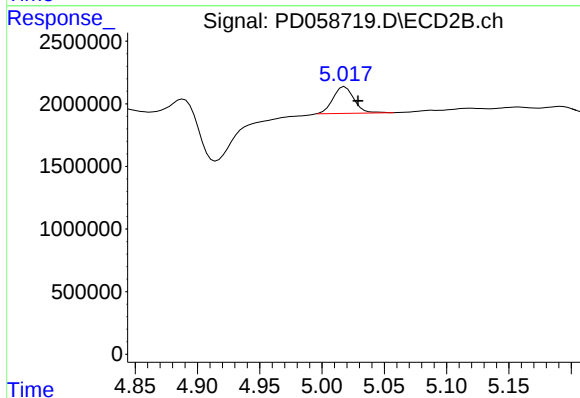


#4 Heptachlor

R.T.: 5.018 min
Delta R.T.: -0.011 min
Response: 2508861
Conc: 0.86 ng/ml

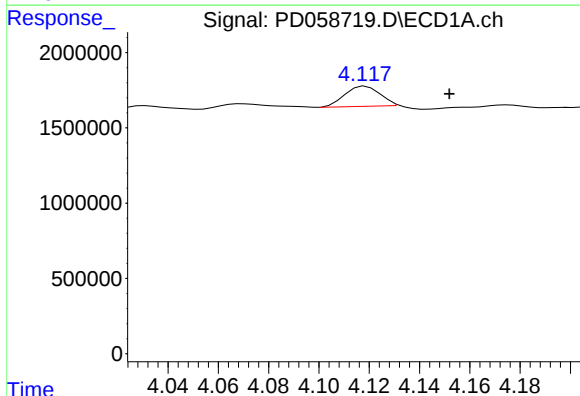


#6 beta-BHC

R.T.: 4.119 min
Delta R.T.: -0.033 min
Response: 1331464
Conc: 1.40 ng/ml

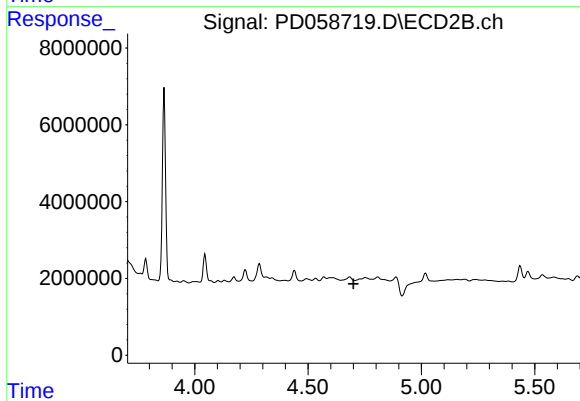

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.701 min
Response: 0
Conc: N.D.

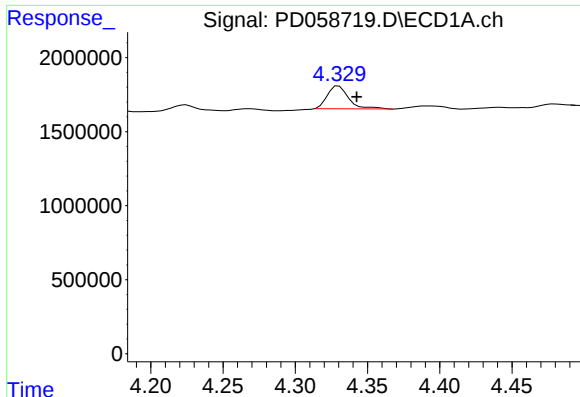

#7 delta-BHC


R.T.: 4.330 min
Delta R.T.: -0.012 min
Response: 1597159
Conc: 0.69 ng/ml

Instrument :
ECD_D
ClientSampleId :

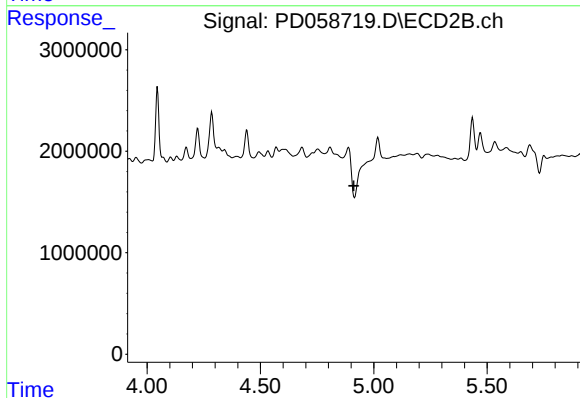


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.912 min
Response: 0
Conc: N.D.

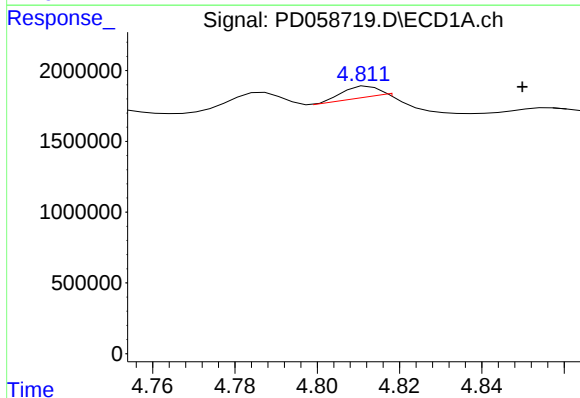


#8 Heptachlor epoxide

R.T.: 4.813 min
Delta R.T.: -0.037 min
Response: 552207
Conc: 0.31 ng/ml

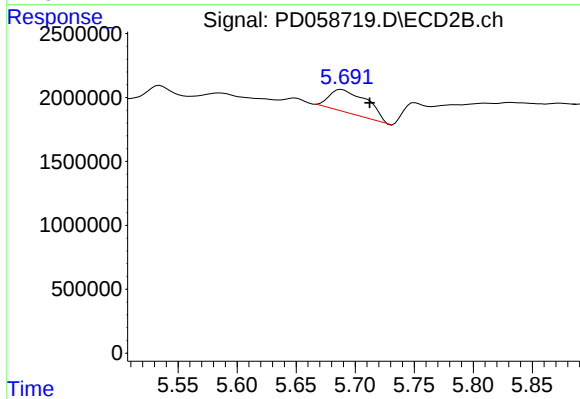

#8 Heptachlor epoxide


R.T.: 5.689 min
Delta R.T.: -0.024 min
Response: 4082118
Conc: 1.58 ng/ml

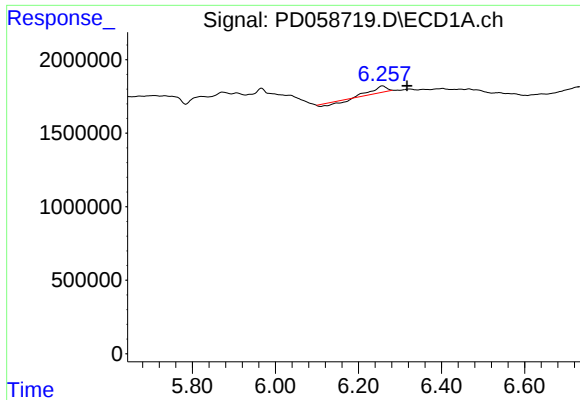

#19 Endosulfan Sulfate


R.T.: 6.258 min
Delta R.T.: -0.059 min
Response: 654855
Conc: 0.43 ng/ml

Instrument :
ECD_D
ClientSampleId :

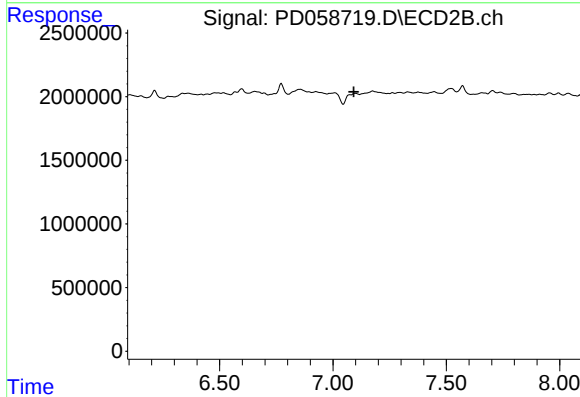


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.092 min
Response: 0
Conc: N.D.

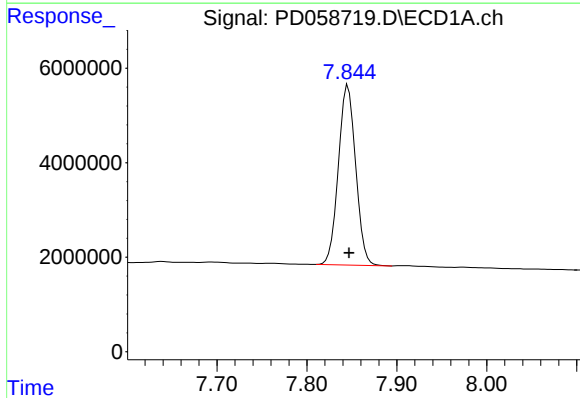

#27 Decachlorobiphenyl

R.T.: 7.846 min
Delta R.T.: 0.000 min
Response: 50910724
Conc: 28.80 ng/ml

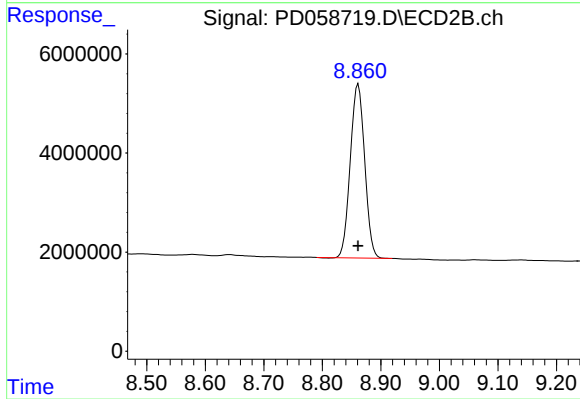

#27 Decachlorobiphenyl

R.T.: 8.861 min
Delta R.T.: 0.000 min
Response: 59918411
Conc: 28.20 ng/ml