

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072720\
 Data File : PD058720.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2020 16:43
 Operator : AJ\MA
 Sample : L3443-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 28 00:59:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070220CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 02 16:12:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.866	33326471	48453618	19.828	21.264
27)	SA Decachlor...	7.847	8.862	47863835	57339486	27.074	26.988
Target Compounds							
2)	A alpha-BHC	3.620	4.224	865544	573825	0.348	0.170 #
3)	MA gamma-BHC...	0.000	4.493f	0	439542	N.D.	0.142
4)	MA Heptachlor	0.000	5.019	0	2841179	N.D.	0.977
6)	B beta-BHC	4.119f	0.000	1405087	0	1.483	N.D. #
7)	B delta-BHC	4.331	4.889	1402036	10380132	0.609	4.686 #
8)	B Heptachlo...	4.813f	5.688	4886484	9301461	2.771	3.596 #
10)	B trans-Chl...	5.060	0.000	2700108	0	1.371	N.D. #
11)	B cis-Chlor...	5.060f	0.000	2700108	0	1.363	N.D. #
18)	B Endrin al...	0.000	6.846	0	3025328	N.D.	1.588
24)	Toxaphene-3	0.000	6.846	0	3025328	N.D.	146.391


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072720\
Data File : PD058720.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2020 16:43
Operator : AJ\MA
Sample : L3443-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 00:59:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070220CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 02 16:12:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

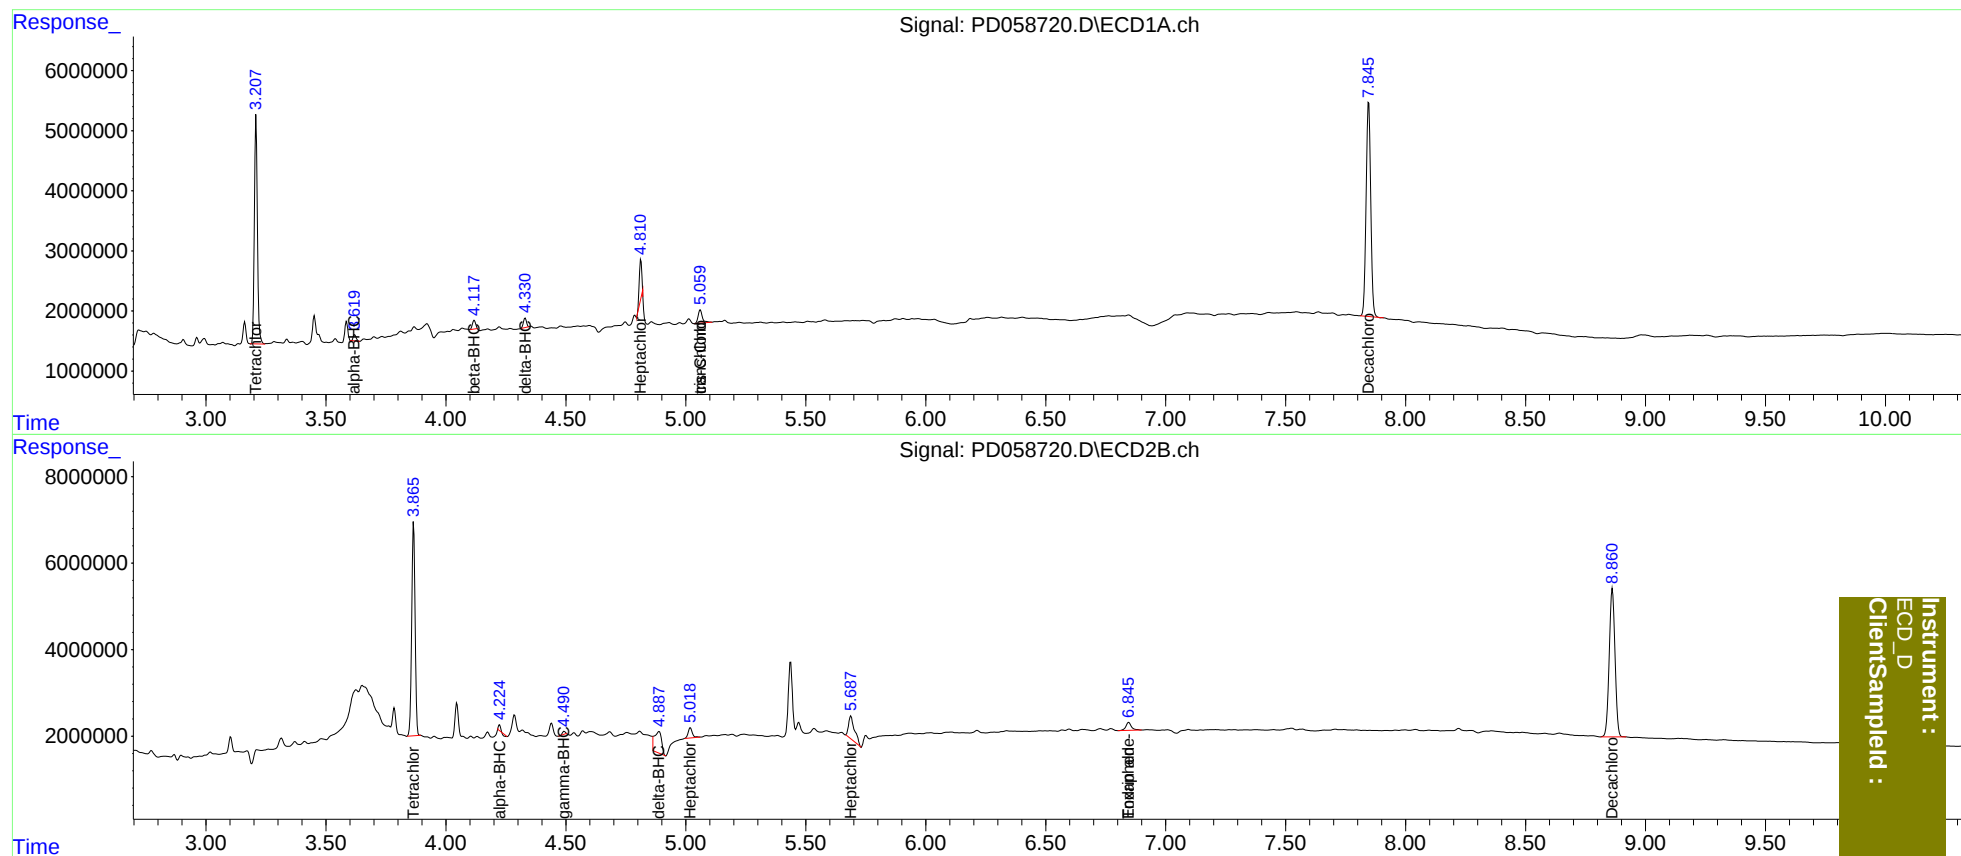


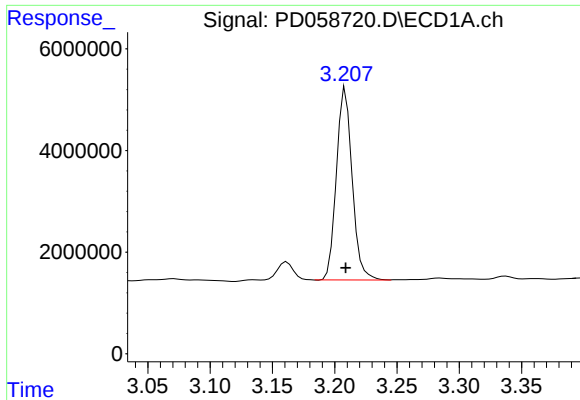

#1 Tetrachloro-m-xylene


R.T.: 3.209 min
Delta R.T.: 0.000 min
Response: 33326471
Conc: 19.83 ng/ml

Instrument :
ECD_D
ClientSampleId :

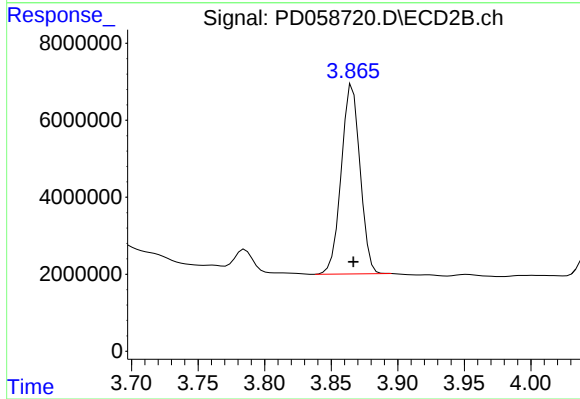


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.000 min
Response: 48453618
Conc: 21.26 ng/ml

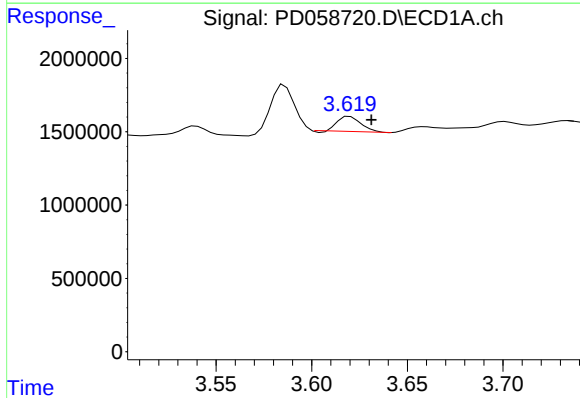


#2 alpha-BHC

R.T.: 3.620 min
Delta R.T.: -0.011 min
Response: 865544
Conc: 0.35 ng/ml

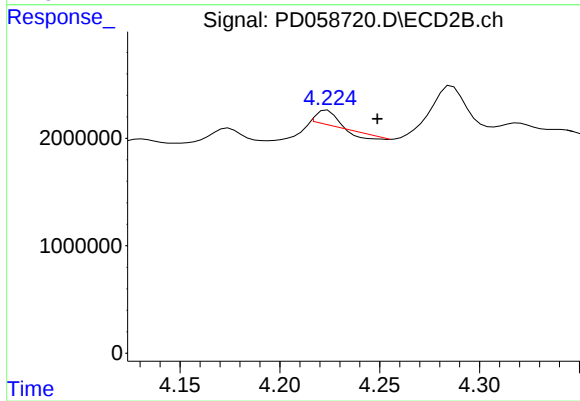

#2 alpha-BHC


R.T.: 4.224 min
Delta R.T.: -0.025 min
Response: 573825
Conc: 0.17 ng/ml

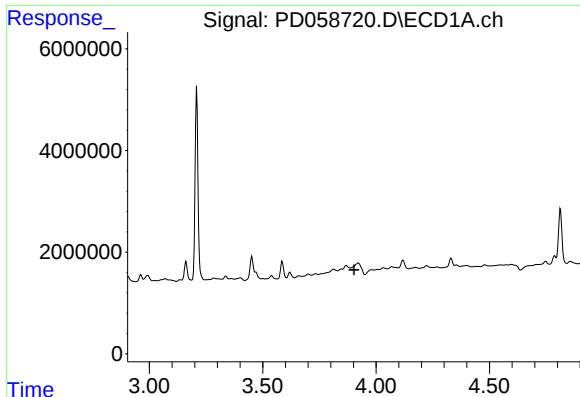

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 3.903 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

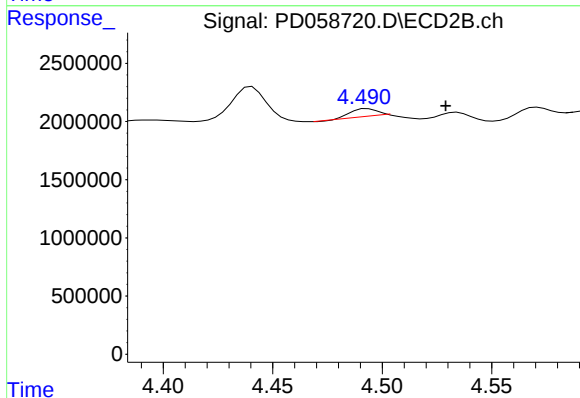


#3 gamma-BHC (Lindane)

R.T.: 4.493 min
Delta R.T.: -0.036 min
Response: 439542
Conc: 0.14 ng/ml

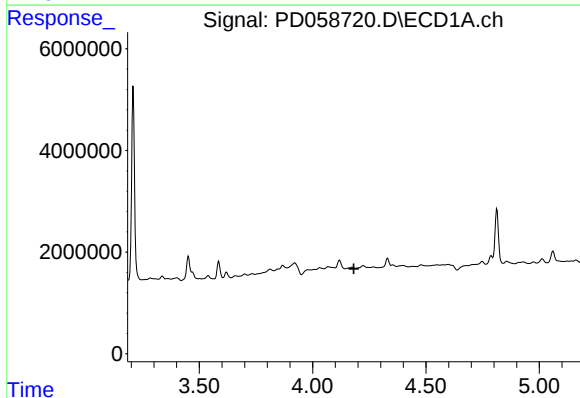


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.182 min
Response: 0
Conc: N.D.

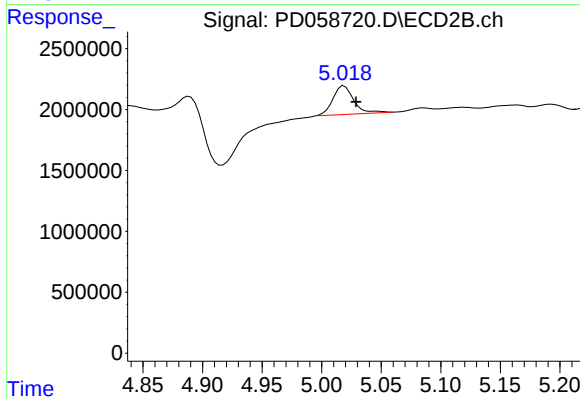

#4 Heptachlor


R.T.: 5.019 min
Delta R.T.: -0.010 min
Response: 2841179
Conc: 0.98 ng/ml

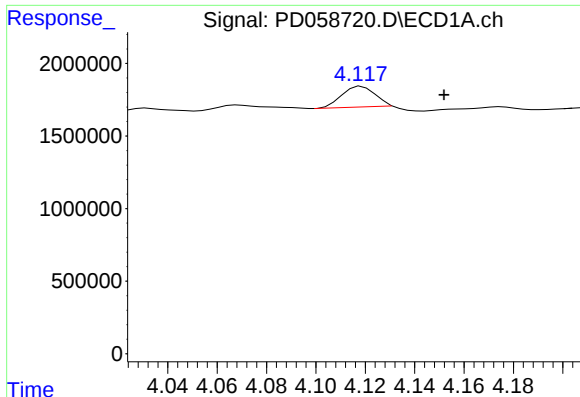

#6 beta-BHC


R.T.: 4.119 min
Delta R.T.: -0.033 min
Response: 1405087
Conc: 1.48 ng/ml

Instrument :
ECD_D
ClientSampleId :

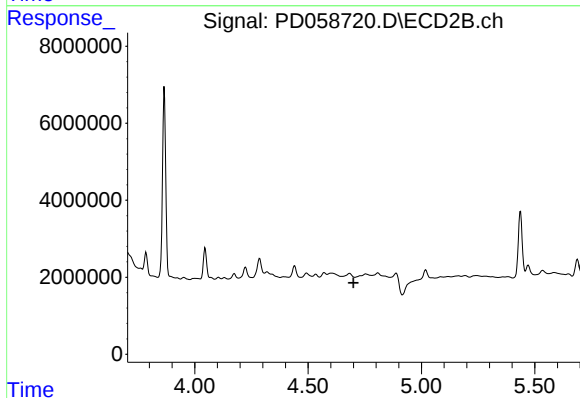


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.701 min
Response: 0
Conc: N.D.

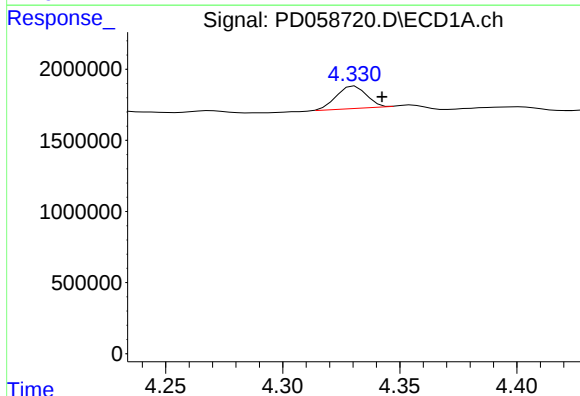


#7 delta-BHC

R.T.: 4.331 min
Delta R.T.: -0.012 min
Response: 1402036
Conc: 0.61 ng/ml

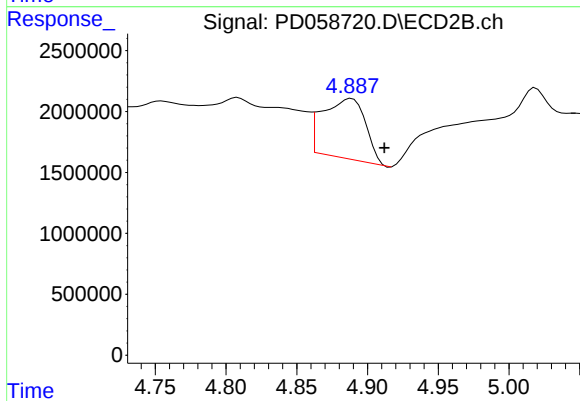

#7 delta-BHC


R.T.: 4.889 min
Delta R.T.: -0.023 min
Response: 10380132
Conc: 4.69 ng/ml

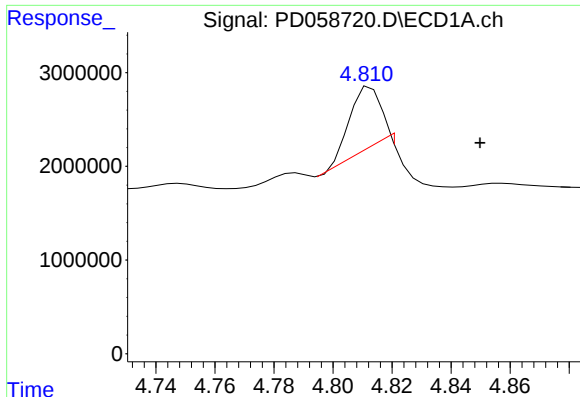

#8 Heptachlor epoxide


R.T.: 4.813 min
Delta R.T.: -0.037 min
Response: 4886484
Conc: 2.77 ng/ml

Instrument :
ECD_D
ClientSampleId :

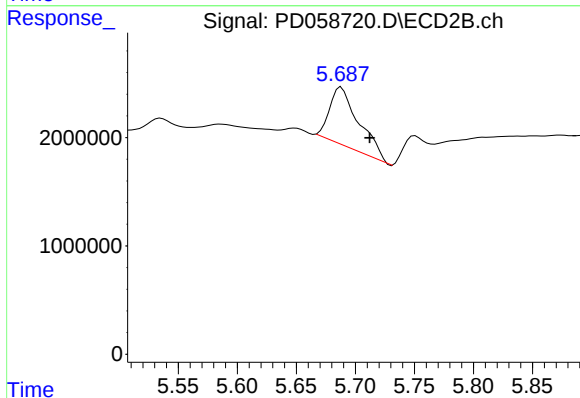


#8 Heptachlor epoxide

R.T.: 5.688 min
Delta R.T.: -0.024 min
Response: 9301461
Conc: 3.60 ng/ml

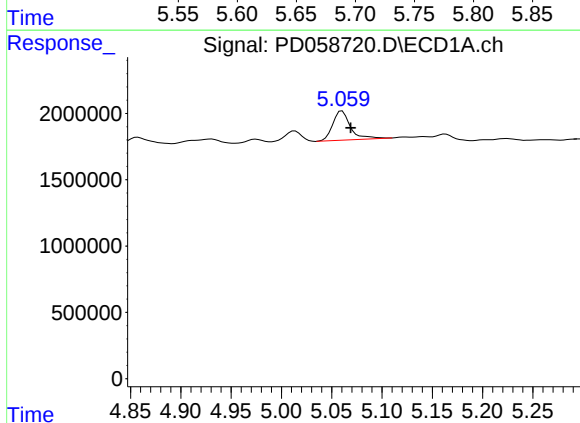


#10 trans-Chlordane

R.T.: 5.060 min
Delta R.T.: -0.009 min
Response: 2700108
Conc: 1.37 ng/ml

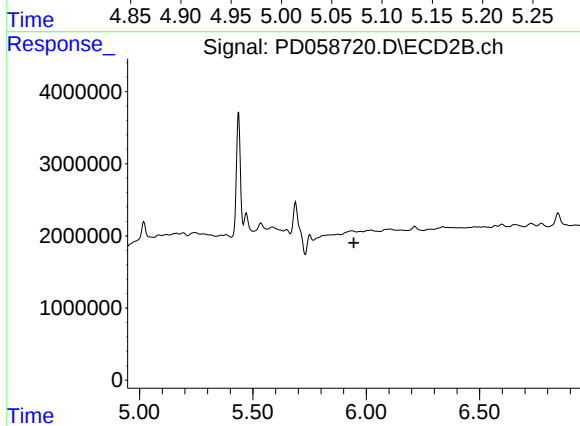

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.945 min
Response: 0
Conc: N.D.

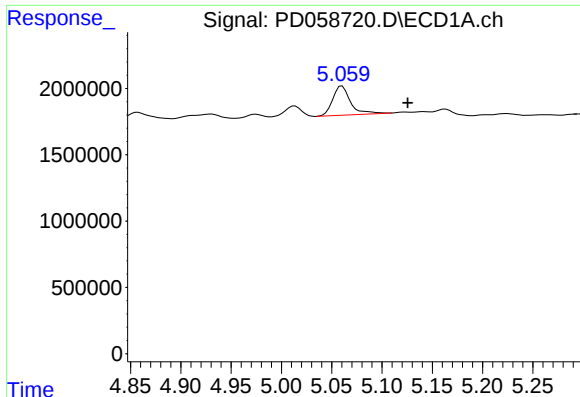

#11 cis-Chlordane


R.T.: 5.060 min
Delta R.T.: -0.065 min
Response: 2700108
Conc: 1.36 ng/ml

Instrument :
ECD_D
ClientSampleId :

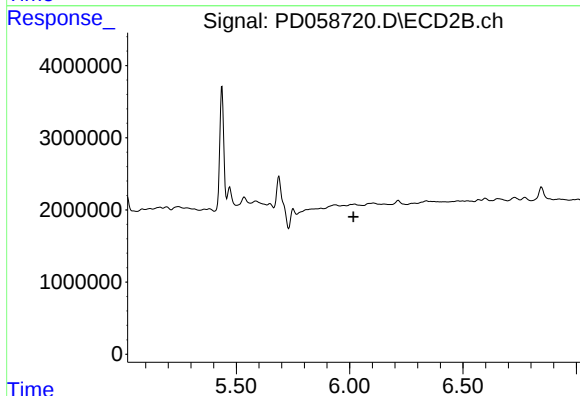


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.017 min
Response: 0
Conc: N.D.

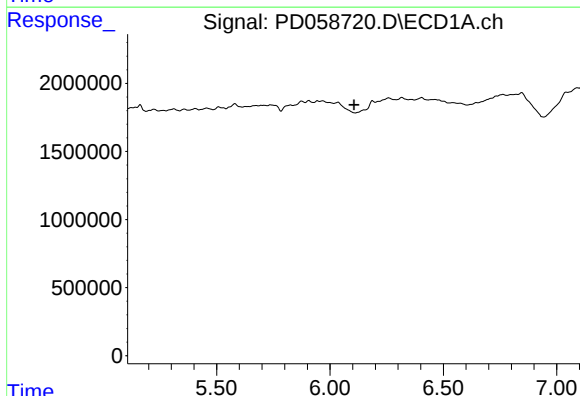


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.107 min
Response: 0
Conc: N.D.

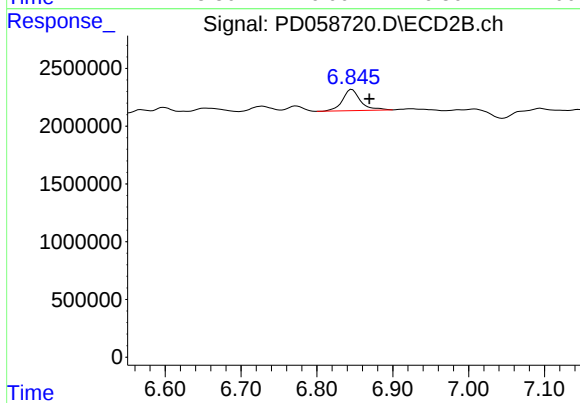

#18 Endrin aldehyde


R.T.: 6.846 min
Delta R.T.: -0.023 min
Response: 3025328
Conc: 1.59 ng/ml

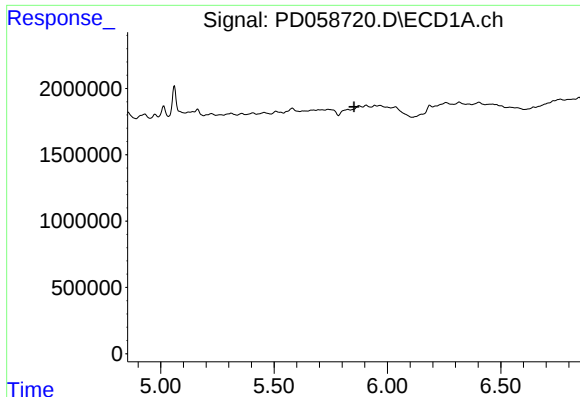

#24 Toxaphene-3


R.T.: 0.000 min
Exp R.T.: 5.854 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

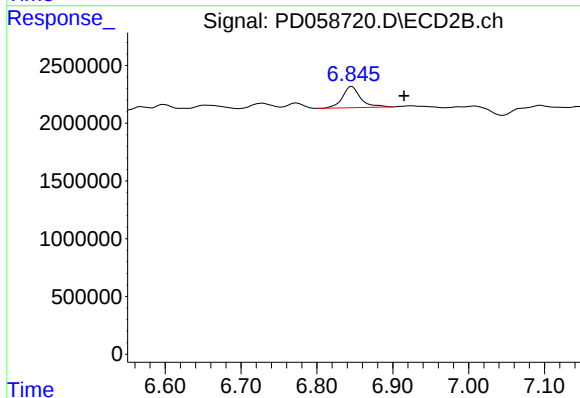


#24 Toxaphene-3

R.T.: 6.846 min
Delta R.T.: -0.069 min
Response: 3025328
Conc: 146.39 ng/ml

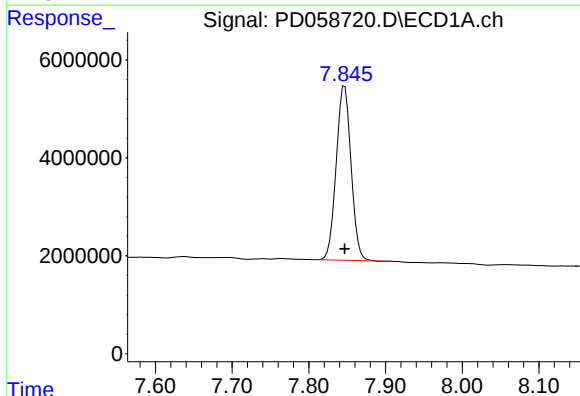

#27 Decachlorobiphenyl

R.T.: 7.847 min
Delta R.T.: 0.000 min
Response: 47863835
Conc: 27.07 ng/ml

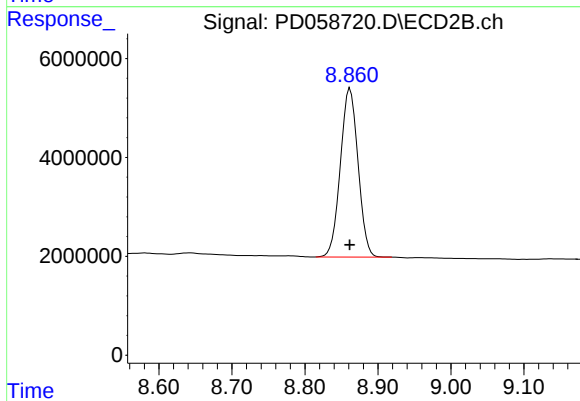

#27 Decachlorobiphenyl

R.T.: 8.862 min
Delta R.T.: 0.000 min
Response: 57339486
Conc: 26.99 ng/ml