

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072720\
 Data File : PD058725.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2020 17:53
 Operator : AJ\MA
 Sample : L3443-08
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 28 01:00:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070220CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 02 16:12:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.865	25784507	49991672	15.341	21.939 #
27)	SA Decachlor...	7.846	8.863	34556568	40729047	19.547	19.170
Target Compounds							
2)	A alpha-BHC	3.620	4.224	1155139	1058915	0.464	0.313 #
3)	MA gamma-BHC...	0.000	4.572f	0	669160	N.D.	0.216
4)	MA Heptachlor	0.000	5.019	0	2750737	N.D.	0.946
6)	B beta-BHC	4.119f	0.000	642089	0	0.677	N.D. #
7)	B delta-BHC	4.331	4.889	1653980	7650182	0.718	3.453 #
8)	B Heptachlo...	4.813f	5.689	9294424	15811453	5.270	6.113
9)	A Endosulfan I	5.162	0.000	2473734	0	1.376	N.D. #
10)	B trans-Chl...	5.060	5.876f	8455431	992665	4.292	0.383 #
11)	B cis-Chlor...	5.162f	0.000	2473734	0	1.249	N.D. #
18)	B Endrin al...	0.000	6.848	0	4519424	N.D.	2.372
24)	Toxaphene-3	0.000	6.848	0	4519424	N.D.	218.688


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072720\
Data File : PD058725.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2020 17:53
Operator : AJ\MA
Sample : L3443-08
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 01:00:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070220CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 02 16:12:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

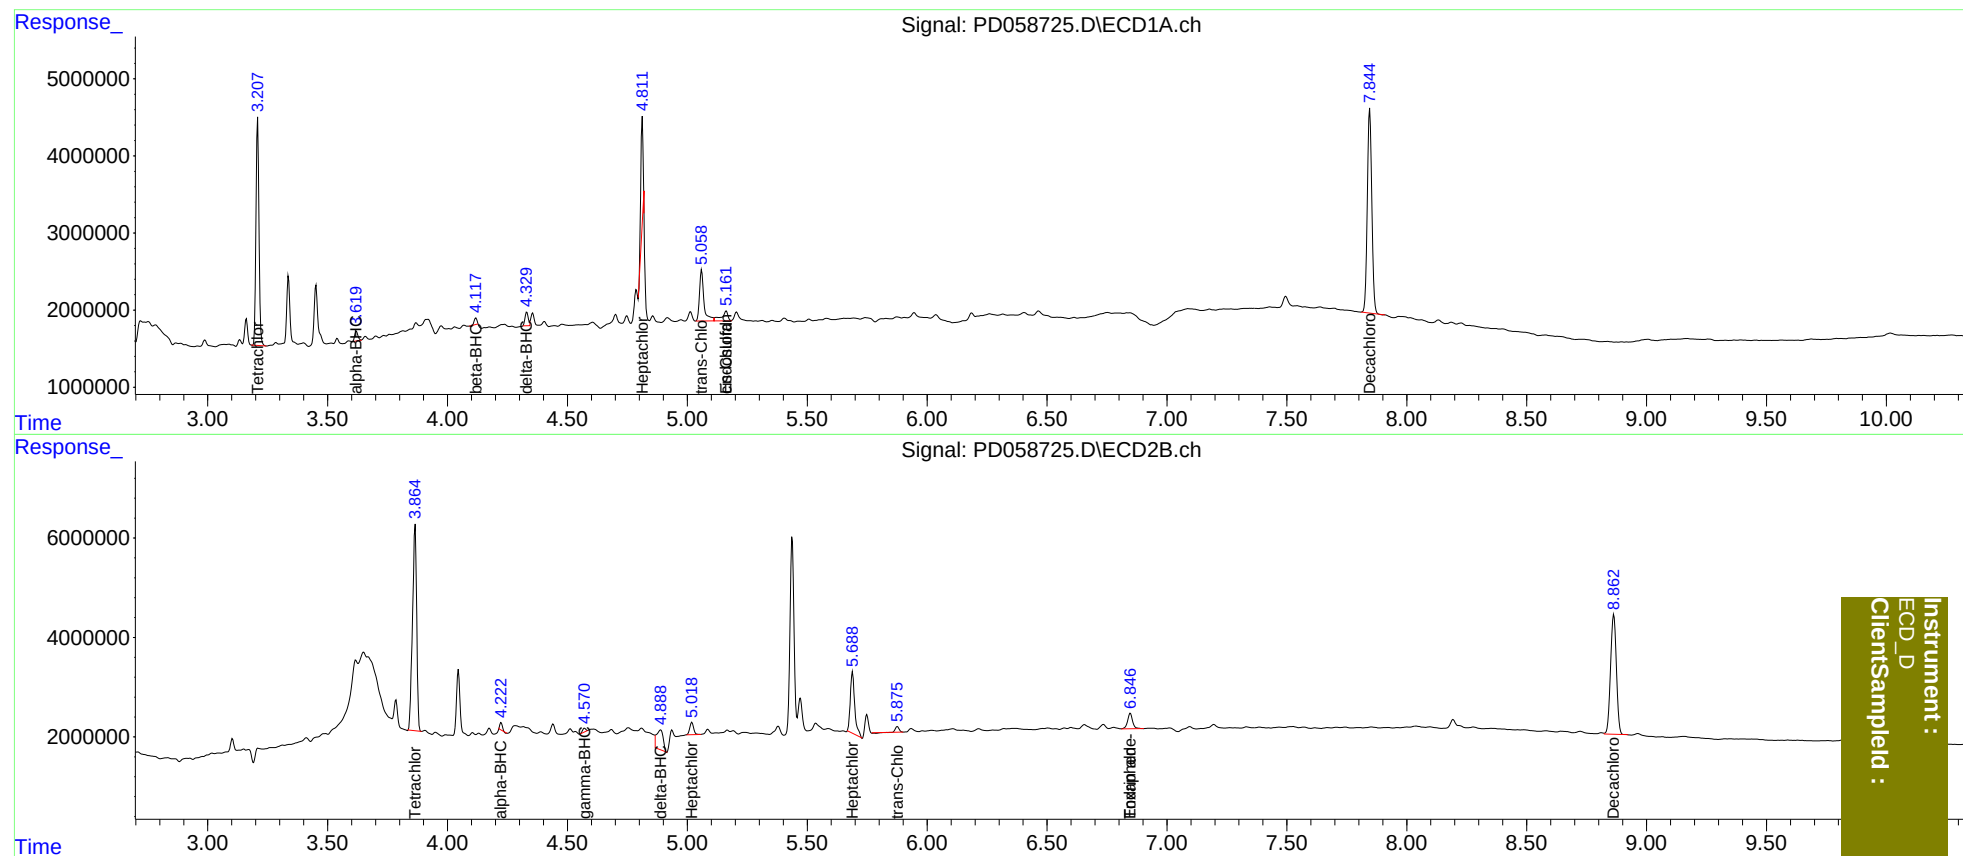


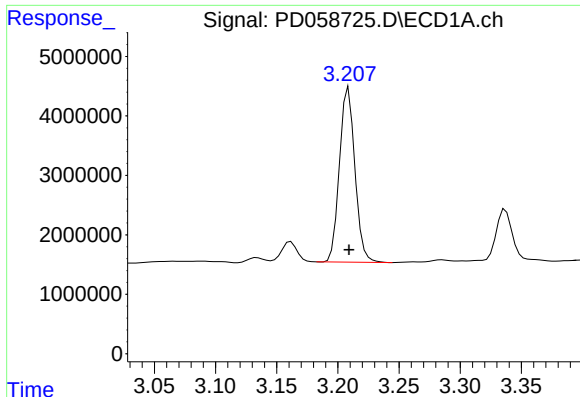

#1 Tetrachloro-m-xylene


R.T.: 3.209 min
Delta R.T.: 0.000 min
Response: 25784507
Conc: 15.34 ng/ml

Instrument :
ECD_D
ClientSampleId :

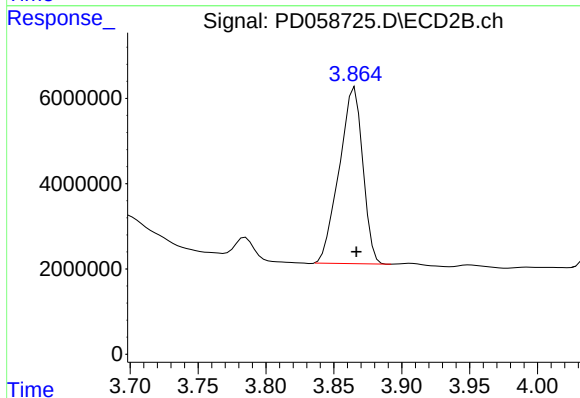


#1 Tetrachloro-m-xylene

R.T.: 3.865 min
Delta R.T.: -0.001 min
Response: 49991672
Conc: 21.94 ng/ml

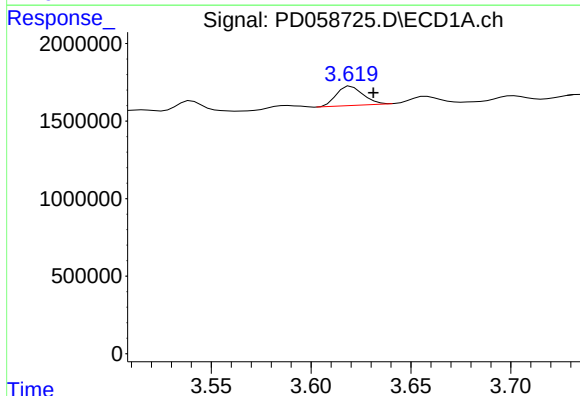


#2 alpha-BHC

R.T.: 3.620 min
Delta R.T.: -0.011 min
Response: 1155139
Conc: 0.46 ng/ml

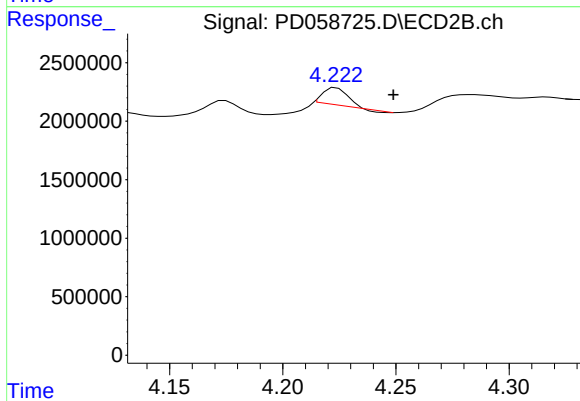

#2 alpha-BHC


R.T.: 4.224 min
Delta R.T.: -0.025 min
Response: 1058915
Conc: 0.31 ng/ml

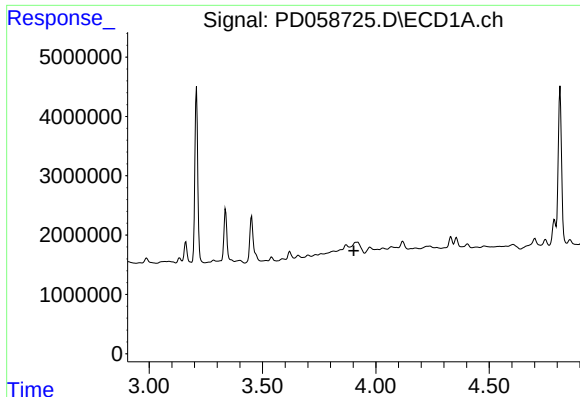

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 3.903 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

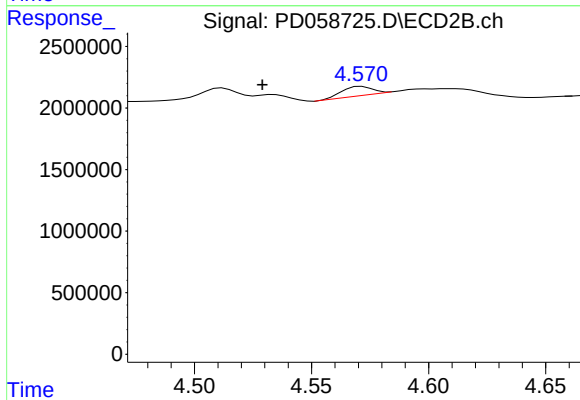


#3 gamma-BHC (Lindane)

R.T.: 4.572 min
Delta R.T.: 0.043 min
Response: 669160
Conc: 0.22 ng/ml

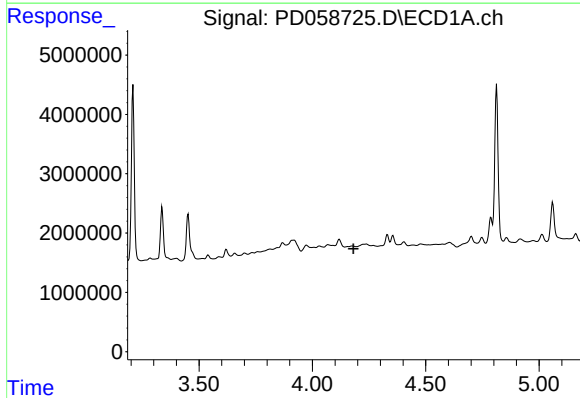


#4 Heptachlor

R.T.: 0.000 min
Exp R.T.: 4.182 min
Response: 0
Conc: N.D.

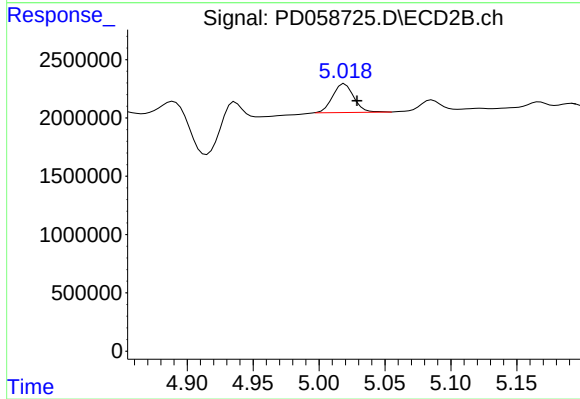

#4 Heptachlor


R.T.: 5.019 min
Delta R.T.: -0.009 min
Response: 2750737
Conc: 0.95 ng/ml

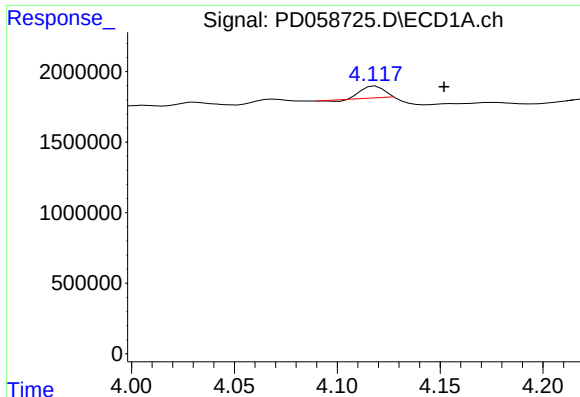

#6 beta-BHC


R.T.: 4.119 min
Delta R.T.: -0.033 min
Response: 642089
Conc: 0.68 ng/ml

Instrument :
ECD_D
ClientSampleId :

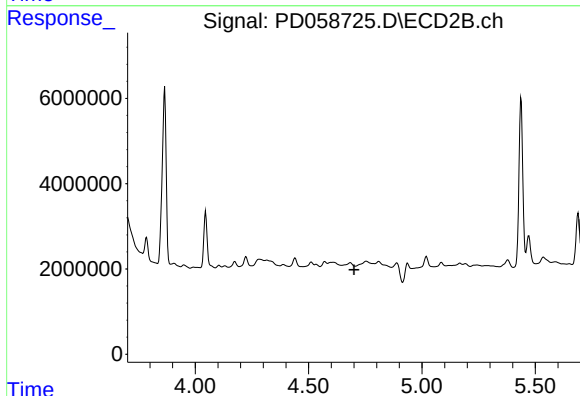


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.701 min
Response: 0
Conc: N.D.

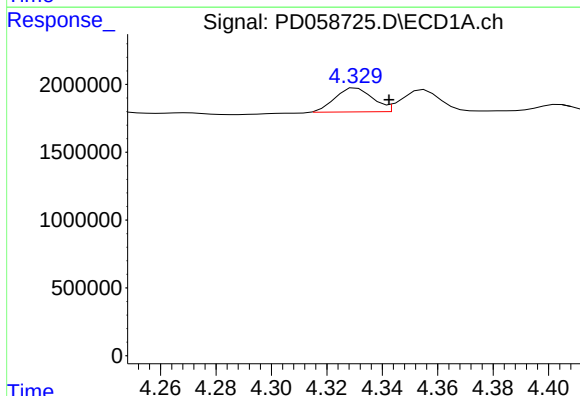


#7 delta-BHC

R.T.: 4.331 min
Delta R.T.: -0.012 min
Response: 1653980
Conc: 0.72 ng/ml

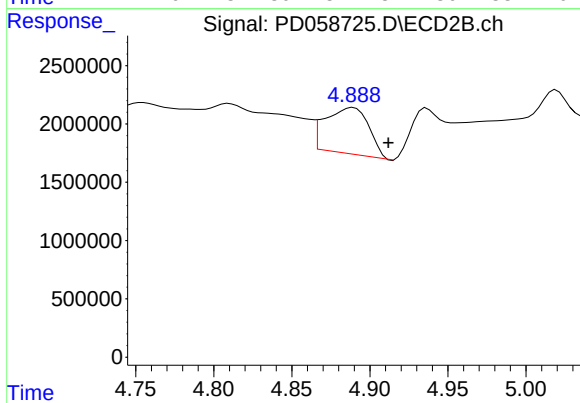

#7 delta-BHC


R.T.: 4.889 min
Delta R.T.: -0.023 min
Response: 7650182
Conc: 3.45 ng/ml

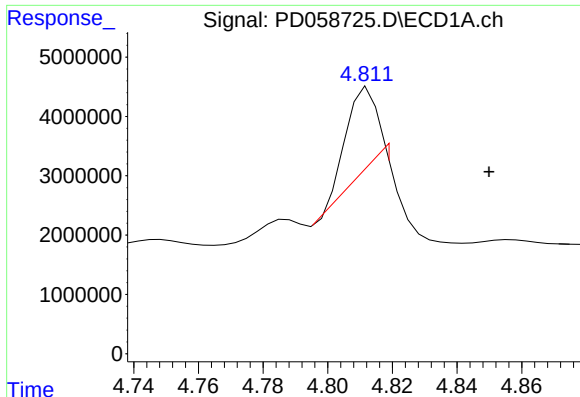

#8 Heptachlor epoxide


R.T.: 4.813 min
Delta R.T.: -0.037 min
Response: 9294424
Conc: 5.27 ng/ml

Instrument :
ECD_D
ClientSampleId :

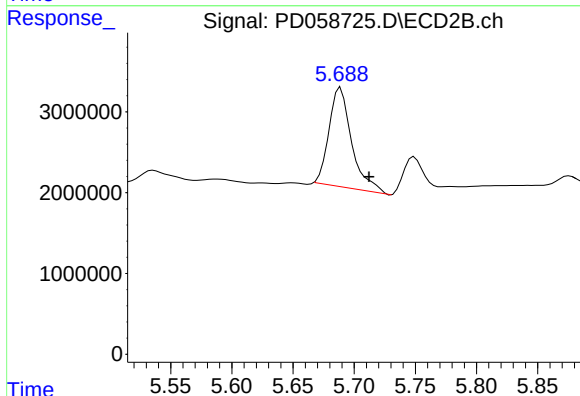


#8 Heptachlor epoxide

R.T.: 5.689 min
Delta R.T.: -0.023 min
Response: 15811453
Conc: 6.11 ng/ml

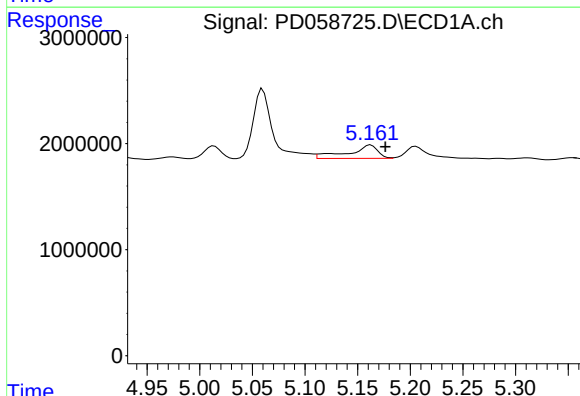


#9 Endosulfan I

R.T.: 5.162 min
Delta R.T.: -0.014 min
Response: 2473734
Conc: 1.38 ng/ml

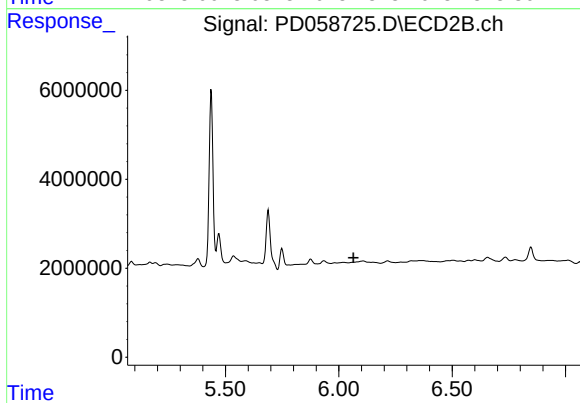

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.065 min
Response: 0
Conc: N.D.

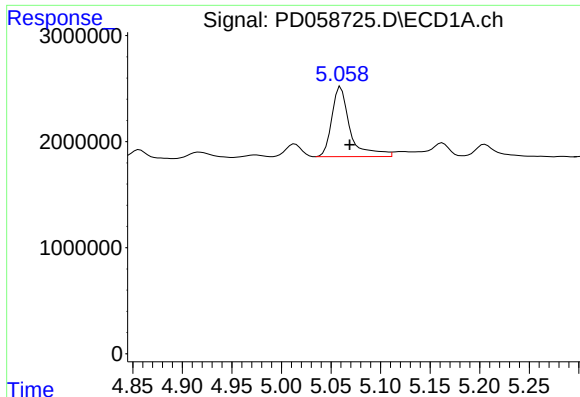

#10 trans-Chlordane


R.T.: 5.060 min
Delta R.T.: -0.009 min
Response: 8455431
Conc: 4.29 ng/ml

Instrument :
ECD_D
ClientSampleId :

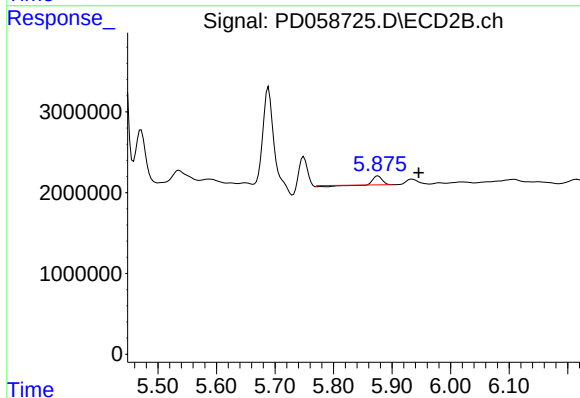


#10 trans-Chlordane

R.T.: 5.876 min
Delta R.T.: -0.069 min
Response: 992665
Conc: 0.38 ng/ml

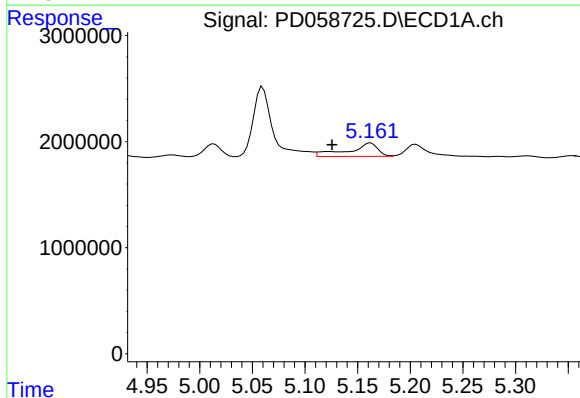


#11 cis-Chlordane

R.T.: 5.162 min
Delta R.T.: 0.037 min
Response: 2473734
Conc: 1.25 ng/ml

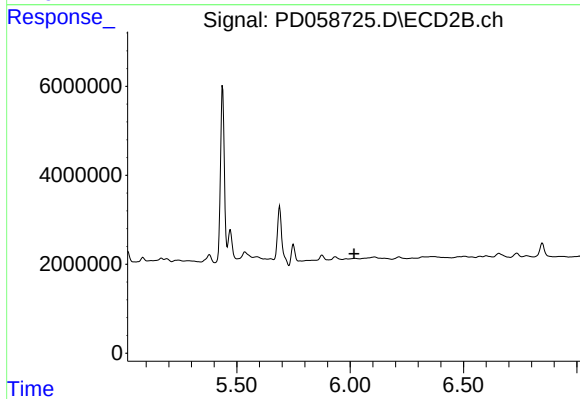

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.017 min
Response: 0
Conc: N.D.

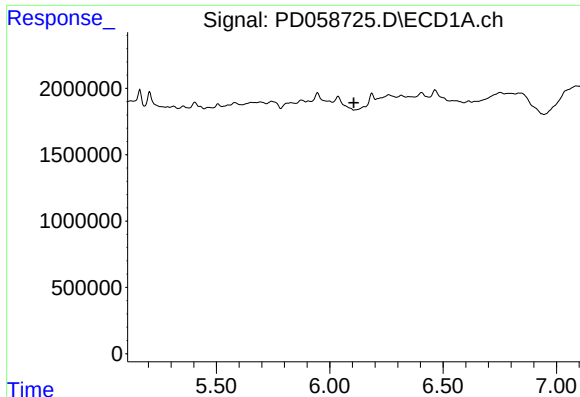

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.107 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

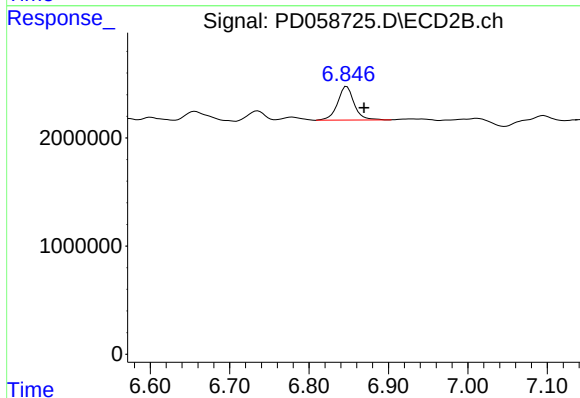


#18 Endrin aldehyde

R.T.: 6.848 min
Delta R.T.: -0.022 min
Response: 4519424
Conc: 2.37 ng/ml

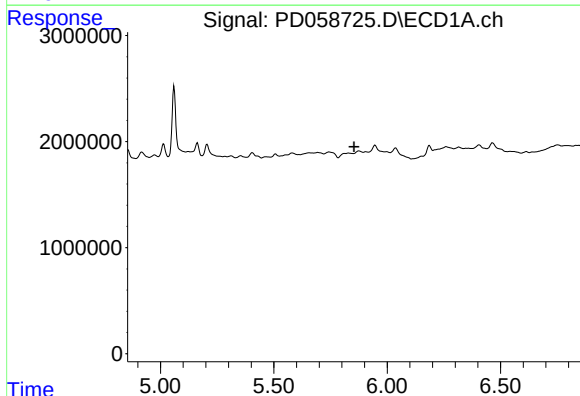


#24 Toxaphene-3

R.T.: 0.000 min
Exp R.T.: 5.854 min
Response: 0
Conc: N.D.

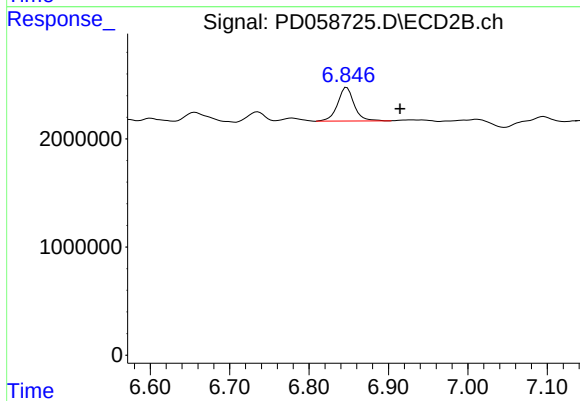

#24 Toxaphene-3


R.T.: 6.848 min
Delta R.T.: -0.067 min
Response: 4519424
Conc: 218.69 ng/ml

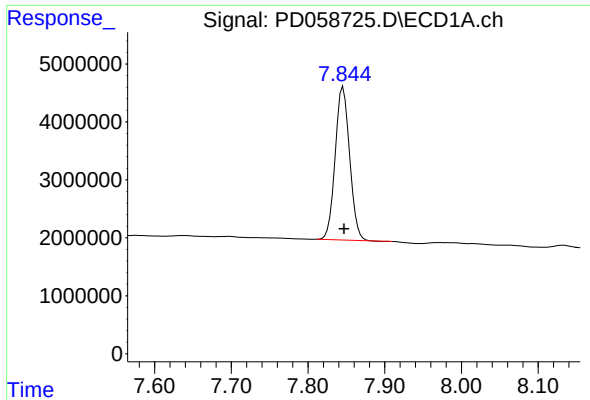

#27 Decachlorobiphenyl

R.T.: 7.846 min
Delta R.T.: -0.001 min
Response: 34556568
Conc: 19.55 ng/ml

Instrument :
ECD_D
ClientSampleId :

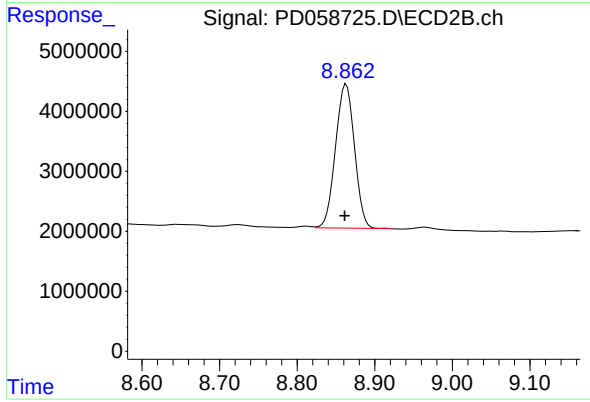

#27 Decachlorobiphenyl

R.T.: 8.863 min
Delta R.T.: 0.002 min
Response: 40729047
Conc: 19.17 ng/ml