

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072720\
 Data File : PD058726.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2020 18:08
 Operator : AJ\MA
 Sample : L3443-09
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 28 01:00:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070220CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 02 16:12:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.866	25824167	43513963	15.364	19.096
27)	SA Decachlor...	7.846	8.863	34546832	41203149	19.541	19.393
Target Compounds							
2)	A alpha-BHC	3.621	4.224	1256934	966199	0.505	0.285 #
3)	MA gamma-BHC...	0.000	4.570f	0	953812	N.D.	0.308
4)	MA Heptachlor	0.000	5.019	0	3379345	N.D.	1.163
6)	B beta-BHC	4.120f	0.000	785746	0	0.829	N.D. #
7)	B delta-BHC	4.331	4.938f	1598500	1850208	0.694	0.835
8)	B Heptachlo...	4.813f	5.688	2905209	10115688	1.647	3.911 #
10)	B trans-Chl...	5.059	0.000	3617325	0	1.836	N.D. #
11)	B cis-Chlor...	5.059f	0.000	3617325	0	1.826	N.D. #
15)	B Endosulfa...	5.945	6.737	1091878	1310271	0.674	0.580
25)	Toxaphene-4	5.945	0.000	1091878	0	41.148	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072720\
Data File : PD058726.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2020 18:08
Operator : AJ\MA
Sample : L3443-09
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 01:00:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070220CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 02 16:12:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

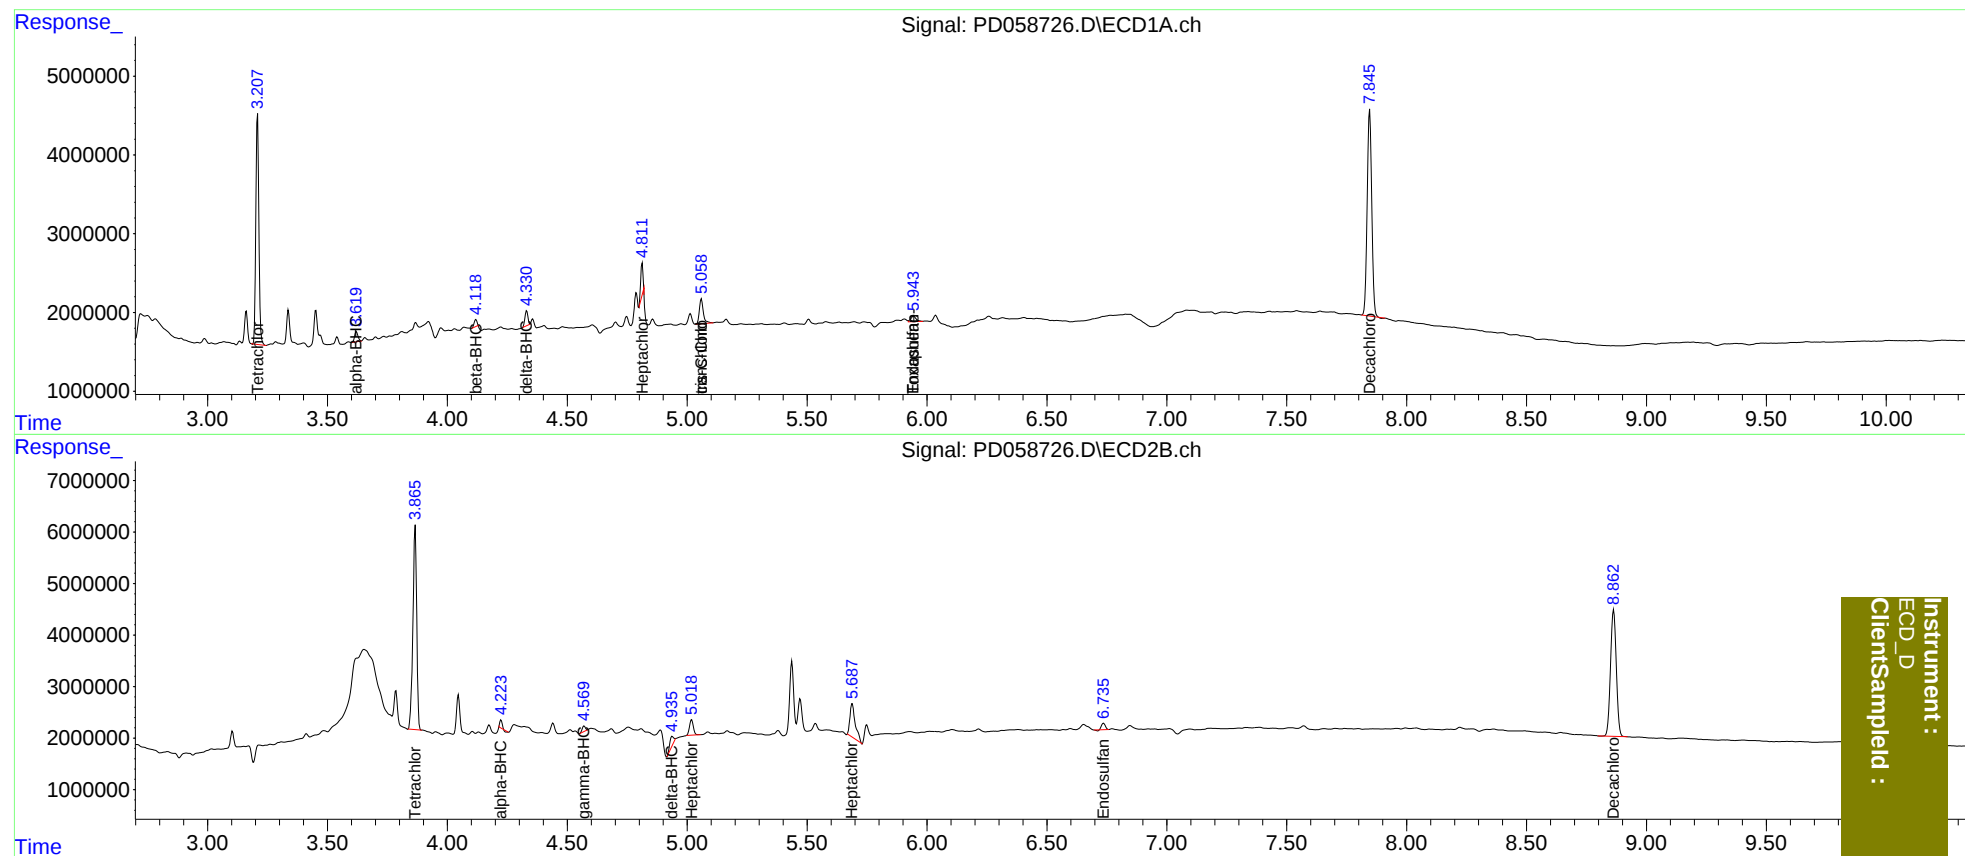


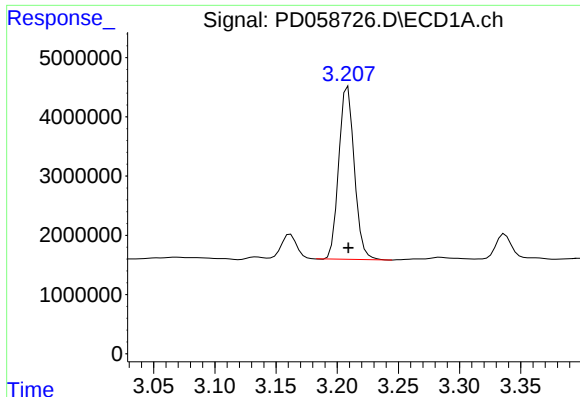

#1 Tetrachloro-m-xylene


R.T.: 3.209 min
Delta R.T.: 0.000 min
Response: 25824167
Conc: 15.36 ng/ml

Instrument :
ECD_D
ClientSampleId :

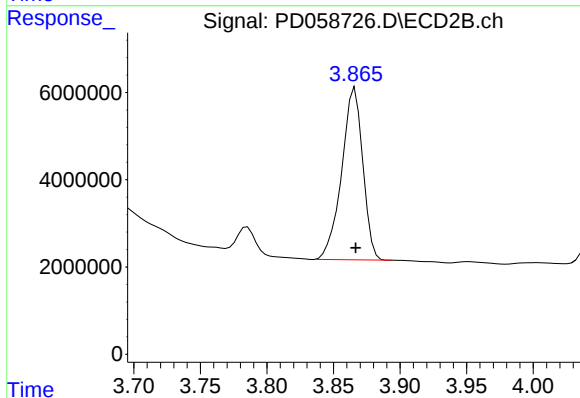


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.000 min
Response: 43513963
Conc: 19.10 ng/ml

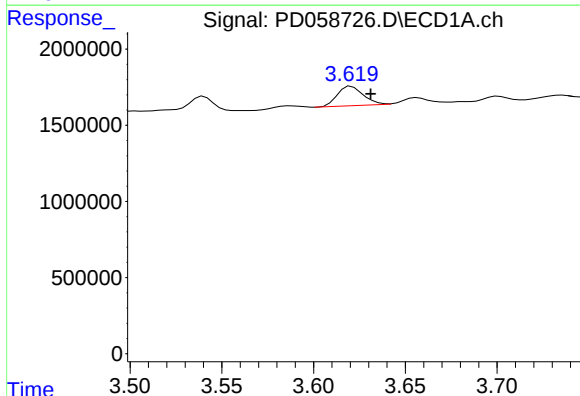


#2 alpha-BHC

R.T.: 3.621 min
Delta R.T.: -0.010 min
Response: 1256934
Conc: 0.51 ng/ml

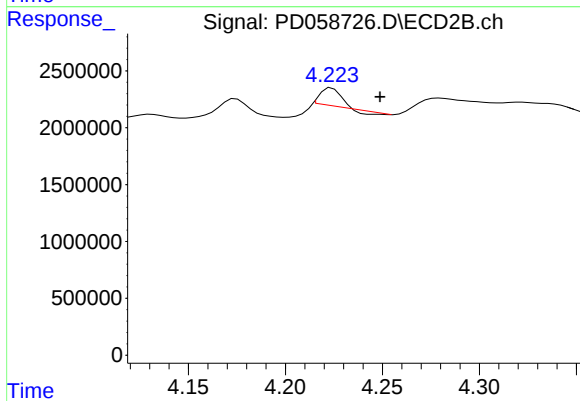

#2 alpha-BHC


R.T.: 4.224 min
Delta R.T.: -0.025 min
Response: 966199
Conc: 0.29 ng/ml

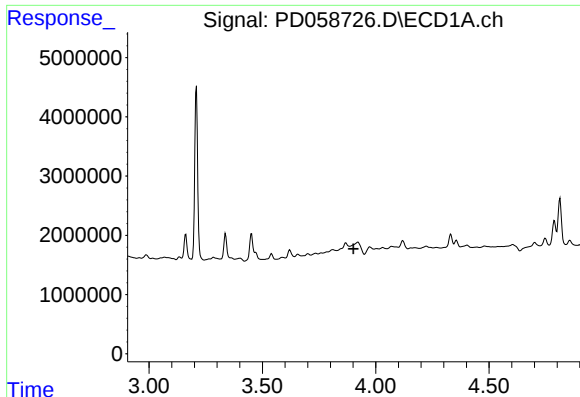

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 3.903 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

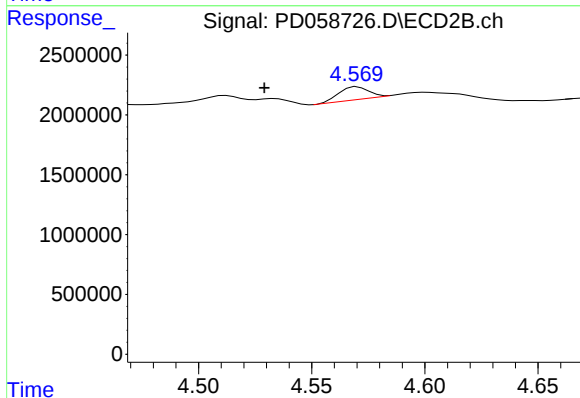


#3 gamma-BHC (Lindane)

R.T.: 4.570 min
Delta R.T.: 0.041 min
Response: 953812
Conc: 0.31 ng/ml

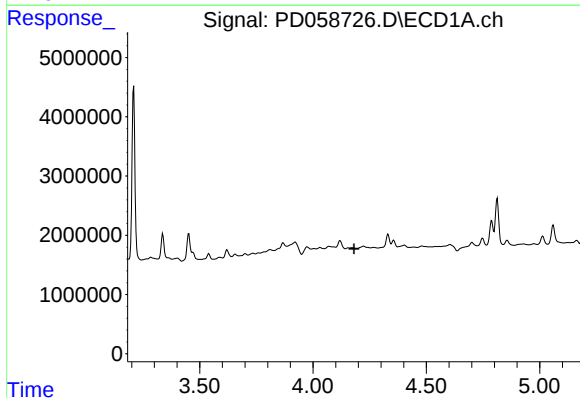


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.182 min
Response: 0
Conc: N.D.

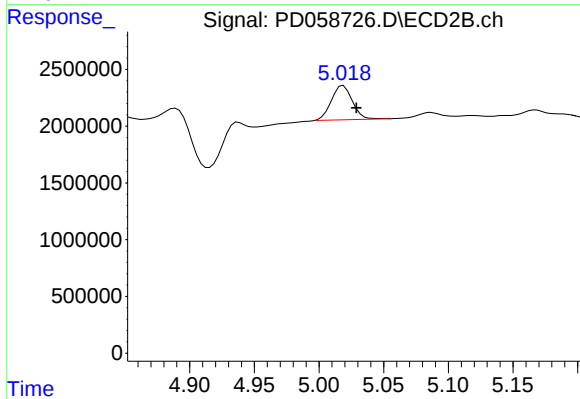

#4 Heptachlor


R.T.: 5.019 min
Delta R.T.: -0.010 min
Response: 3379345
Conc: 1.16 ng/ml

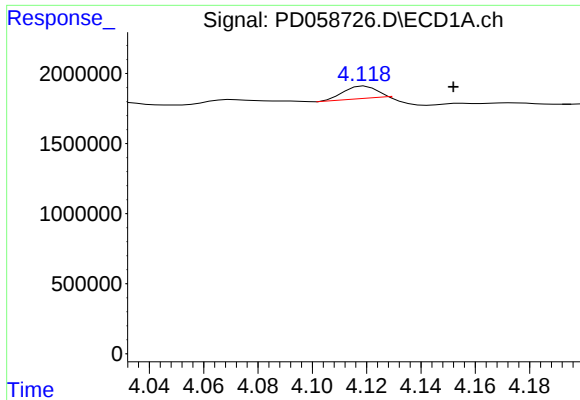

#6 beta-BHC


R.T.: 4.120 min
Delta R.T.: -0.032 min
Response: 785746
Conc: 0.83 ng/ml

Instrument :
ECD_D
ClientSampleId :

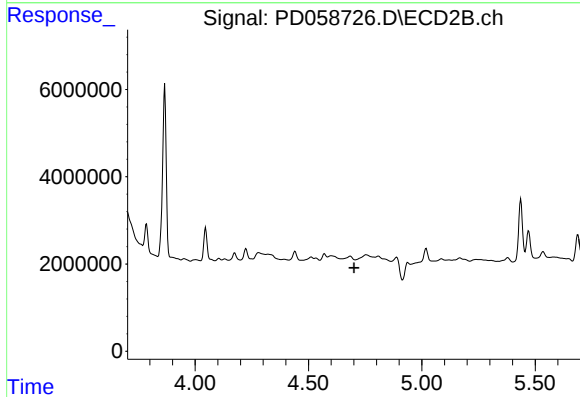


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.701 min
Response: 0
Conc: N.D.

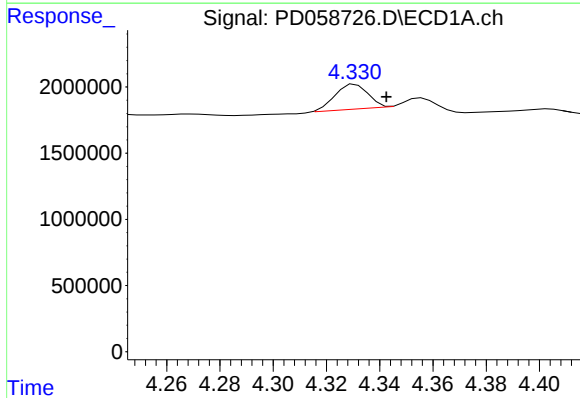


#7 delta-BHC

R.T.: 4.331 min
Delta R.T.: -0.012 min
Response: 1598500
Conc: 0.69 ng/ml

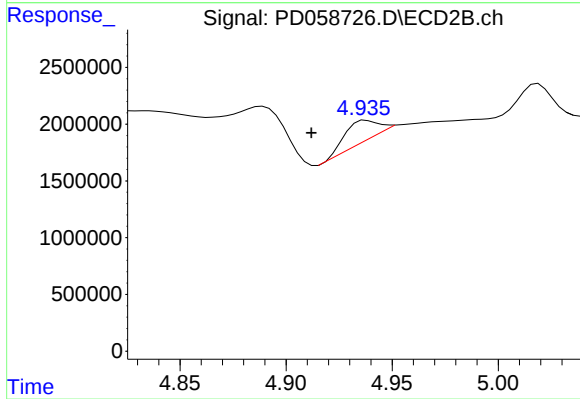

#7 delta-BHC


R.T.: 4.938 min
Delta R.T.: 0.026 min
Response: 1850208
Conc: 0.84 ng/ml

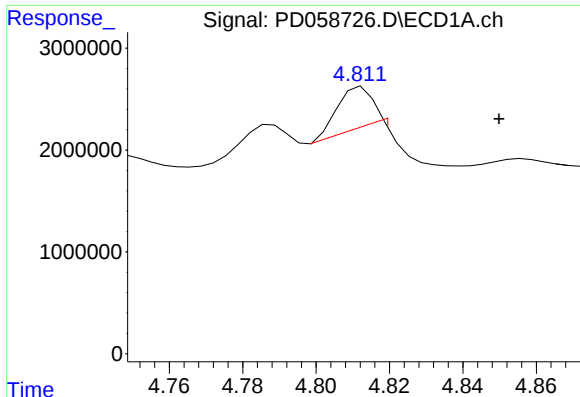

#8 Heptachlor epoxide


R.T.: 4.813 min
Delta R.T.: -0.037 min
Response: 2905209
Conc: 1.65 ng/ml

Instrument :
ECD_D
ClientSampleId :

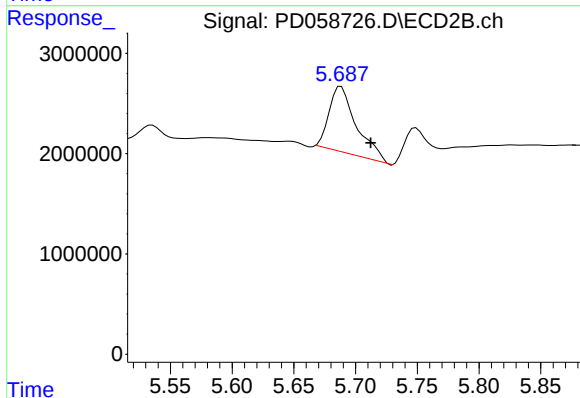


#8 Heptachlor epoxide

R.T.: 5.688 min
Delta R.T.: -0.024 min
Response: 10115688
Conc: 3.91 ng/ml

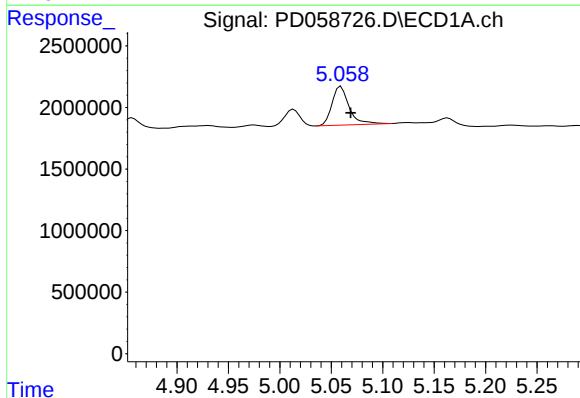


#10 trans-Chlordane

R.T.: 5.059 min
Delta R.T.: -0.010 min
Response: 3617325
Conc: 1.84 ng/ml

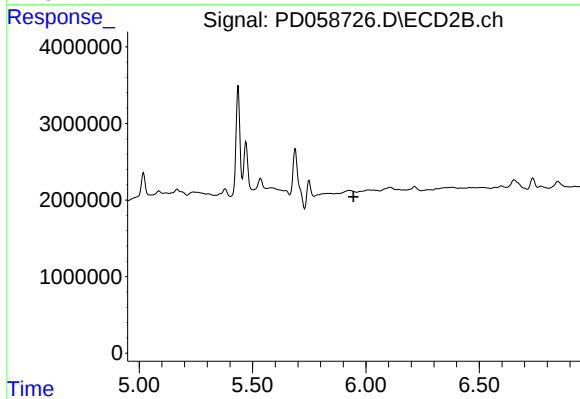

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.945 min
Response: 0
Conc: N.D.

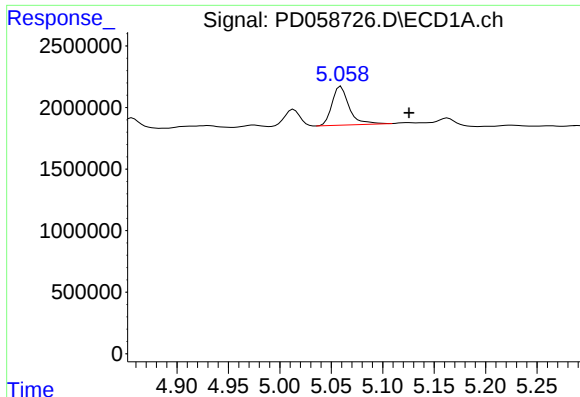

#11 cis-Chlordane


R.T.: 5.059 min
Delta R.T.: -0.066 min
Response: 3617325
Conc: 1.83 ng/ml

Instrument :
ECD_D
ClientSampleId :

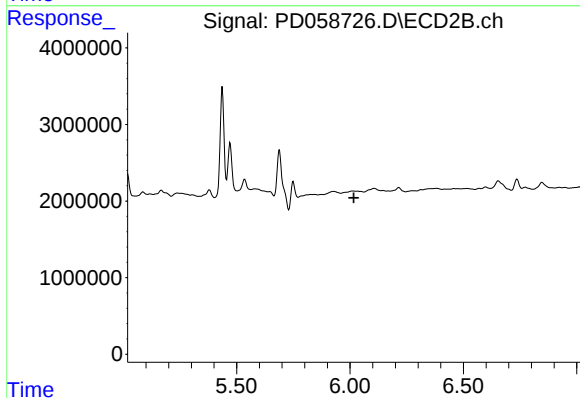


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.017 min
Response: 0
Conc: N.D.

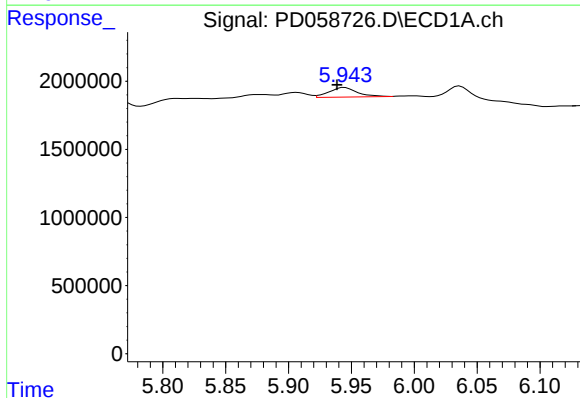


#15 Endosulfan II

R.T.: 5.945 min
Delta R.T.: 0.006 min
Response: 1091878
Conc: 0.67 ng/ml

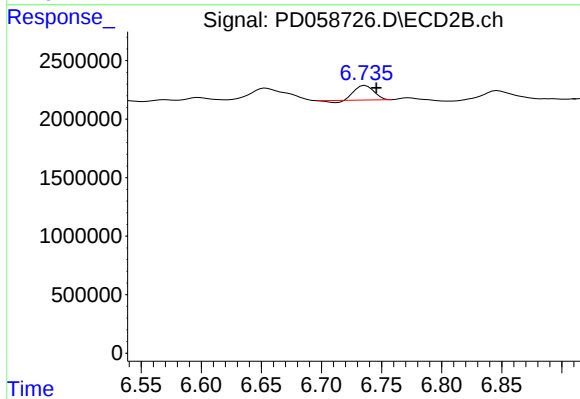

#15 Endosulfan II


R.T.: 6.737 min
Delta R.T.: -0.009 min
Response: 1310271
Conc: 0.58 ng/ml

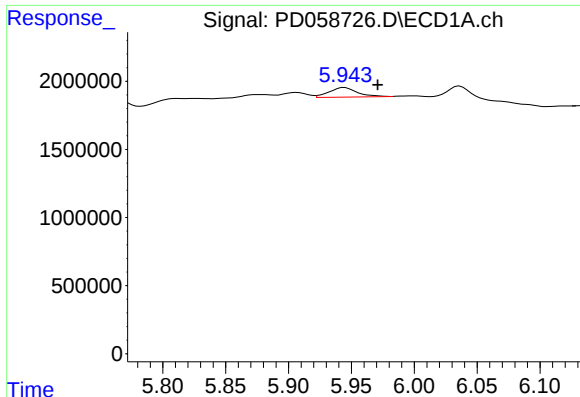

#25 Toxaphene-4


R.T.: 5.945 min
Delta R.T.: -0.026 min
Response: 1091878
Conc: 41.15 ng/ml

Instrument :
ECD_D
ClientSampleId :

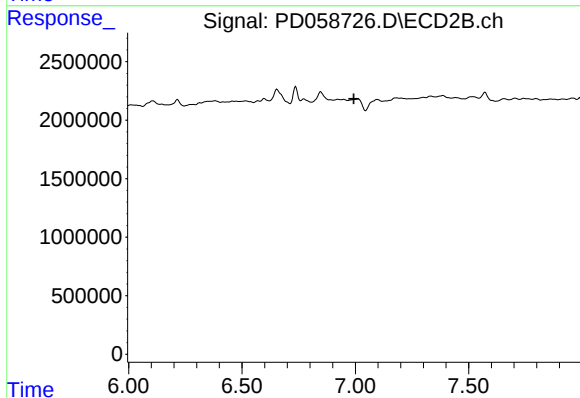


#25 Toxaphene-4

R.T.: 0.000 min
Exp R.T. : 6.993 min
Response: 0
Conc: N.D.

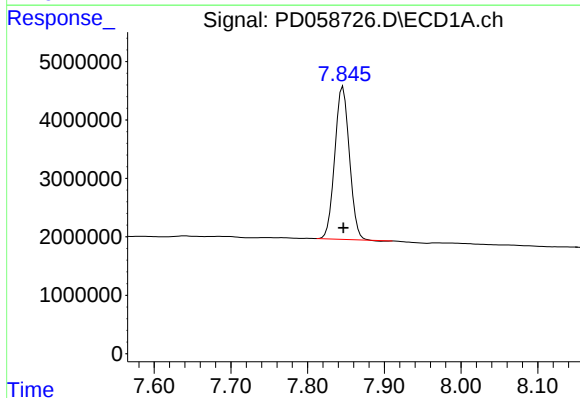

#27 Decachlorobiphenyl

R.T.: 7.846 min
Delta R.T.: 0.000 min
Response: 34546832
Conc: 19.54 ng/ml

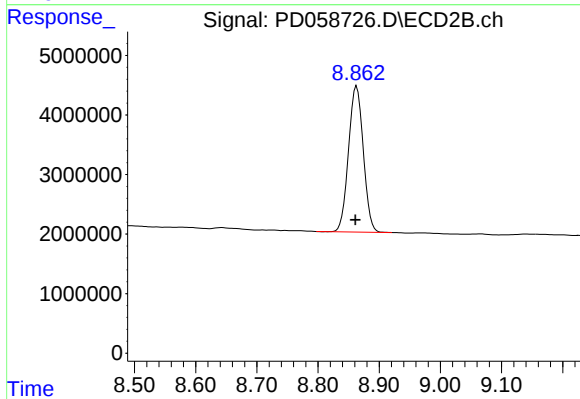

#27 Decachlorobiphenyl

R.T.: 8.863 min
Delta R.T.: 0.002 min
Response: 41203149
Conc: 19.39 ng/ml