

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072720\
 Data File : PD058728.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2020 18:36
 Operator : AJ\MA
 Sample : L3443-11
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 28 01:01:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070220CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 02 16:12:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.867	30121860	44252145	17.921	19.420
27)	SA Decachlor...	7.846	8.862	38326015	45493024	21.679	21.412
Target Compounds							
2)	A alpha-BHC	3.620	4.288f	932588	2994868	0.375	0.885 #
3)	MA gamma-BHC...	3.917	0.000	2387313	0	1.024	N.D. #
4)	MA Heptachlor	0.000	5.019	0	2428092	N.D.	0.835
6)	B beta-BHC	4.118f	0.000	618915	0	0.653	N.D. #
7)	B delta-BHC	4.331	0.000	1279123	0	0.556	N.D. #
8)	B Heptachlo...	4.813f	5.689	2233538	7112221	1.266	2.750 #
10)	B trans-Chl...	5.060	0.000	1437338	0	0.730	N.D. #
11)	B cis-Chlor...	5.060f	0.000	1437338	0	0.725	N.D. #
18)	B Endrin al...	0.000	6.847	0	2180639	N.D.	1.145
24)	Toxaphene-3	0.000	6.847	0	2180639	N.D.	105.518


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072720\
Data File : PD058728.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2020 18:36
Operator : AJ\MA
Sample : L3443-11
Misc :
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 01:01:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070220CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 02 16:12:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

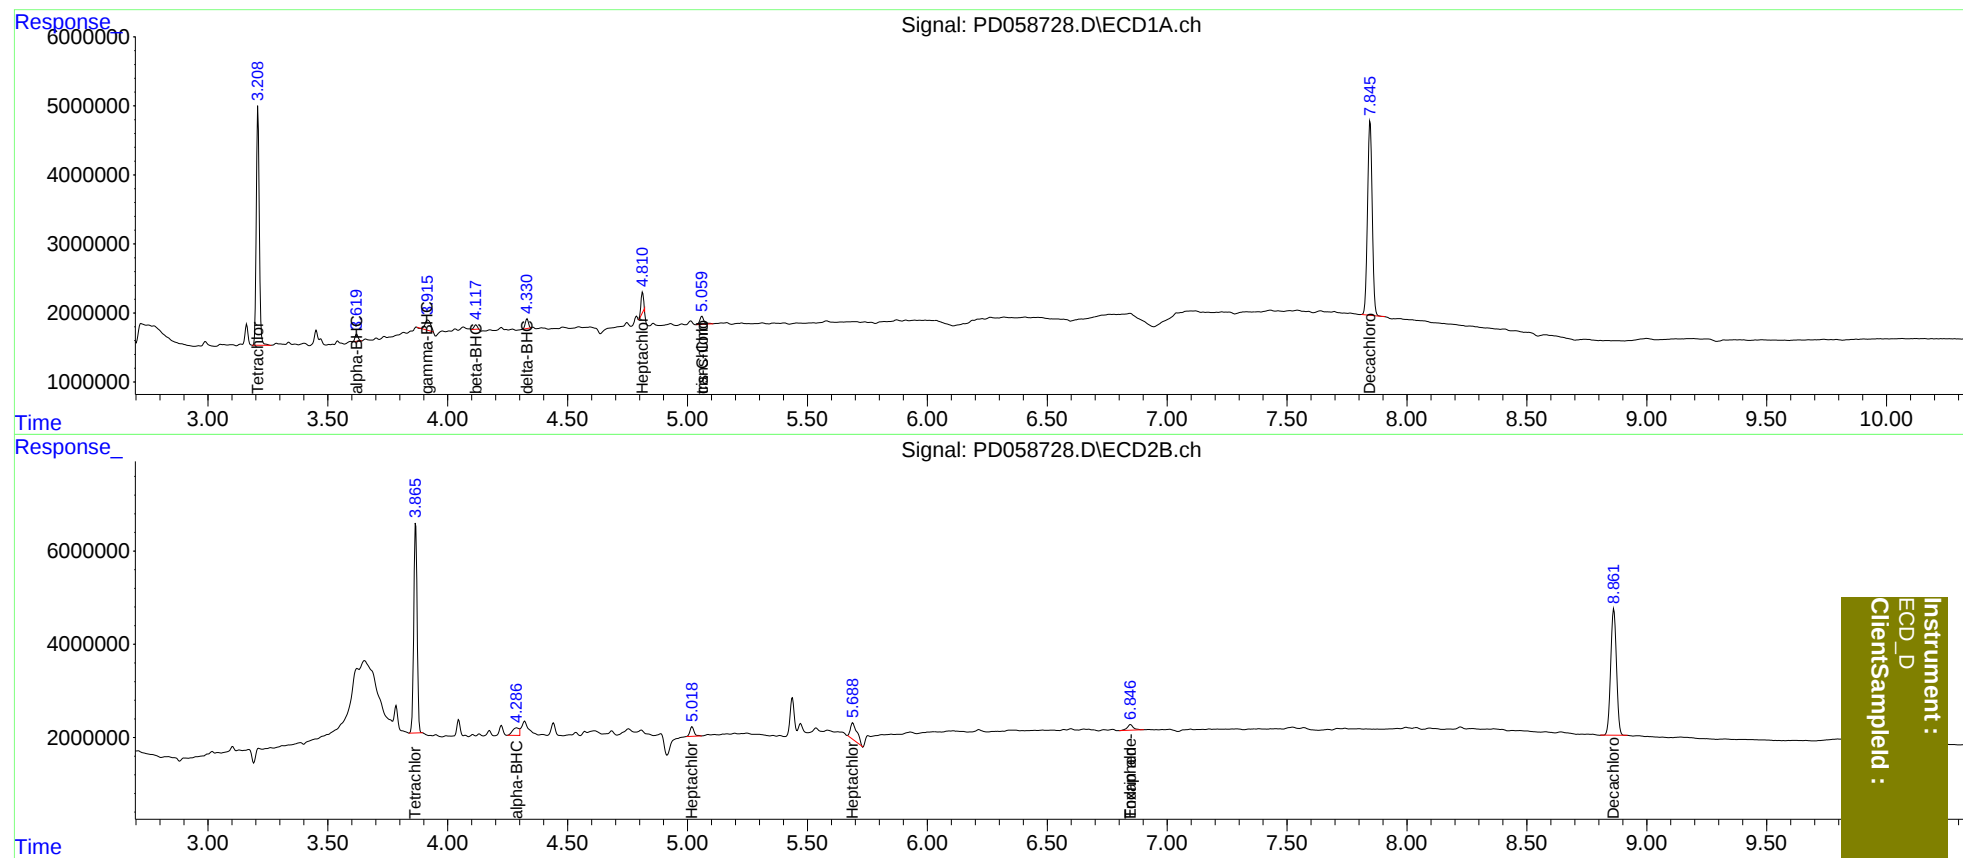


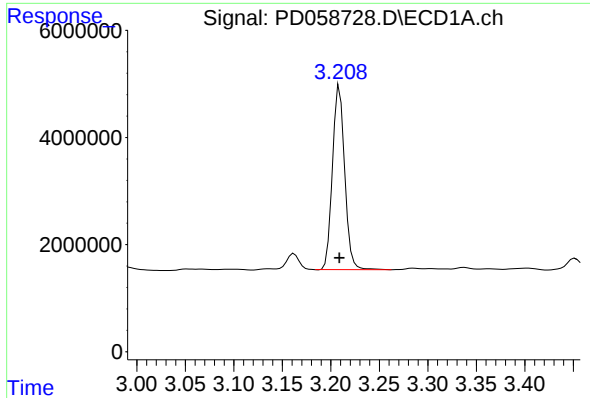

#1 Tetrachloro-m-xylene


R.T.: 3.209 min
Delta R.T.: 0.000 min
Response: 30121860
Conc: 17.92 ng/ml

Instrument :
ECD_D
ClientSampleId :

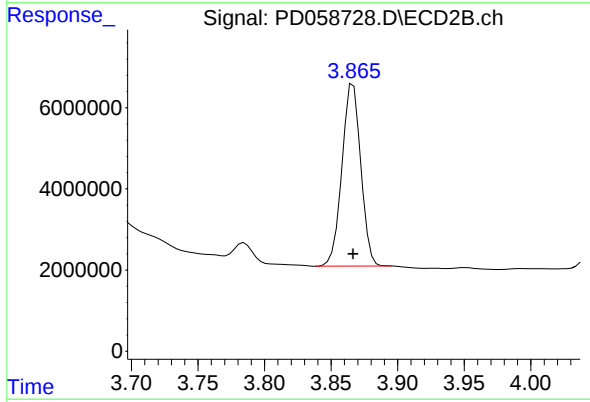


#1 Tetrachloro-m-xylene

R.T.: 3.867 min
Delta R.T.: 0.000 min
Response: 44252145
Conc: 19.42 ng/ml

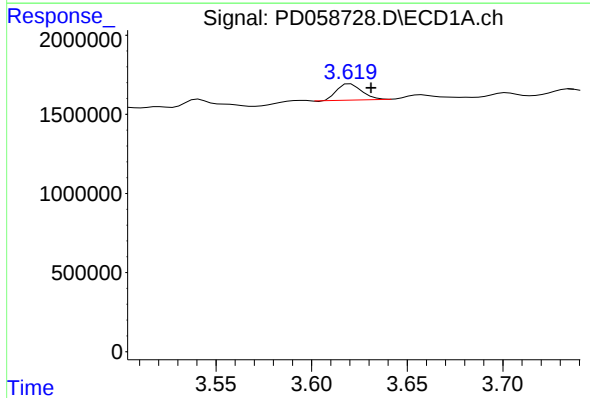


#2 alpha-BHC

R.T.: 3.620 min
Delta R.T.: -0.011 min
Response: 932588
Conc: 0.37 ng/ml

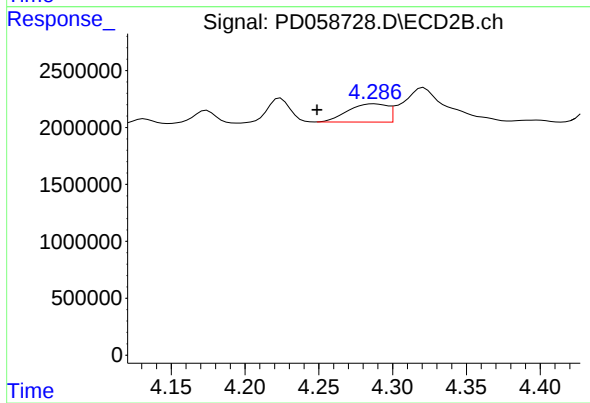

#2 alpha-BHC


R.T.: 4.288 min
Delta R.T.: 0.039 min
Response: 2994868
Conc: 0.88 ng/ml

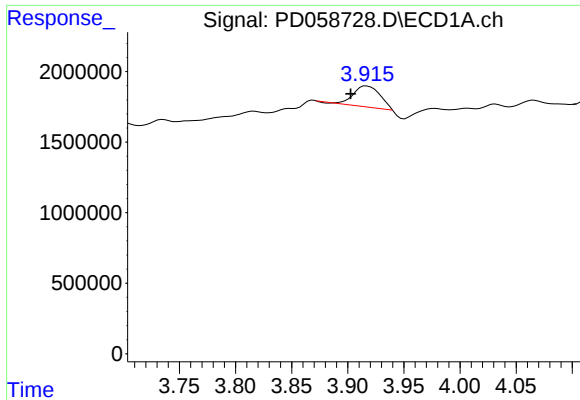

#3 gamma-BHC (Lindane)


R.T.: 3.917 min
Delta R.T.: 0.014 min
Response: 2387313
Conc: 1.02 ng/ml

Instrument :
ECD_D
ClientSampleId :

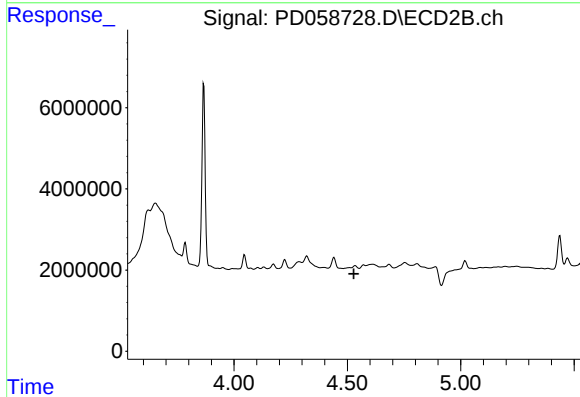


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.529 min
Response: 0
Conc: N.D.

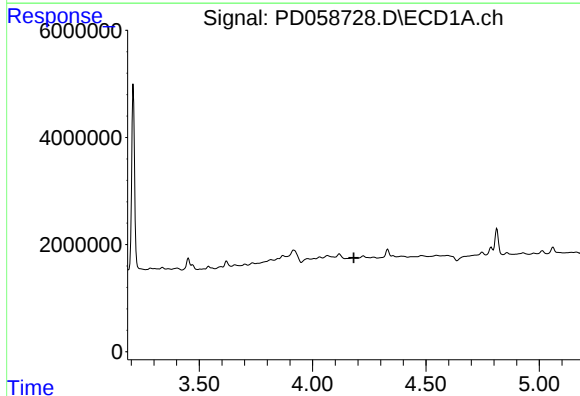


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.182 min
Response: 0
Conc: N.D.

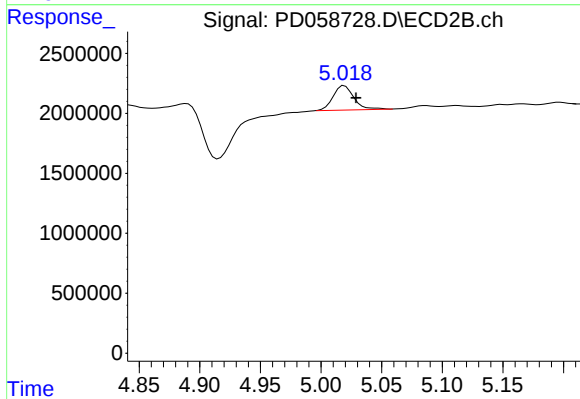

#4 Heptachlor


R.T.: 5.019 min
Delta R.T.: -0.010 min
Response: 2428092
Conc: 0.84 ng/ml

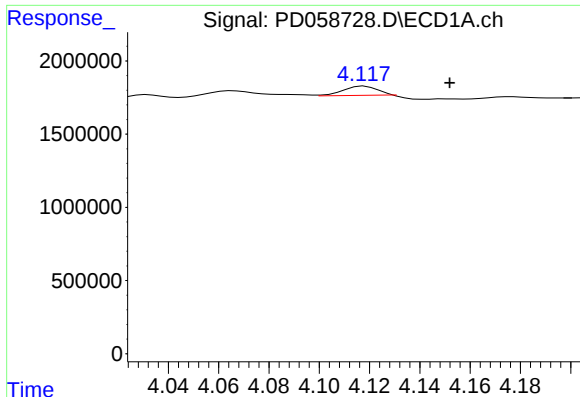

#6 beta-BHC


R.T.: 4.118 min
Delta R.T.: -0.034 min
Response: 618915
Conc: 0.65 ng/ml

Instrument :
ECD_D
ClientSampleId :

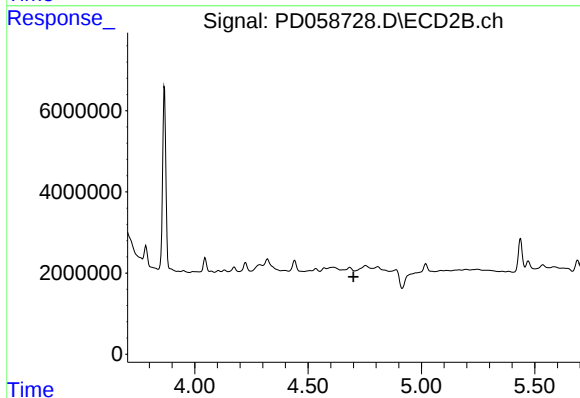


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.701 min
Response: 0
Conc: N.D.

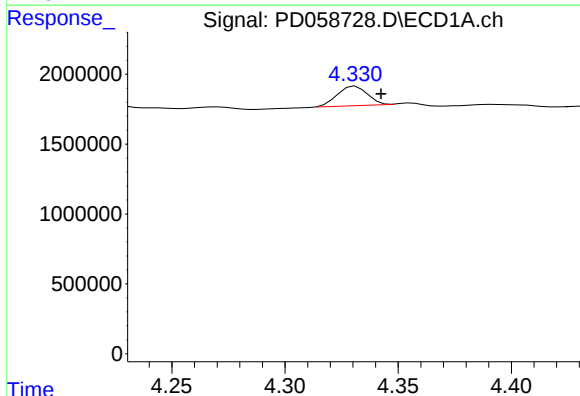


#7 delta-BHC

R.T.: 4.331 min
Delta R.T.: -0.011 min
Response: 1279123
Conc: 0.56 ng/ml

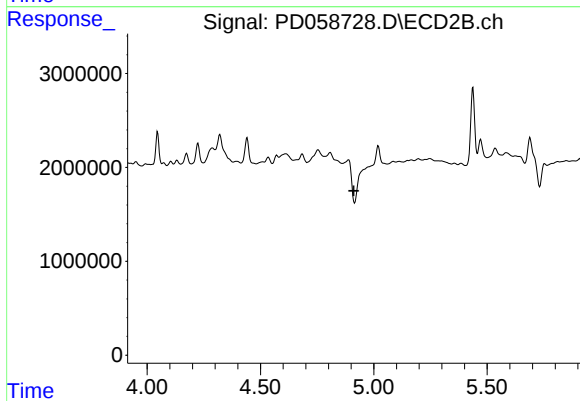

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.912 min
Response: 0
Conc: N.D.

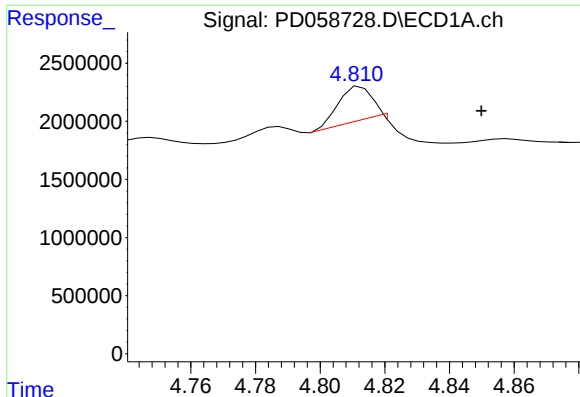

#8 Heptachlor epoxide


R.T.: 4.813 min
Delta R.T.: -0.037 min
Response: 2233538
Conc: 1.27 ng/ml

Instrument :
ECD_D
ClientSampleId :

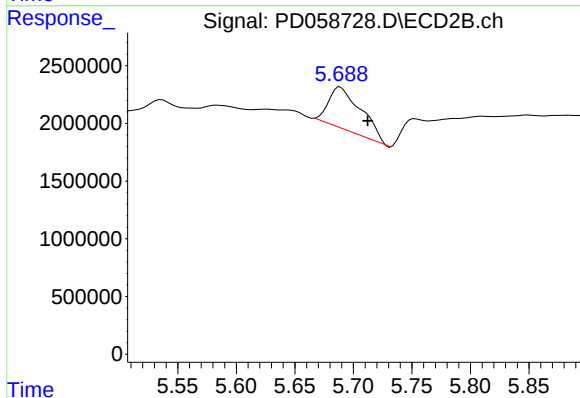


#8 Heptachlor epoxide

R.T.: 5.689 min
Delta R.T.: -0.023 min
Response: 7112221
Conc: 2.75 ng/ml

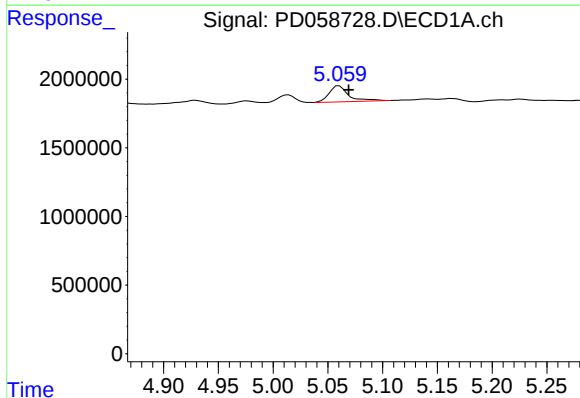


#10 trans-Chlordane

R.T.: 5.060 min
Delta R.T.: -0.009 min
Response: 1437338
Conc: 0.73 ng/ml

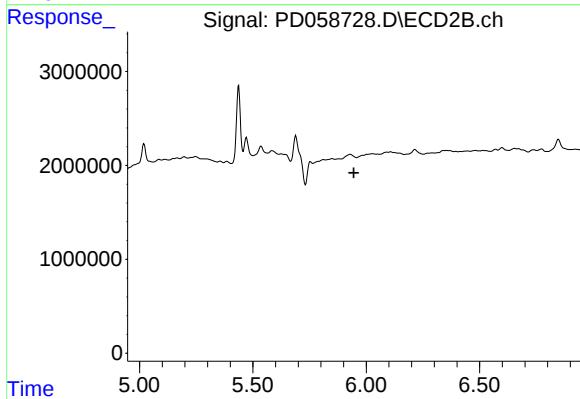

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.945 min
Response: 0
Conc: N.D.

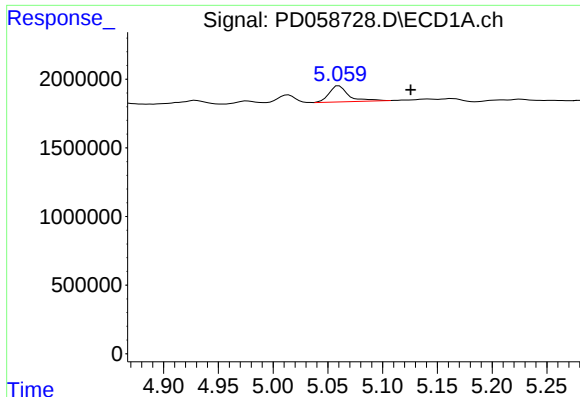

#11 cis-Chlordane


R.T.: 5.060 min
Delta R.T.: -0.065 min
Response: 1437338
Conc: 0.73 ng/ml

Instrument :
ECD_D
ClientSampleId :

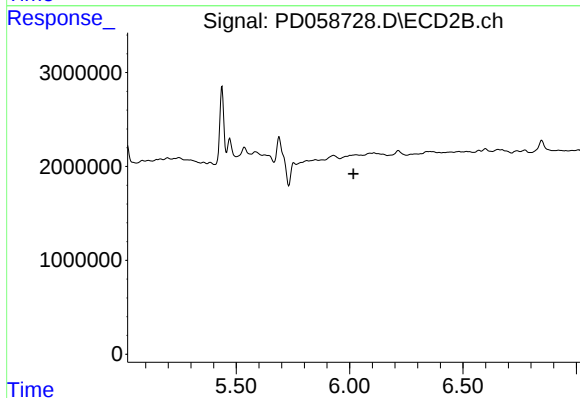


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.017 min
Response: 0
Conc: N.D.

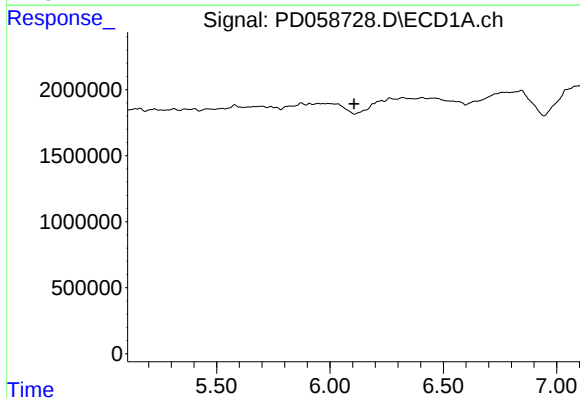


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.107 min
Response: 0
Conc: N.D.

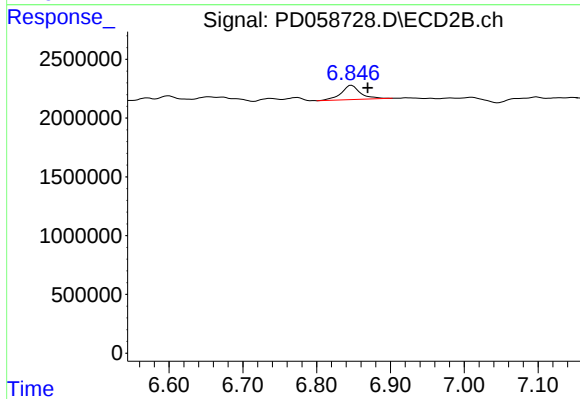

#18 Endrin aldehyde


R.T.: 6.847 min
Delta R.T.: -0.022 min
Response: 2180639
Conc: 1.14 ng/ml

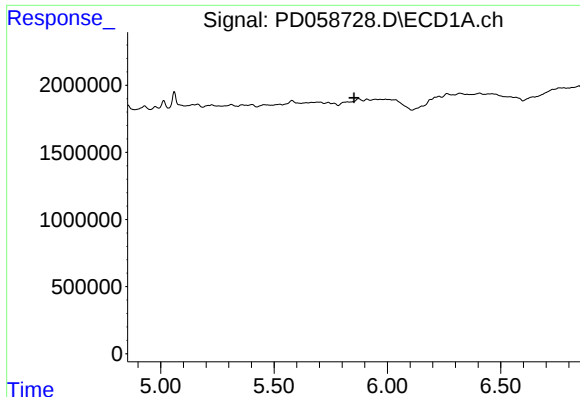

#24 Toxaphene-3


R.T.: 0.000 min
Exp R.T.: 5.854 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

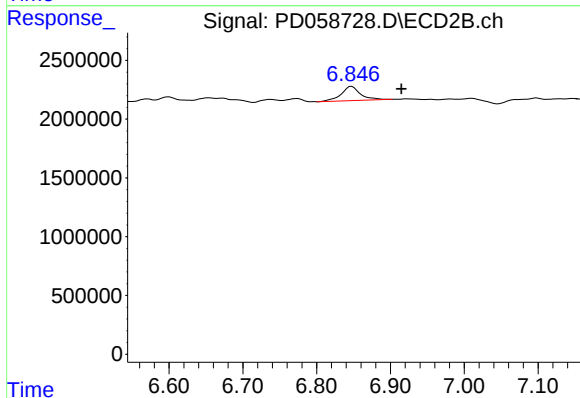


#24 Toxaphene-3

R.T.: 6.847 min
Delta R.T.: -0.067 min
Response: 2180639
Conc: 105.52 ng/ml

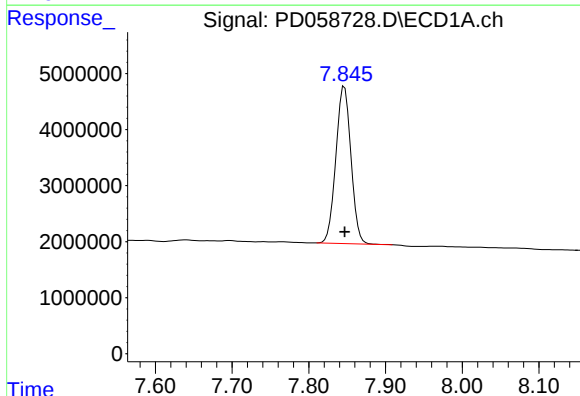

#27 Decachlorobiphenyl

R.T.: 7.846 min
Delta R.T.: 0.000 min
Response: 38326015
Conc: 21.68 ng/ml

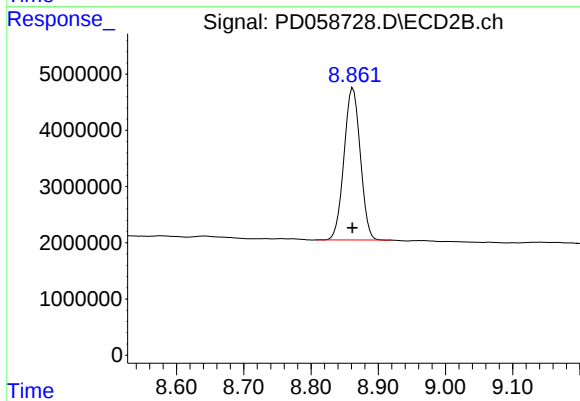

#27 Decachlorobiphenyl

R.T.: 8.862 min
Delta R.T.: 0.001 min
Response: 45493024
Conc: 21.41 ng/ml