

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072720\
Data File : PD058707.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2020 11:54
Operator : AJ\MA
Sample : PEM27
Misc :
ALS Vial : 3 Sample Multiplier: 1


Instrument :
ECD_D
LabSampleId :
PEM27

Manual Integrations
APPROVED

Ankita
7/28/2020 1:22:51 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 00:56:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070220CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 02 16:12:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

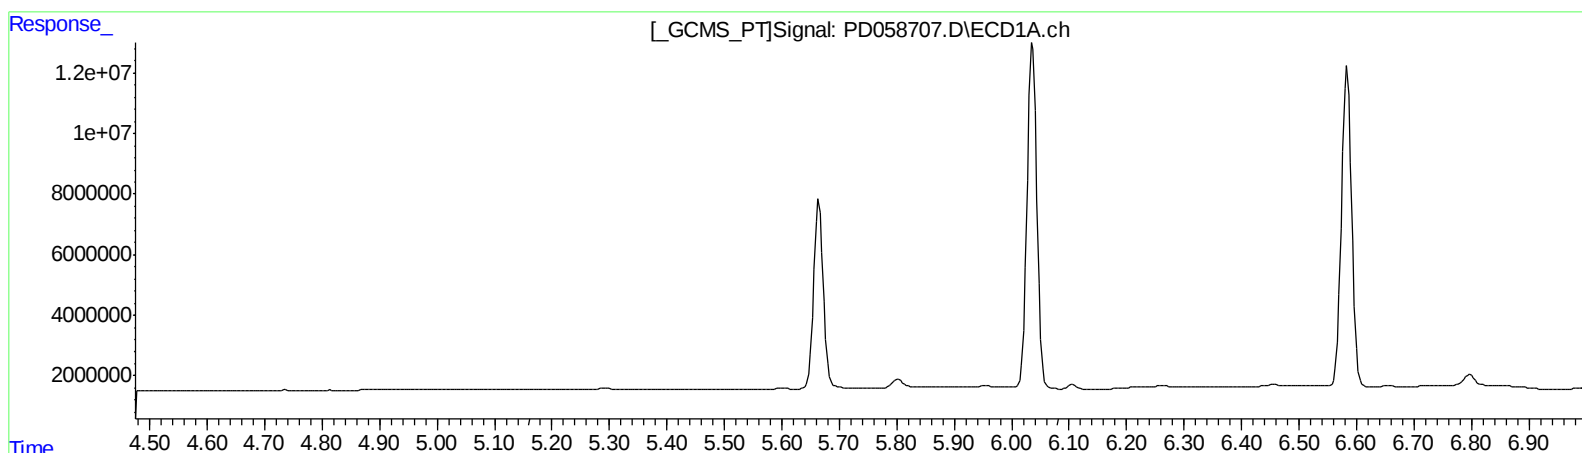

(12) 4,4'-DDE (B)
0.000min 0.000 ng/ml
response 0

(12) 4,4'-DDE #2 (B)
0.000min 0.000 ng/ml
response 0

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072720\
 Data File : PD058707.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2020 11:54
 Operator : AJ\MA
 Sample : PEM27
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_D
 LabSampleId :
 PEM27

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 28 00:56:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070220CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 02 16:12:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Manual Integrations
 APPROVED

Ankita
 7/28/2020 1:22:51 PM

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.208	3.865	30858498	45786909	18.359	20.093
27) SA Decachlor...	7.845	8.861	31455970	37531976	17.793	17.665
Target Compounds						
2) A alpha-BHC	3.631	4.248	22485929	32651885	9.036	9.647
3) MA gamma-BHC...	3.902	4.528	21580461	29569195	9.255	9.540
6) B beta-BHC	4.151	4.700	9666208	13522035	10.199	9.781
12) B 4,4'-DDE	5.293	6.175	520856	768956	0.259m	0.300m
14) MA Endrin	5.665	6.535	71627025	104.1E6	48.488	45.565
16) A 4,4'-DDD	5.802	6.664	3248645	4777812	2.688	2.198
17) MA 4,4'-DDT	6.036	6.961	134.9E6	203.8E6	95.028	90.379
18) B Endrin al...	6.107	6.869	1716826	2631555	1.406	1.381
20) A Methoxychlor	6.585	7.422	130.3E6	232.1E6	238.933	198.390
21) B Endrin ke...	6.797	7.557	4928534	4270978	3.058	1.782 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

AJ
 07/31/20