

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072721\
 Data File : PD064442.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jul 2021 00:42
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 28 02:11:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 28 02:11:09 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	5.405	4.620	6379861	50032127	5.470	5.507
27)	SA Decachlor...	11.305	10.365	14278337	63541607	10.900	10.612
Target Compounds							
2)	A alpha-BHC	5.988	5.322	8014477	66553085	5.027	5.495
3)	MA gamma-BHC...	6.385	5.742	7817573	65677961	5.023	5.985
4)	MA Heptachlor	7.035	6.151	8901961	59464506	5.388	5.232
9)	A Endosulfan I	8.279	7.450	7450531	40795100	5.409	5.216
13)	MA Dieldrin	8.570	7.735	14801465	95866191	10.088	12.696 #
14)	MA Endrin	8.808	8.025	13923701	57311191	11.318	9.999
16)	A 4,4'-DDD	8.962	8.188	12838539	63058486	10.734	11.058
17)	MA 4,4'-DDT	9.280	8.450	13219553	53657936	10.358	9.822
20)	A Methoxychlor	9.771	9.042	37878634	148.0E6	53.766	58.684


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072721\
Data File : PD064442.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jul 2021 00:42
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 02:11:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 28 02:11:09 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

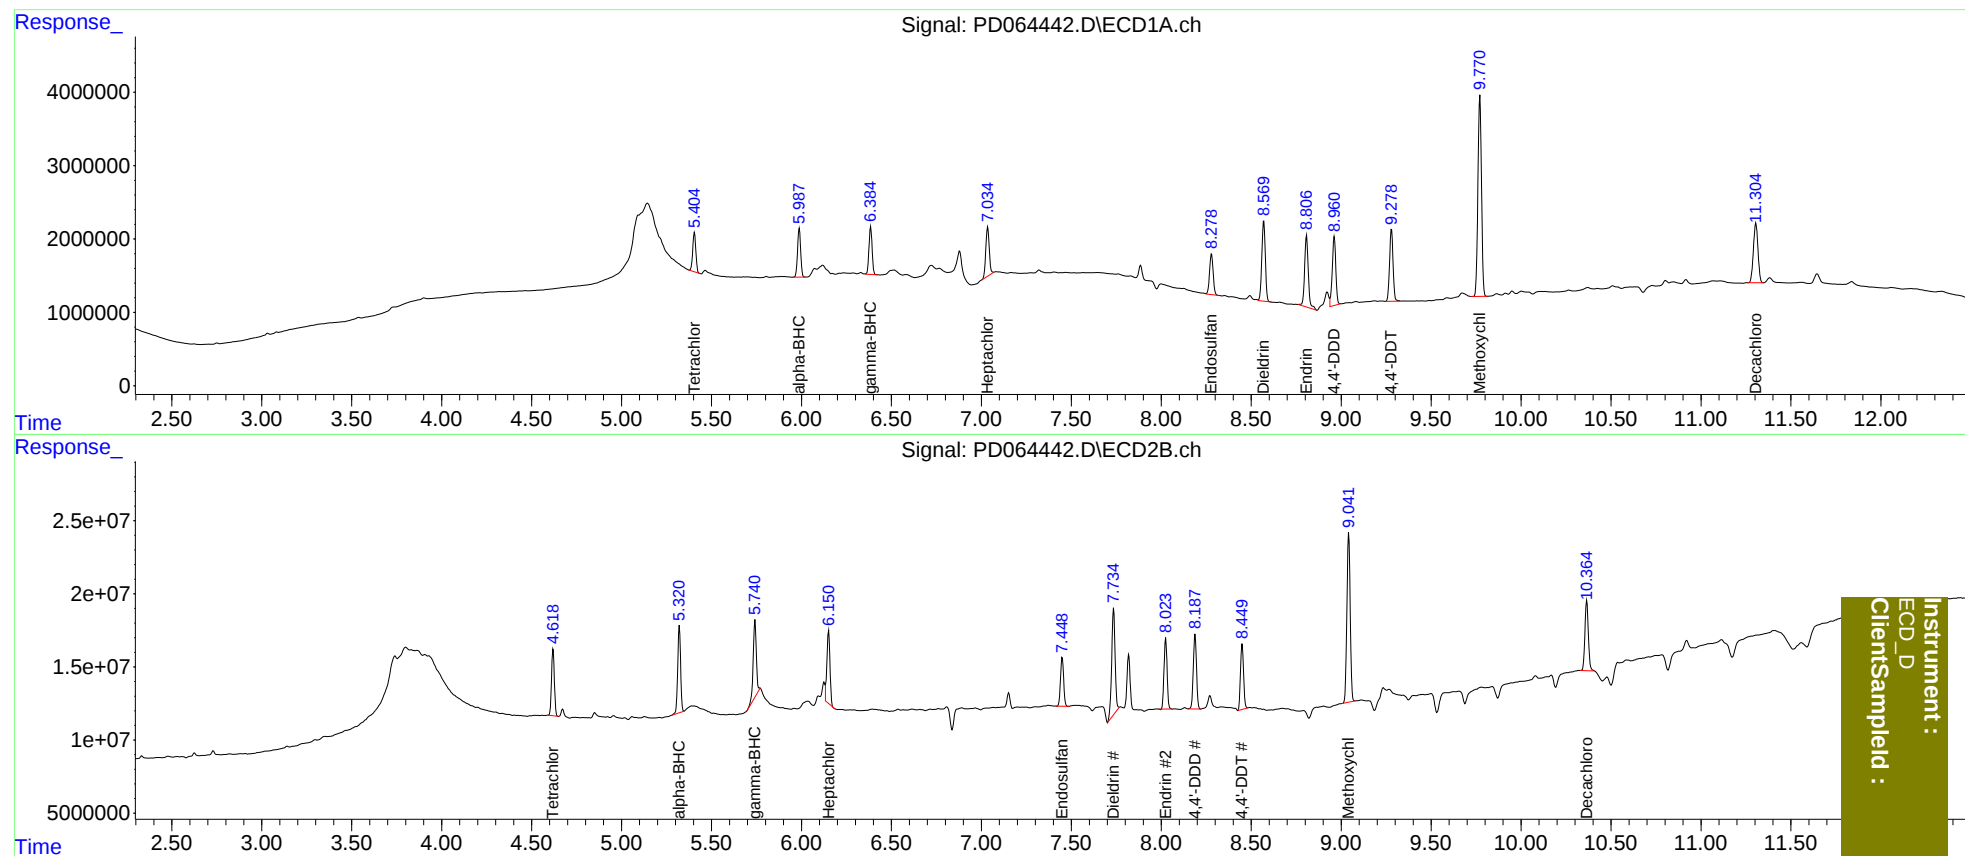


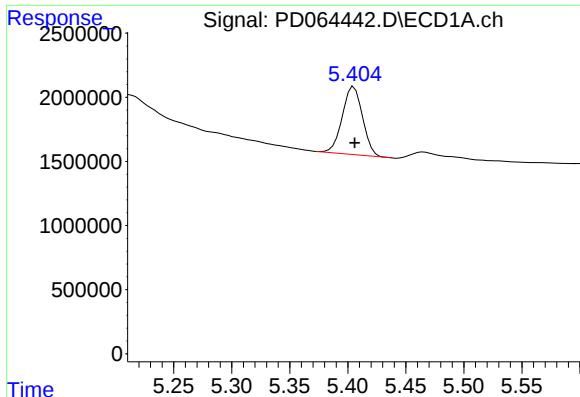

#1 Tetrachloro-m-xylene


R.T.: 5.405 min
Delta R.T.: 0.000 min
Response: 6379861
Conc: 5.47 ng/ml

Instrument :
ECD_D
ClientSampleId :

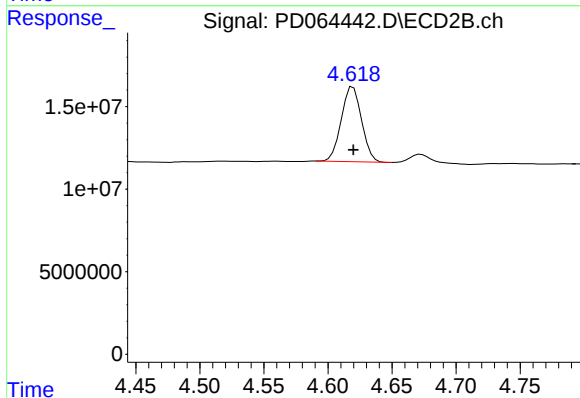


#1 Tetrachloro-m-xylene

R.T.: 4.620 min
Delta R.T.: 0.000 min
Response: 50032127
Conc: 5.51 ng/ml

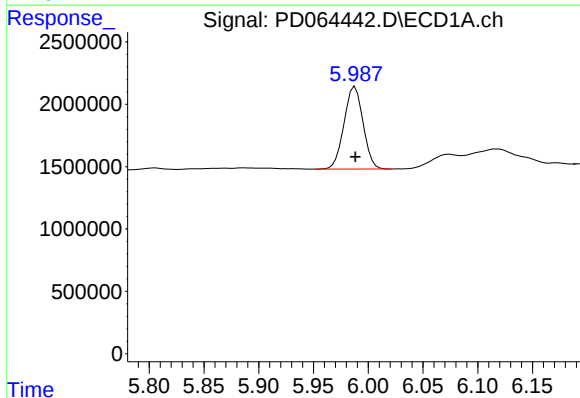


#2 alpha-BHC

R.T.: 5.988 min
Delta R.T.: 0.000 min
Response: 8014477
Conc: 5.03 ng/ml

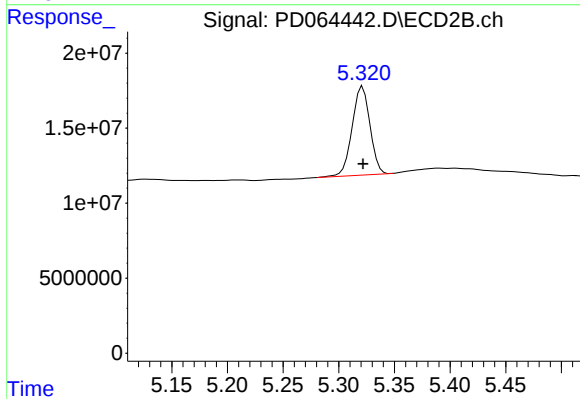

#2 alpha-BHC


R.T.: 5.322 min
Delta R.T.: 0.000 min
Response: 66553085
Conc: 5.49 ng/ml

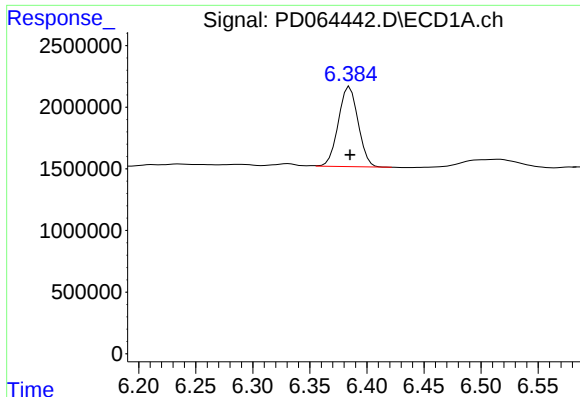

#3 gamma-BHC (Lindane)


R.T.: 6.385 min
Delta R.T.: 0.000 min
Response: 7817573
Conc: 5.02 ng/ml

Instrument :
ECD_D
ClientSampleId :

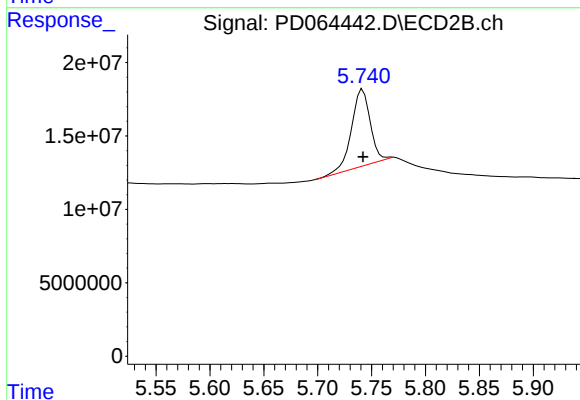


#3 gamma-BHC (Lindane)

R.T.: 5.742 min
Delta R.T.: 0.000 min
Response: 65677961
Conc: 5.98 ng/ml

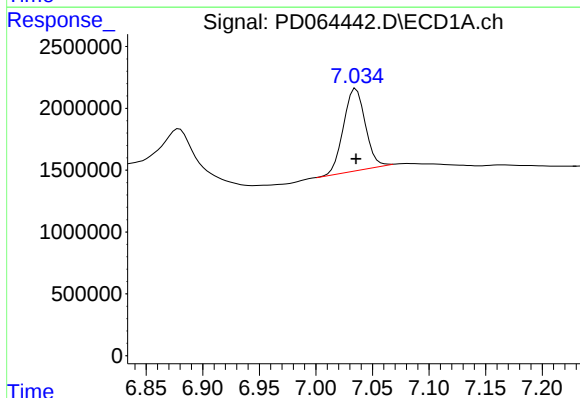


#4 Heptachlor

R.T.: 7.035 min
Delta R.T.: 0.000 min
Response: 8901961
Conc: 5.39 ng/ml

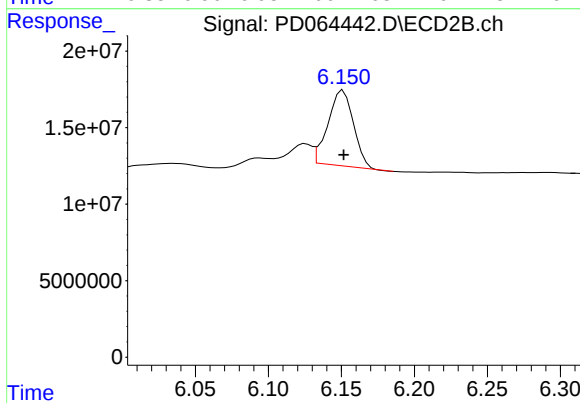

#4 Heptachlor


R.T.: 6.151 min
Delta R.T.: 0.000 min
Response: 59464506
Conc: 5.23 ng/ml

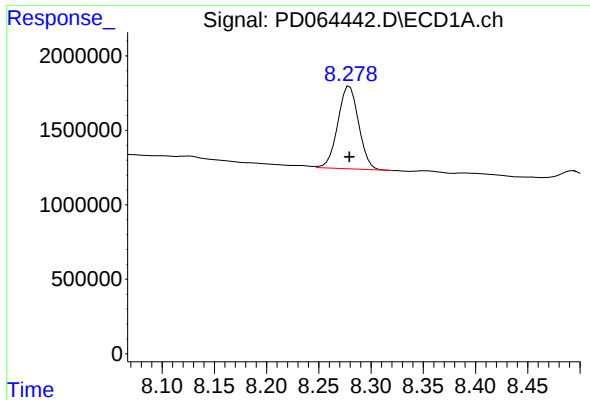

#9 Endosulfan I


R.T.: 8.279 min
Delta R.T.: 0.000 min
Response: 7450531
Conc: 5.41 ng/ml

Instrument :
ECD_D
ClientSampleId :

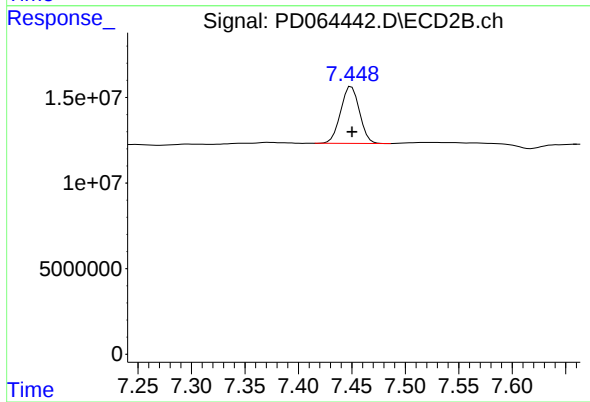


#9 Endosulfan I

R.T.: 7.450 min
Delta R.T.: 0.000 min
Response: 40795100
Conc: 5.22 ng/ml

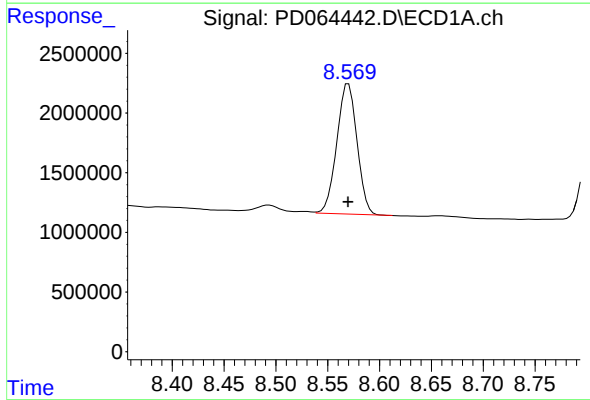


#13 Dieldrin

R.T.: 8.570 min
Delta R.T.: 0.000 min
Response: 14801465
Conc: 10.09 ng/ml

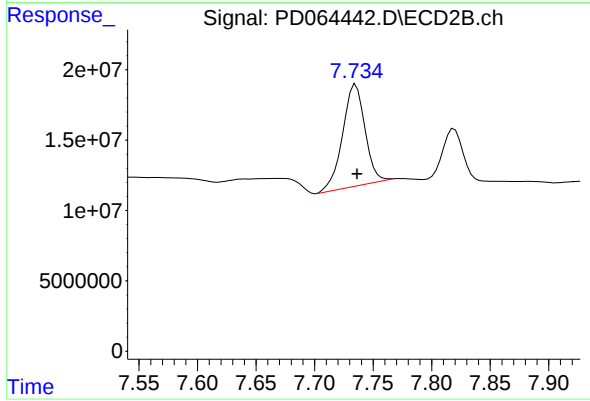

#13 Dieldrin


R.T.: 7.735 min
Delta R.T.: 0.000 min
Response: 95866191
Conc: 12.70 ng/ml

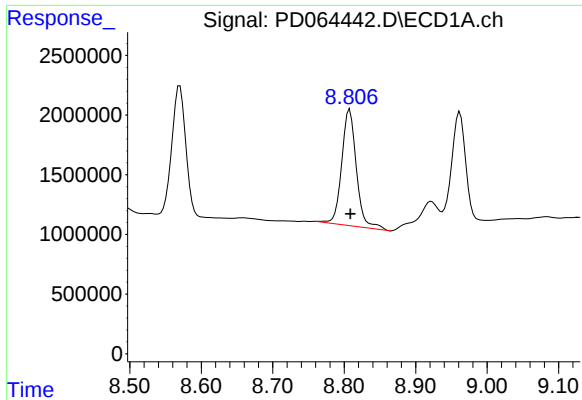

#14 Endrin


R.T.: 8.808 min
Delta R.T.: -0.001 min
Response: 13923701
Conc: 11.32 ng/ml

Instrument :
ECD_D
ClientSampleId :

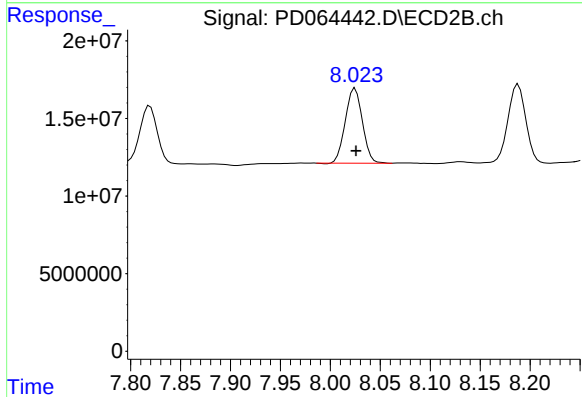


#14 Endrin

R.T.: 8.025 min
Delta R.T.: -0.001 min
Response: 57311191
Conc: 10.00 ng/ml

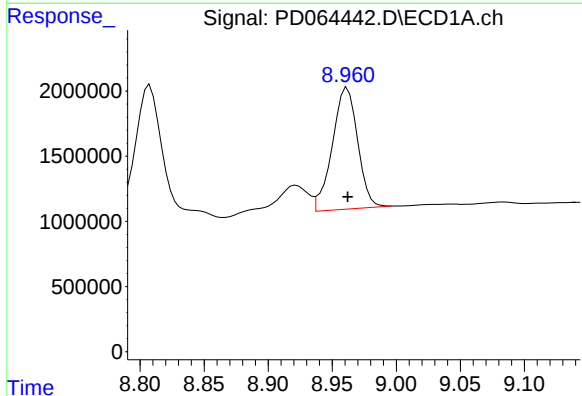


#16 4,4'-DDD

R.T.: 8.962 min
Delta R.T.: 0.000 min
Response: 12838539
Conc: 10.73 ng/ml

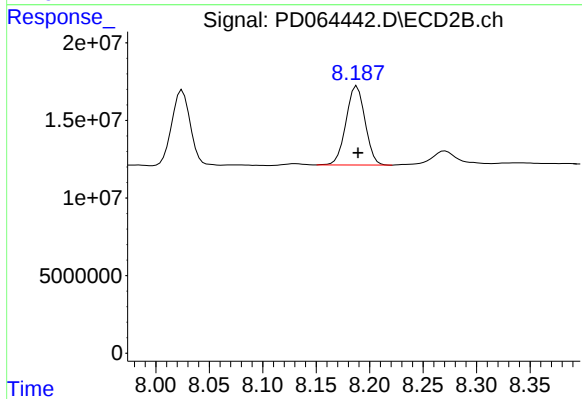

#16 4,4'-DDD


R.T.: 8.188 min
Delta R.T.: 0.000 min
Response: 63058486
Conc: 11.06 ng/ml

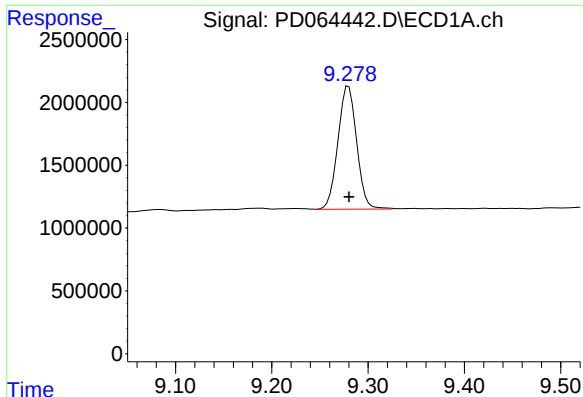

#17 4,4'-DDT


R.T.: 9.280 min
Delta R.T.: 0.000 min
Response: 13219553
Conc: 10.36 ng/ml

Instrument :
ECD_D
ClientSampleId :

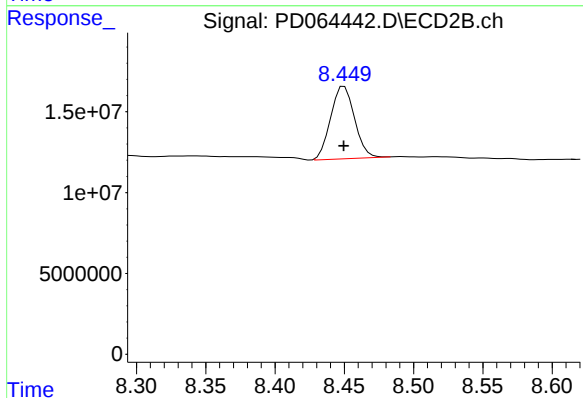


#17 4,4'-DDT

R.T.: 8.450 min
Delta R.T.: 0.000 min
Response: 53657936
Conc: 9.82 ng/ml

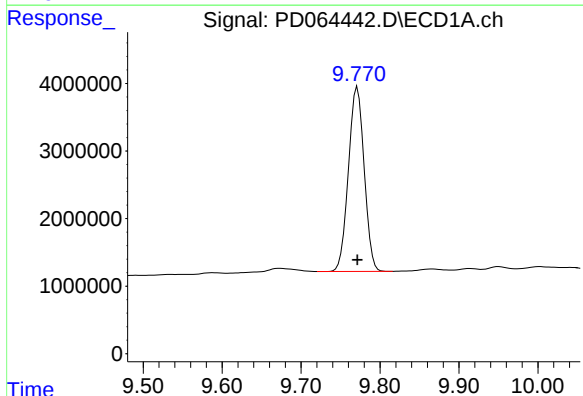


#20 Methoxychlor

R.T.: 9.771 min
Delta R.T.: 0.000 min
Response: 37878634
Conc: 53.77 ng/ml

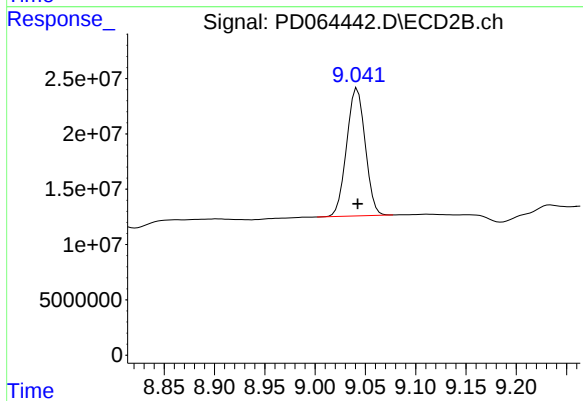

#20 Methoxychlor

R.T.: 9.042 min
Delta R.T.: 0.000 min
Response: 148001344
Conc: 58.68 ng/ml

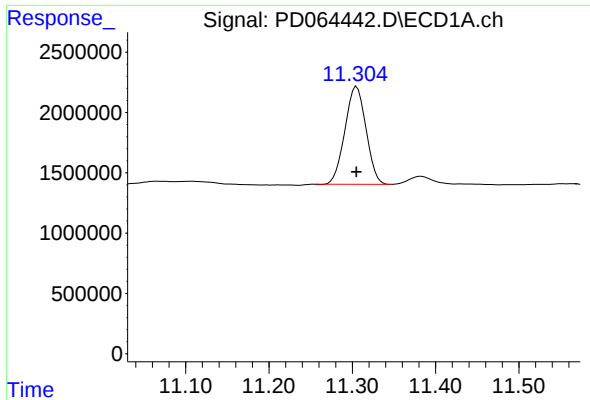

#27 Decachlorobiphenyl


R.T.: 11.305 min

Delta R.T.: 0.000 min

Response: 14278337

Conc: 10.90 ng/ml

Instrument :
ECD_D
ClientSampleId :

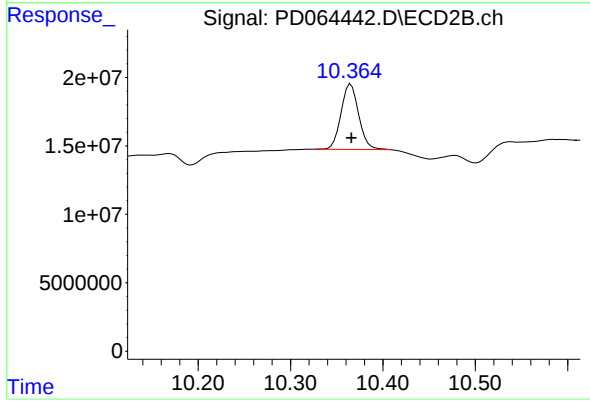

#27 Decachlorobiphenyl

R.T.: 10.365 min

Delta R.T.: 0.000 min

Response: 63541607

Conc: 10.61 ng/ml