

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072721\
 Data File : PD064444.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jul 2021 01:14
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 28 02:11:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 28 02:11:09 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	5.405	4.619	12377433	97254487	10.612	10.705
27)	SA Decachlor...	11.304	10.365	27957873	125.8E6	21.343	21.013
Target Compounds							
2)	A alpha-BHC	5.988	5.322	16061521	130.5E6	10.075	10.777
3)	MA gamma-BHC...	6.385	5.742	15636683	122.2E6	10.048	11.133
4)	MA Heptachlor	7.035	6.152	17296734	124.3E6	10.469	10.933
9)	A Endosulfan I	8.279	7.449	14612398	80813545	10.608	10.333
13)	MA Dieldrin	8.570	7.735	29726248	176.1E6	20.260	23.324
14)	MA Endrin	8.808	8.026	27498219	129.7E6	22.353	22.622
16)	A 4,4'-DDD	8.962	8.188	25092988	121.2E6	20.981	21.252
17)	MA 4,4'-DDT	9.279	8.449	26206757	119.3E6	20.533	21.842
20)	A Methoxychlor	9.771	9.041	73011859	279.2E6	103.634	110.687

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072721\
Data File : PD064444.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jul 2021 01:14
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 02:11:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 28 02:11:09 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

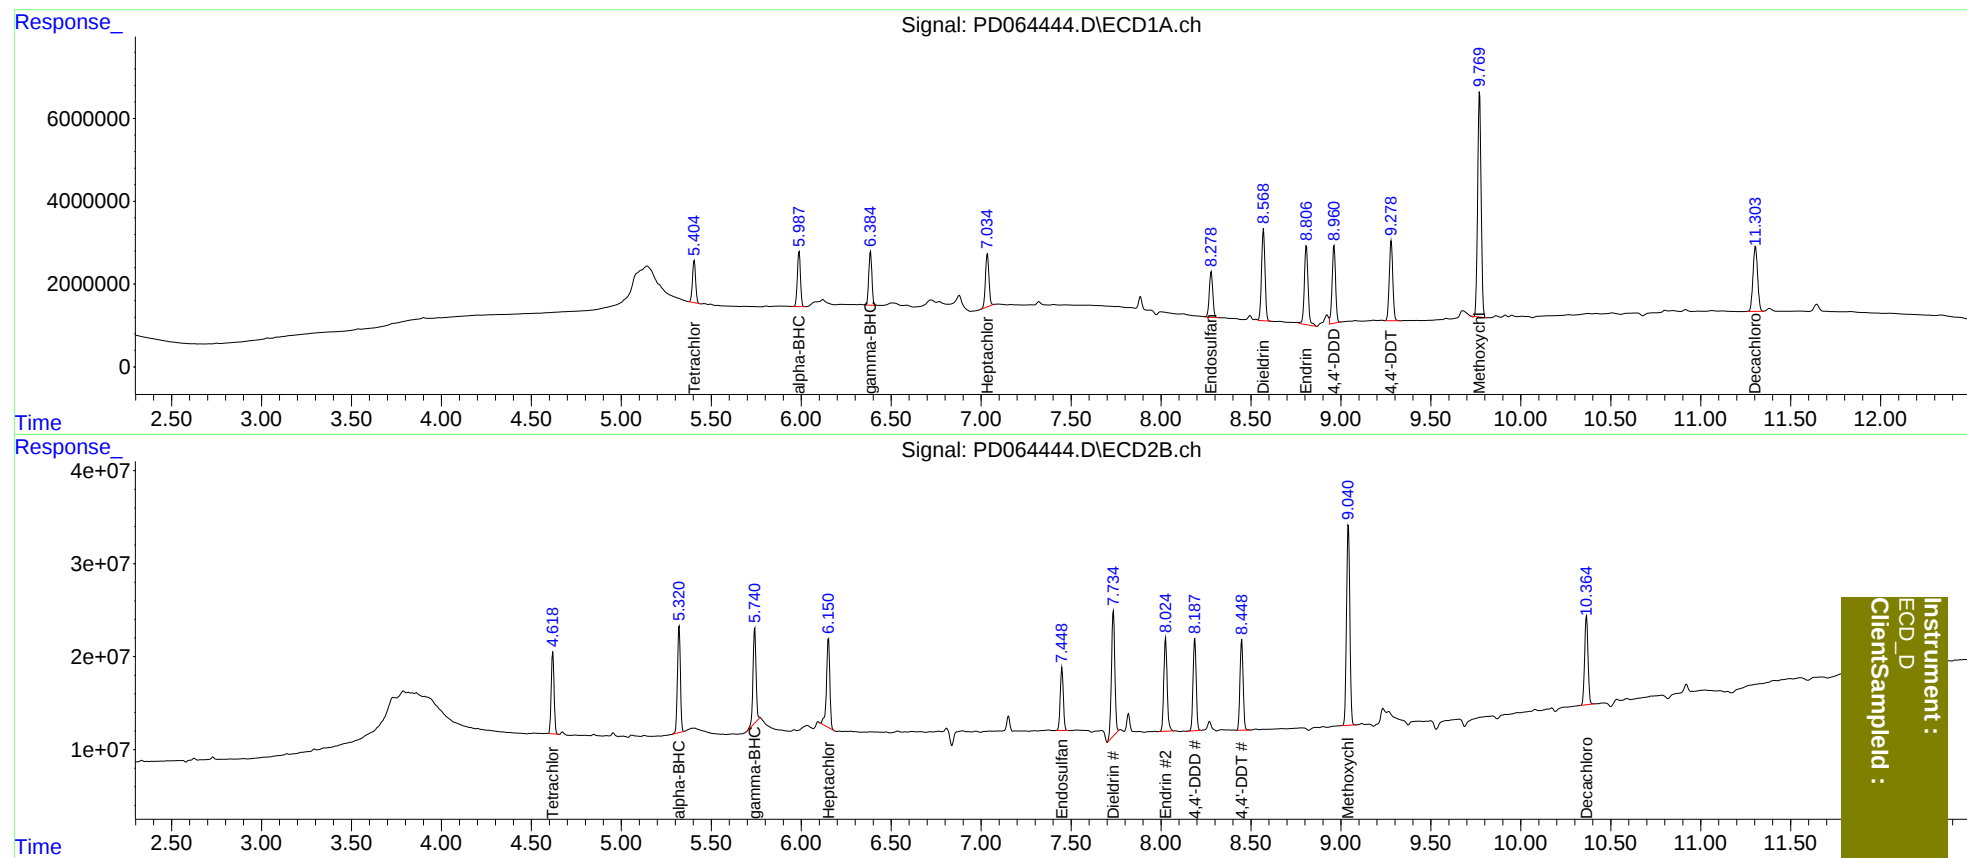


Instrument :
ECD_D
ClientSampled :

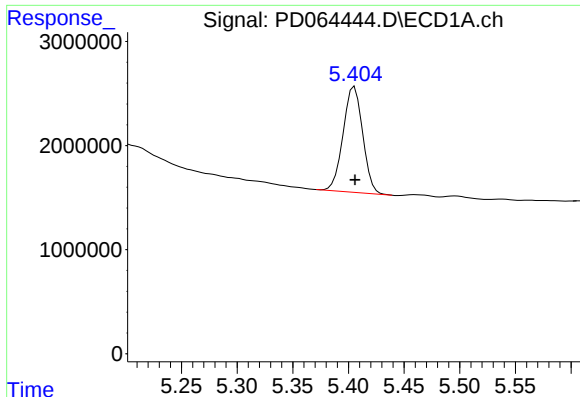

#1 Tetrachloro-m-xylene


R.T.: 5.405 min
Delta R.T.: 0.000 min
Response: 12377433
Conc: 10.61 ng/ml

Instrument :
ECD_D
ClientSampleId :

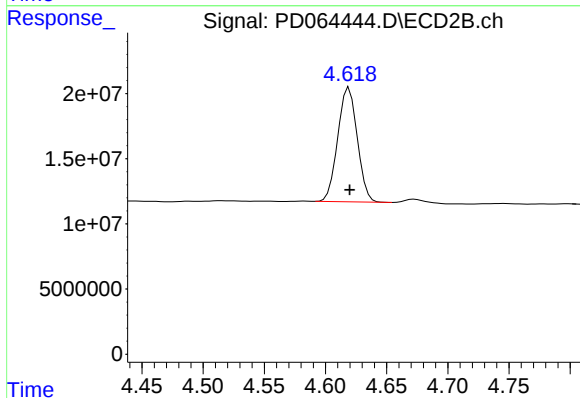


#1 Tetrachloro-m-xylene

R.T.: 4.619 min
Delta R.T.: 0.000 min
Response: 97254487
Conc: 10.71 ng/ml

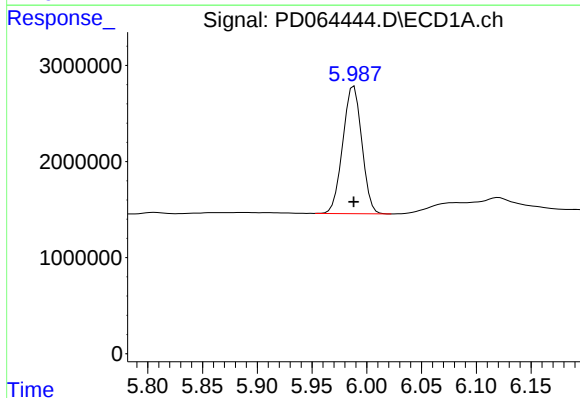


#2 alpha-BHC

R.T.: 5.988 min
Delta R.T.: 0.000 min
Response: 16061521
Conc: 10.07 ng/ml

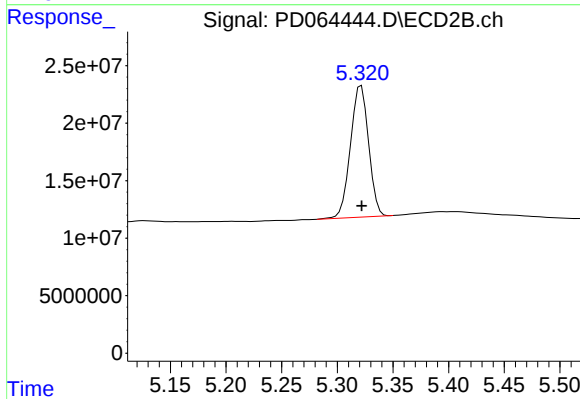

#2 alpha-BHC


R.T.: 5.322 min
Delta R.T.: 0.000 min
Response: 130533526
Conc: 10.78 ng/ml

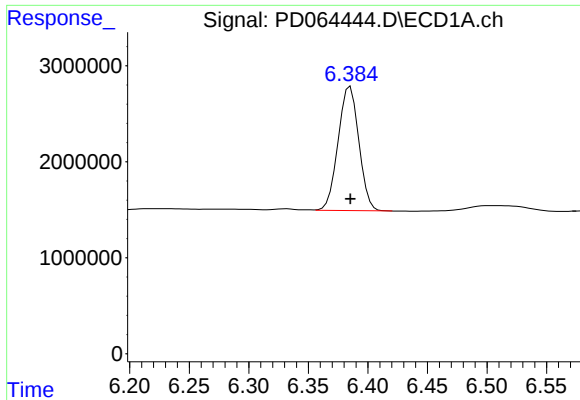

#3 gamma-BHC (Lindane)


R.T.: 6.385 min
Delta R.T.: 0.000 min
Response: 15636683
Conc: 10.05 ng/ml

Instrument :
ECD_D
ClientSampleId :

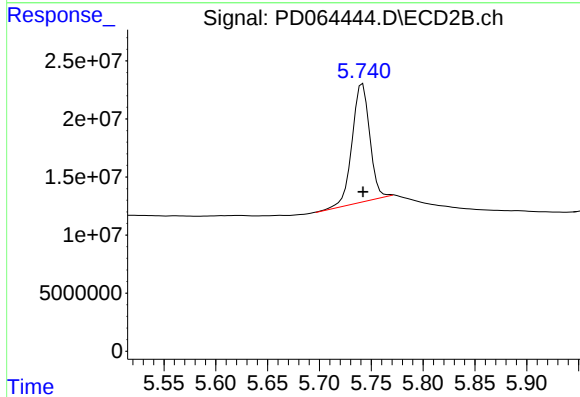


#3 gamma-BHC (Lindane)

R.T.: 5.742 min
Delta R.T.: 0.000 min
Response: 122182758
Conc: 11.13 ng/ml

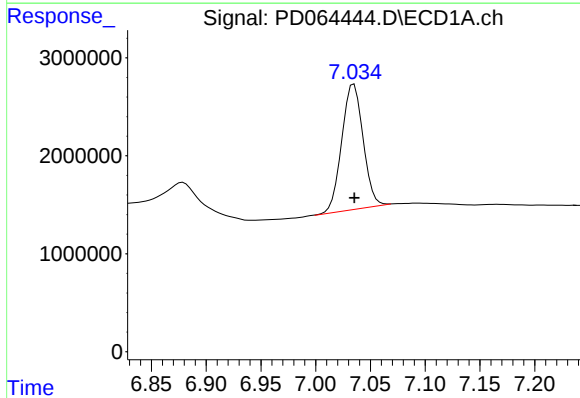


#4 Heptachlor

R.T.: 7.035 min
Delta R.T.: 0.000 min
Response: 17296734
Conc: 10.47 ng/ml

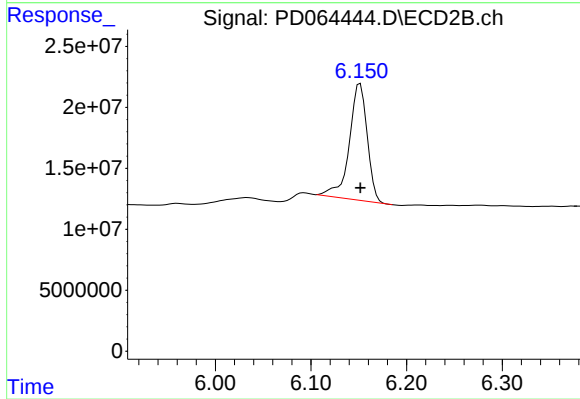

#4 Heptachlor


R.T.: 6.152 min
Delta R.T.: 0.000 min
Response: 124252079
Conc: 10.93 ng/ml

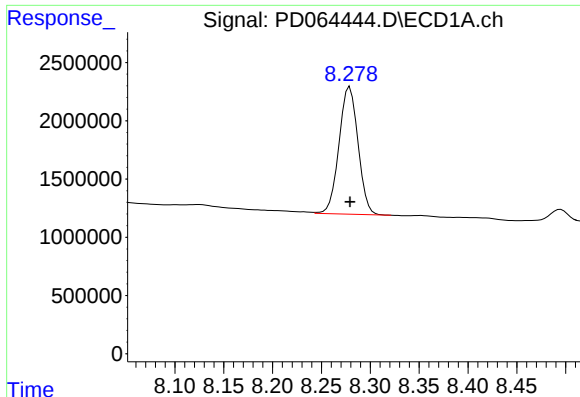

#9 Endosulfan I


R.T.: 8.279 min
Delta R.T.: 0.000 min
Response: 14612398
Conc: 10.61 ng/ml

Instrument :
ECD_D
ClientSampleId :

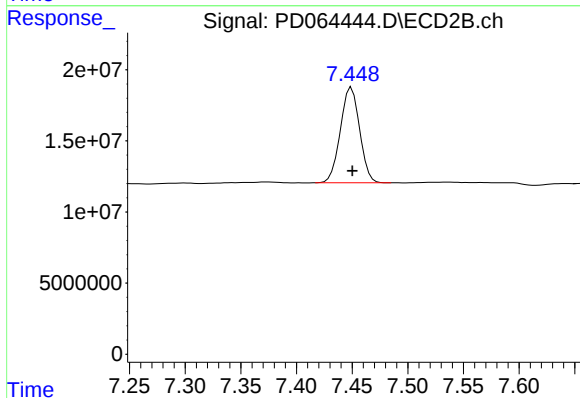


#9 Endosulfan I

R.T.: 7.449 min
Delta R.T.: 0.000 min
Response: 80813545
Conc: 10.33 ng/ml

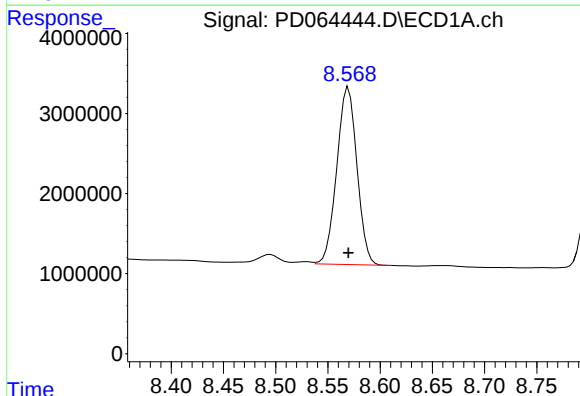


#13 Dieldrin

R.T.: 8.570 min
Delta R.T.: 0.000 min
Response: 29726248
Conc: 20.26 ng/ml

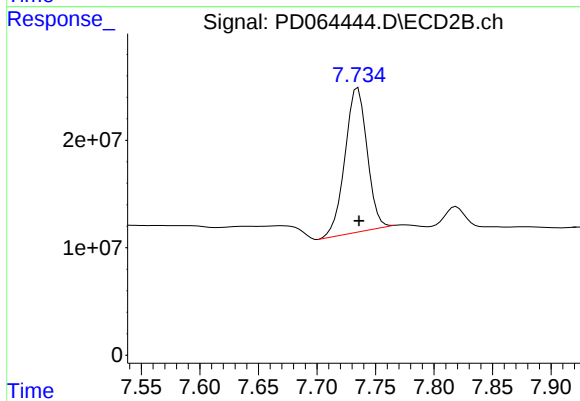

#13 Dieldrin


R.T.: 7.735 min
Delta R.T.: -0.001 min
Response: 176110900
Conc: 23.32 ng/ml

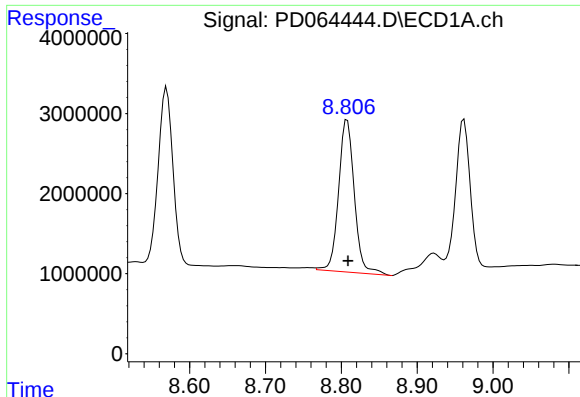

#14 Endrin


R.T.: 8.808 min
Delta R.T.: -0.001 min
Response: 27498219
Conc: 22.35 ng/ml

Instrument :
ECD_D
ClientSampleId :

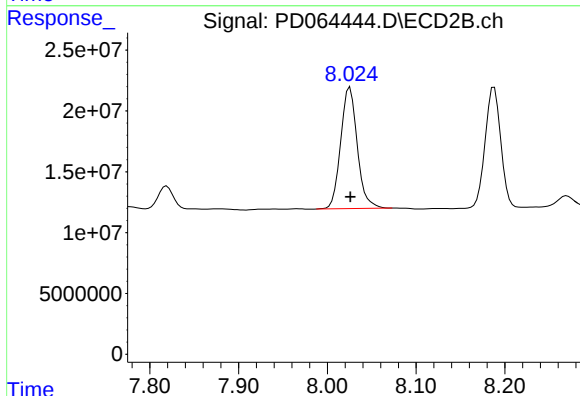


#14 Endrin

R.T.: 8.026 min
Delta R.T.: 0.000 min
Response: 129658624
Conc: 22.62 ng/ml

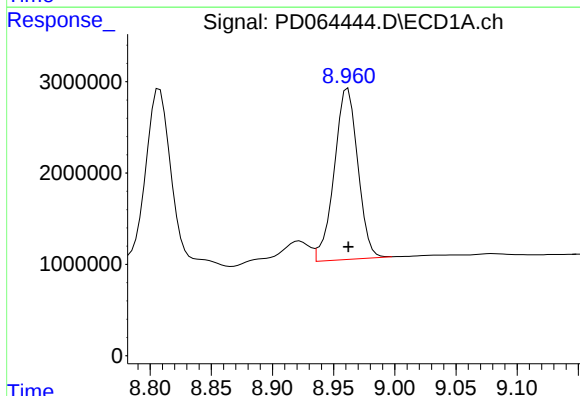


#16 4,4'-DDD

R.T.: 8.962 min
Delta R.T.: 0.000 min
Response: 25092988
Conc: 20.98 ng/ml

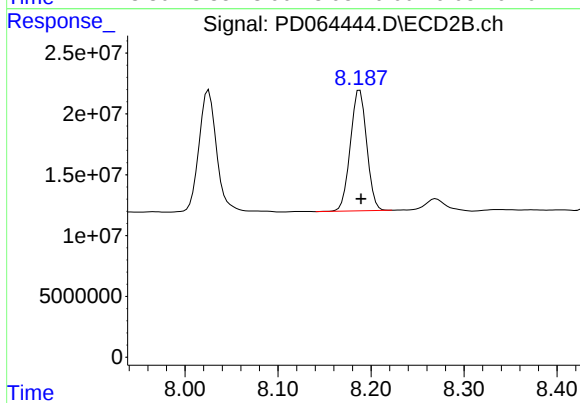

#16 4,4'-DDD


R.T.: 8.188 min
Delta R.T.: -0.001 min
Response: 121191601
Conc: 21.25 ng/ml

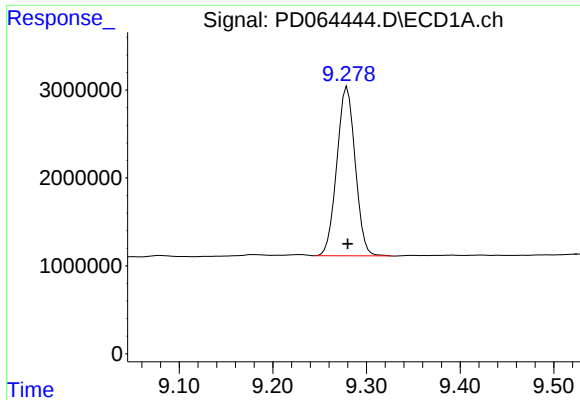

#17 4,4'-DDT


R.T.: 9.279 min
Delta R.T.: 0.000 min
Response: 26206757
Conc: 20.53 ng/ml

Instrument :
ECD_D
ClientSampleId :

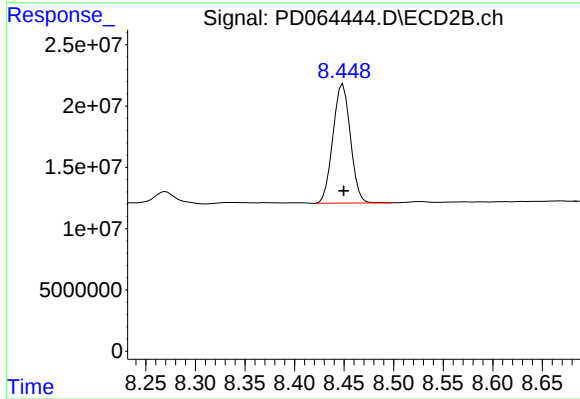


#17 4,4'-DDT

R.T.: 8.449 min
Delta R.T.: 0.000 min
Response: 119326739
Conc: 21.84 ng/ml

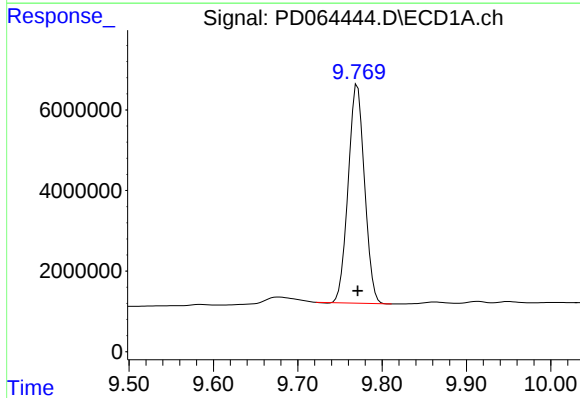


#20 Methoxychlor

R.T.: 9.771 min
Delta R.T.: 0.000 min
Response: 73011859
Conc: 103.63 ng/ml

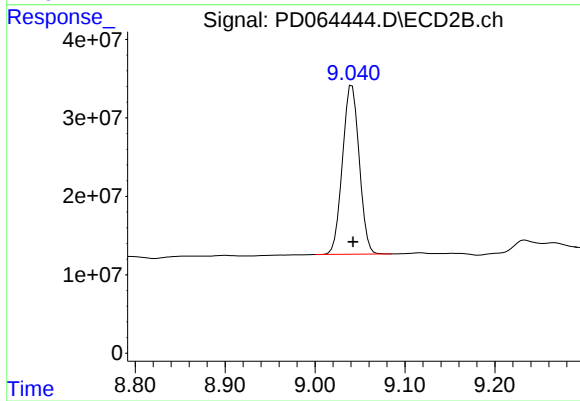

#20 Methoxychlor


R.T.: 9.041 min
Delta R.T.: -0.001 min
Response: 279151731
Conc: 110.69 ng/ml

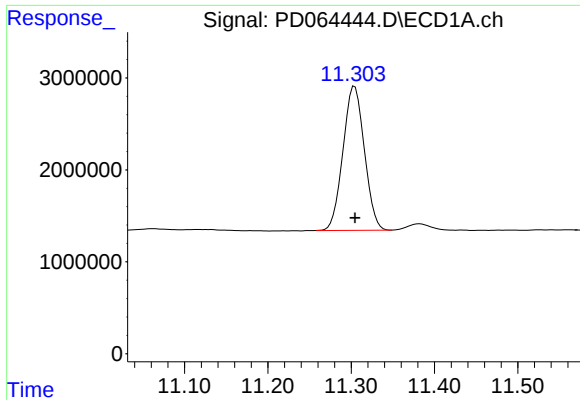

#27 Decachlorobiphenyl

R.T.: 11.304 min
Delta R.T.: 0.000 min
Response: 27957873
Conc: 21.34 ng/ml

Instrument :
ECD_D
ClientSampleId :

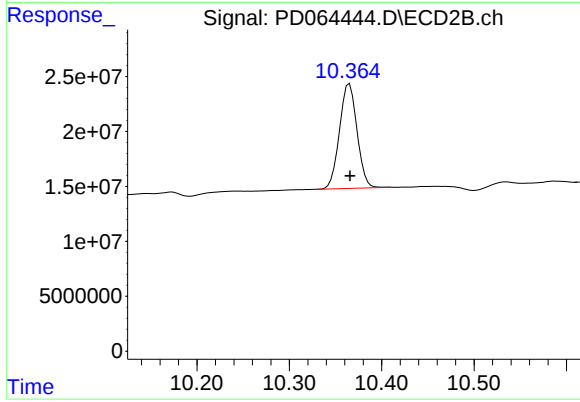

#27 Decachlorobiphenyl

R.T.: 10.365 min
Delta R.T.: 0.000 min
Response: 125821942
Conc: 21.01 ng/ml