

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072721\
 Data File : PD064448.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jul 2021 02:18
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 28 02:53:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 28 02:11:09 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	5.405	4.620	45599137	343.4E6	39.095	37.794
27)	SA Decachlor...	11.305	10.365	99274338	453.4E6	75.784	75.719
Target Compounds							
2)	A alpha-BHC	5.988	5.322	65042743	465.3E6	40.798	38.419
3)	MA gamma-BHC...	6.385	5.742	61890798	417.5E6	39.769	38.045
4)	MA Heptachlor	7.035	6.152	64189493	429.7E6	38.852	37.810
9)	A Endosulfan I	8.280	7.450	53937219	293.9E6	39.155	37.578
13)	MA Dieldrin	8.570	7.736	118.1E6	571.4E6	80.520	75.677
14)	MA Endrin	8.808	8.026	98847288	434.5E6	80.351	75.805
16)	A 4,4'-DDD	8.962	8.189	95740929	433.1E6	80.050	75.946
17)	MA 4,4'-DDT	9.280	8.449	102.5E6	426.9E6	80.348	78.146
20)	A Methoxychlor	9.771	9.042	276.9E6	932.0E6	392.977	369.535


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072721\
Data File : PD064448.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jul 2021 02:18
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 02:53:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 28 02:11:09 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

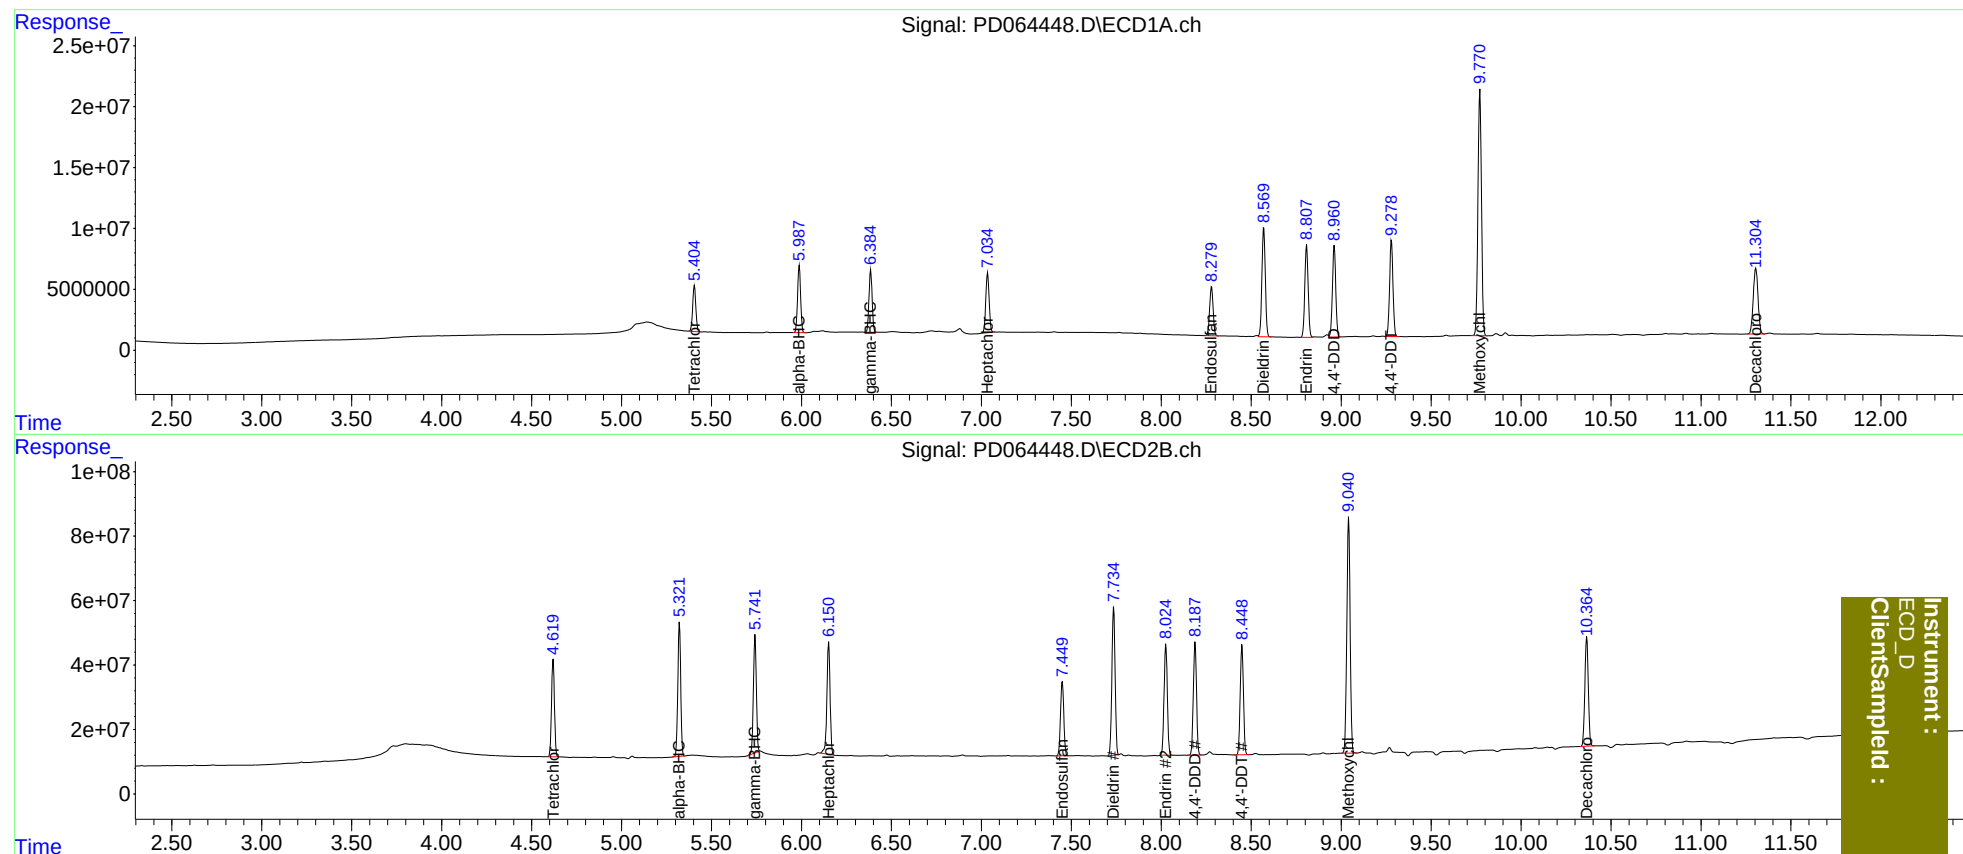


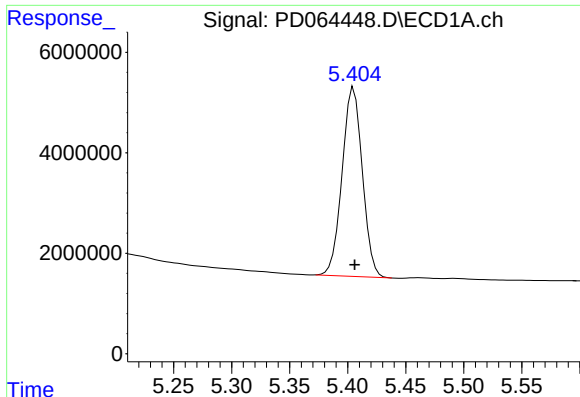

#1 Tetrachloro-m-xylene


R.T.: 5.405 min
Delta R.T.: 0.000 min
Response: 45599137
Conc: 39.09 ng/ml

Instrument :
ECD_D
ClientSampleId :

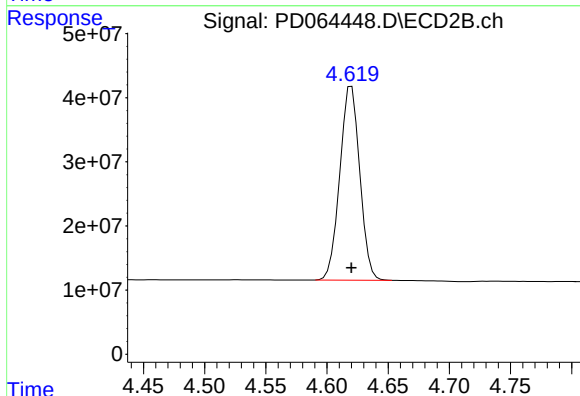


#1 Tetrachloro-m-xylene

R.T.: 4.620 min
Delta R.T.: 0.000 min
Response: 343352700
Conc: 37.79 ng/ml

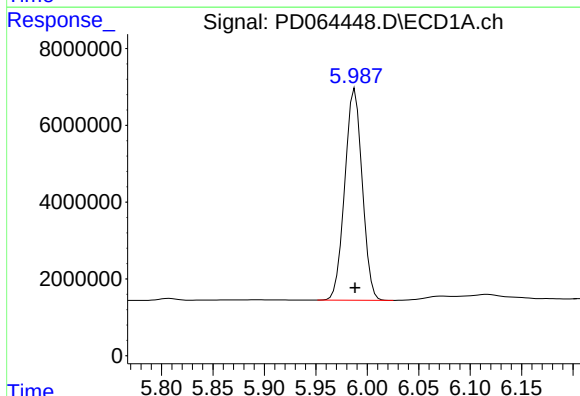


#2 alpha-BHC

R.T.: 5.988 min
Delta R.T.: 0.000 min
Response: 65042743
Conc: 40.80 ng/ml

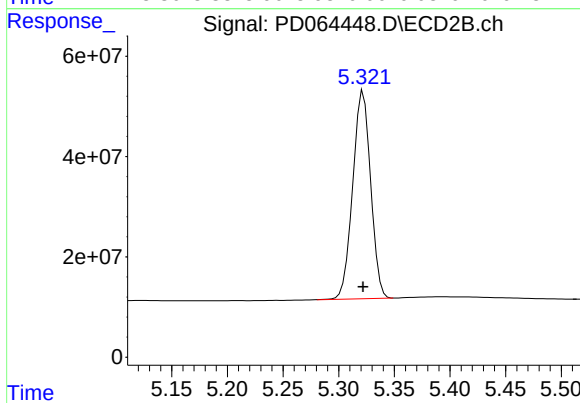

#2 alpha-BHC


R.T.: 5.322 min
Delta R.T.: 0.000 min
Response: 465327738
Conc: 38.42 ng/ml

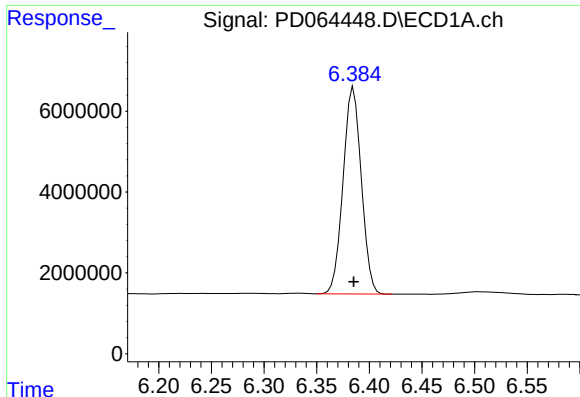

#3 gamma-BHC (Lindane)


R.T.: 6.385 min
Delta R.T.: 0.000 min
Response: 61890798
Conc: 39.77 ng/ml

Instrument :
ECD_D
ClientSampleId :

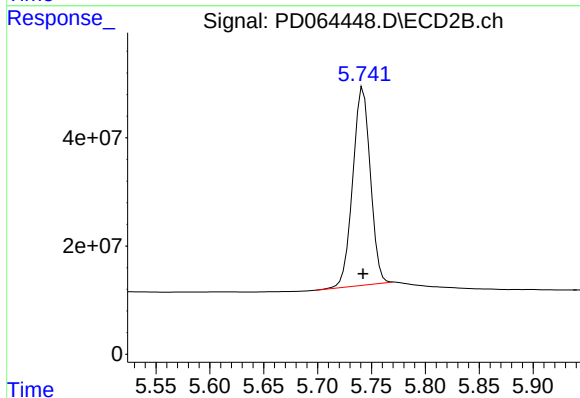


#3 gamma-BHC (Lindane)

R.T.: 5.742 min
Delta R.T.: 0.000 min
Response: 417521062
Conc: 38.04 ng/ml

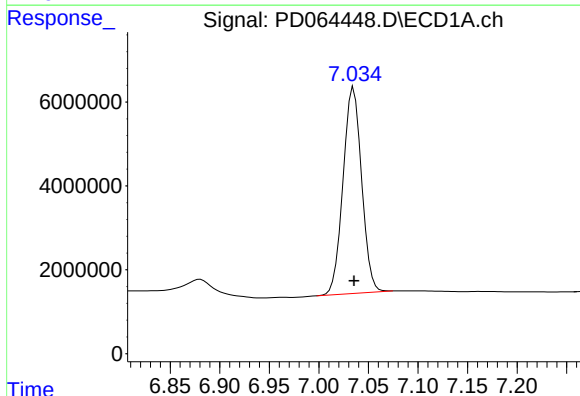


#4 Heptachlor

R.T.: 7.035 min
Delta R.T.: 0.000 min
Response: 64189493
Conc: 38.85 ng/ml

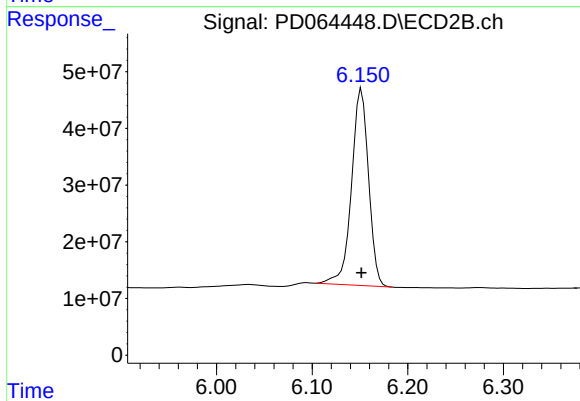

#4 Heptachlor


R.T.: 6.152 min
Delta R.T.: 0.000 min
Response: 429702662
Conc: 37.81 ng/ml

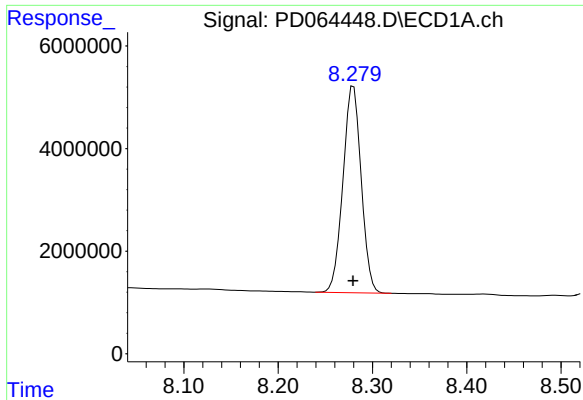

#9 Endosulfan I


R.T.: 8.280 min
Delta R.T.: 0.000 min
Response: 53937219
Conc: 39.15 ng/ml

Instrument :
ECD_D
ClientSampleId :

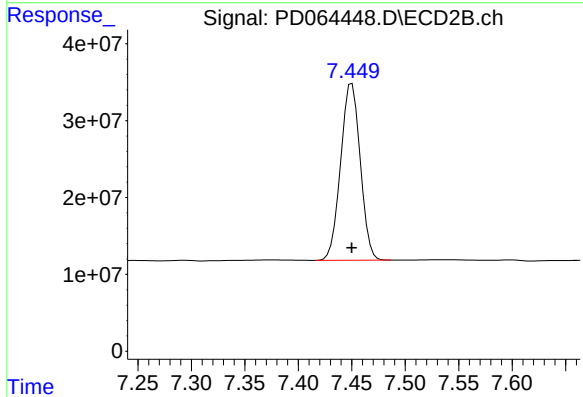


#9 Endosulfan I

R.T.: 7.450 min
Delta R.T.: 0.000 min
Response: 293894806
Conc: 37.58 ng/ml

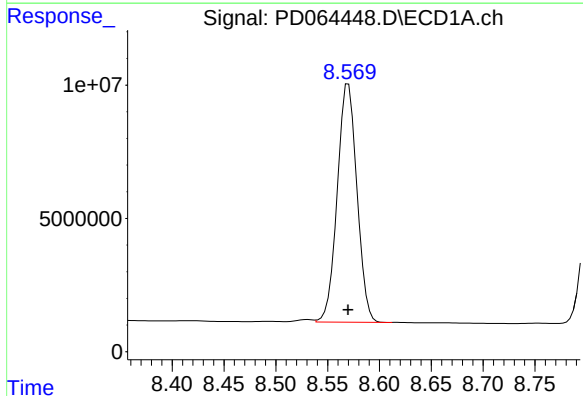


#13 Dieldrin

R.T.: 8.570 min
Delta R.T.: 0.000 min
Response: 118143695
Conc: 80.52 ng/ml

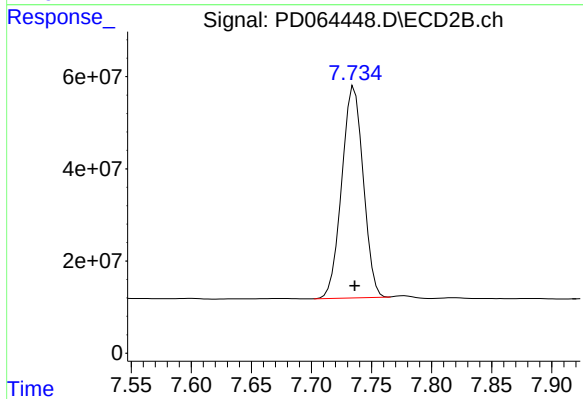

#13 Dieldrin


R.T.: 7.736 min
Delta R.T.: 0.000 min
Response: 571414653
Conc: 75.68 ng/ml

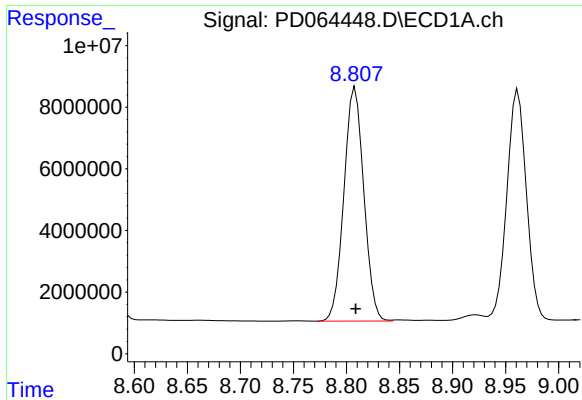

#14 Endrin


R.T.: 8.808 min
Delta R.T.: 0.000 min
Response: 98847288
Conc: 80.35 ng/ml

Instrument :
ECD_D
ClientSampleId :

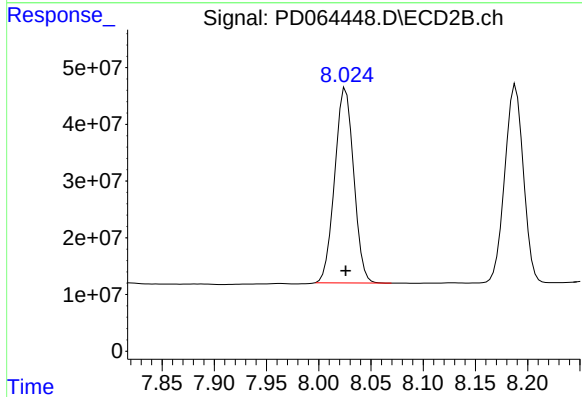


#14 Endrin

R.T.: 8.026 min
Delta R.T.: 0.000 min
Response: 434476607
Conc: 75.81 ng/ml

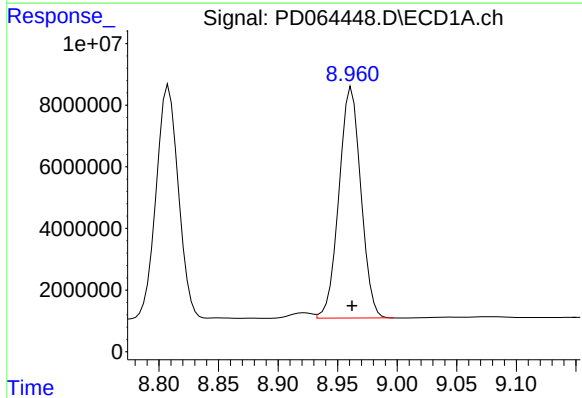


#16 4,4'-DDD

R.T.: 8.962 min
Delta R.T.: 0.000 min
Response: 95740929
Conc: 80.05 ng/ml

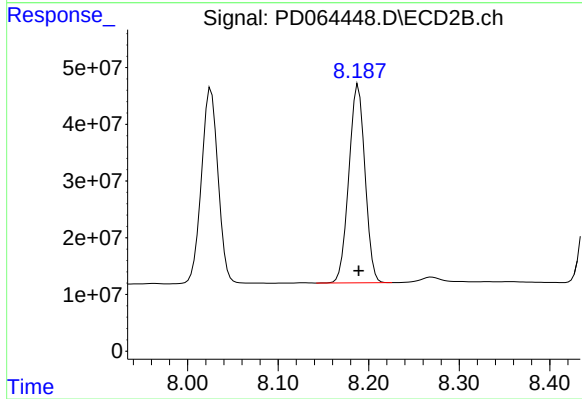

#16 4,4'-DDD


R.T.: 8.189 min
Delta R.T.: 0.000 min
Response: 433090929
Conc: 75.95 ng/ml

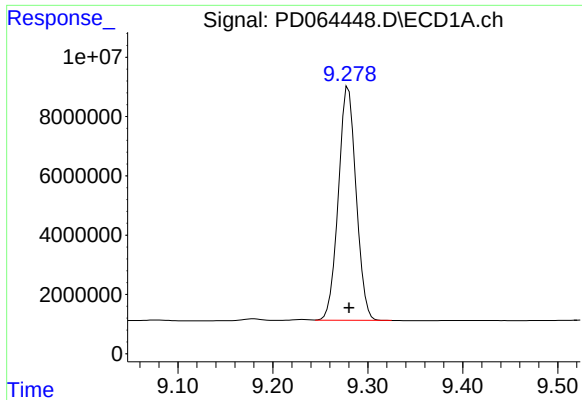

#17 4,4'-DDT


R.T.: 9.280 min
Delta R.T.: 0.000 min
Response: 102548523
Conc: 80.35 ng/ml

Instrument :
ECD_D
ClientSampleId :

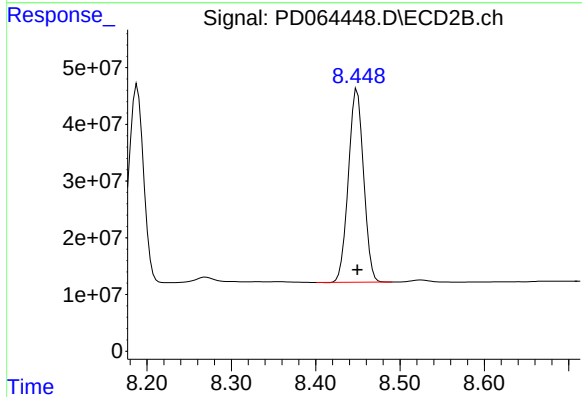


#17 4,4'-DDT

R.T.: 8.449 min
Delta R.T.: 0.000 min
Response: 426930517
Conc: 78.15 ng/ml

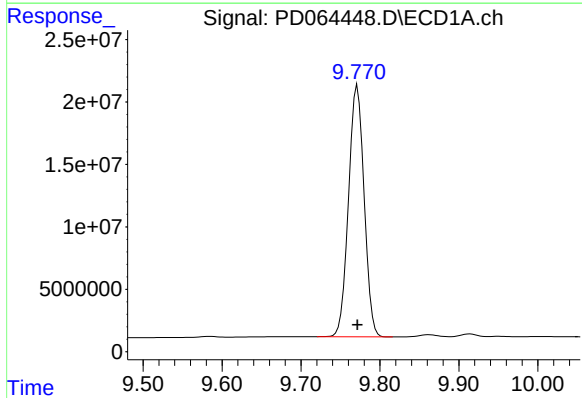


#20 Methoxychlor

R.T.: 9.771 min
Delta R.T.: 0.000 min
Response: 276858097
Conc: 392.98 ng/ml

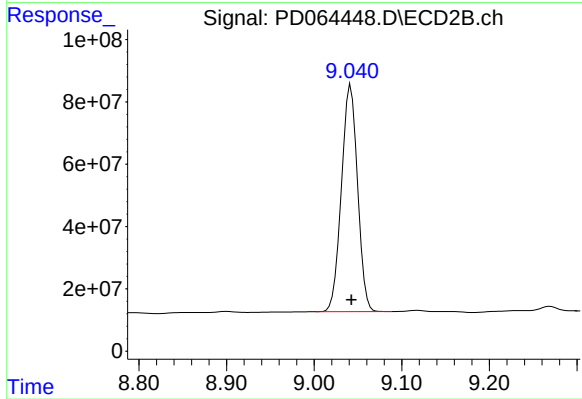

#20 Methoxychlor


R.T.: 9.042 min
Delta R.T.: 0.000 min
Response: 931963182
Conc: 369.54 ng/ml

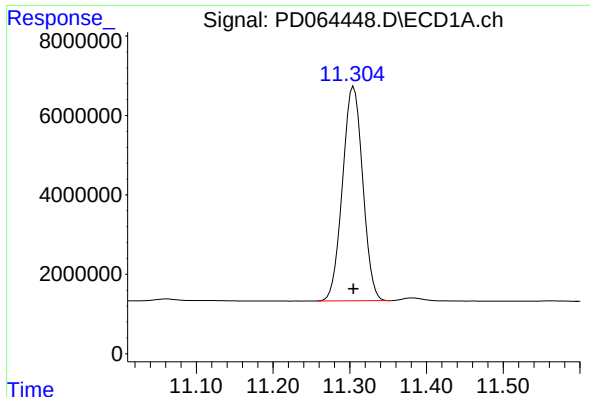

#27 Decachlorobiphenyl

R.T.: 11.305 min
Delta R.T.: 0.000 min
Response: 99274338
Conc: 75.78 ng/ml

Instrument :
ECD_D
ClientSampleId :

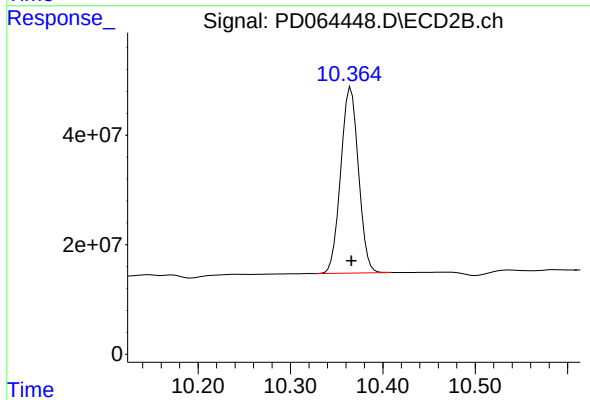

#27 Decachlorobiphenyl

R.T.: 10.365 min
Delta R.T.: 0.000 min
Response: 453400670
Conc: 75.72 ng/ml