

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072721\
 Data File : PD064471.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jul 2021 13:25
 Operator : AR\AJ
 Sample : PB137780BS
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS780

Manual Integrations
 APPROVED

mohammad
 7/29/2021 11:43:38 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 04:22:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 28 07:07:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	5.404	4.619	23139635	178.0E6	19.398	19.477
2)	SA Decachlor...	11.302	10.364	50124548	238.6E6	38.077	40.124
Target Compounds							
2)	A alpha-BHC	5.986	5.320	6431632	55173302	3.948	4.476
3)	MA gamma-BHC...	6.384	5.741	6754952	59470027	4.307	5.215
4)	MA Heptachlor	7.034	6.150	8212755	58763034	4.887	5.183
5)	MB Aldrin	7.404	6.474	7007502	50503640	4.449	4.801
6)	B beta-BHC	6.642	6.115	3742247	31336101	4.797	5.165m
7)	B delta-BHC	6.907	6.378	1264800	15229442	0.727m	1.402 #
8)	B Heptachlo...	7.874	7.047	7936203	46318380	4.623	5.004
9)	A Endosulfan I	8.277	7.448	6792769	39381726	4.819	5.121
10)	B trans-Chl...	8.143	7.323	7380192	43973357	4.606	4.848
11)	B cis-Chlor...	8.225	7.392	7332724	44770577	4.706	5.033
12)	B 4,4'-DDE	8.420	7.604	12783569	74995817	8.869	9.939
13)	MA Dieldrin	8.568	7.734	13712207	81803952	9.195	10.185
14)	MA Endrin	8.806	8.024	11278742	59639278	8.809	10.382
15)	B Endosulfa...	9.042	8.333	12682490	58097175	9.766	10.065
16)	A 4,4'-DDD	8.960	8.187	11812414	57947966	9.623	10.061
17)	MA 4,4'-DDT	9.278	8.448	11639887	52633507	8.916	9.562
18)	B Endrin al...	9.178	8.520	11626203	49450520	10.262	10.020
19)	B Endosulfa...	9.416	8.750	10803852	40509794	7.839	7.515
20)	A Methoxychlor	9.769	9.040	34243421	141.5E6	47.855	55.241
21)	B Endrin ke...	9.912	9.269	14381595	61440477	9.506	10.243

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072721\
Data File : PD064471.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jul 2021 13:25
Operator : AR\AJ
Sample : PB137780BS
Misc :
ALS Vial : 35 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 04:22:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 28 07:07:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

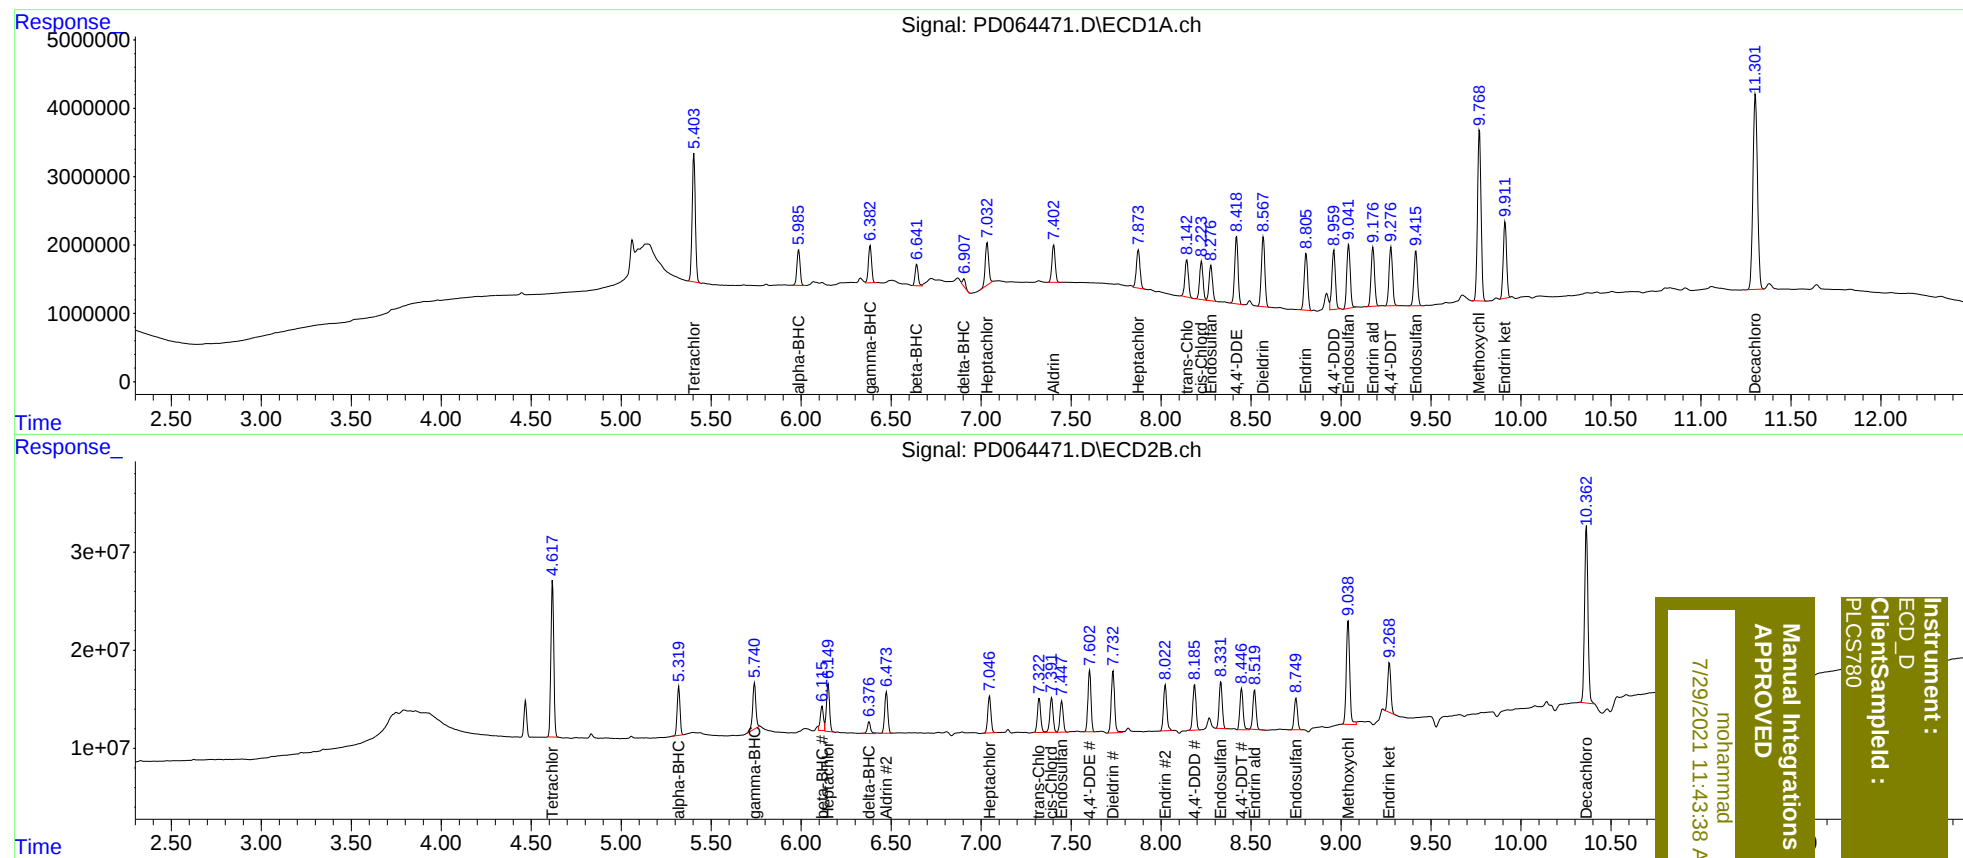

7/29/2021 11:43:38 AM
mohammad

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sample :
PLC5780