

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072721\
 Data File : PD064461.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jul 2021 09:34
 Operator : AR\AJ
 Sample : M3009-03MS
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGEE2MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 04:18:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 28 07:07:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	5.406	4.619	13969000	81273304	11.710	8.894
2)	SA Decachlor...	11.304	10.365	19683477	90241573	14.953	15.175
Target Compounds							
2)	A alpha-BHC	5.988	5.322	70861999	515.3E6	43.498	41.811
3)	MA gamma-BHC...	6.385	5.742	69652324	469.9E6	44.411	41.203
4)	MA Heptachlor	7.034	6.151	75473681	502.7E6	44.909	44.339
5)	MB Aldrin	7.405	6.475	70141766	452.7E6	44.530	43.039
6)	B beta-BHC	6.644	6.117	32783016	221.9E6	42.020	36.571
7)	B delta-BHC	6.908	6.378	22087938	155.8E6	12.693	14.341
8)	B Heptachlo...	7.874	7.048	67184123	390.5E6	39.132	42.180
9)	A Endosulfan I	8.279	7.450	62147219	338.0E6	44.087	43.952
10)	B trans-Chl...	8.145	7.324	68589474	385.0E6	42.802	42.444
11)	B cis-Chlor...	8.226	7.394	66430708	368.7E6	42.636	41.448
12)	B 4,4'-DDE	8.420	7.606	132.7E6	687.7E6	92.069	91.146
13)	MA Dieldrin	8.569	7.736	138.3E6	673.0E6	92.716	83.791
14)	MA Endrin	8.807	8.026	115.9E6	546.6E6	90.484	95.147
15)	B Endosulfa...	9.043	8.334	117.3E6	516.4E6	90.310	89.467
16)	A 4,4'-DDD	8.961	8.188	112.9E6	520.7E6	91.944	90.399
17)	MA 4,4'-DDT	9.279	8.449	118.9E6	502.9E6	91.060	91.367
18)	B Endrin al...	9.179	8.522	102.4E6	426.5E6	90.361	86.415
19)	B Endosulfa...	9.417	8.752	100.7E6	390.8E6	73.079	72.494
20)	A Methoxychlor	9.770	9.041	324.8E6	1102.8E6	453.922	430.660
21)	B Endrin ke...	9.914	9.270	140.7E6	543.0E6	93.031	90.523

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072721\
Data File : PD064461.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jul 2021 09:34
Operator : AR\AJ
Sample : M3009-03MS
Misc :
ALS Vial : 26 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 04:18:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 28 07:07:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

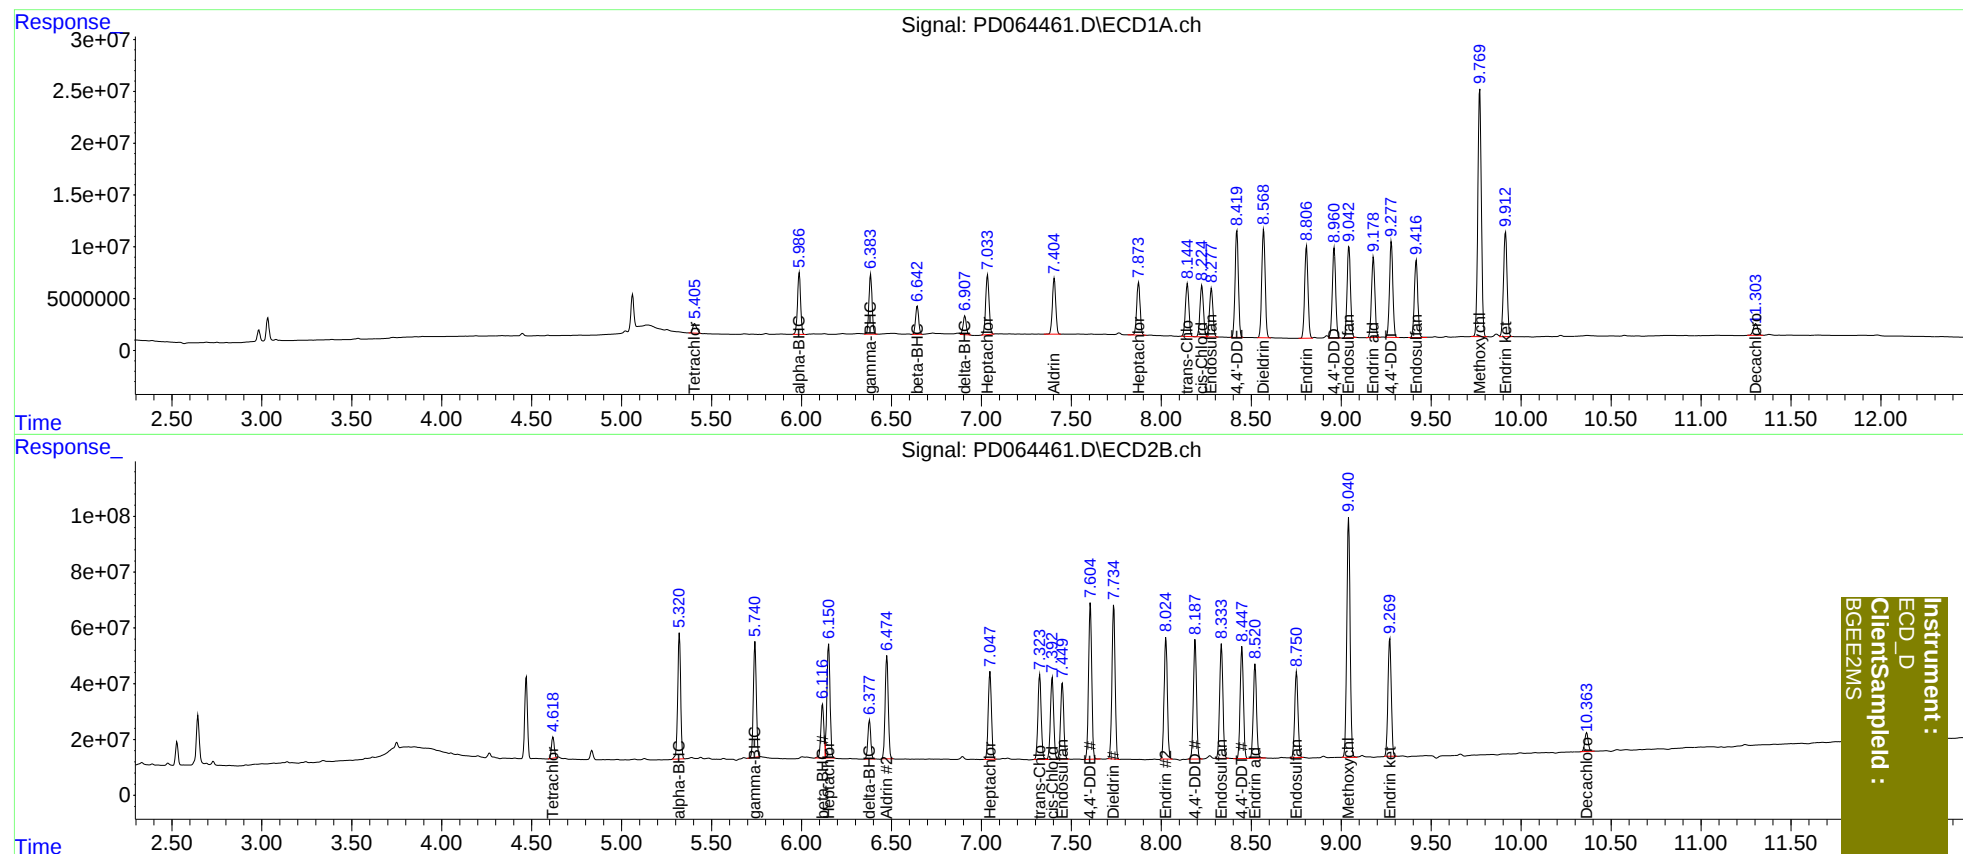

Instrument :
ECD_D
ClientSampled :
BGEE2MS