

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072722\
 Data File : PD071178.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jul 2022 13:13
 Operator : AR\AJ
 Sample : PB146420BS
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS420

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/27/2022
 Supervised By : Ankita Jodhani 07/27/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 27 03:23:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 14 05:14:58 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.473	4.124	52054030	530.7E6	21.634	22.615
27)	SA Decachlor...	8.239	9.320	74177322	244.3E6	29.217	26.448
Target Compounds							
2)	A alpha-BHC	3.913	4.529	19170564	148.8E6	5.110	4.931
3)	MA gamma-BHC...	4.197	4.823	17969056	129.5E6	4.936	5.003
4)	MA Heptachlor	4.497	5.339	16185742	84974632	4.645	4.240
5)	MB Aldrin	4.745	5.651	15976371	77940433	4.421	4.478
6)	B beta-BHC	4.448	5.000	7601270	68722897	4.852	5.139
7)	B delta-BHC	4.652	5.224	15714146	102.3E6	4.511	4.511
8)	B Heptachlo...	5.190	6.045	15771184	57781915	4.737	3.891m
9)	A Endosulfan I	5.530	6.411	14238112	51069590	4.723	3.851
10)	B trans-Chl...	5.417	6.283	13761863	54645796	3.954	3.629
11)	B cis-Chlor...	5.475	6.356	15340217	53058520	4.489	3.674
12)	B 4,4'-DDE	5.641	6.511	28581760	111.4E6	8.883	8.122
13)	MA Dieldrin	5.774	6.672	30425640	117.3E6	9.086	8.472
14)	MA Endrin	6.032	6.895	24962619	80640477	9.005	7.723
15)	B Endosulfa...	6.306	7.110	23903745	85314774	8.716	7.407
16)	A 4,4'-DDD	6.158	7.012	22852562	87157209	8.775	7.969
17)	MA 4,4'-DDT	6.400	7.312	20149156	98417522	7.531	8.794
18)	B Endrin al...	6.476	7.235	17240152	67047002	7.526	6.896
19)	B Endosulfa...	6.689	7.458	21224735	69096835	7.577	6.095m
20)	A Methoxychlor	6.950	7.772	60857266	196.3E6	44.010	37.514
21)	B Endrin ke...	7.183	7.939	25453079	101.1E6	8.211	8.185m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072722\
Data File : PD071178.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jul 2022 13:13
Operator : AR\AJ
Sample : PB146420BS
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 27 03:23:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 14 05:14:58 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

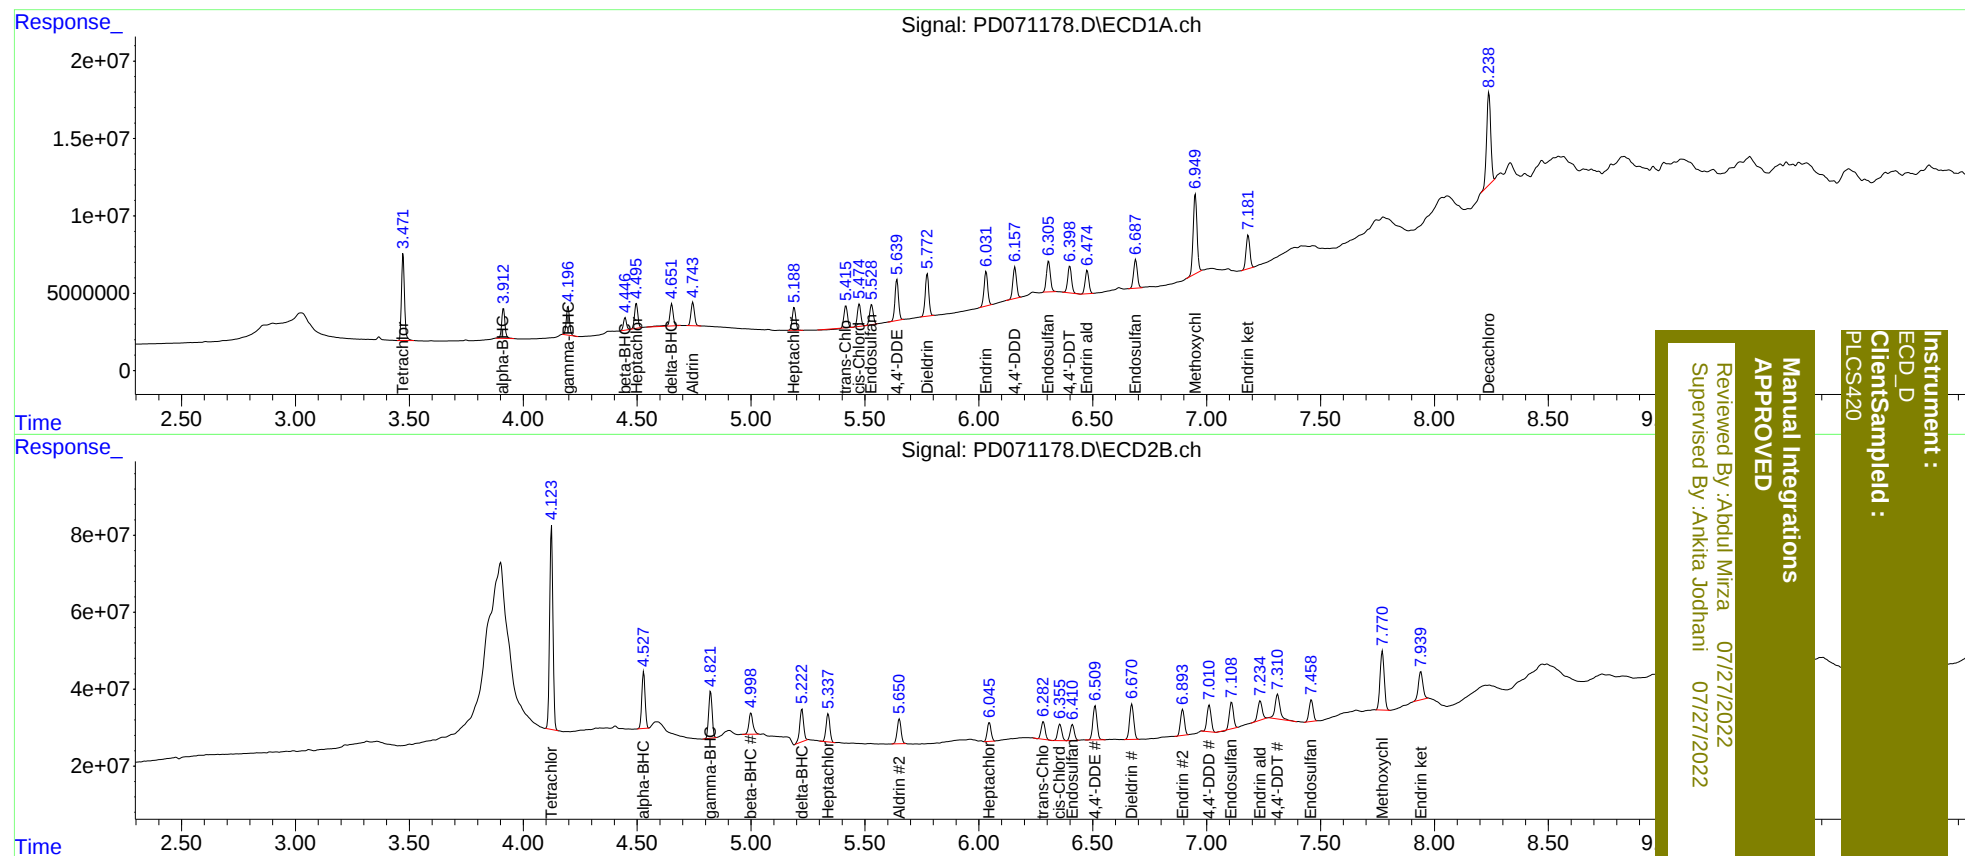

Instrument :
ECD_D
ClientSampled :
PLCS420

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 07/27/2022
Supervised By: Ankita Jodhani 07/27/2022