

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072722\
 Data File : PD071185.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jul 2022 19:09
 Operator : AR\AJ
 Sample : N3741-02MS
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 H0B12MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/27/2022
 Supervised By : Ankita Jodhani 07/27/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 27 03:26:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 14 05:14:58 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.473	4.124	33284706	358.0E6	13.833	15.253
27)	SA Decachlor...	8.240	9.319	43901667	166.8E6	17.292	18.062
Target Compounds							
2)	A alpha-BHC	3.914	4.529	186.4E6	1493.9E6	49.701	49.495
3)	MA gamma-BHC...	4.198	4.823	183.6E6	1298.6E6	50.438	50.180
4)	MA Heptachlor	4.497	5.339	181.3E6	893.3E6	52.042	44.572
5)	MB Aldrin	4.746	5.651	178.1E6	783.8E6	49.288	45.039
6)	B beta-BHC	4.448	4.999	69556605	492.9E6	44.397	36.853
7)	B delta-BHC	4.653	5.223	174.9E6	988.4E6	50.215	43.577
8)	B Heptachlo...	5.191	6.046	160.8E6	595.7E6	48.306	40.116
9)	A Endosulfan I	5.530	6.411	146.8E6	565.7E6	48.708	42.657
10)	B trans-Chl...	5.417	6.283	166.6E6	637.3E6	47.870	42.322
11)	B cis-Chlor...	5.476	6.356	164.4E6	605.1E6	48.108	41.898
12)	B 4,4'-DDE	5.642	6.512	313.6E6	1173.8E6	97.454	85.582
13)	MA Dieldrin	5.774	6.673	341.7E6	1233.5E6	102.046	89.083
14)	MA Endrin	6.033	6.896	296.7E6	1010.8E6	107.031	96.812
15)	B Endosulfa...	6.307	7.110	258.2E6	987.3E6	94.144	85.715
16)	A 4,4'-DDD	6.159	7.011	249.0E6	981.0E6	95.592	89.698
17)	MA 4,4'-DDT	6.401	7.313	260.5E6	987.6E6	97.344	88.249
18)	B Endrin al...	6.477	7.235	192.5E6	775.0E6	84.012	79.715
19)	B Endosulfa...	6.688	7.459	222.1E6	900.5E6	79.271m	79.426
20)	A Methoxychlor	6.951	7.772	667.3E6	2325.8E6	482.579	444.534
21)	B Endrin ke...	7.183	7.941	298.4E6	977.2E6	96.249	79.140

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072722\
Data File : PD071185.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jul 2022 19:09
Operator : AR\AJ
Sample : N3741-02MS
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 27 03:26:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 14 05:14:58 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

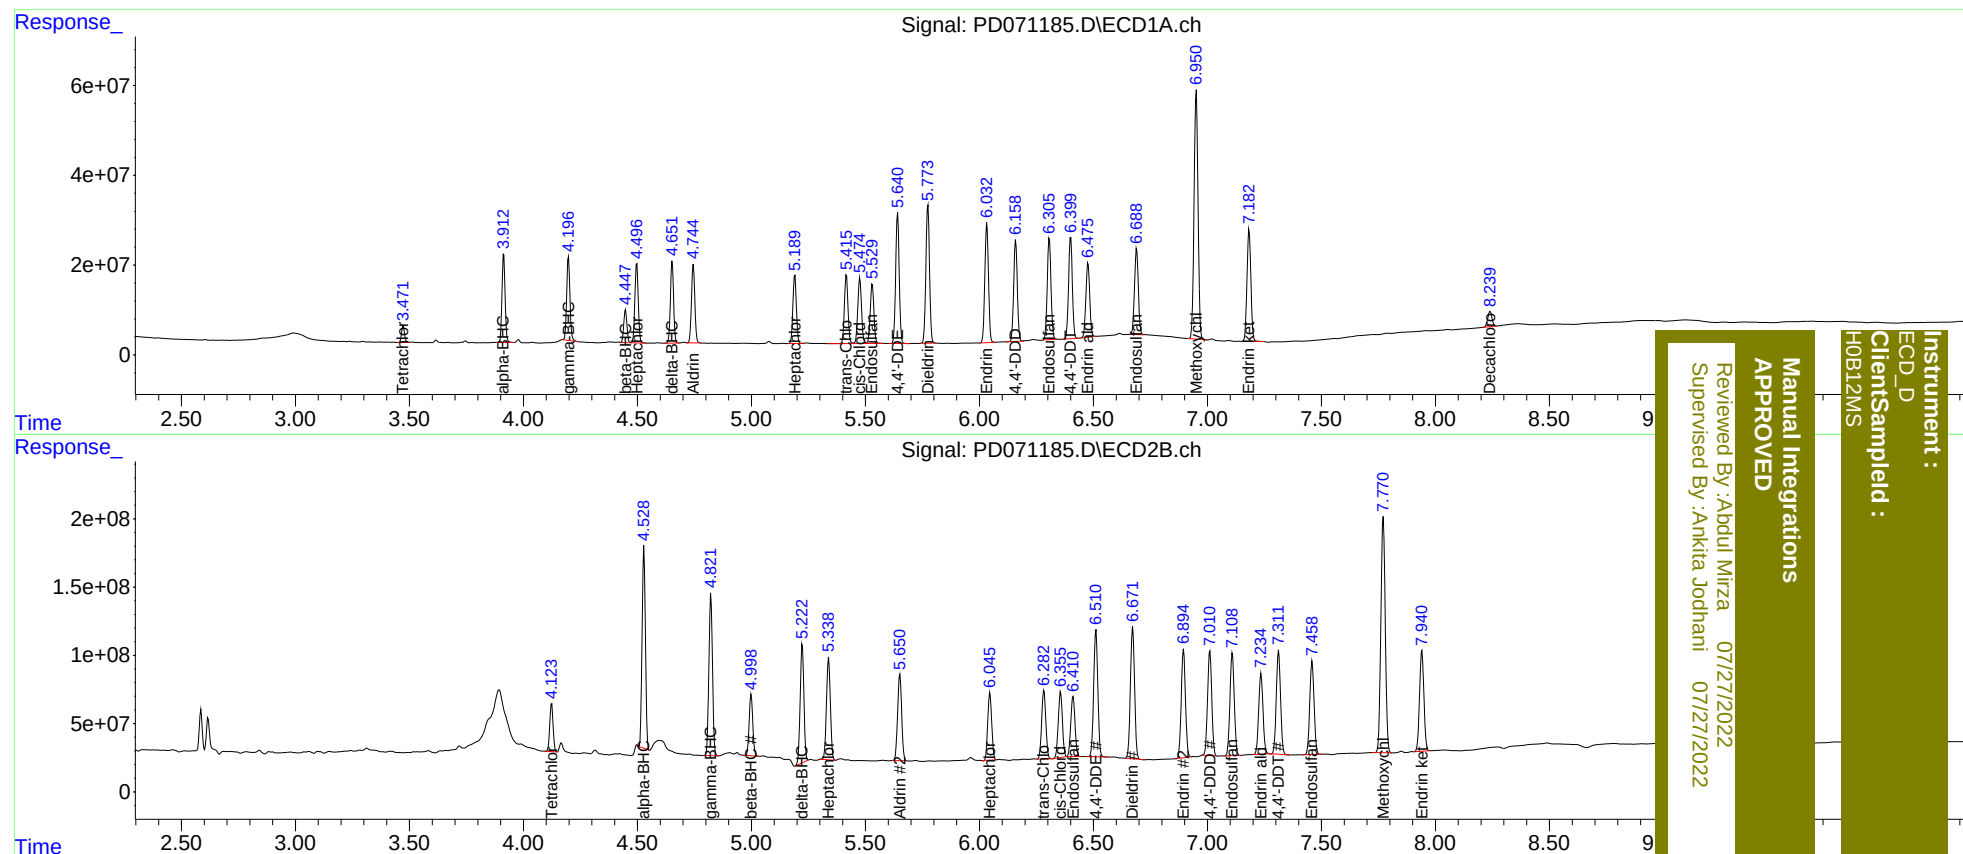

Instrument :
ECD_D
ClientSampled :
HOB12MS

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/27/2022
Supervised By :Ankita Jodhani 07/27/2022