

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072722\
 Data File : PD071191.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jul 2022 20:36
 Operator : AR\AJ
 Sample : N3741-12
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 H0B37

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/28/2022
 Supervised By :Ankita Jodhani 07/28/2022

Supervised By :Ankita
 Jodhani
 07/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 27 03:28:59 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 14 05:14:58 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.472	4.124	31799088	354.8E6	13.216	15.120
2)	SA Decachlor...	8.240	9.318	53127835	191.5E6	20.926	20.740
Target Compounds							
12)	B 4,4'-DDE	5.639	6.509	1969102	18217815	0.612m	1.328m#
16)	A 4,4'-DDD	6.157	7.013	1187030	6103744	0.456m	0.558m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072722\
Data File : PD071191.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jul 2022 20:36
Operator : AR\AJ
Sample : N3741-12
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 27 03:28:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 14 05:14:58 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

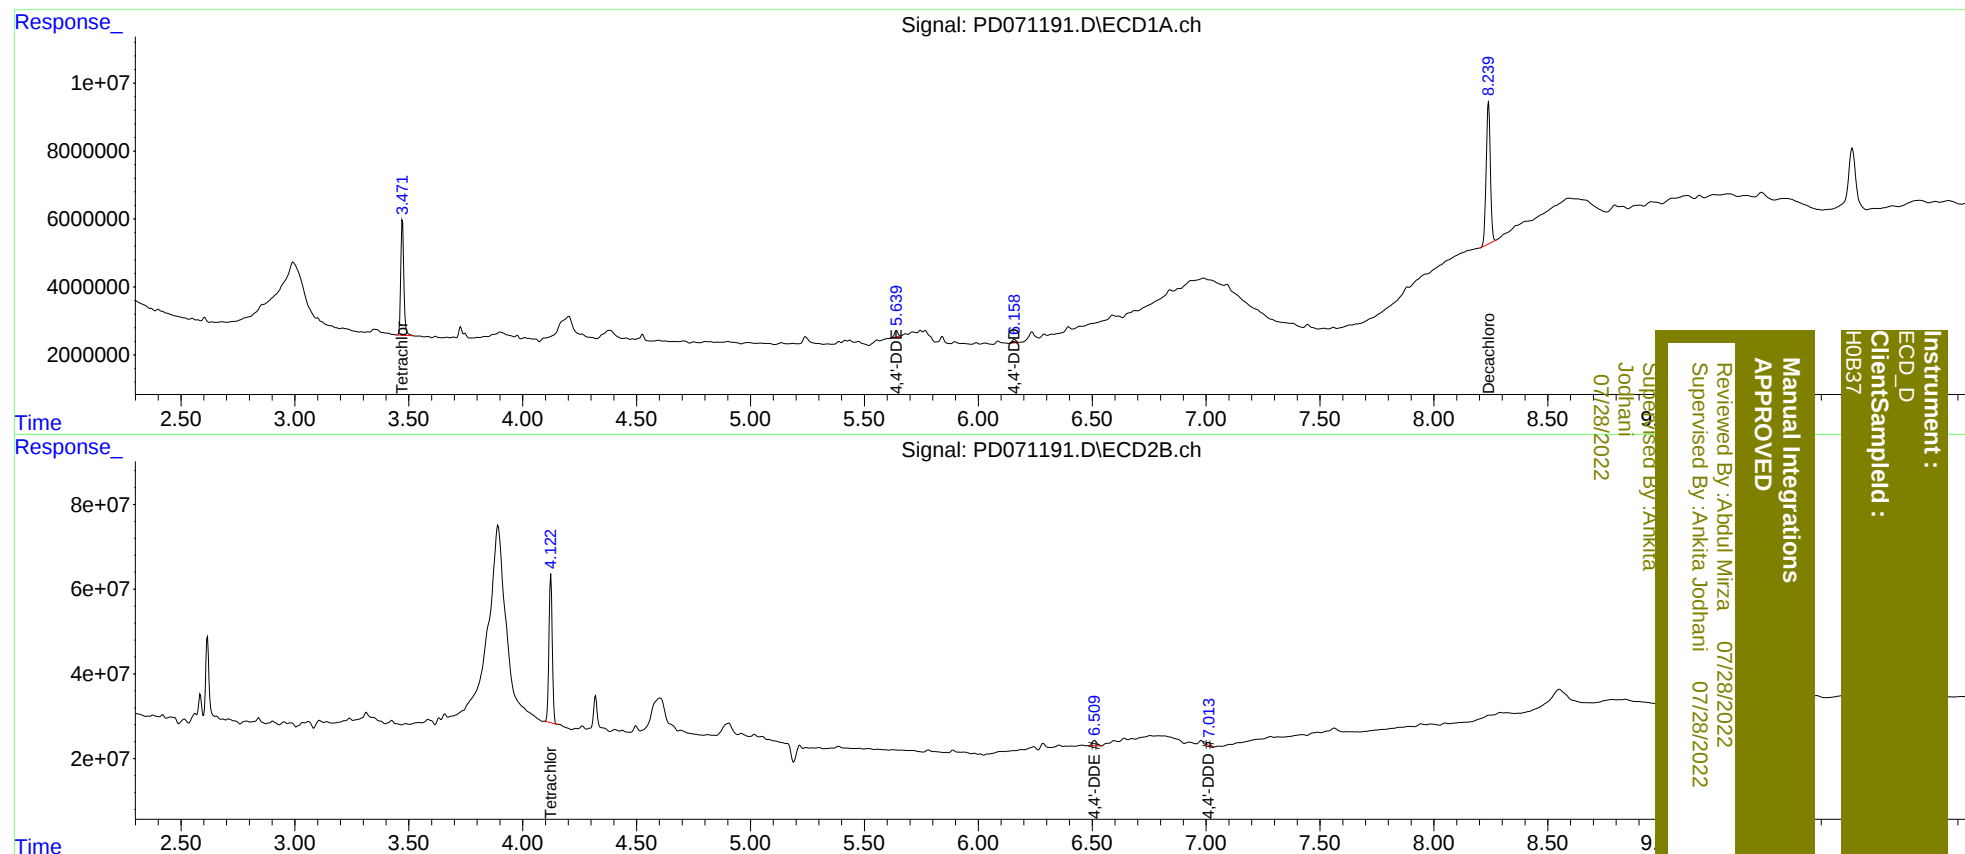

Supervised By: Ankitia
Jodhani
07/28/2022

Reviewed By: Abdul Mirza 07/28/2022
Supervised By: Ankitia Jodhani 07/28/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
HOB37