

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072820\
 Data File : PD058731.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jul 2020 10:36
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 28 13:40:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 08 08:01:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

3) MA	gamma-BHC...	0.000	4.536	0	1325008	N.D.	0.383 #
7) B	delta-BHC	0.000	4.893f	0	1350242	N.D.	0.439 #
15) B	Endosulfa...	0.000	6.770f	0	923437	N.D.	0.374 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072820\
Data File : PD058731.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jul 2020 10:36
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 13:40:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
Quant Title : GC Extractables
QLast Update : Wed Jul 08 08:01:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

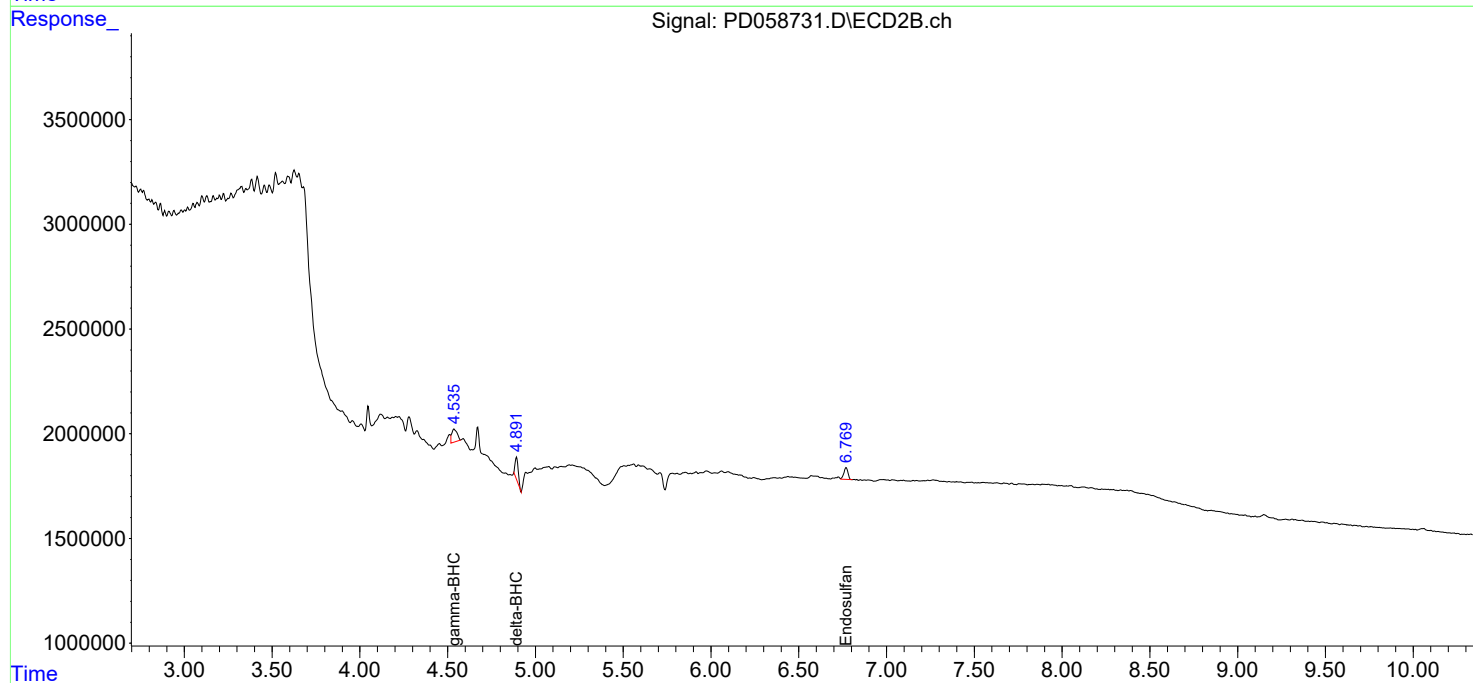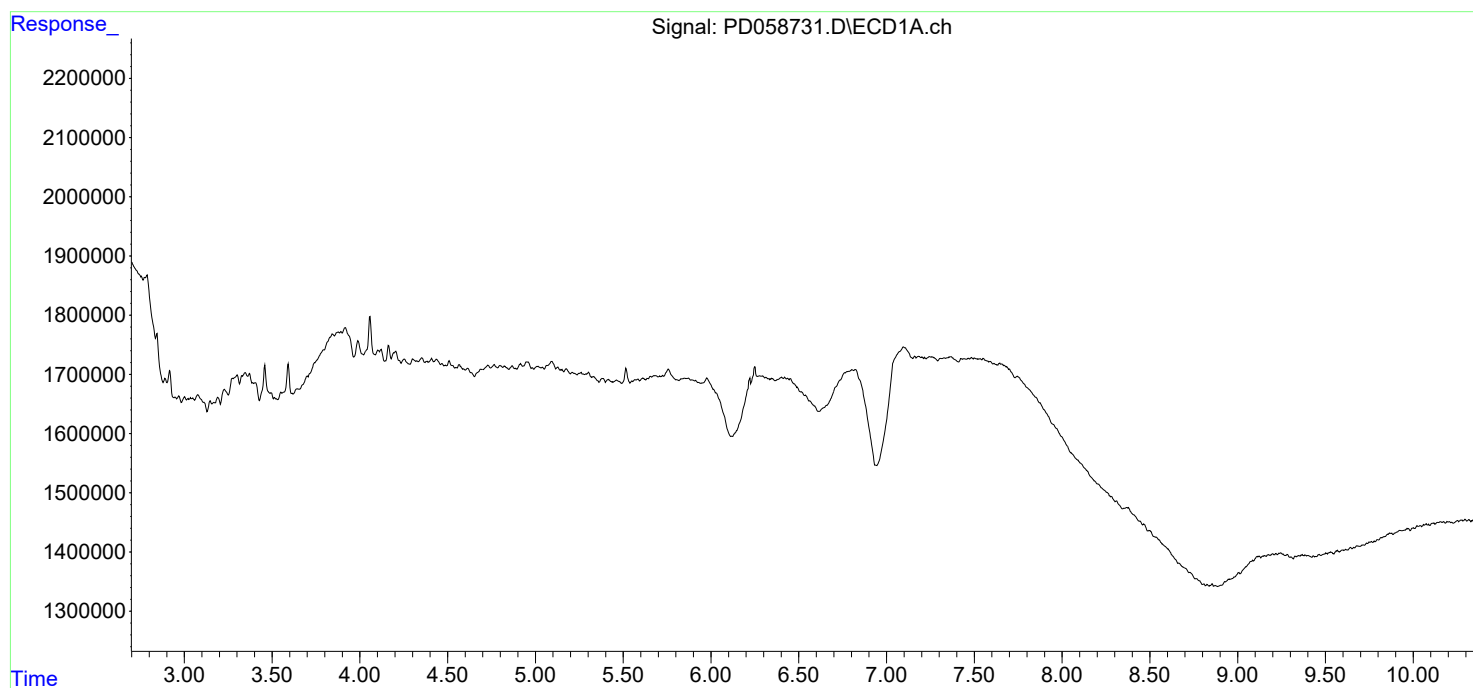


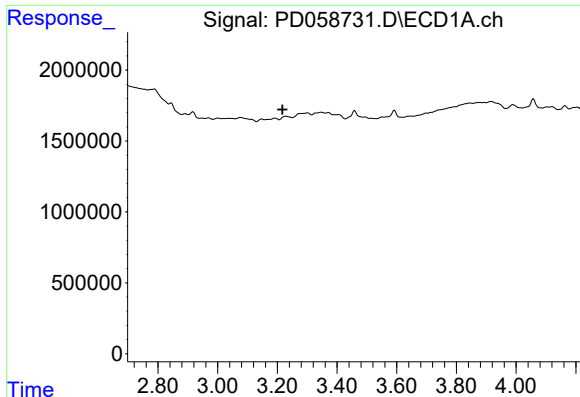

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.217 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

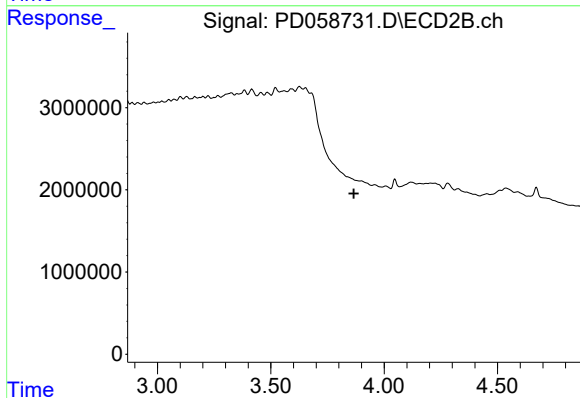


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.866 min
Response: 0
Conc: N.D.

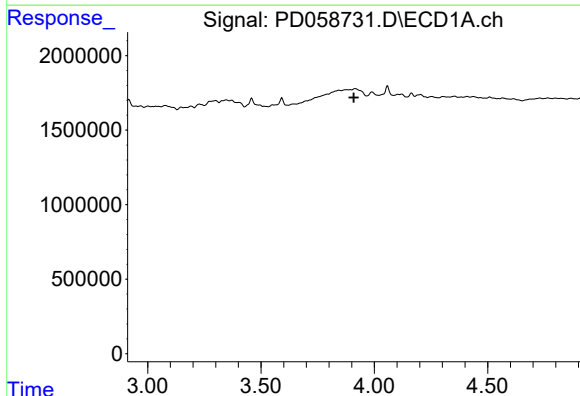


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 3.910 min
Response: 0
Conc: N.D.

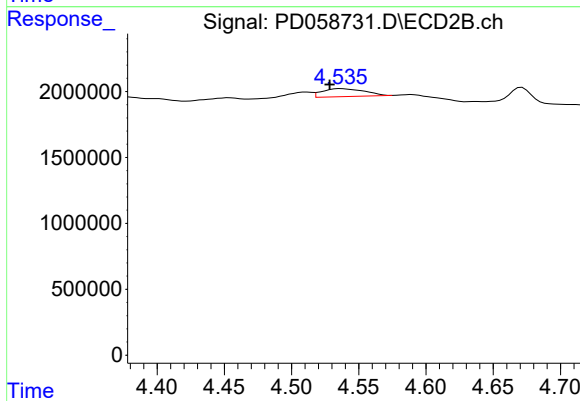

#3 gamma-BHC (Lindane)


R.T.: 4.536 min
Delta R.T.: 0.008 min
Response: 1325008
Conc: 0.38 ng/ml

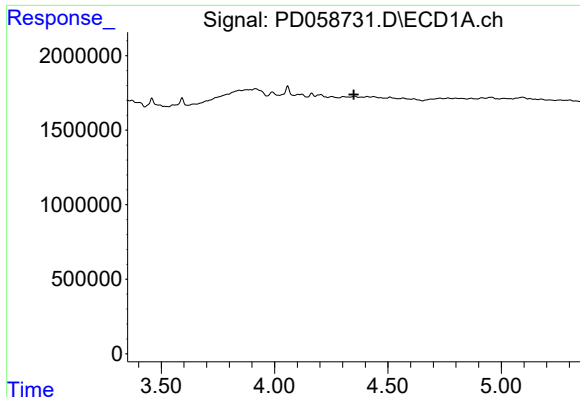

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.350 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

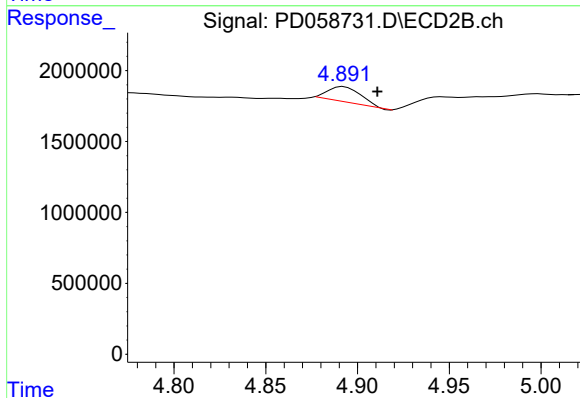


#7 delta-BHC

R.T.: 4.893 min
Delta R.T.: -0.018 min
Response: 1350242
Conc: 0.44 ng/ml

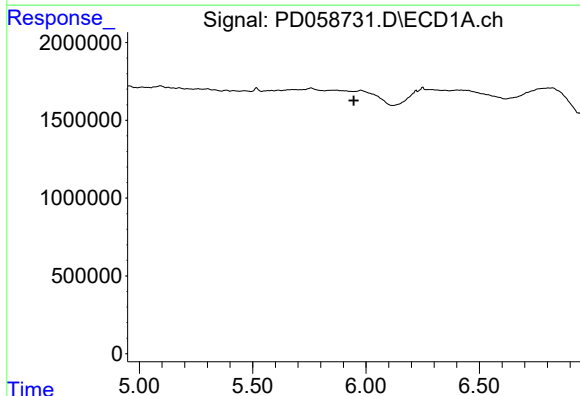


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 5.946 min
Response: 0
Conc: N.D.

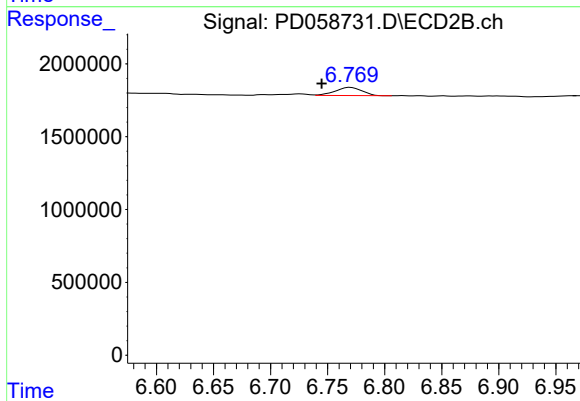

#15 Endosulfan II


R.T.: 6.770 min
Delta R.T.: 0.025 min
Response: 923437
Conc: 0.37 ng/ml

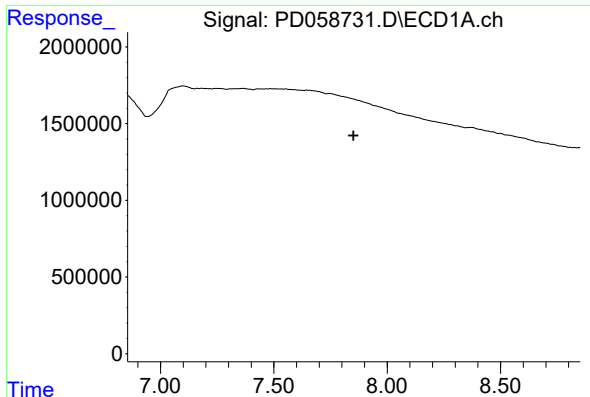

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.852 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

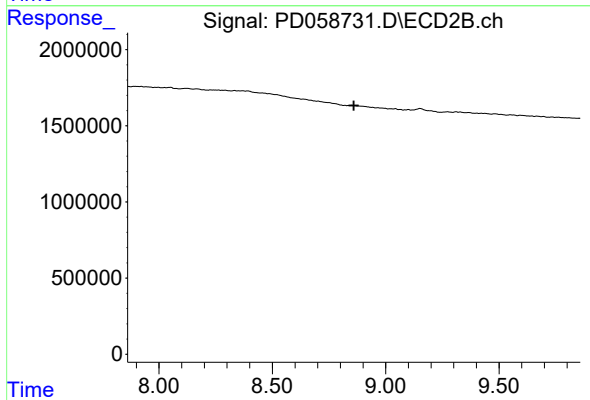

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.859 min
Response: 0
Conc: N.D.