

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072820\
 Data File : PD058739.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jul 2020 13:07
 Operator : AJ\MA
 Sample : PB130543BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 28 13:42:19 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 08 08:01:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.208	3.866	32062321	47479826	17.585	19.217
28)	SA Decachlor...	7.845	8.861	34408516	41954526	19.054	19.243
Target Compounds							
8)	B Heptachlo...	0.000	5.708	0	4239200	N.D.	1.456 #
9)	A Endosulfan I	0.000	6.087f	0	2141338	N.D.	0.812 #
10)	B gamma-Chl...	0.000	5.928f	0	2995576	N.D.	1.029 #
15)	B Endosulfa...	0.000	6.771f	0	757494	N.D.	0.307 #
25)	Chlordane-3	0.000	5.928f	0	2995576	N.D.	8.054 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072820\
Data File : PD058739.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jul 2020 13:07
Operator : AJ\MA
Sample : PB130543BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 13:42:19 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
Quant Title : GC Extractables
QLast Update : Wed Jul 08 08:01:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

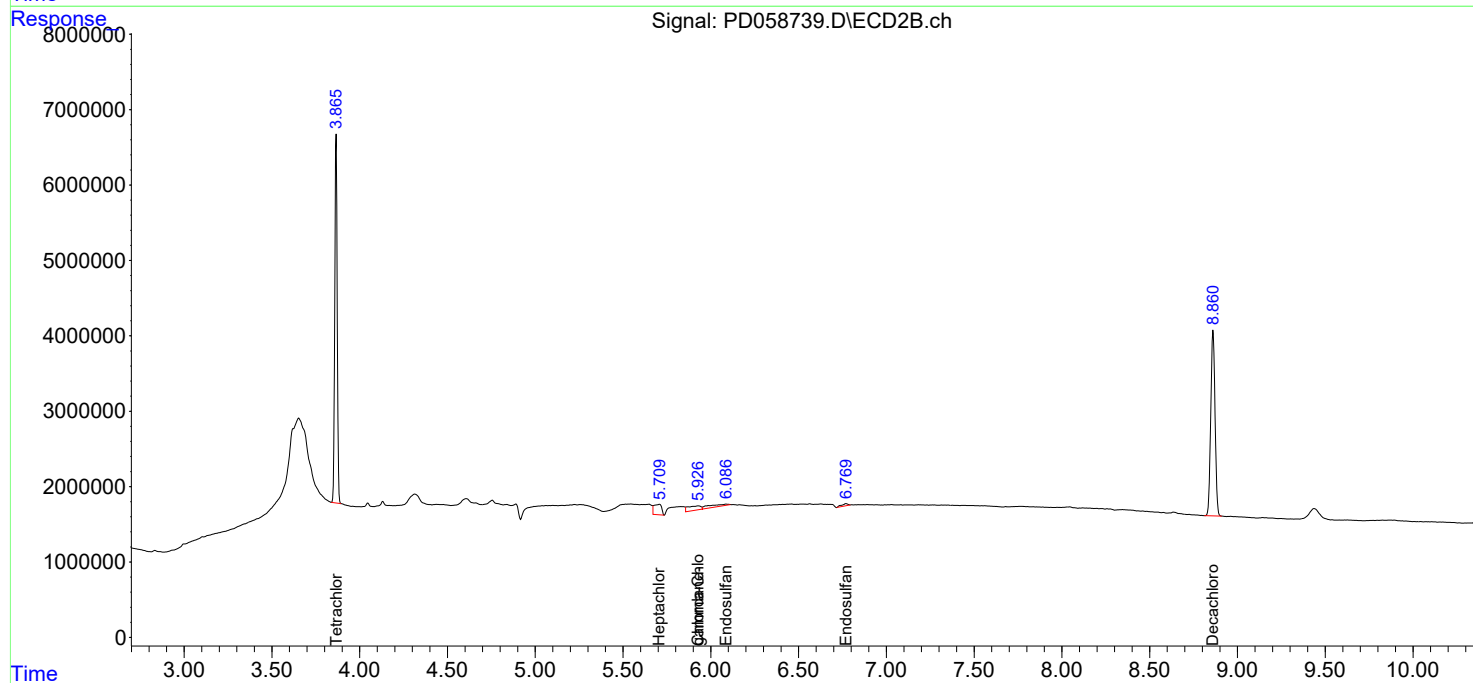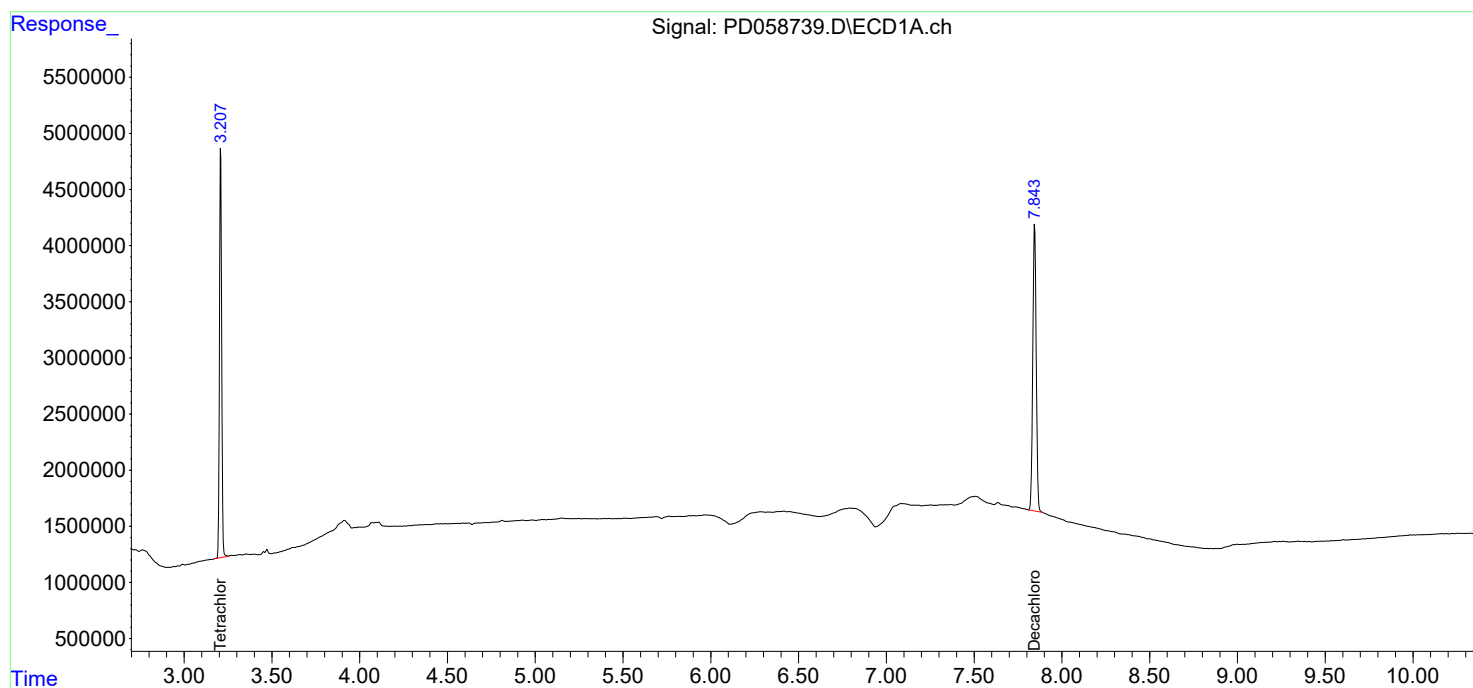


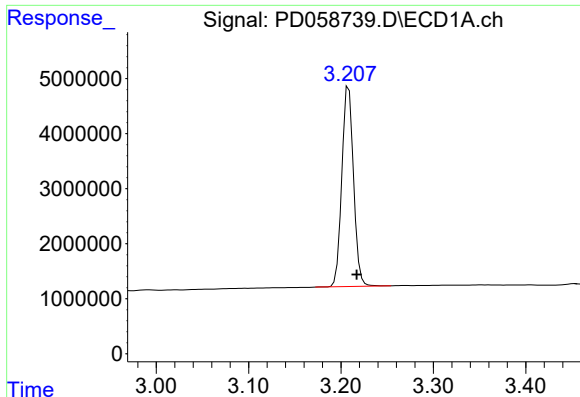

#1 Tetrachloro-m-xylene


R.T.: 3.208 min
Delta R.T.: -0.009 min
Response: 32062321
Conc: 17.58 ng/ml

Instrument :
ECD_D
ClientSampleId :

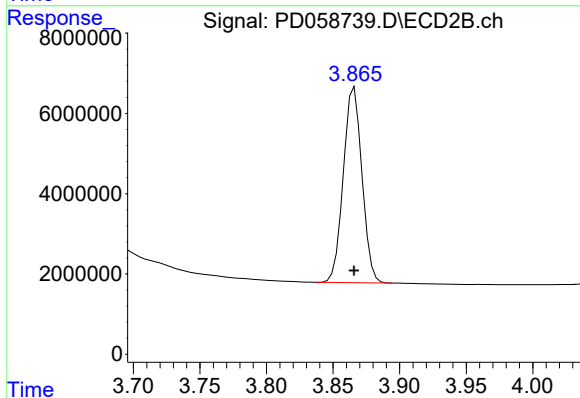


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.000 min
Response: 47479826
Conc: 19.22 ng/ml

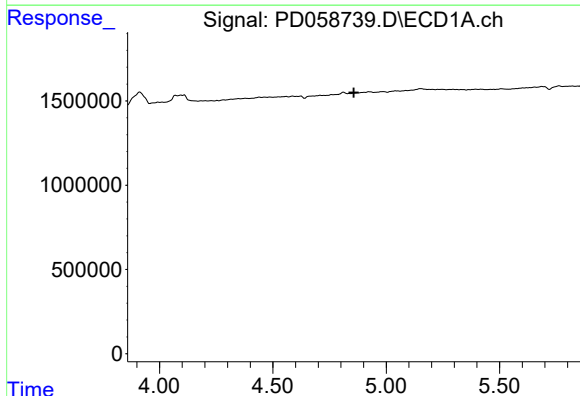


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.857 min
Response: 0
Conc: N.D.

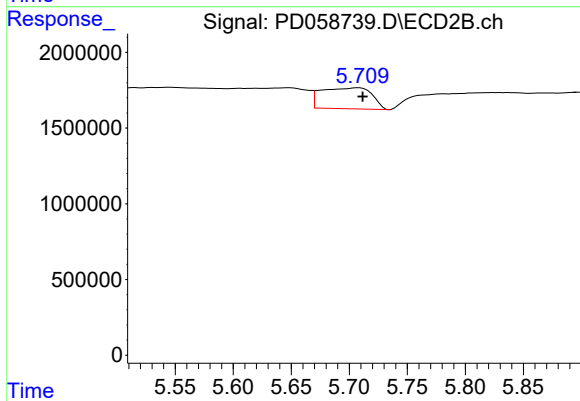

#8 Heptachlor epoxide


R.T.: 5.708 min
Delta R.T.: -0.004 min
Response: 4239200
Conc: 1.46 ng/ml

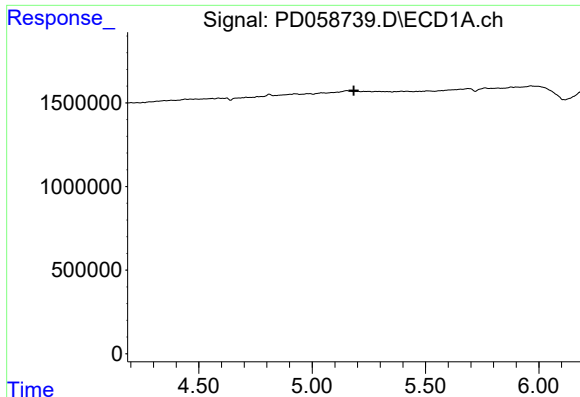

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.184 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

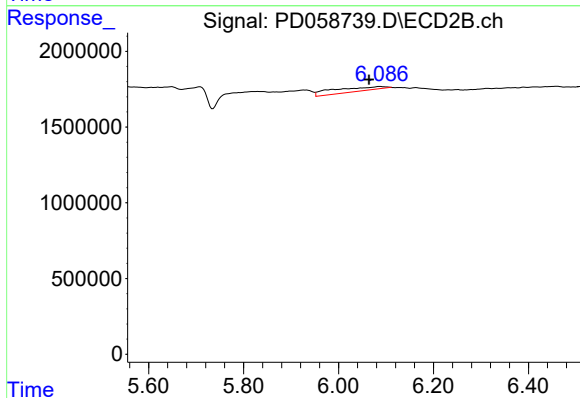


#9 Endosulfan I

R.T.: 6.087 min
Delta R.T.: 0.023 min
Response: 2141338
Conc: 0.81 ng/ml

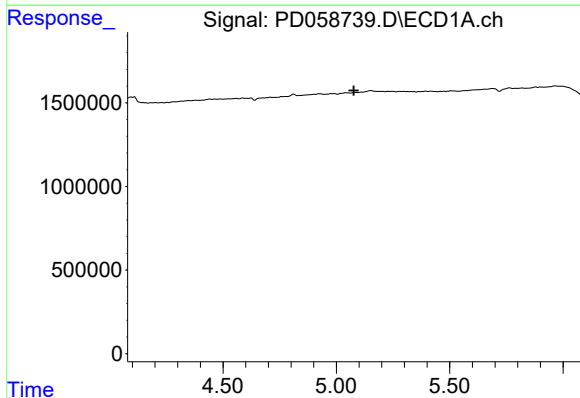


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.077 min
Response: 0
Conc: N.D.

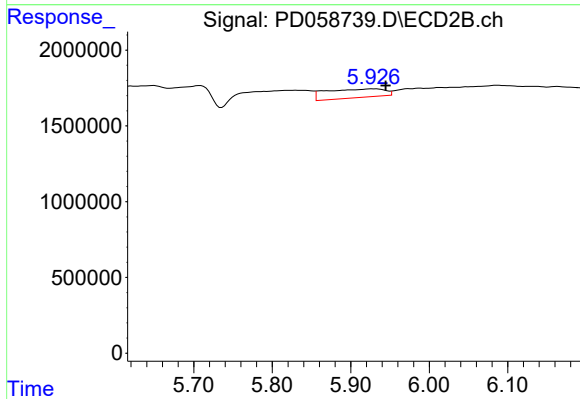

#10 gamma-Chlordane


R.T.: 5.928 min
Delta R.T.: -0.017 min
Response: 2995576
Conc: 1.03 ng/ml

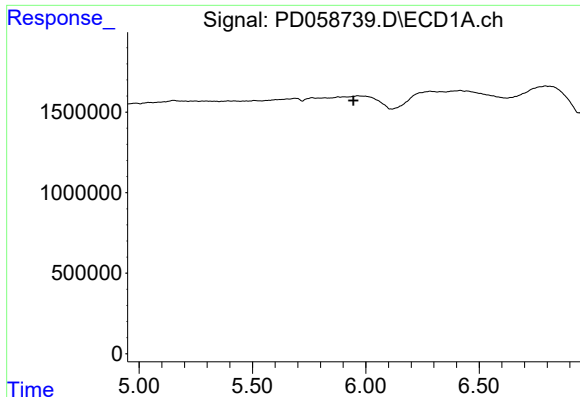

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 5.946 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

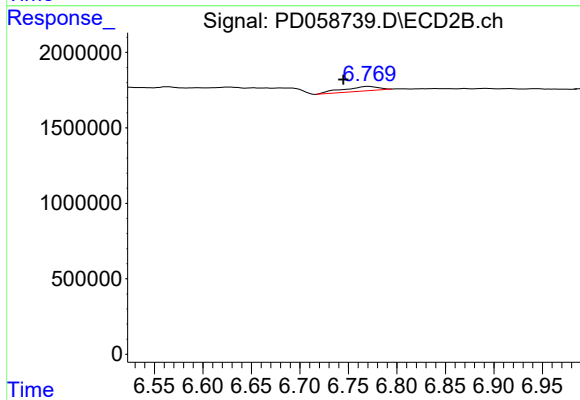


#15 Endosulfan II

R.T.: 6.771 min
Delta R.T.: 0.026 min
Response: 757494
Conc: 0.31 ng/ml

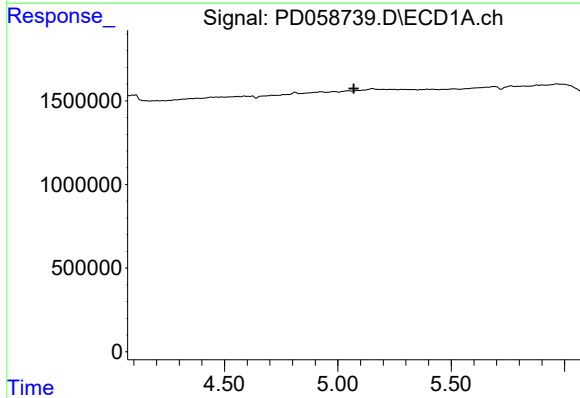


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.070 min
Response: 0
Conc: N.D.

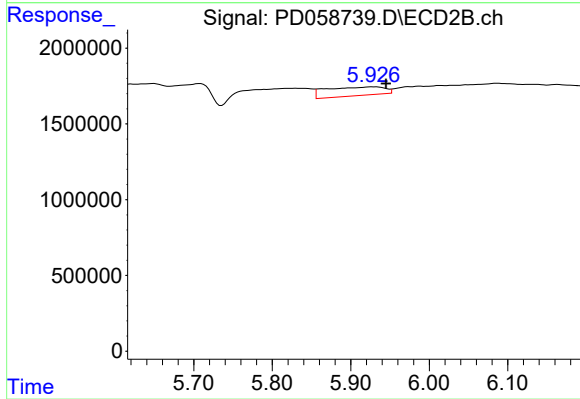

#25 Chlordane-3


R.T.: 5.928 min
Delta R.T.: -0.017 min
Response: 2995576
Conc: 8.05 ng/ml

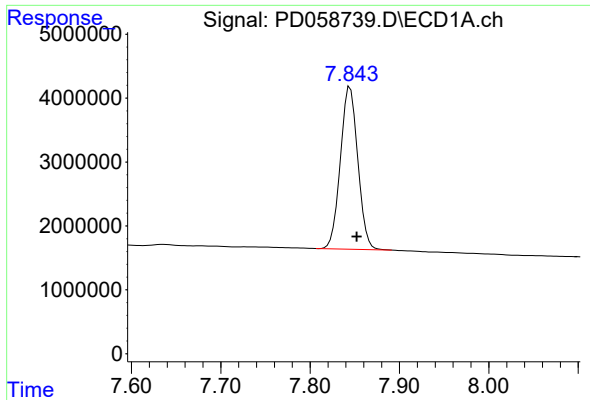

#28 Decachlorobiphenyl

R.T.: 7.845 min
Delta R.T.: -0.007 min
Response: 34408516
Conc: 19.05 ng/ml

Instrument :
ECD_D
ClientSampleId :

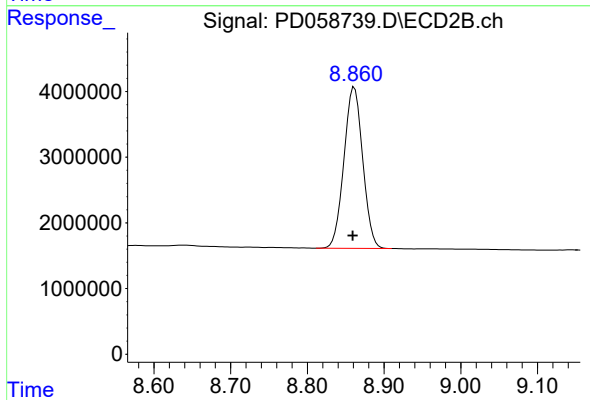

#28 Decachlorobiphenyl

R.T.: 8.861 min
Delta R.T.: 0.002 min
Response: 41954526
Conc: 19.24 ng/ml