

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072820\
 Data File : PD058747.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jul 2020 15:19
 Operator : AJ\MA
 Sample : L3185-01 10X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 04:18:48 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 08 08:01:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	0.000	3.865	0	2280321	N.D.	0.923 #
28)	SA Decachlor...	0.000	8.860	0	2978069	N.D.	1.366 #
Target Compounds							
3)	MA gamma-BHC...	0.000	4.508f	0	1243877	N.D.	0.360 #
7)	B delta-BHC	0.000	4.889f	0	1758513	N.D.	0.572 #
9)	A Endosulfan I	5.204f	0.000	2704268	0	1.365	N.D. #
10)	B gamma-Chl...	0.000	5.944	0	3352789	N.D.	1.152 #
11)	B alpha-Chl...	0.000	6.019	0	3262344	N.D.	1.134 #
16)	A 4,4'-DDD	0.000	6.664	0	2018449	N.D.	0.875 #
25)	Chlordane-3	0.000	5.944	0	3352789	N.D.	9.014 #
26)	Chlordane-4	0.000	6.019	0	3262344	N.D.	7.500 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072820\
Data File : PD058747.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jul 2020 15:19
Operator : AJ\MA
Sample : L3185-01 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 04:18:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
Quant Title : GC Extractables
QLast Update : Wed Jul 08 08:01:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

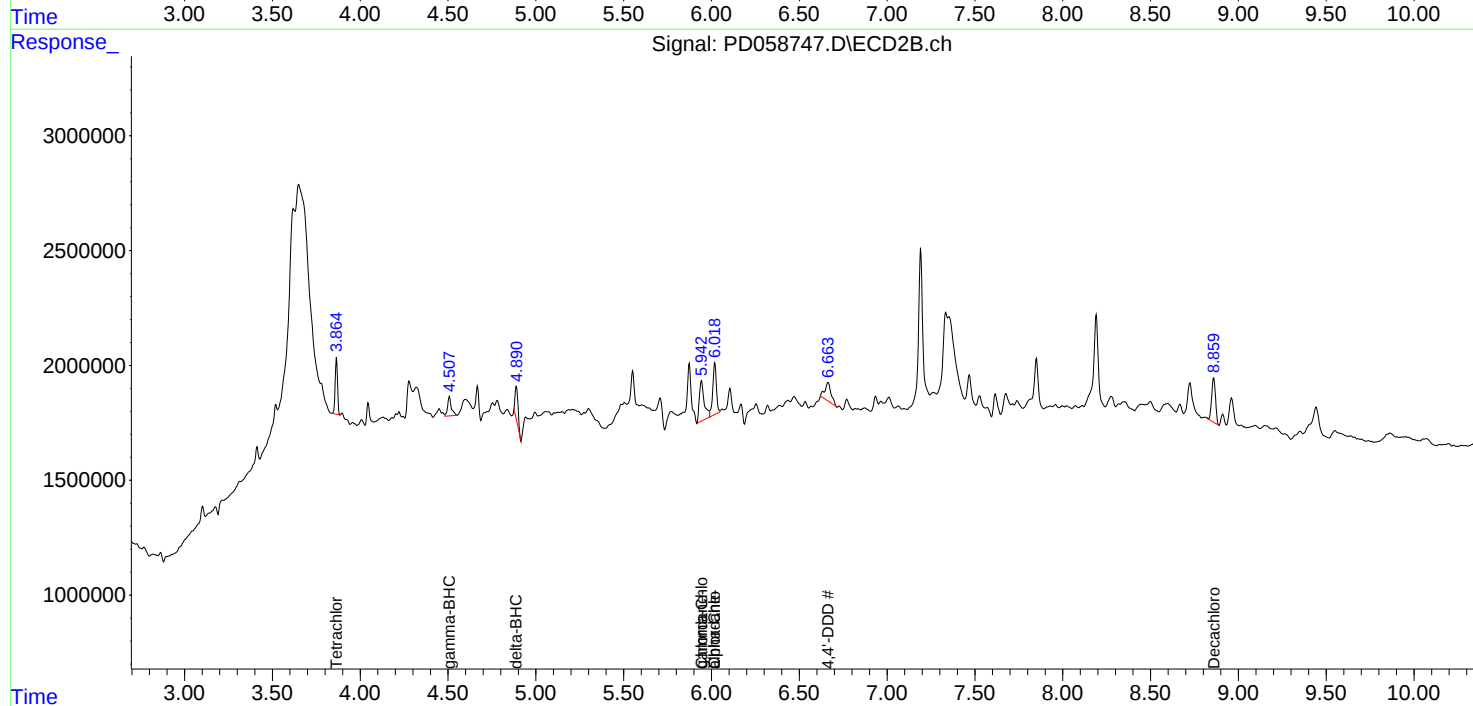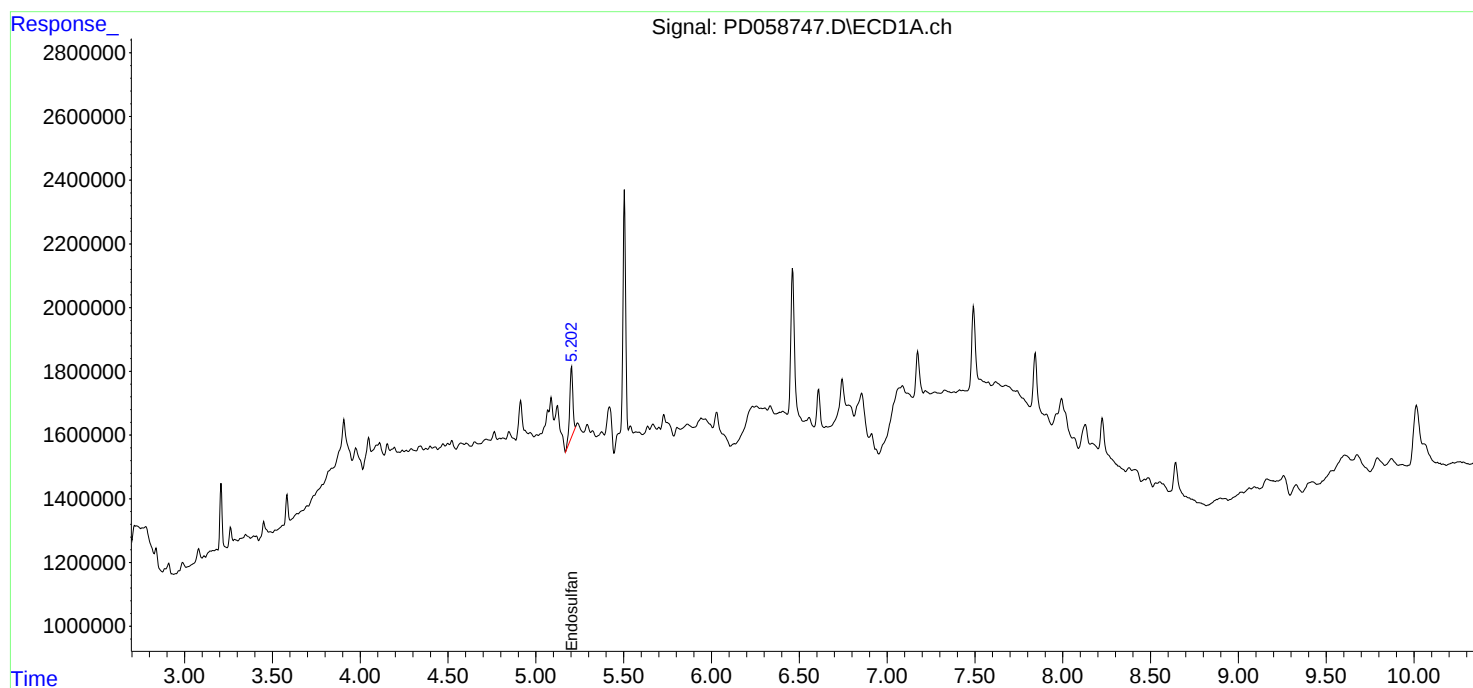


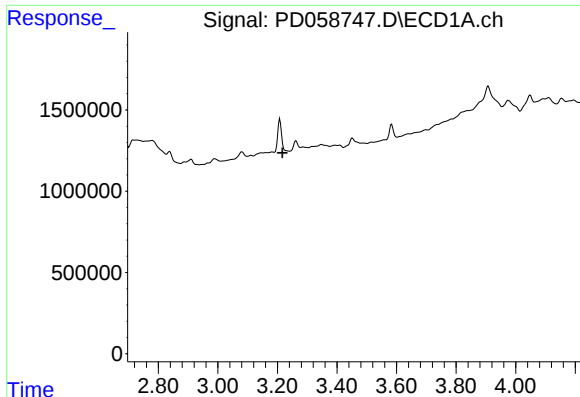

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.217 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

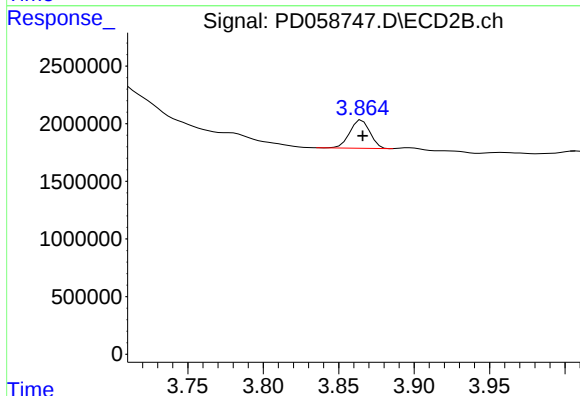


#1 Tetrachloro-m-xylene

R.T.: 3.865 min
Delta R.T.: 0.000 min
Response: 2280321
Conc: 0.92 ng/ml

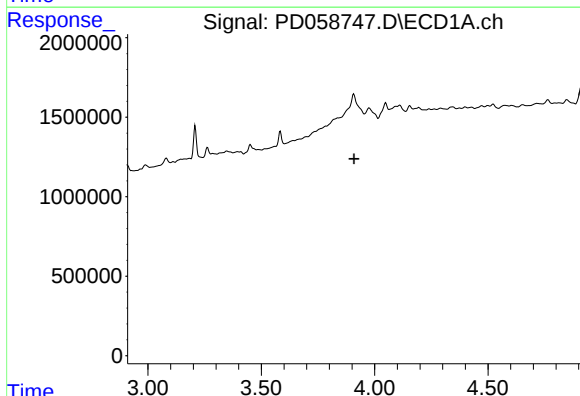


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T.: 3.910 min
Response: 0
Conc: N.D.

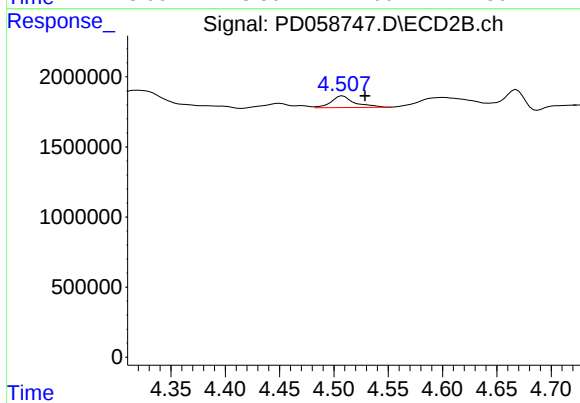

#3 gamma-BHC (Lindane)


R.T.: 4.508 min
Delta R.T.: -0.020 min
Response: 1243877
Conc: 0.36 ng/ml

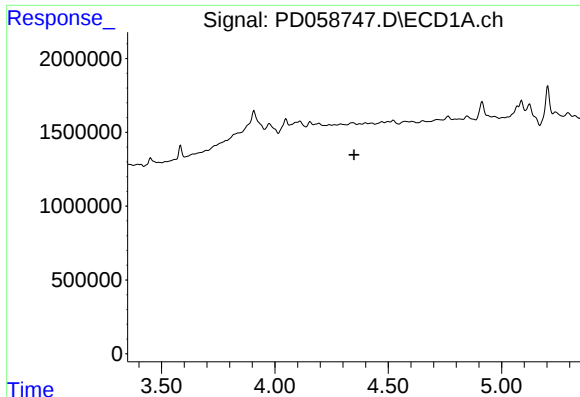

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.350 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

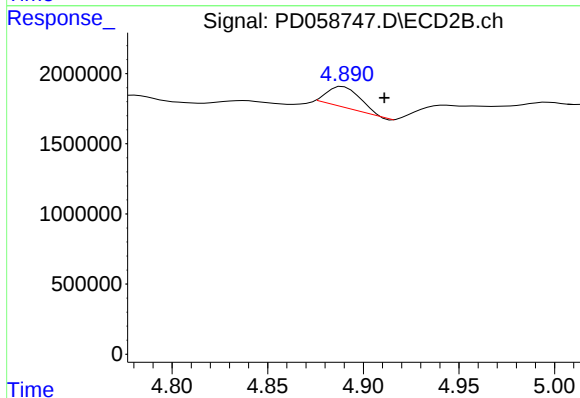


#7 delta-BHC

R.T.: 4.889 min
Delta R.T.: -0.022 min
Response: 1758513
Conc: 0.57 ng/ml

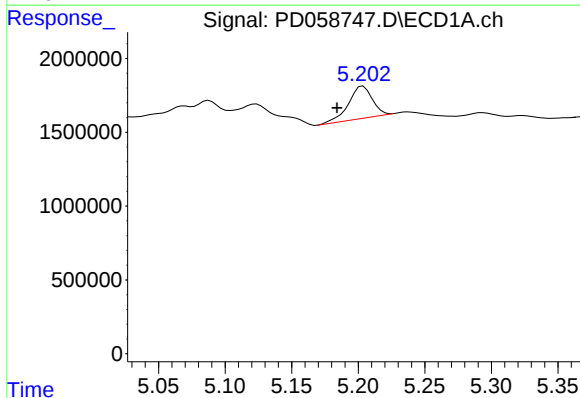


#9 Endosulfan I

R.T.: 5.204 min
Delta R.T.: 0.020 min
Response: 2704268
Conc: 1.36 ng/ml

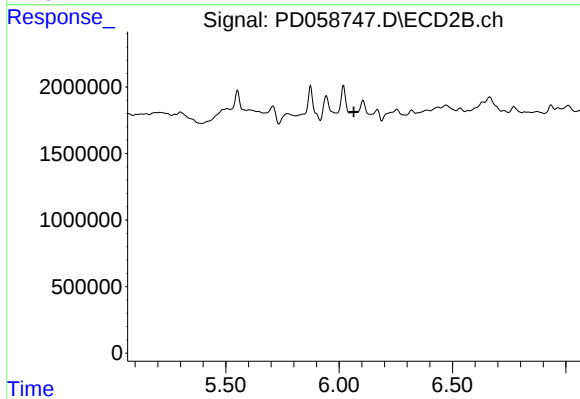

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.064 min
Response: 0
Conc: N.D.

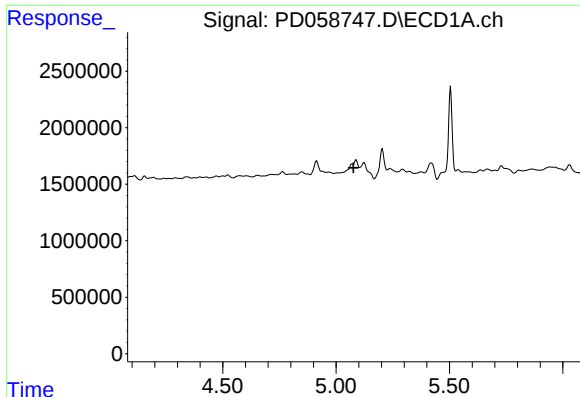

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.077 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

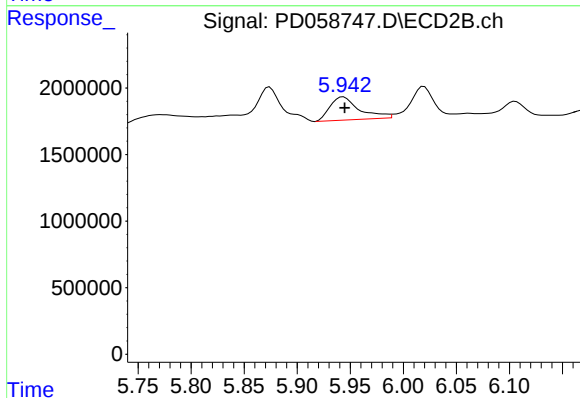


#10 gamma-Chlordane

R.T.: 5.944 min
Delta R.T.: -0.001 min
Response: 3352789
Conc: 1.15 ng/ml

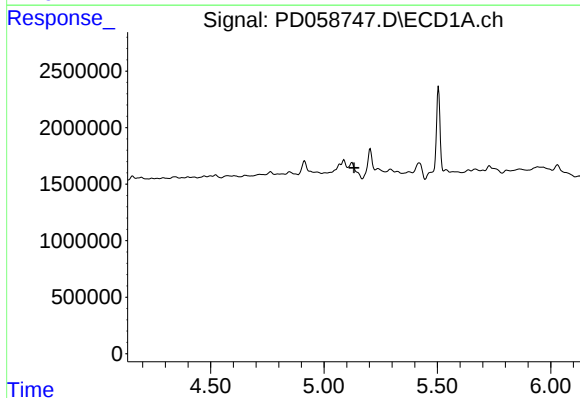


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.133 min
Response: 0
Conc: N.D.

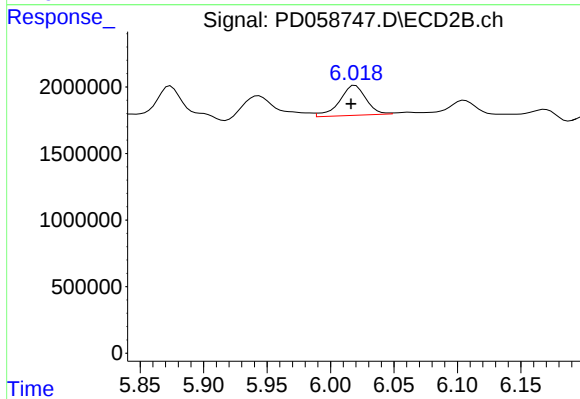

#11 alpha-Chlordane


R.T.: 6.019 min
Delta R.T.: 0.003 min
Response: 3262344
Conc: 1.13 ng/ml

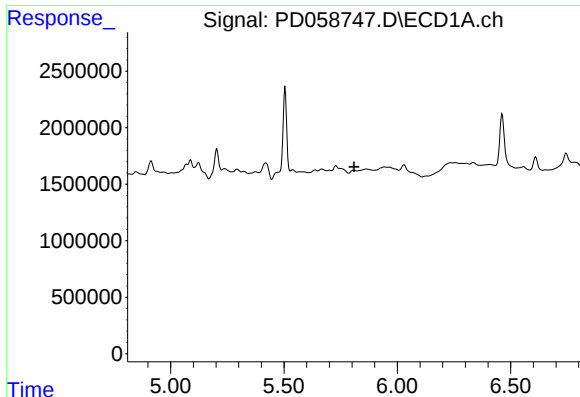

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.810 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

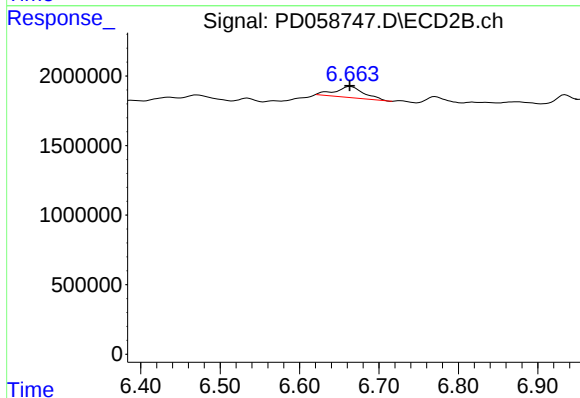


#16 4,4'-DDD

R.T.: 6.664 min
Delta R.T.: 0.000 min
Response: 2018449
Conc: 0.88 ng/ml

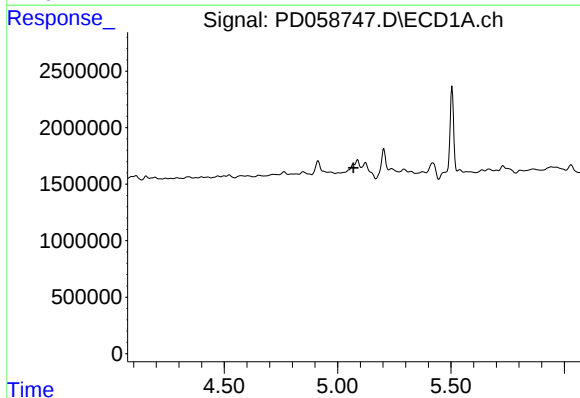


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.070 min
Response: 0
Conc: N.D.

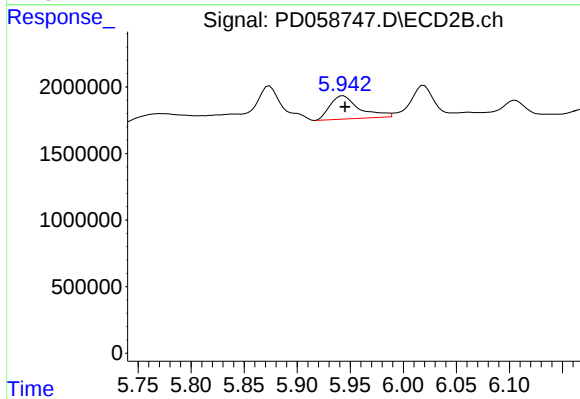

#25 Chlordane-3


R.T.: 5.944 min
Delta R.T.: -0.002 min
Response: 3352789
Conc: 9.01 ng/ml

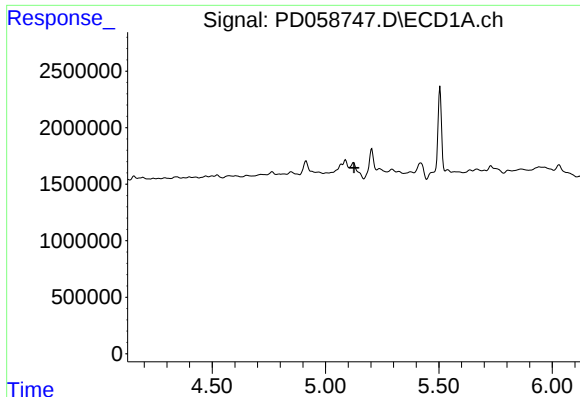

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.126 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

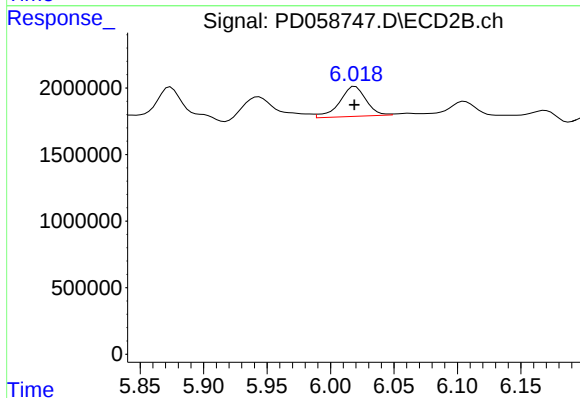


#26 Chlordane-4

R.T.: 6.019 min
Delta R.T.: 0.000 min
Response: 3262344
Conc: 7.50 ng/ml

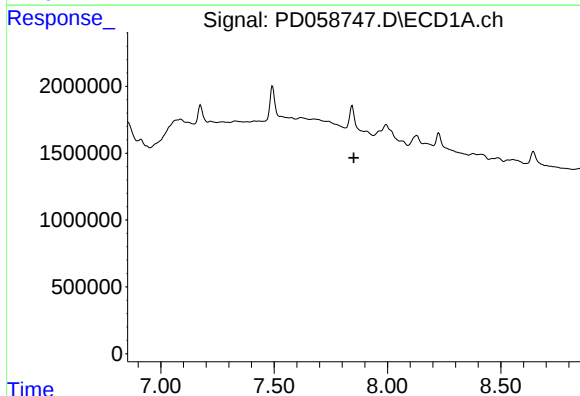

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 7.852 min
Response: 0
Conc: N.D.

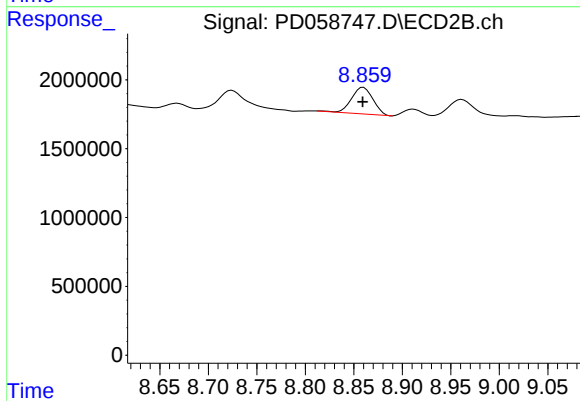

#28 Decachlorobiphenyl

R.T.: 8.860 min
Delta R.T.: 0.000 min
Response: 2978069
Conc: 1.37 ng/ml