

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072820\
 Data File : PD058750.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jul 2020 16:01
 Operator : AJ\MA
 Sample : L3434-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 04:19:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 08 08:01:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.208	3.866	32266279	47457880	17.697	19.208
28)	SA Decachlor...	7.845	8.862	34763569	45205370	19.251	20.734
Target Compounds							
4)	MA Heptachlor	0.000	5.009f	0	762047	N.D.	0.242 #
6)	B beta-BHC	0.000	4.689	0	624124	N.D.	0.441 #
7)	B delta-BHC	0.000	4.891f	0	2625272	N.D.	0.854 #
9)	A Endosulfan I	0.000	6.057	0	2253129	N.D.	0.855 #
10)	B gamma-Chl...	0.000	5.935	0	4650677	N.D.	1.598 #
15)	B Endosulfa...	0.000	6.771f	0	983990	N.D.	0.399 #
21)	B Endrin ke...	0.000	7.572f	0	916672	N.D.	0.337 #
25)	Chlordane-3	0.000	5.935	0	4650677	N.D.	12.504 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072820\
Data File : PD058750.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jul 2020 16:01
Operator : AJ\MA
Sample : L3434-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 04:19:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
Quant Title : GC Extractables
QLast Update : Wed Jul 08 08:01:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

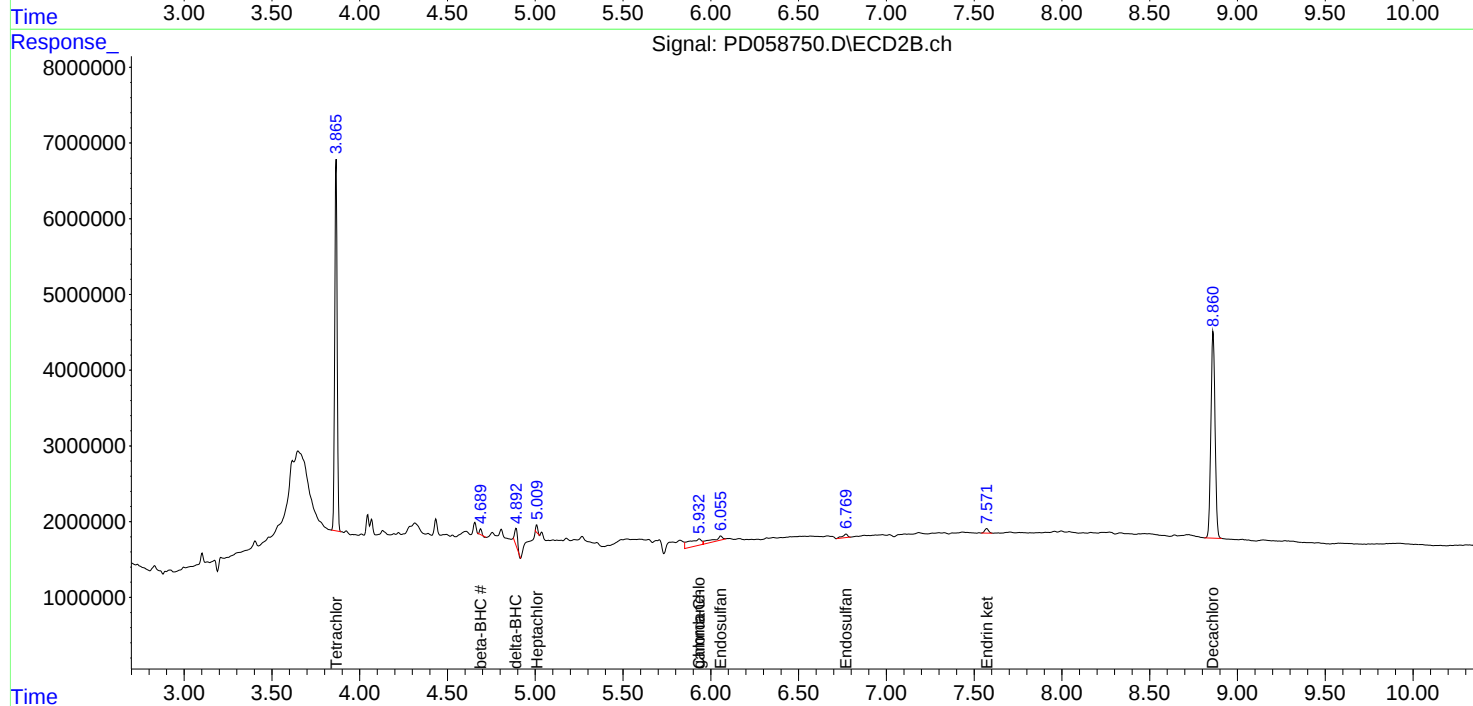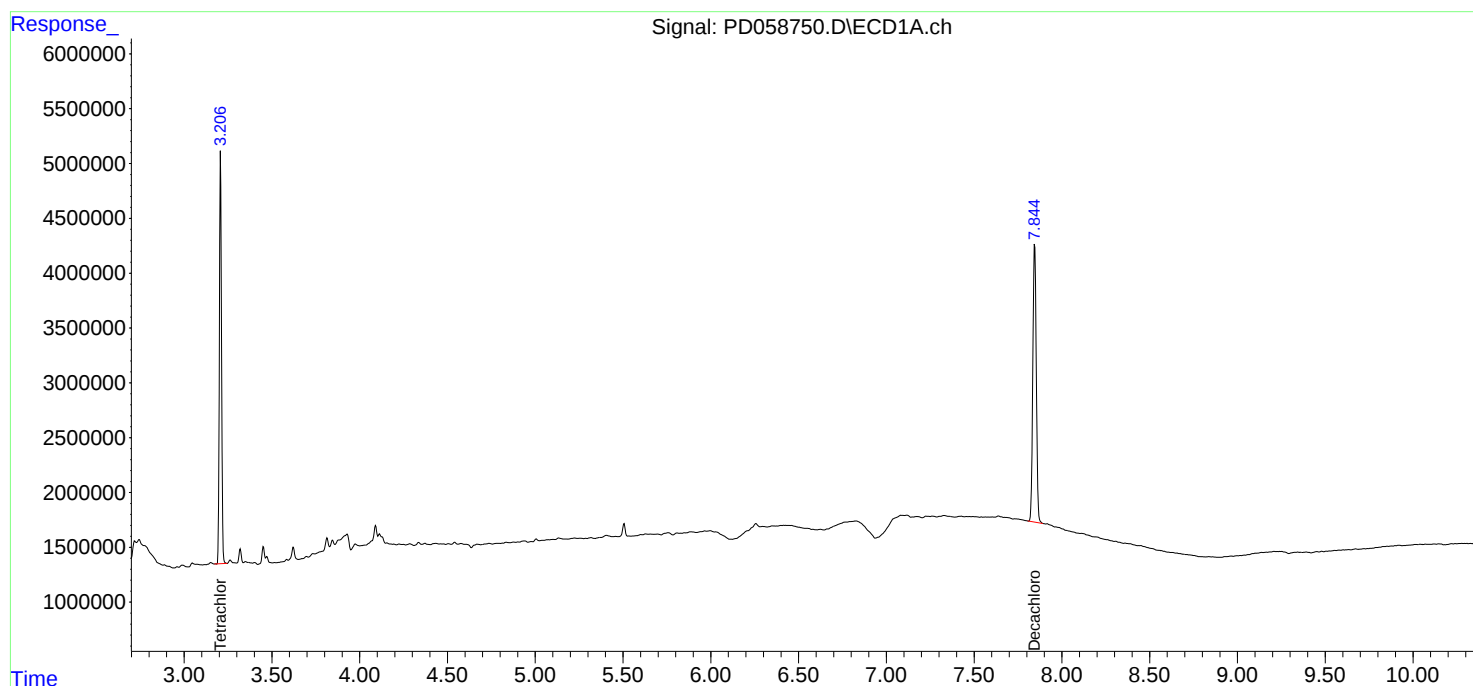


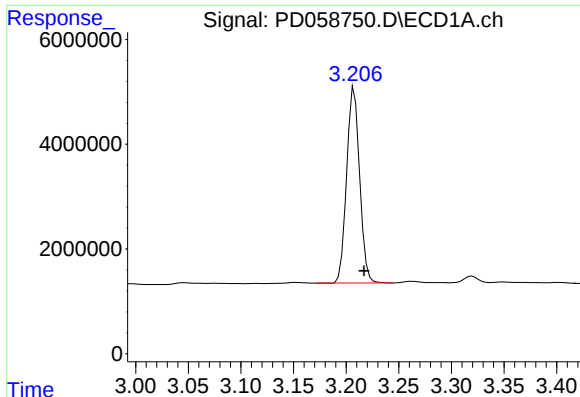

#1 Tetrachloro-m-xylene


R.T.: 3.208 min
Delta R.T.: -0.009 min
Response: 32266279
Conc: 17.70 ng/ml

Instrument :
ECD_D
ClientSampleId :

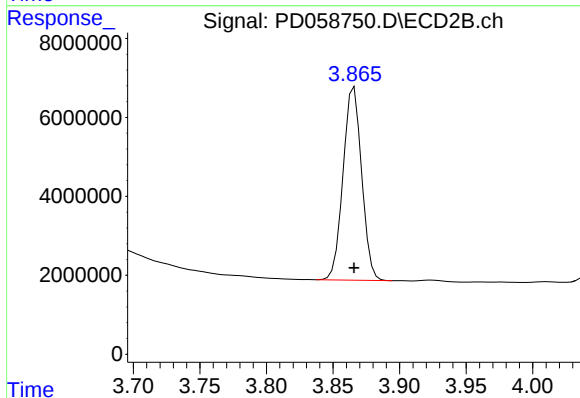


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.000 min
Response: 47457880
Conc: 19.21 ng/ml

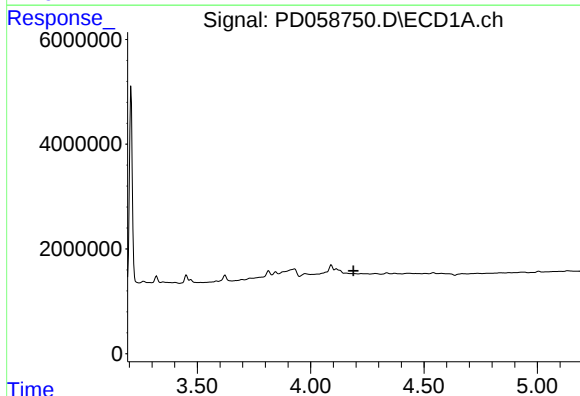


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.189 min
Response: 0
Conc: N.D.

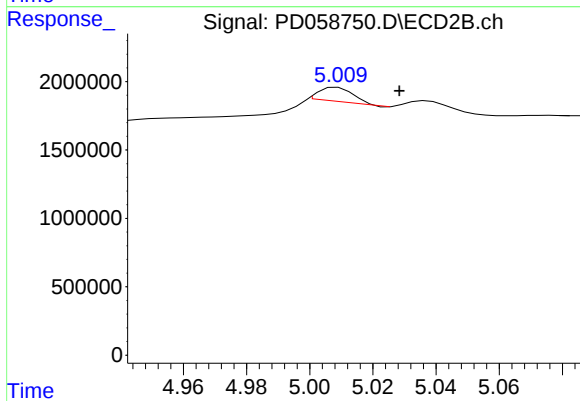

#4 Heptachlor


R.T.: 5.009 min
Delta R.T.: -0.020 min
Response: 762047
Conc: 0.24 ng/ml

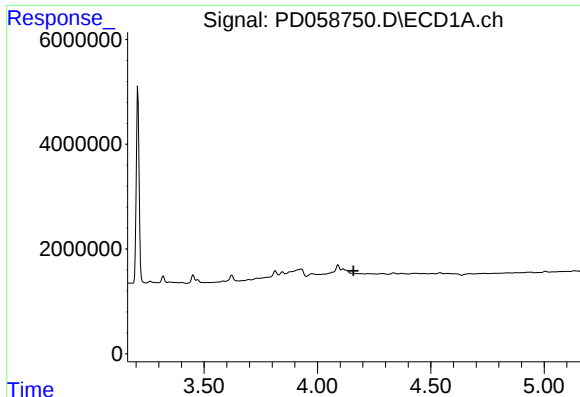

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.159 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

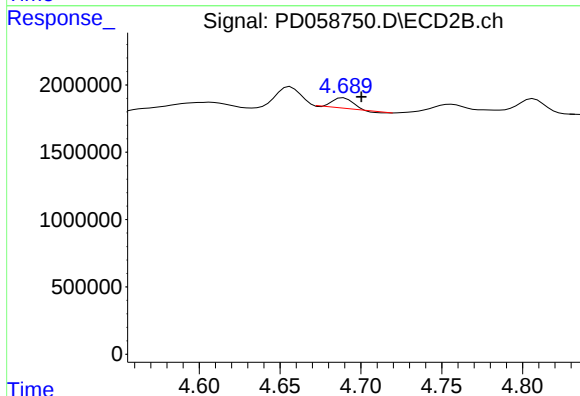


#6 beta-BHC

R.T.: 4.689 min
Delta R.T.: -0.011 min
Response: 624124
Conc: 0.44 ng/ml

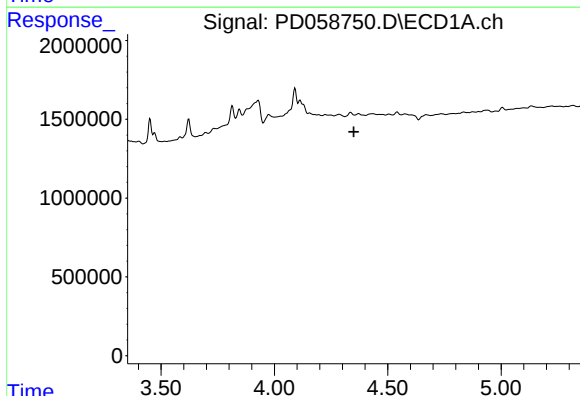


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.350 min
Response: 0
Conc: N.D.

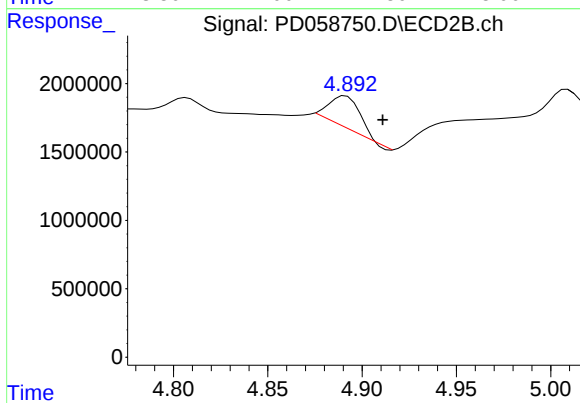

#7 delta-BHC


R.T.: 4.891 min
Delta R.T.: -0.020 min
Response: 2625272
Conc: 0.85 ng/ml

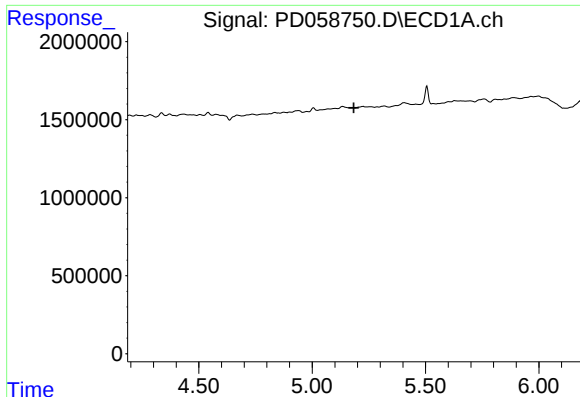

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.184 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

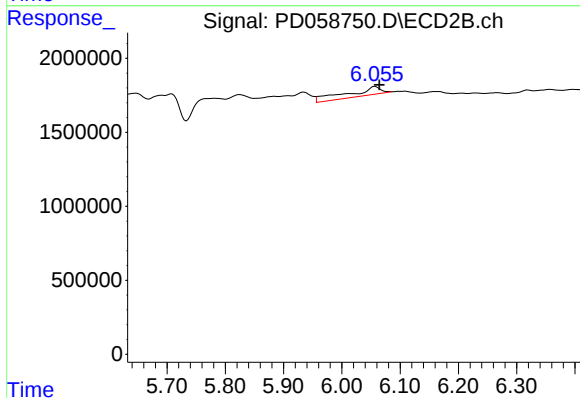


#9 Endosulfan I

R.T.: 6.057 min
Delta R.T.: -0.008 min
Response: 2253129
Conc: 0.85 ng/ml

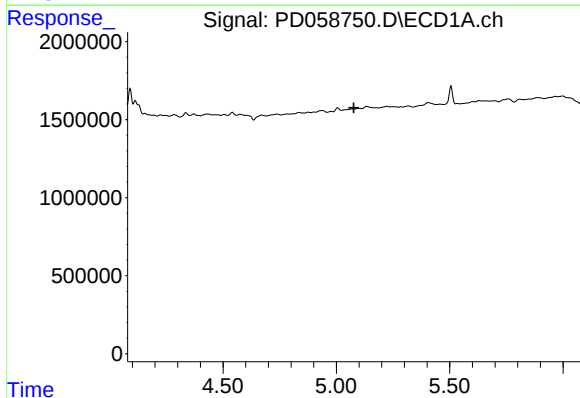


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.077 min
Response: 0
Conc: N.D.

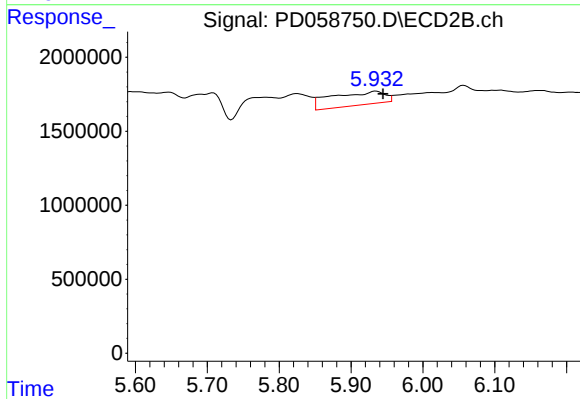

#10 gamma-Chlordane


R.T.: 5.935 min
Delta R.T.: -0.010 min
Response: 4650677
Conc: 1.60 ng/ml

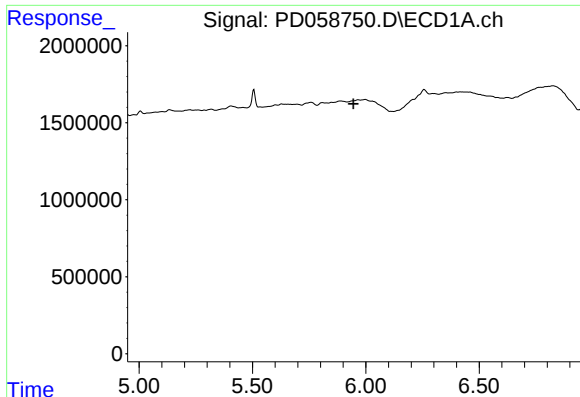

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.946 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

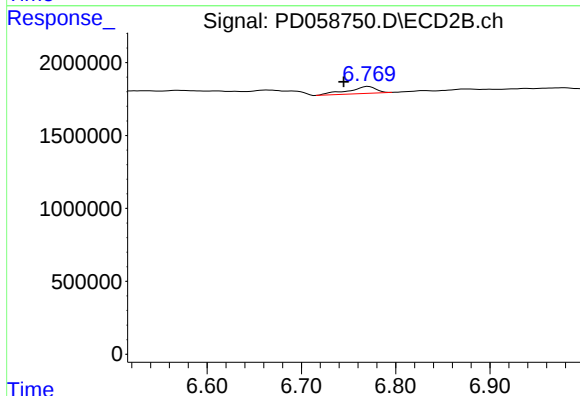


#15 Endosulfan II

R.T.: 6.771 min
Delta R.T.: 0.026 min
Response: 983990
Conc: 0.40 ng/ml

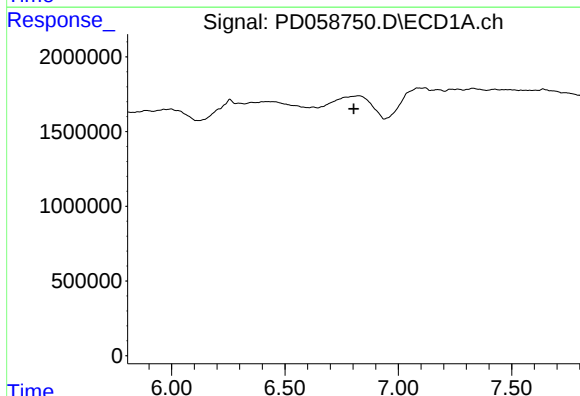


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 6.804 min
Response: 0
Conc: N.D.

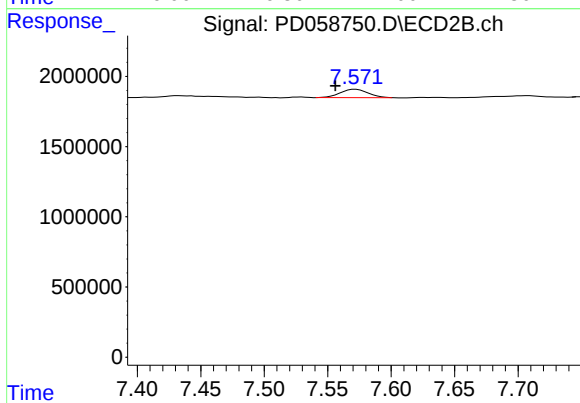

#21 Endrin ketone


R.T.: 7.572 min
Delta R.T.: 0.016 min
Response: 916672
Conc: 0.34 ng/ml

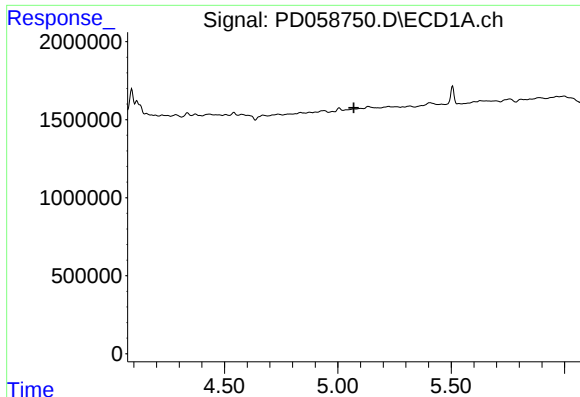

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.070 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

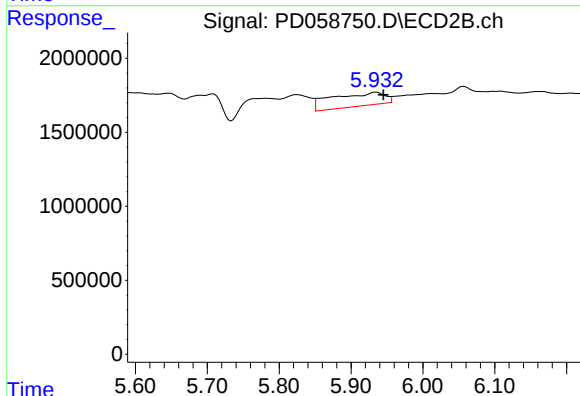


#25 Chlordane-3

R.T.: 5.935 min
Delta R.T.: -0.011 min
Response: 4650677
Conc: 12.50 ng/ml

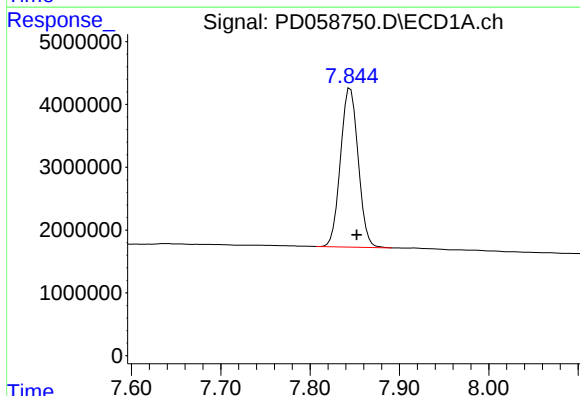

#28 Decachlorobiphenyl

R.T.: 7.845 min
Delta R.T.: -0.007 min
Response: 34763569
Conc: 19.25 ng/ml

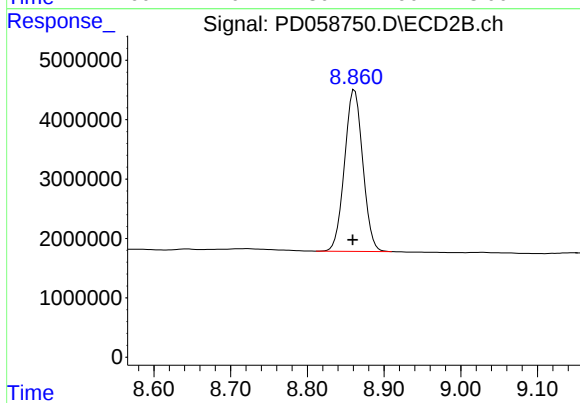

#28 Decachlorobiphenyl

R.T.: 8.862 min
Delta R.T.: 0.002 min
Response: 45205370
Conc: 20.73 ng/ml