

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072820\
 Data File : PD058755.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jul 2020 17:12
 Operator : AJ\MA
 Sample : L3439-09
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 04:20:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 08 08:01:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.866	31927945	45658287	17.511	18.479
28)	SA Decachlor...	7.845	8.863	25327267	32649507	14.025	14.975
Target Compounds							
5)	MB Aldrin	0.000	5.311f	0	2327393	N.D.	0.734 #
7)	B delta-BHC	0.000	4.891f	0	2409797	N.D.	0.783 #
8)	B Heptachlo...	0.000	5.707	0	5899177	N.D.	2.027 #
10)	B gamma-Chl...	0.000	5.954	0	9211608	N.D.	3.165 #
11)	B alpha-Chl...	0.000	6.019	0	417349	N.D.	0.145 #
13)	MA Dieldrin	0.000	6.307	0	695623	N.D.	0.244 #
15)	B Endosulfa...	0.000	6.771f	0	1173577	N.D.	0.476 #
24)	Chlordane-2	0.000	5.311	0	2327393	N.D.	23.560 #
25)	Chlordane-3	0.000	5.954	0	9211608	N.D.	24.766 #
26)	Chlordane-4	0.000	6.019	0	417349	N.D.	0.959 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072820\
Data File : PD058755.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jul 2020 17:12
Operator : AJ\MA
Sample : L3439-09
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 04:20:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
Quant Title : GC Extractables
QLast Update : Wed Jul 08 08:01:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

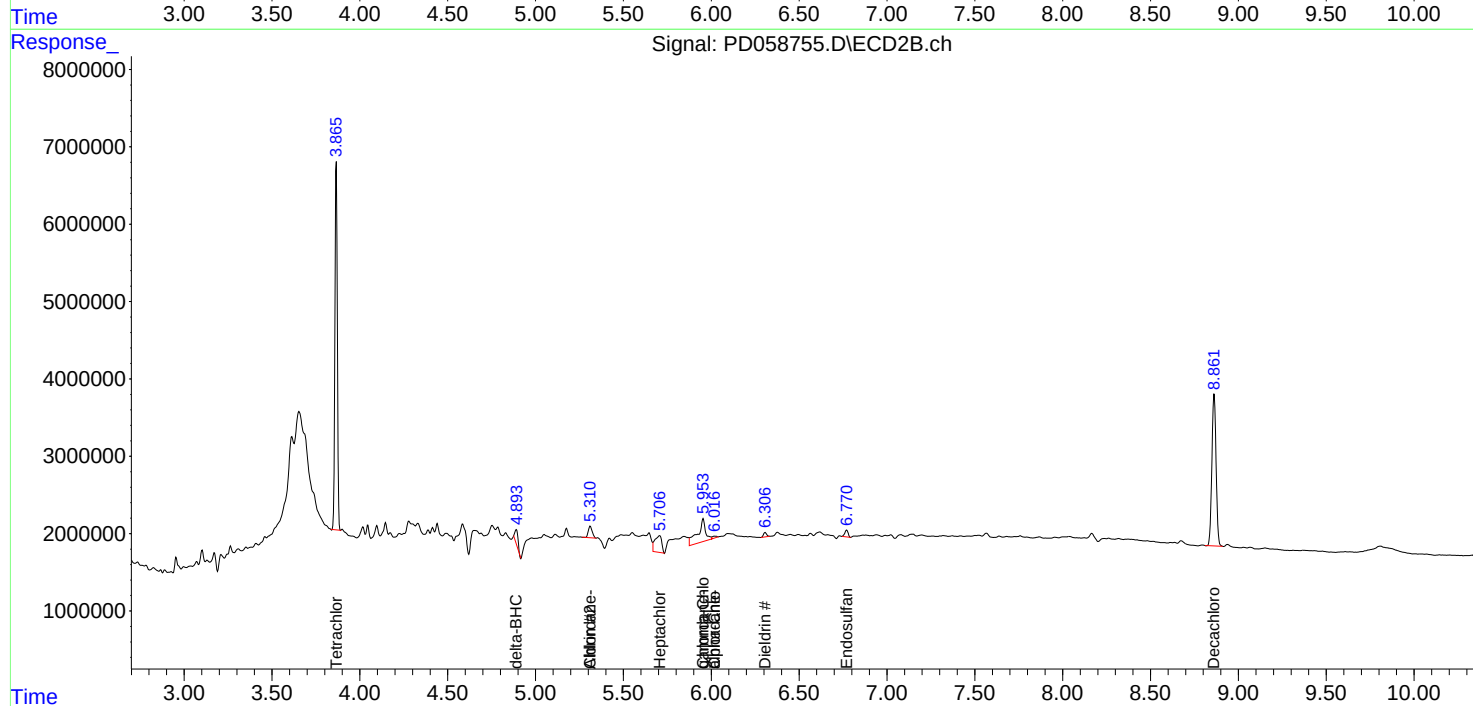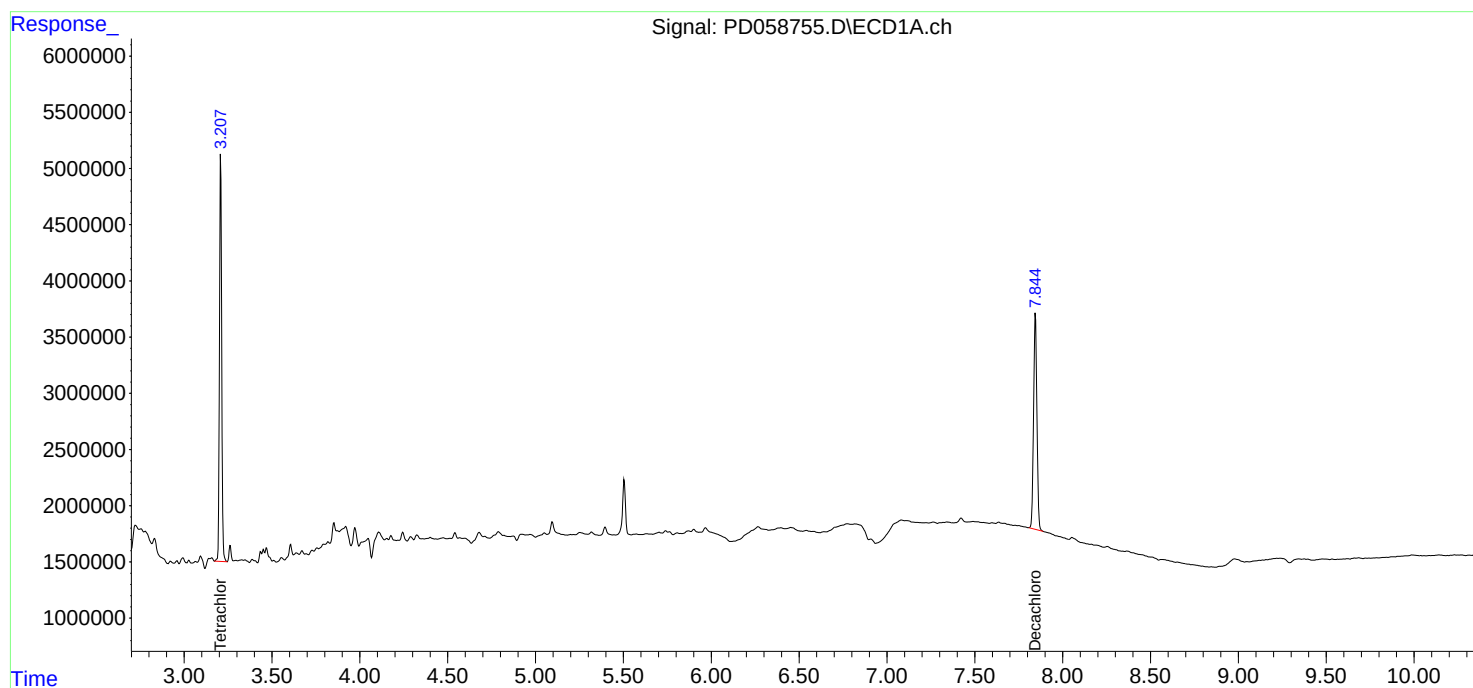


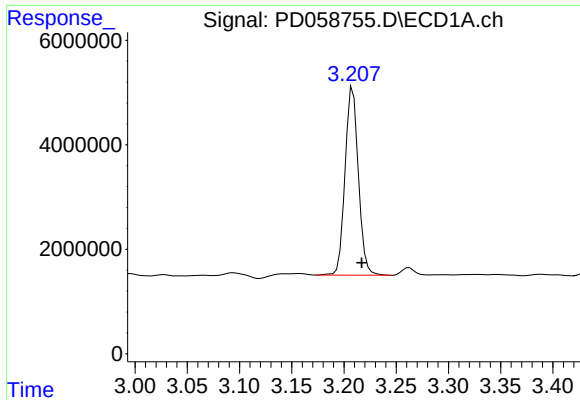

#1 Tetrachloro-m-xylene


R.T.: 3.209 min
Delta R.T.: -0.008 min
Response: 31927945
Conc: 17.51 ng/ml

Instrument :
ECD_D
ClientSampleId :

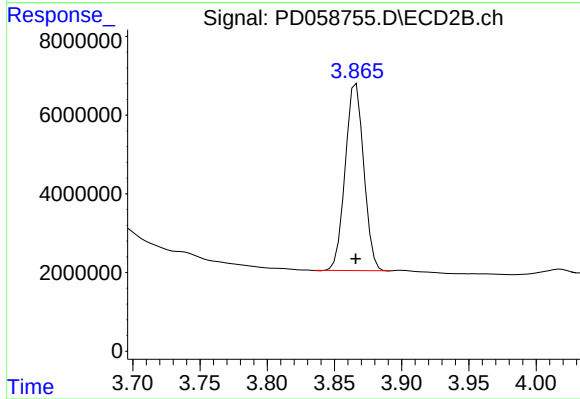


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.000 min
Response: 45658287
Conc: 18.48 ng/ml

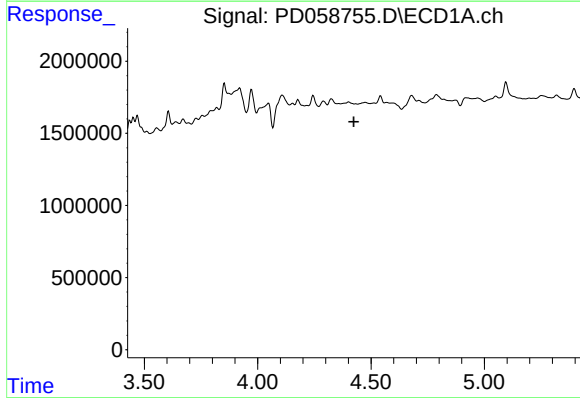


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.424 min
Response: 0
Conc: N.D.

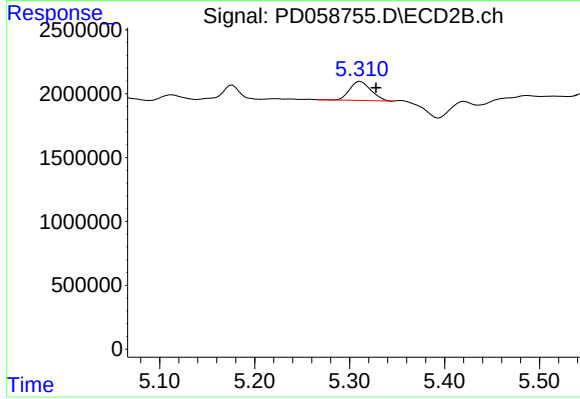

#5 Aldrin


R.T.: 5.311 min
Delta R.T.: -0.017 min
Response: 2327393
Conc: 0.73 ng/ml

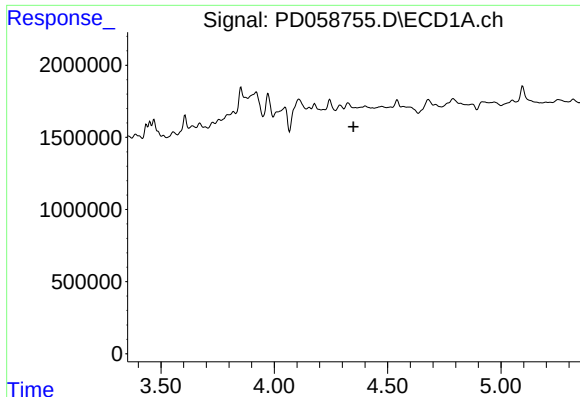

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.350 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

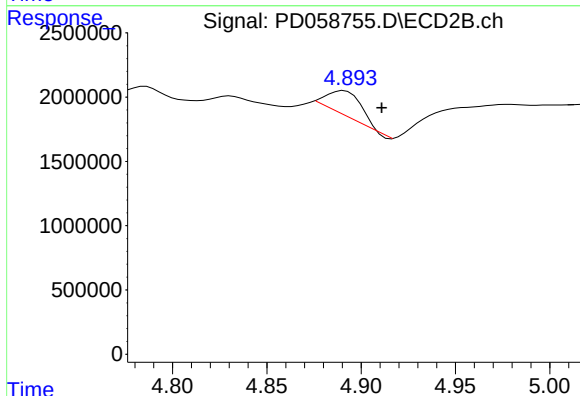


#7 delta-BHC

R.T.: 4.891 min
Delta R.T.: -0.020 min
Response: 2409797
Conc: 0.78 ng/ml

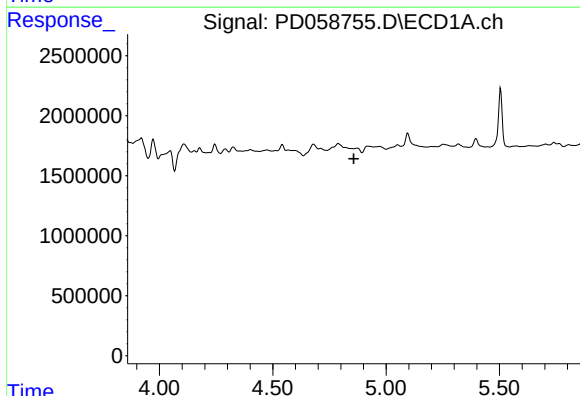


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 4.857 min
Response: 0
Conc: N.D.

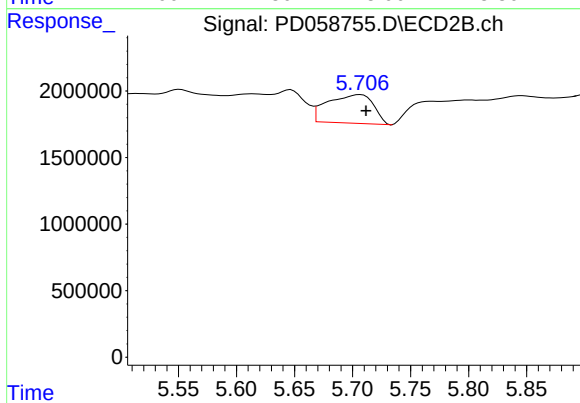

#8 Heptachlor epoxide


R.T.: 5.707 min
Delta R.T.: -0.005 min
Response: 5899177
Conc: 2.03 ng/ml

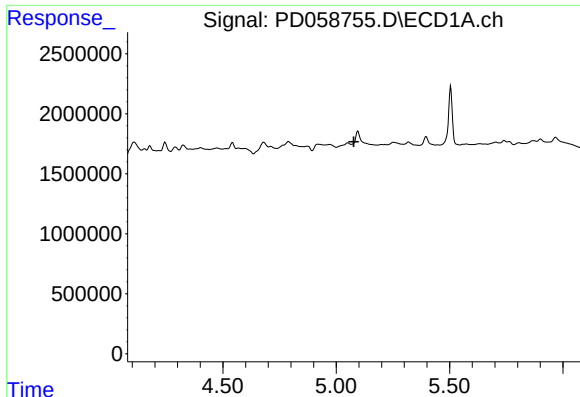

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.077 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

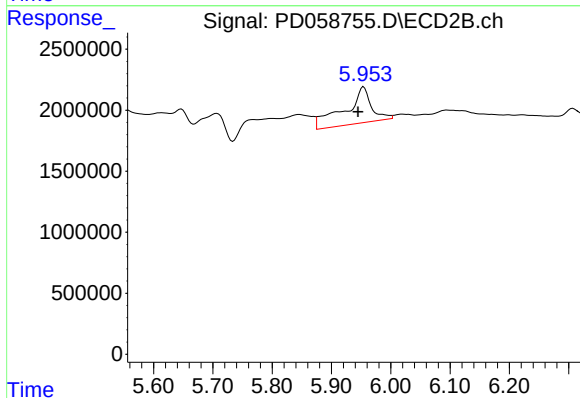


#10 gamma-Chlordane

R.T.: 5.954 min
Delta R.T.: 0.010 min
Response: 9211608
Conc: 3.17 ng/ml

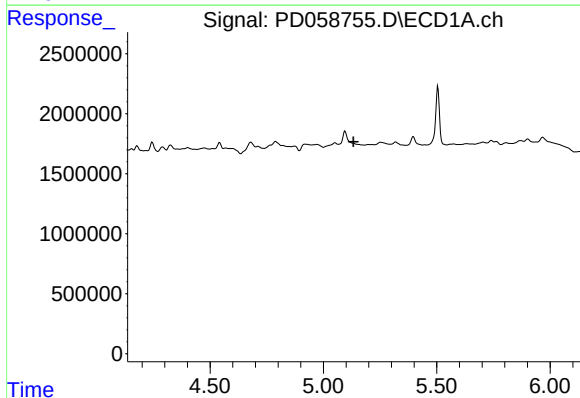


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.133 min
Response: 0
Conc: N.D.

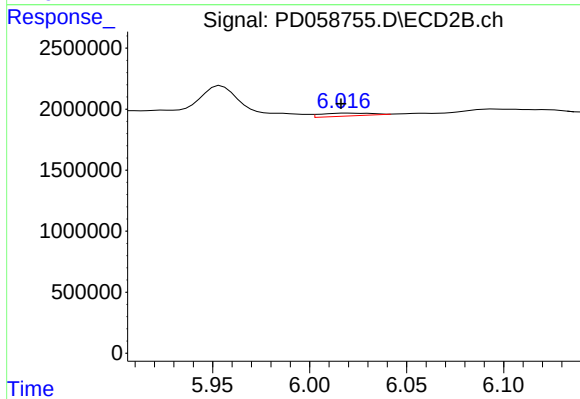

#11 alpha-Chlordane


R.T.: 6.019 min
Delta R.T.: 0.003 min
Response: 417349
Conc: 0.15 ng/ml

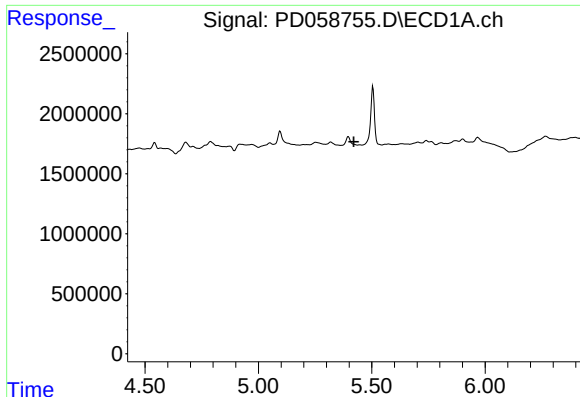

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.421 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

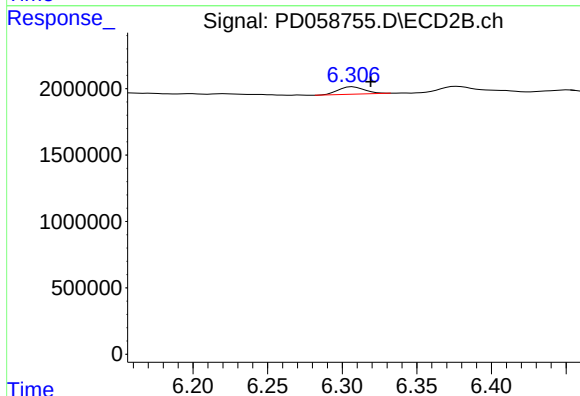


#13 Dieldrin

R.T.: 6.307 min
Delta R.T.: -0.012 min
Response: 695623
Conc: 0.24 ng/ml

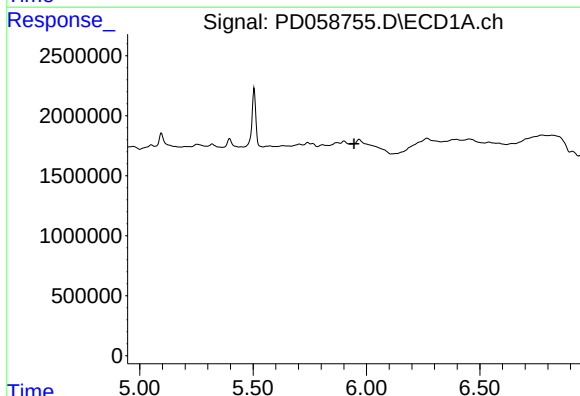


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 5.946 min
Response: 0
Conc: N.D.

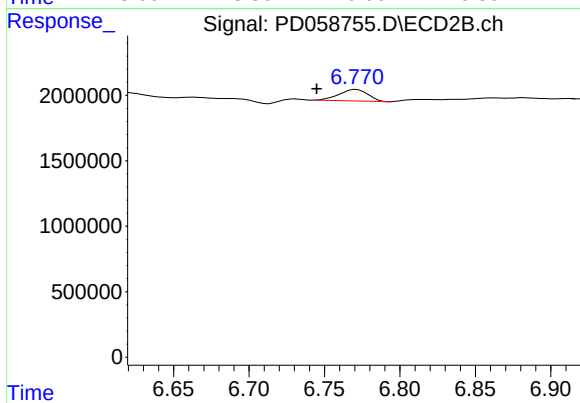

#15 Endosulfan II


R.T.: 6.771 min
Delta R.T.: 0.026 min
Response: 1173577
Conc: 0.48 ng/ml

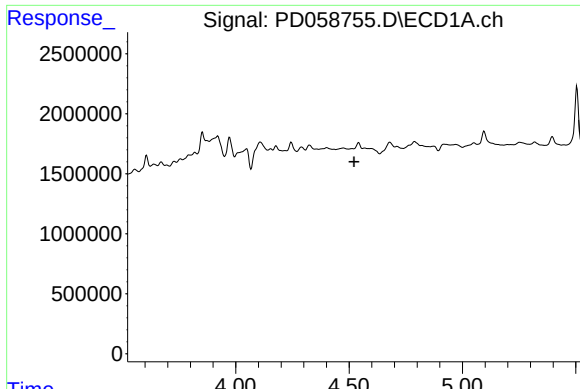

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.522 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

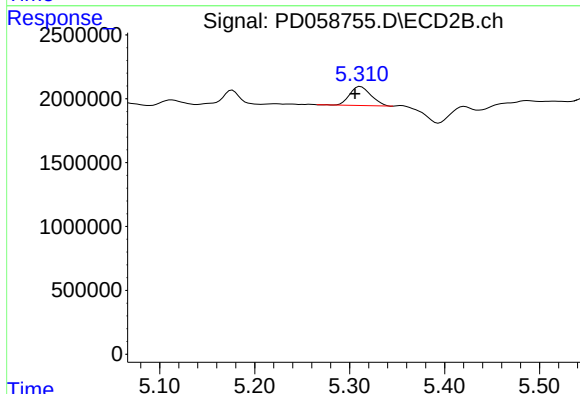


#24 Chlordane-2

R.T.: 5.311 min
Delta R.T.: 0.006 min
Response: 2327393
Conc: 23.56 ng/ml

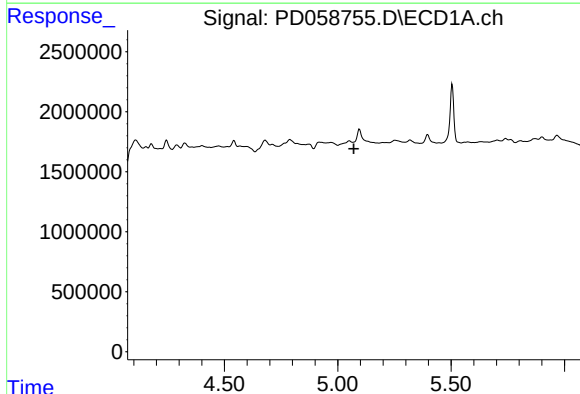


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.070 min
Response: 0
Conc: N.D.

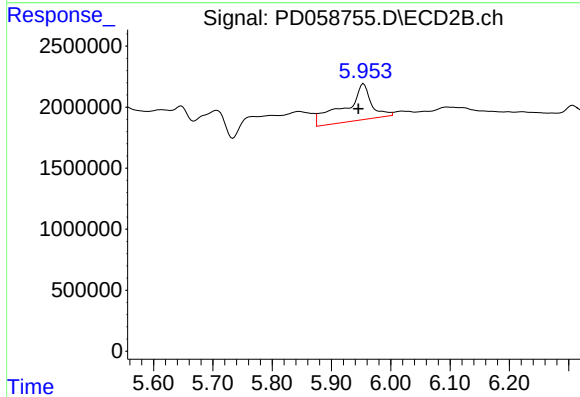

#25 Chlordane-3


R.T.: 5.954 min
Delta R.T.: 0.009 min
Response: 9211608
Conc: 24.77 ng/ml

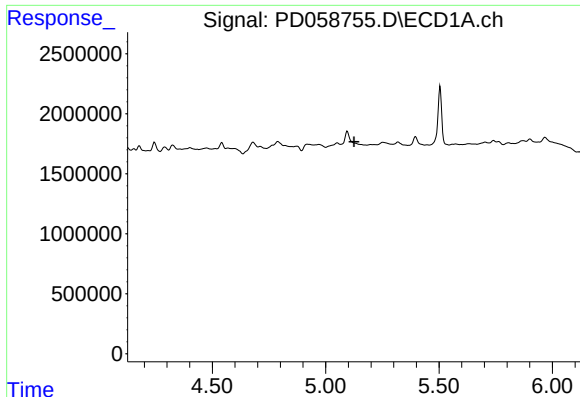

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.126 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

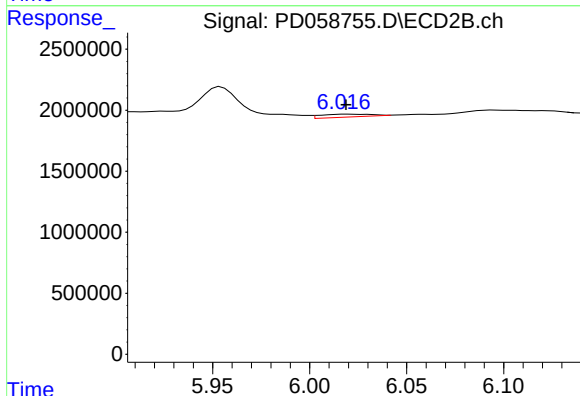


#26 Chlordane-4

R.T.: 6.019 min
Delta R.T.: 0.000 min
Response: 417349
Conc: 0.96 ng/ml

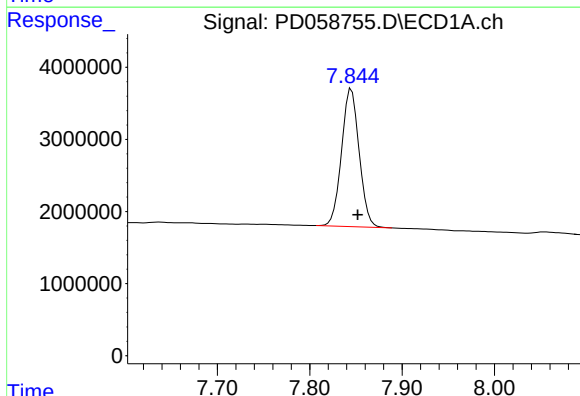

#28 Decachlorobiphenyl

R.T.: 7.845 min
Delta R.T.: -0.007 min
Response: 25327267
Conc: 14.03 ng/ml

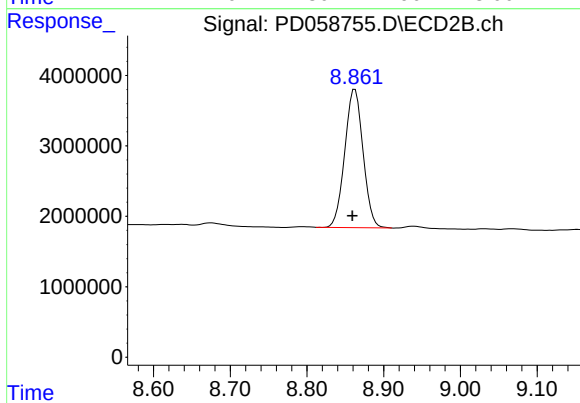

#28 Decachlorobiphenyl

R.T.: 8.863 min
Delta R.T.: 0.003 min
Response: 32649507
Conc: 14.97 ng/ml