

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072820\
 Data File : PD058764.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jul 2020 19:20
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 04:22:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 08 08:01:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.866	28579109	41856310	15.674	16.941
28)	SA Decachlor...	7.845	8.861	31514448	41392321	17.451	18.985
Target Compounds							
8)	B Heptachlo...	0.000	5.709	0	2949229	N.D.	1.013 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072820\
Data File : PD058764.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jul 2020 19:20
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 04:22:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
Quant Title : GC Extractables
QLast Update : Wed Jul 08 08:01:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

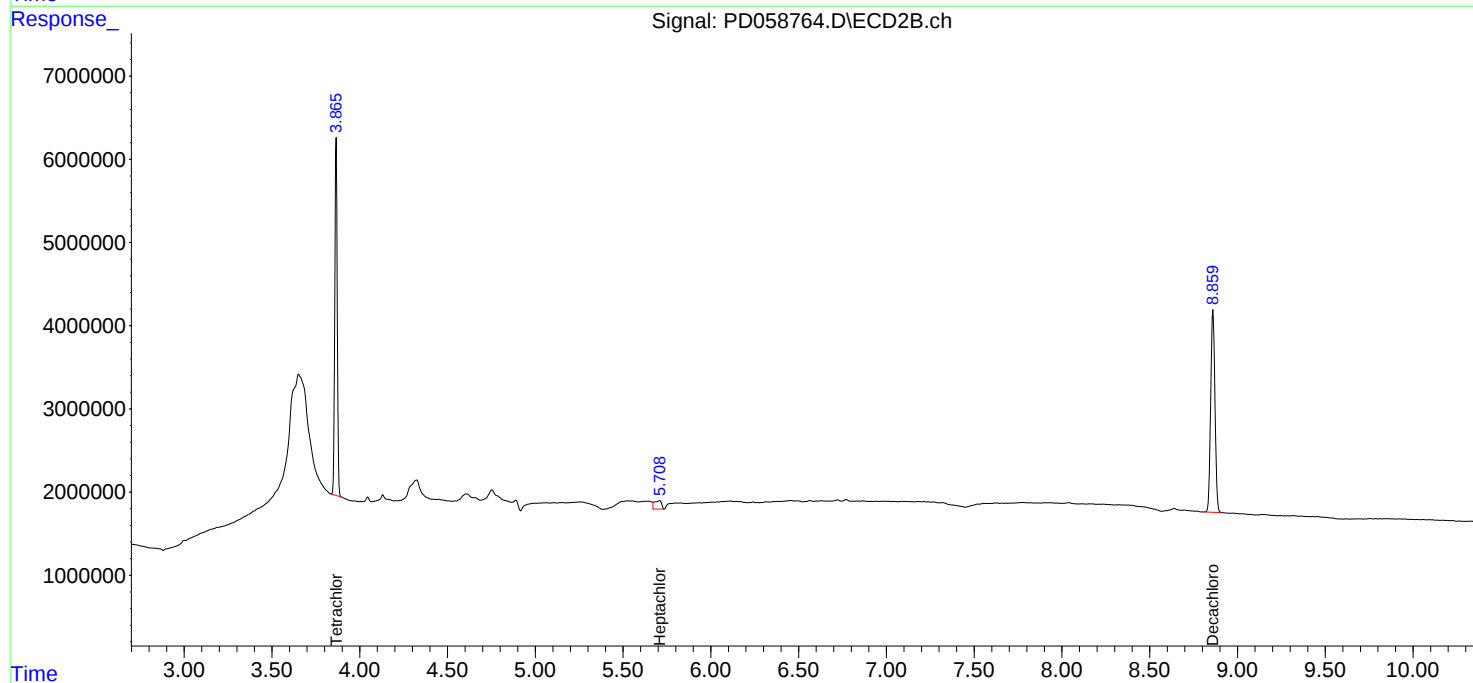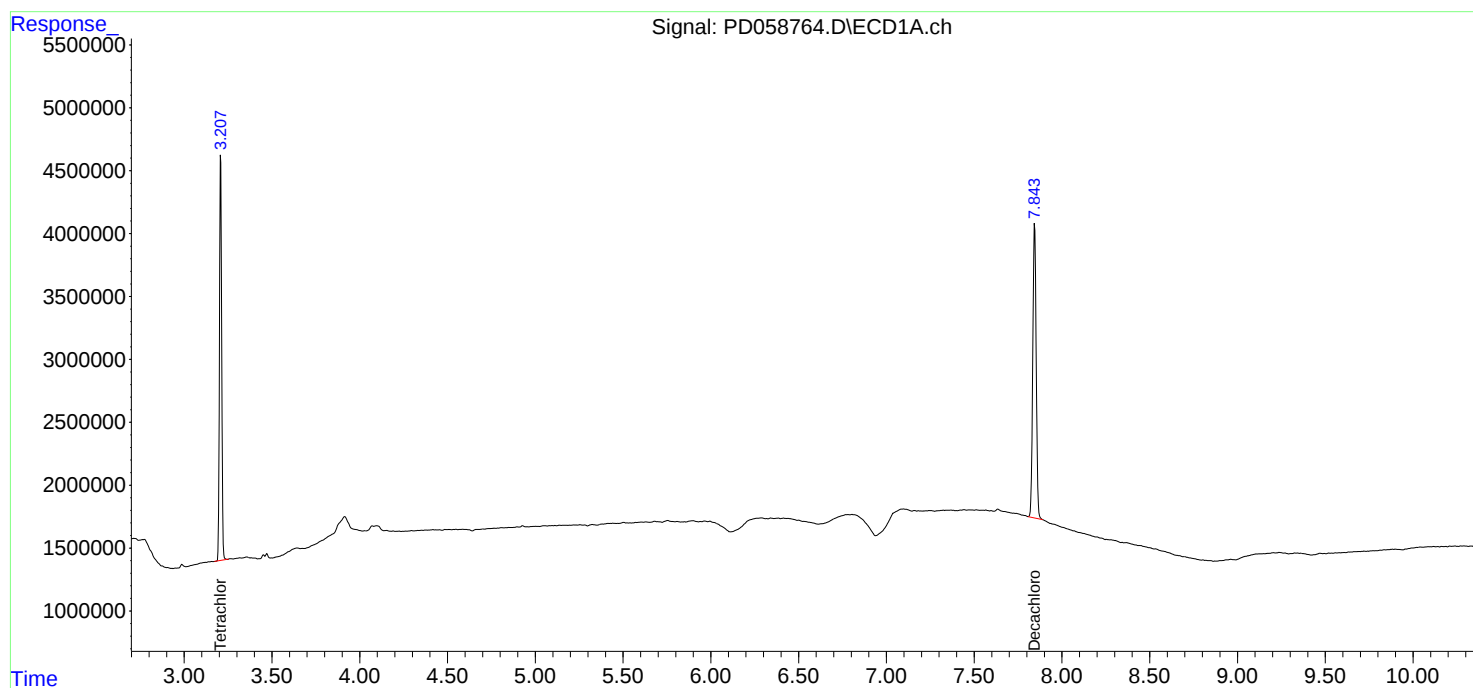


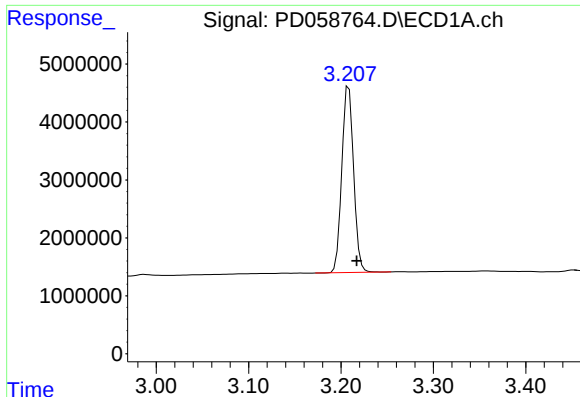

#1 Tetrachloro-m-xylene


R.T.: 3.209 min
Delta R.T.: -0.008 min
Response: 28579109
Conc: 15.67 ng/ml

Instrument :
ECD_D
ClientSampleId :

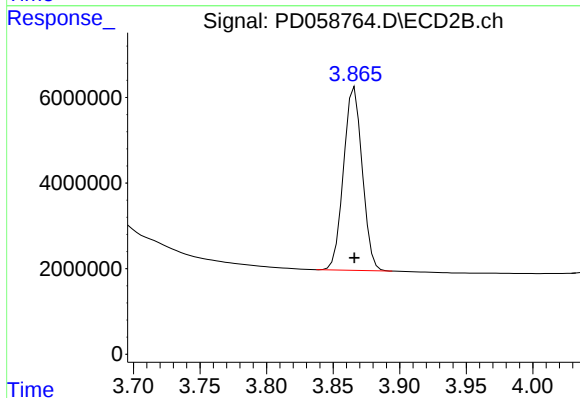


#1 Tetrachloro-m-xylene

R.T.: 3.866 min
Delta R.T.: 0.000 min
Response: 41856310
Conc: 16.94 ng/ml

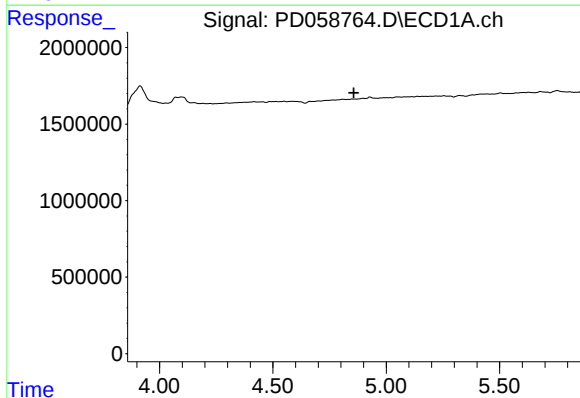


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.857 min
Response: 0
Conc: N.D.

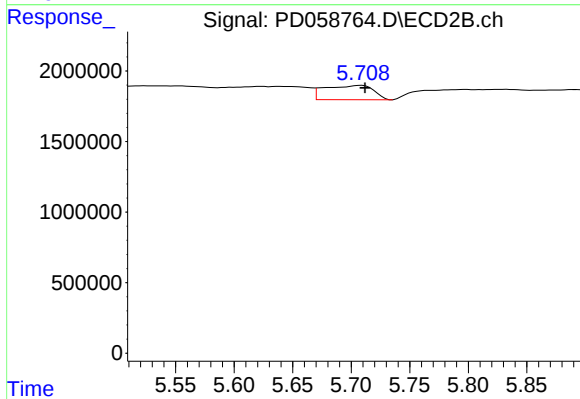

#8 Heptachlor epoxide


R.T.: 5.709 min
Delta R.T.: -0.002 min
Response: 2949229
Conc: 1.01 ng/ml

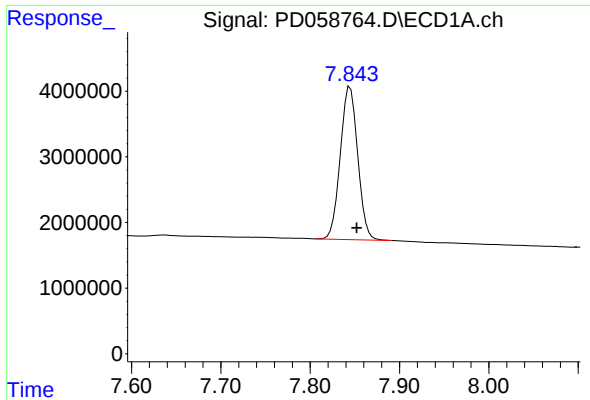

#28 Decachlorobiphenyl

R.T.: 7.845 min
Delta R.T.: -0.007 min
Response: 31514448
Conc: 17.45 ng/ml

Instrument :
ECD_D
ClientSampleId :

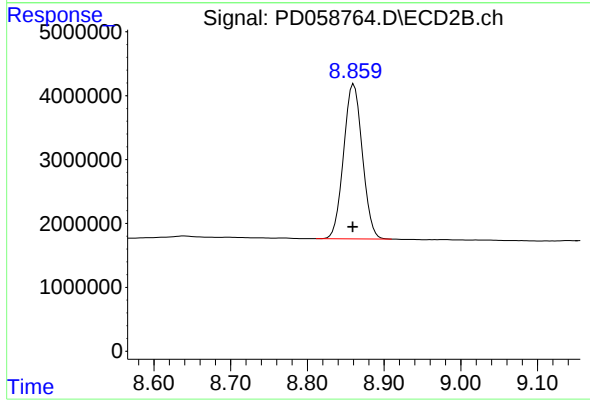

#28 Decachlorobiphenyl

R.T.: 8.861 min
Delta R.T.: 0.001 min
Response: 41392321
Conc: 18.98 ng/ml