

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072820\
 Data File : PD058770.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jul 2020 20:59
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 04:23:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 08 08:01:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.208	3.867	28823338	41117268	15.808	16.641
28)	SA Decachlor...	7.844	8.862	26535982	31802210	14.695	14.586
Target Compounds							
8)	B Heptachlo...	0.000	5.710	0	4453053	N.D.	1.530 #
10)	B gamma-Chl...	0.000	5.927f	0	1845928	N.D.	0.634 #
20)	A Methoxychlor	0.000	7.447f	0	505456	N.D.	0.420 #
22)	Mirex	0.000	8.020	0	2209204	N.D.	1.145 #
25)	Chlordane-3	0.000	5.927f	0	1845928	N.D.	4.963 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072820\
Data File : PD058770.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jul 2020 20:59
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 04:23:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
Quant Title : GC Extractables
QLast Update : Wed Jul 08 08:01:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

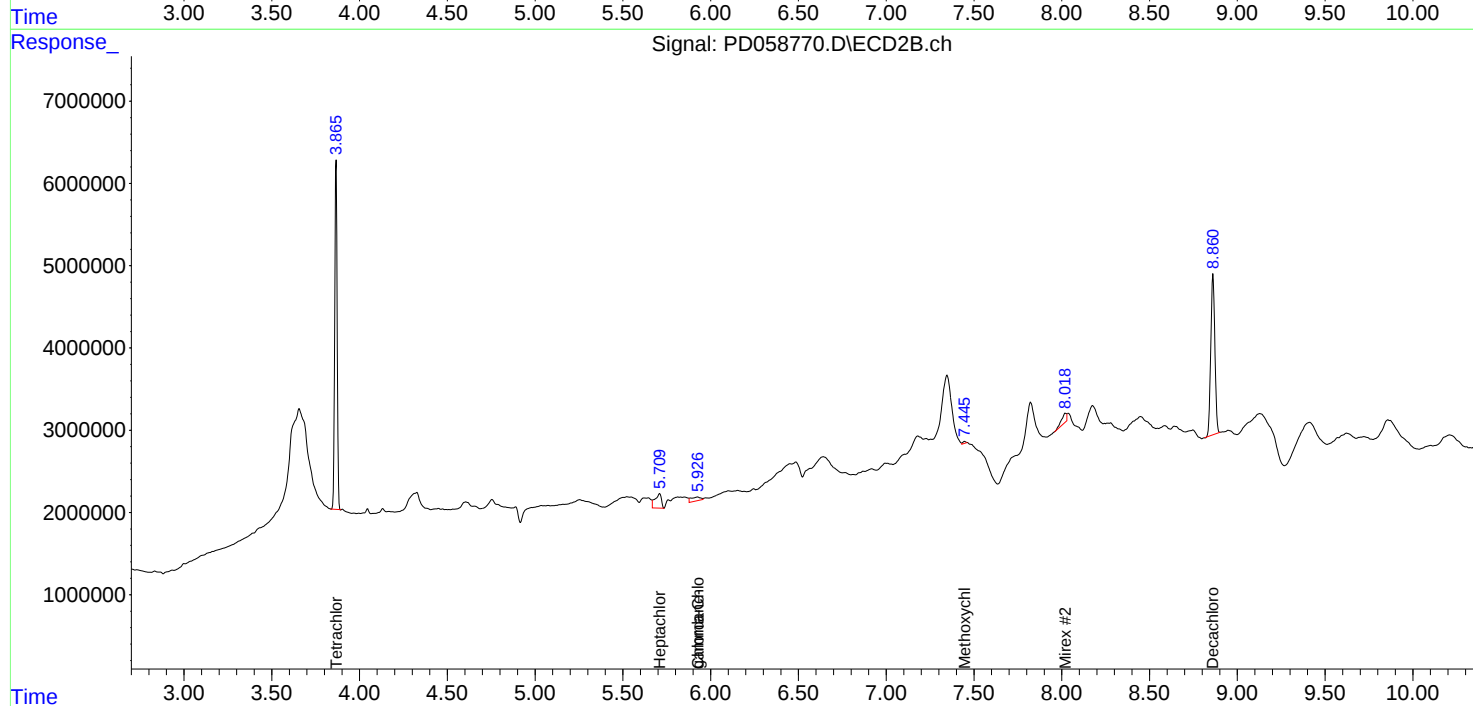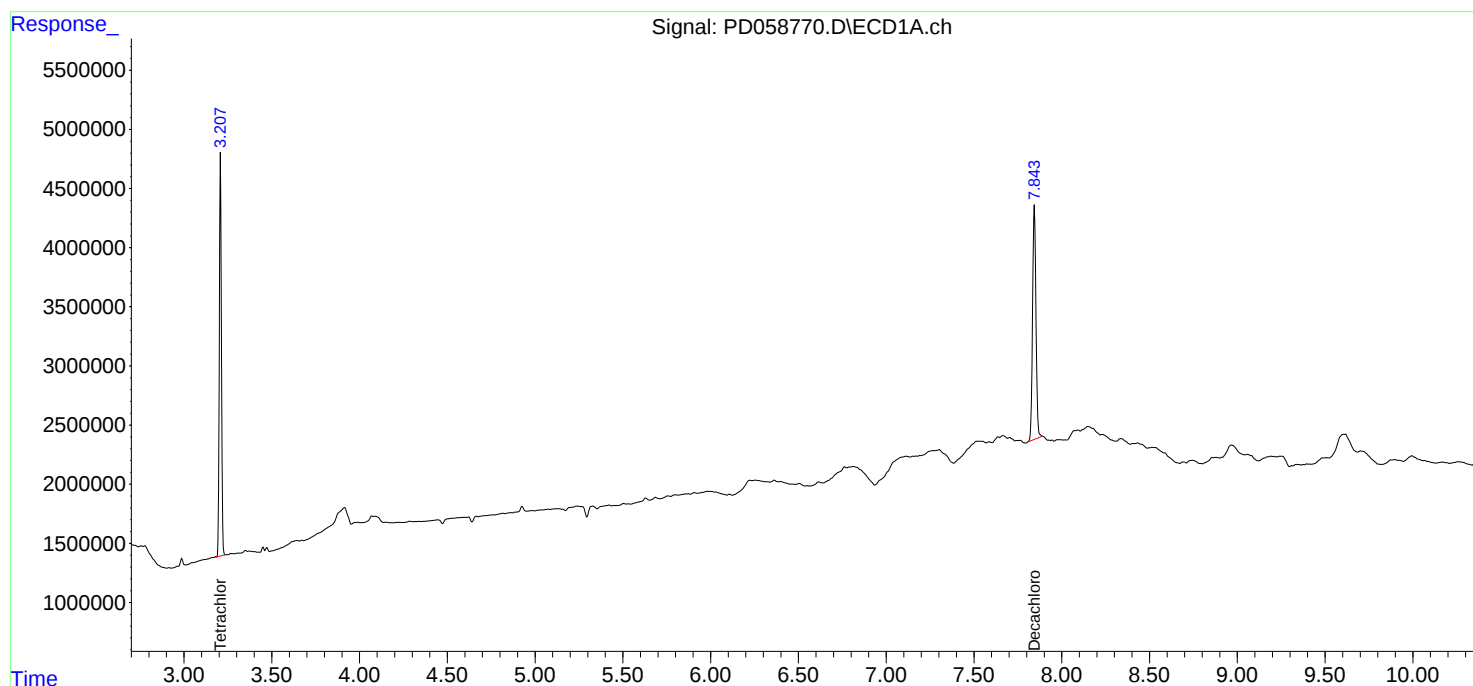


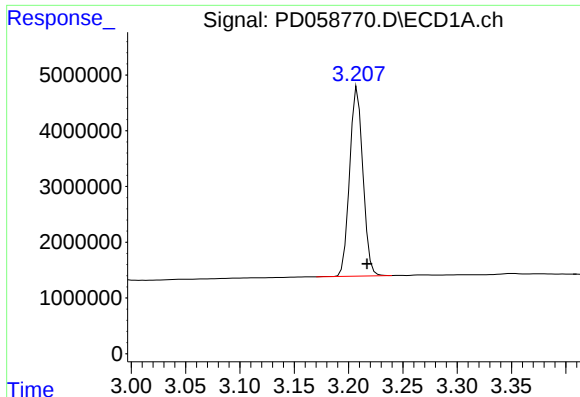

#1 Tetrachloro-m-xylene


R.T.: 3.208 min
Delta R.T.: -0.009 min
Response: 2882338
Conc: 15.81 ng/ml

Instrument :
ECD_D
ClientSampleId :

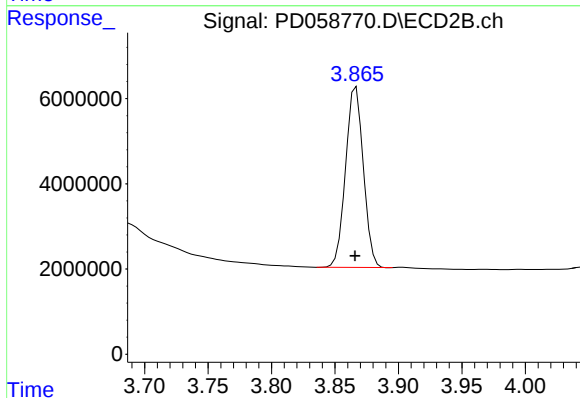


#1 Tetrachloro-m-xylene

R.T.: 3.867 min
Delta R.T.: 0.000 min
Response: 41117268
Conc: 16.64 ng/ml

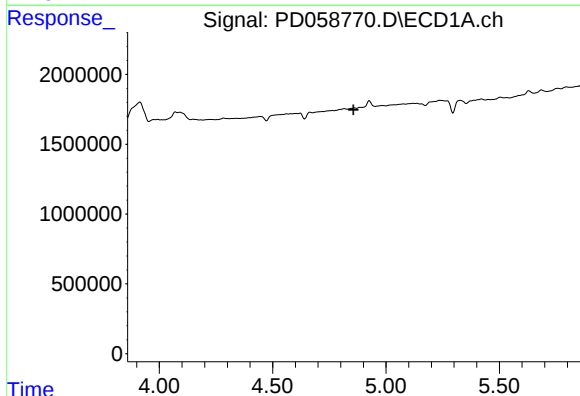


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.857 min
Response: 0
Conc: N.D.

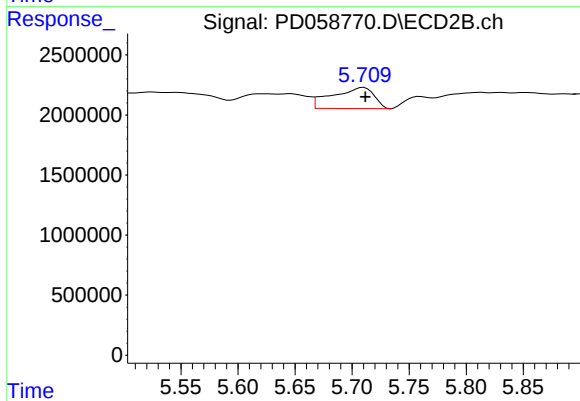

#8 Heptachlor epoxide


R.T.: 5.710 min
Delta R.T.: -0.001 min
Response: 4453053
Conc: 1.53 ng/ml

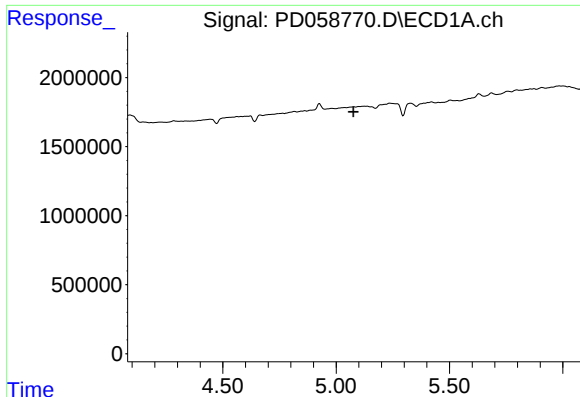

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.077 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

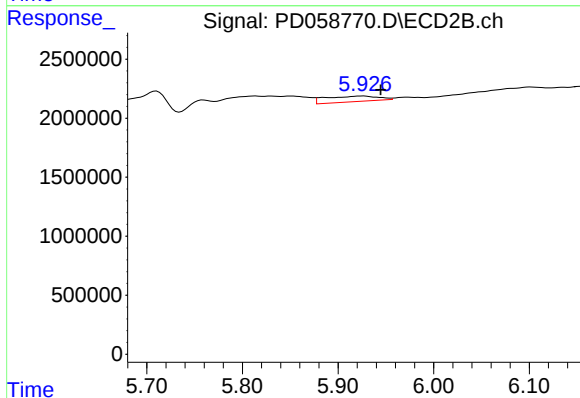


#10 gamma-Chlordane

R.T.: 5.927 min
Delta R.T.: -0.018 min
Response: 1845928
Conc: 0.63 ng/ml

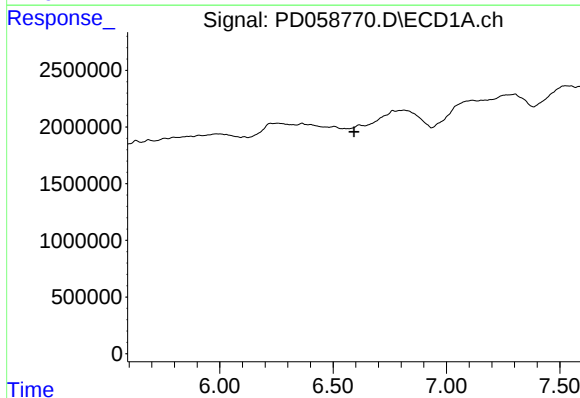


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 6.592 min
Response: 0
Conc: N.D.

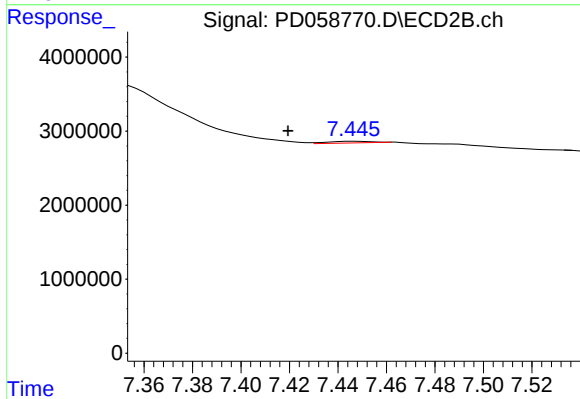

#20 Methoxychlor


R.T.: 7.447 min
Delta R.T.: 0.027 min
Response: 505456
Conc: 0.42 ng/ml

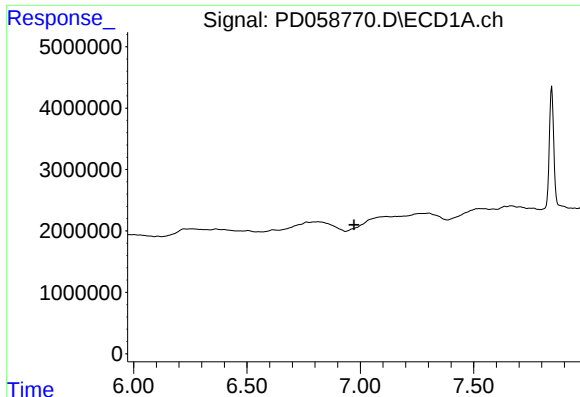

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 6.973 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

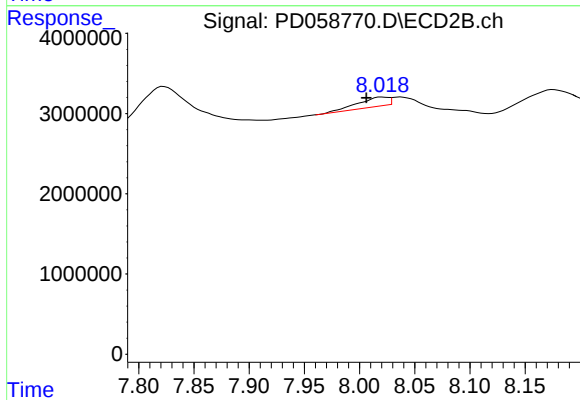


#22 Mirex

R.T.: 8.020 min
Delta R.T.: 0.014 min
Response: 2209204
Conc: 1.15 ng/ml

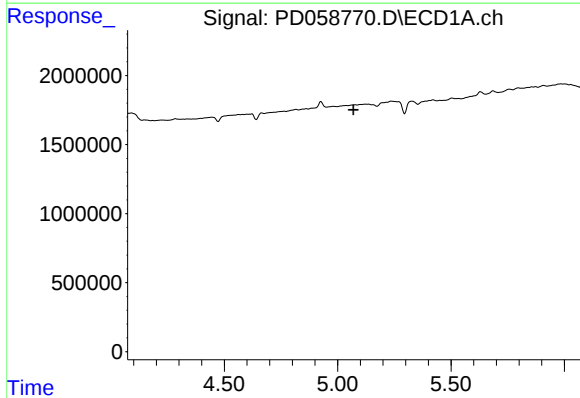


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.070 min
Response: 0
Conc: N.D.

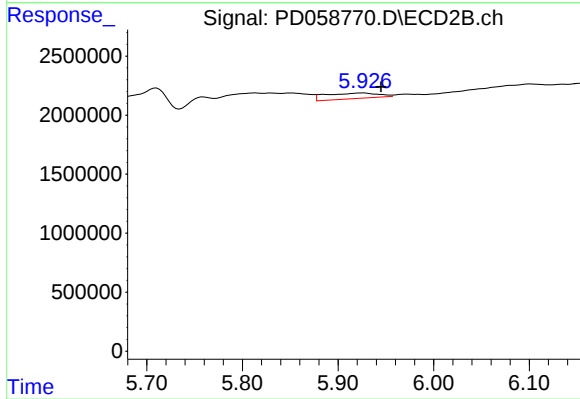

#25 Chlordane-3


R.T.: 5.927 min
Delta R.T.: -0.019 min
Response: 1845928
Conc: 4.96 ng/ml

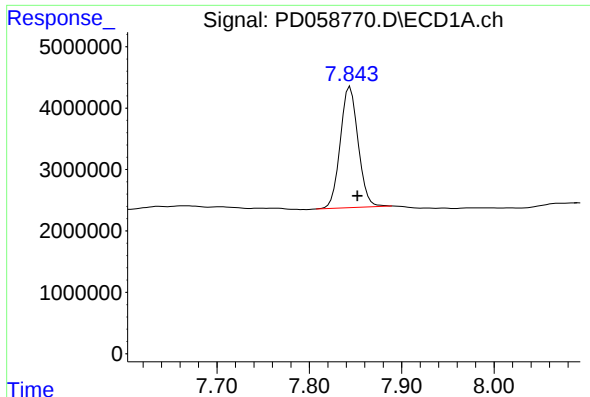

#28 Decachlorobiphenyl

R.T.: 7.844 min
Delta R.T.: -0.008 min
Response: 26535982
Conc: 14.69 ng/ml

Instrument :
ECD_D
ClientSampleId :

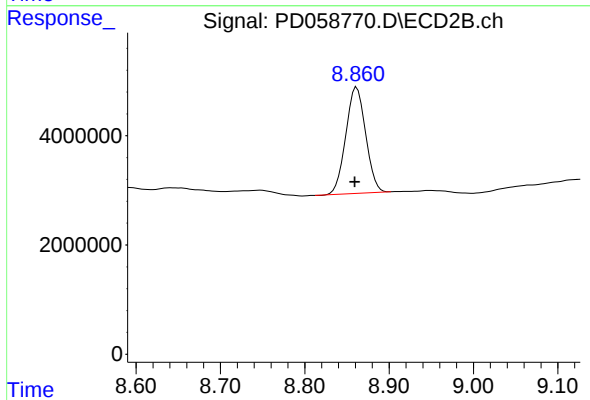

#28 Decachlorobiphenyl

R.T.: 8.862 min
Delta R.T.: 0.002 min
Response: 31802210
Conc: 14.59 ng/ml