

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072820\
 Data File : PD058747.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jul 2020 15:19
 Operator : AJ\MA
 Sample : L3185-01 10X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PL-05-072720

Manual Integrations
 APPROVED

Ankita
 7/29/2020 4:36:56 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 04:18:48 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 08 08:01:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.207	3.865	1806834	2280321	0.991m	0.923
28)	SA Decachlor...	7.842	8.860	2568616	2978069	1.422m	1.366
Target Compounds							
10)	B gamma-Chl...	5.068	5.942	697978	2783867	0.314m	0.957m#
11)	B alpha-Chl...	5.122	6.018	1287121	2860930	0.581m	0.995m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072820\
Data File : PD058747.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jul 2020 15:19
Operator : AJ\MA
Sample : L3185-01 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
PL-05-072720


Manual Integrations
APPROVED

Ankita
7/29/2020 4:36:56 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 04:18:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070720.M
Quant Title : GC Extractables
QLast Update : Wed Jul 08 08:01:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

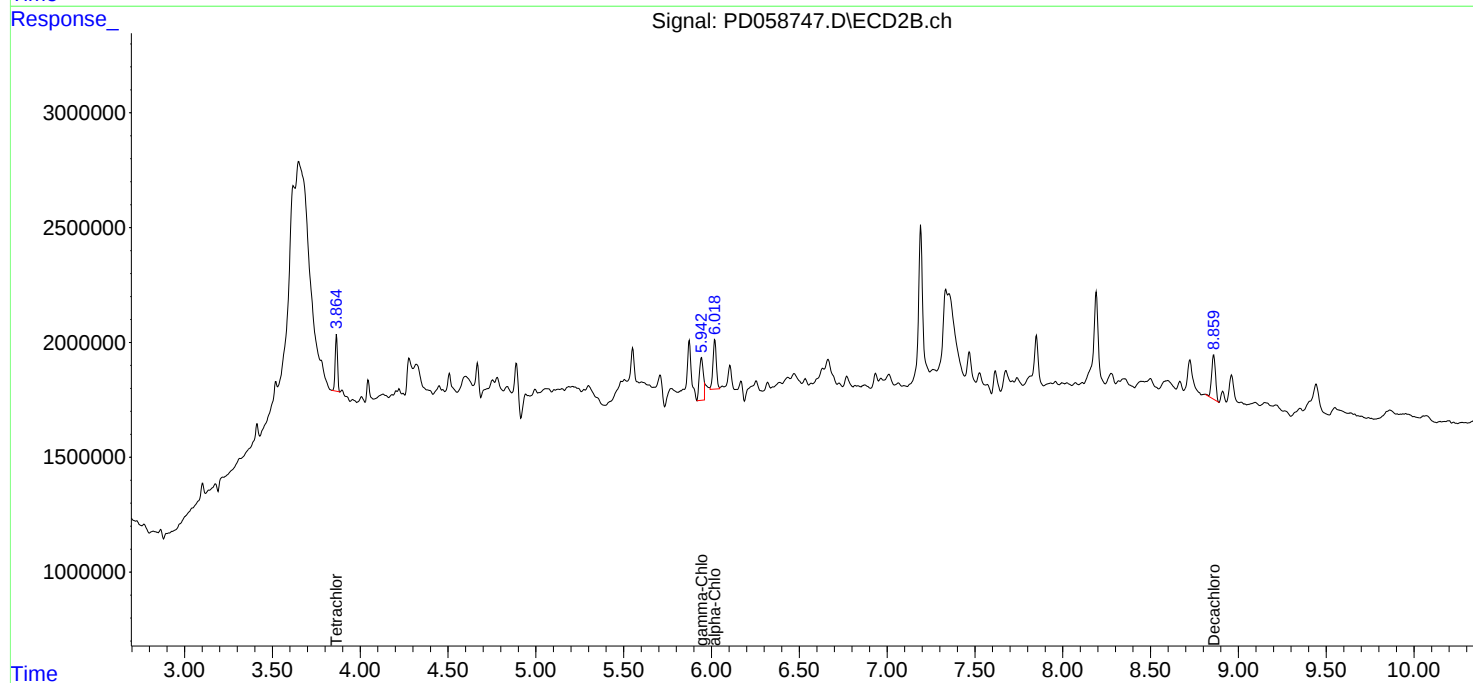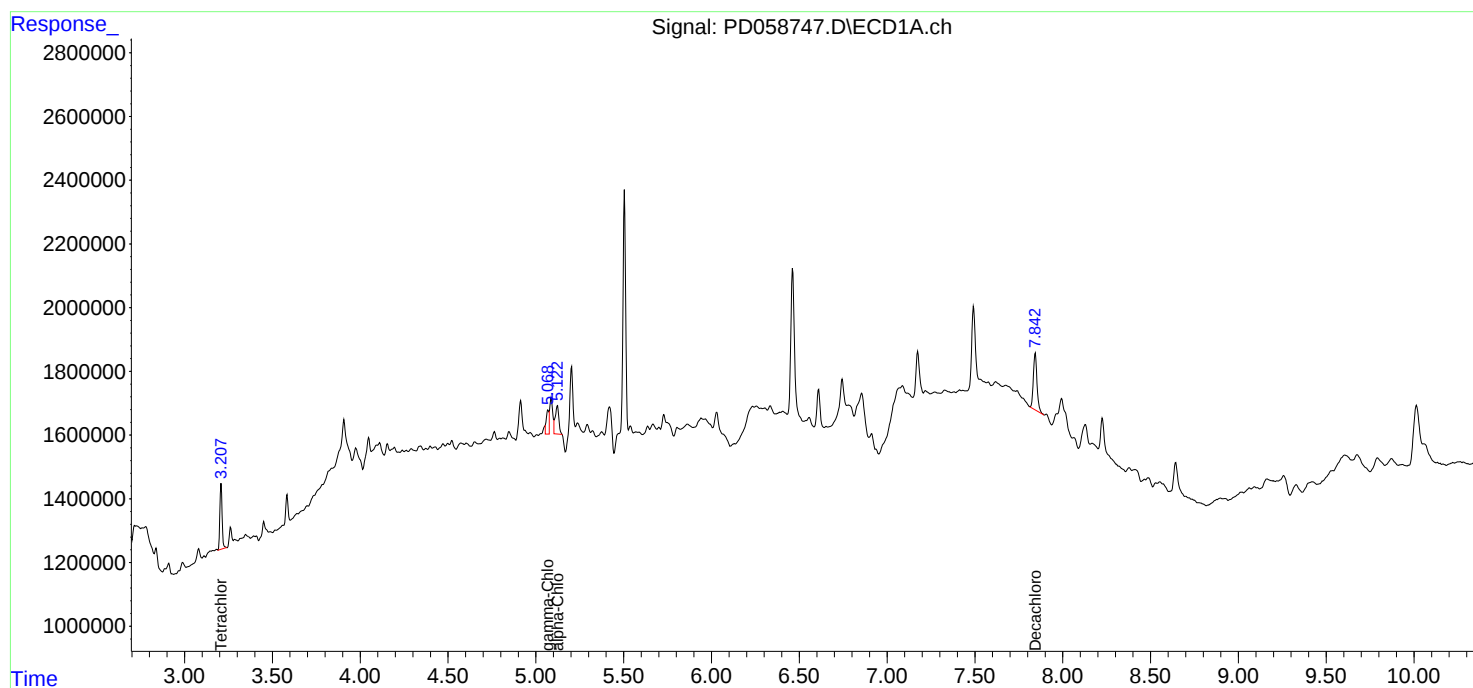

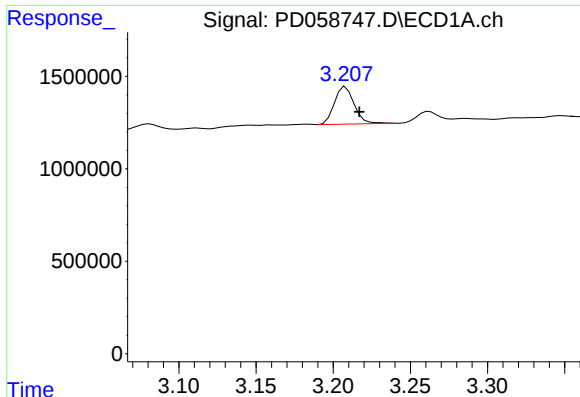


#1 Tetrachloro-m-xylene

R.T.: 3.207 min
Delta R.T.: -0.010 min
Response: 1806834
Conc: 0.99 ng/ml m

Instrument :
ECD_D
ClientSampleId :
PL-05-072720


Manual Integrations
APPROVED

Ankita
7/29/2020 4:36:56 PM

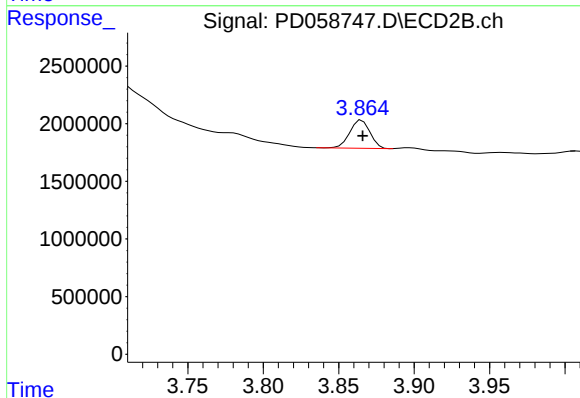


#1 Tetrachloro-m-xylene

R.T.: 3.865 min
Delta R.T.: 0.000 min
Response: 2280321
Conc: 0.92 ng/ml

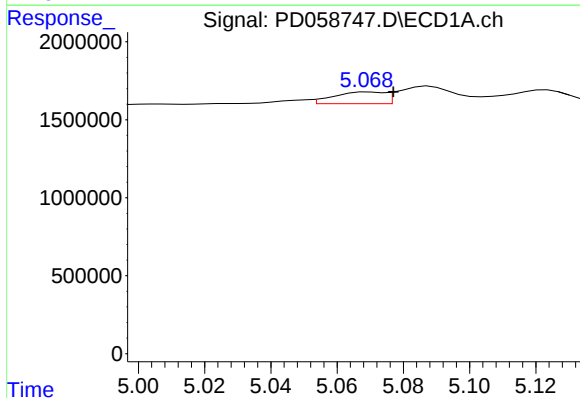


#10 gamma-Chlordane

R.T.: 5.068 min
Delta R.T.: -0.009 min
Response: 697978
Conc: 0.31 ng/ml m

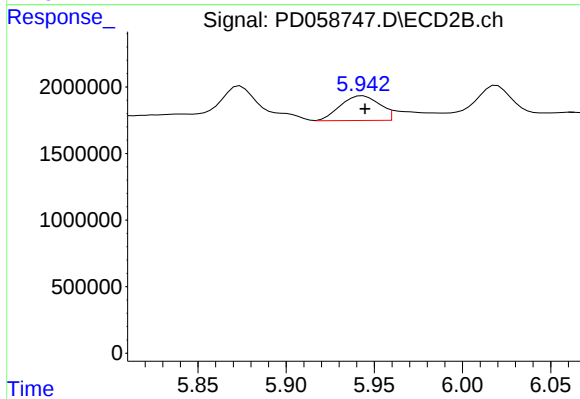

#10 gamma-Chlordane

R.T.: 5.942 min
Delta R.T.: -0.003 min
Response: 2783867
Conc: 0.96 ng/ml m

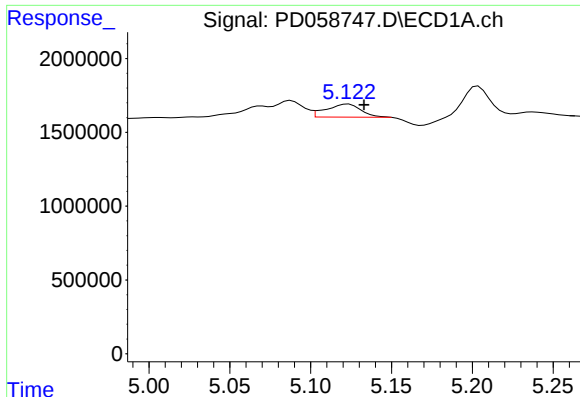


#11 alpha-Chlordane

R.T.: 5.122 min
Delta R.T.: -0.011 min
Response: 1287121
Conc: 0.58 ng/ml m

Instrument :
ECD_D
ClientSampleId :
PL-05-072720


Manual Integrations
APPROVED

Ankita
7/29/2020 4:36:56 PM

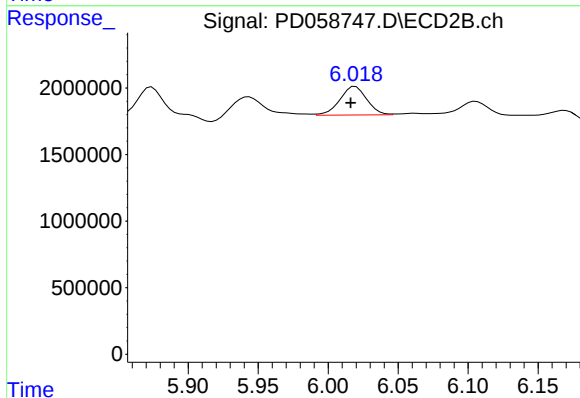


#11 alpha-Chlordane

R.T.: 6.018 min
Delta R.T.: 0.002 min
Response: 2860930
Conc: 0.99 ng/ml m

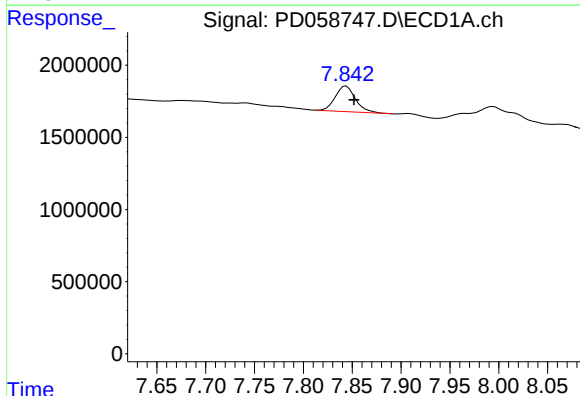

#28 Decachlorobiphenyl

R.T.: 7.842 min
Delta R.T.: -0.010 min
Response: 2568616
Conc: 1.42 ng/ml m

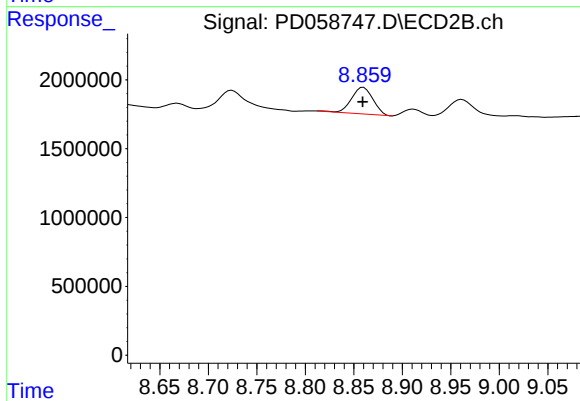

#28 Decachlorobiphenyl

R.T.: 8.860 min
Delta R.T.: 0.000 min
Response: 2978069
Conc: 1.37 ng/ml