

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072821\
 Data File : PD064498.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2021 06:18
 Operator : AR\AJ
 Sample : M3084-07
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0025

Manual Integrations
 APPROVED

mohammad
 7/30/2021 2:28:06 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 06:50:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 28 07:07:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	5.406	4.618	18730814	141.4E6	15.702	15.475m
27)	SA Decachlor...	11.307	10.364	44679942	172.2E6	33.941m	28.953
Target Compounds							
3)	MA gamma-BHC...	6.396	5.736	2035006	110.0E6	1.298	9.643 #
6)	B beta-BHC	6.640	6.124	687843	56047811	0.882	9.238m#
12)	B 4,4'-DDE	8.435	7.607	19638383	30746200	13.625m	4.075m#
13)	MA Dieldrin	8.571	7.740	58594948	137.2E6	39.292m	17.078m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072821\
Data File : PD064498.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jul 2021 06:18
Operator : AR\AJ
Sample : M3084-07
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 06:50:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 28 07:07:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

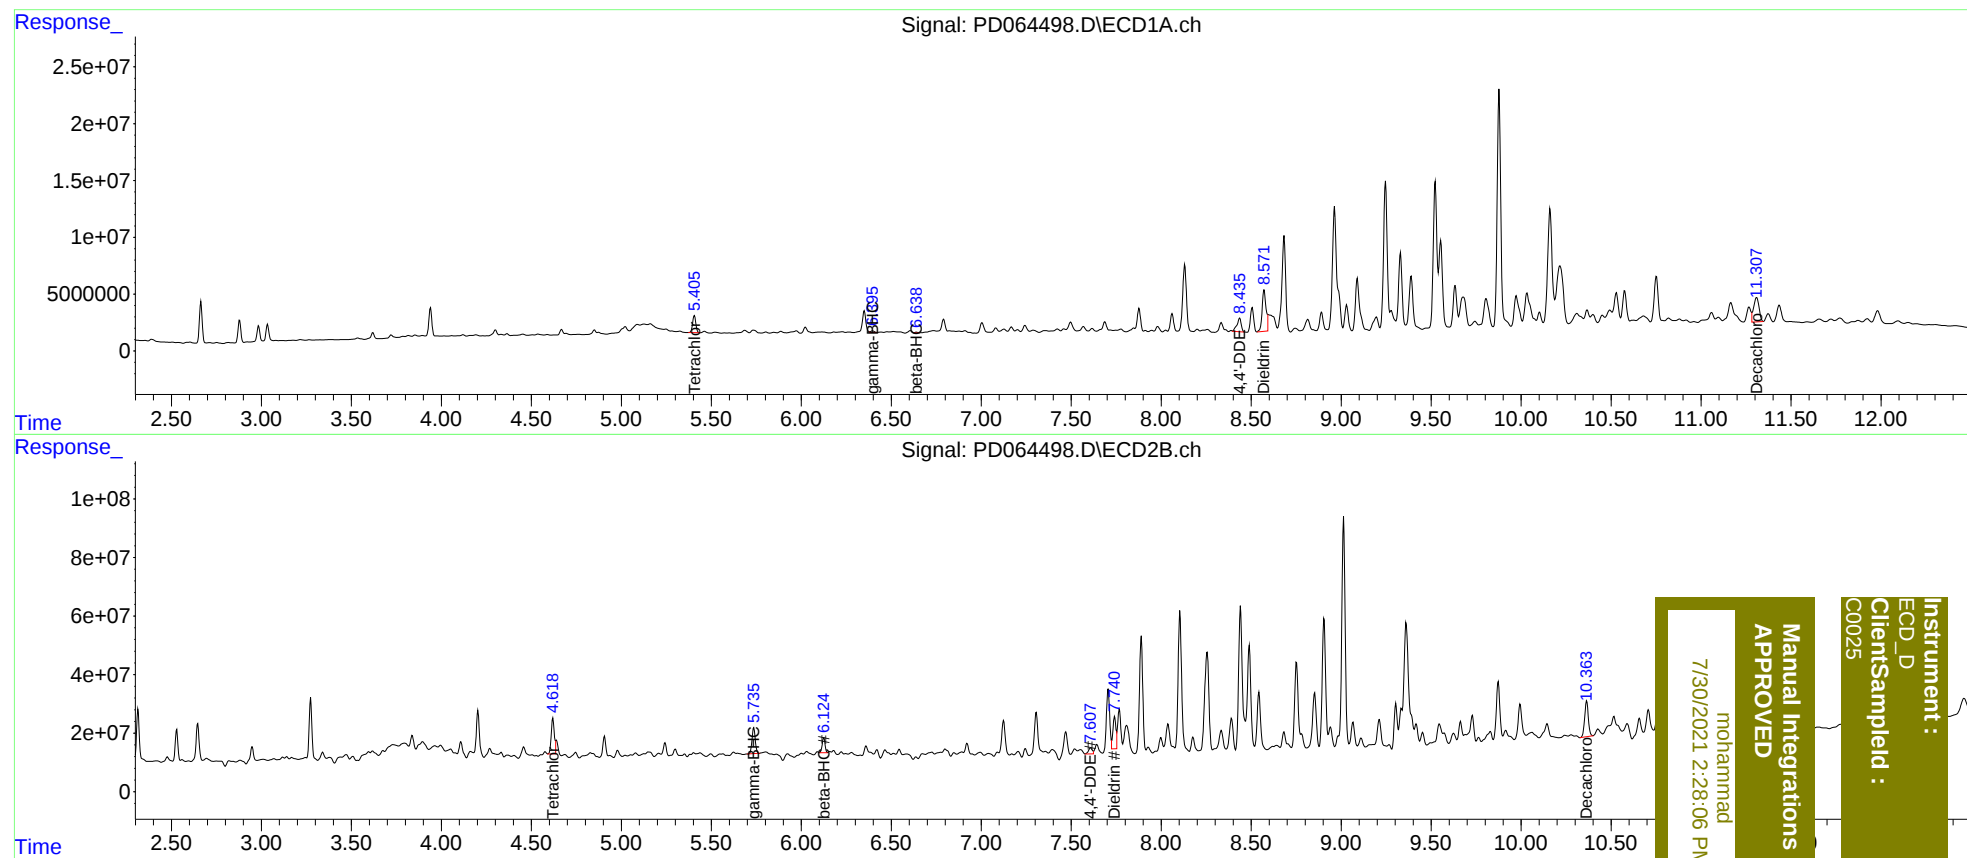

Manual Integrations
APPROVED

mohammad
7/30/2021 2:28:06 PM

Instrument :
ECD_D
ClientSampled :
C0025