

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072821\
Data File : PD064483.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jul 2021 02:20
Operator : AR\AJ
Sample : INDA335
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_D
LabSampleId :
INDA335

Manual Integrations
APPROVED

mohammad
7/30/2021 2:24:03 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 06:11:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 28 07:07:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

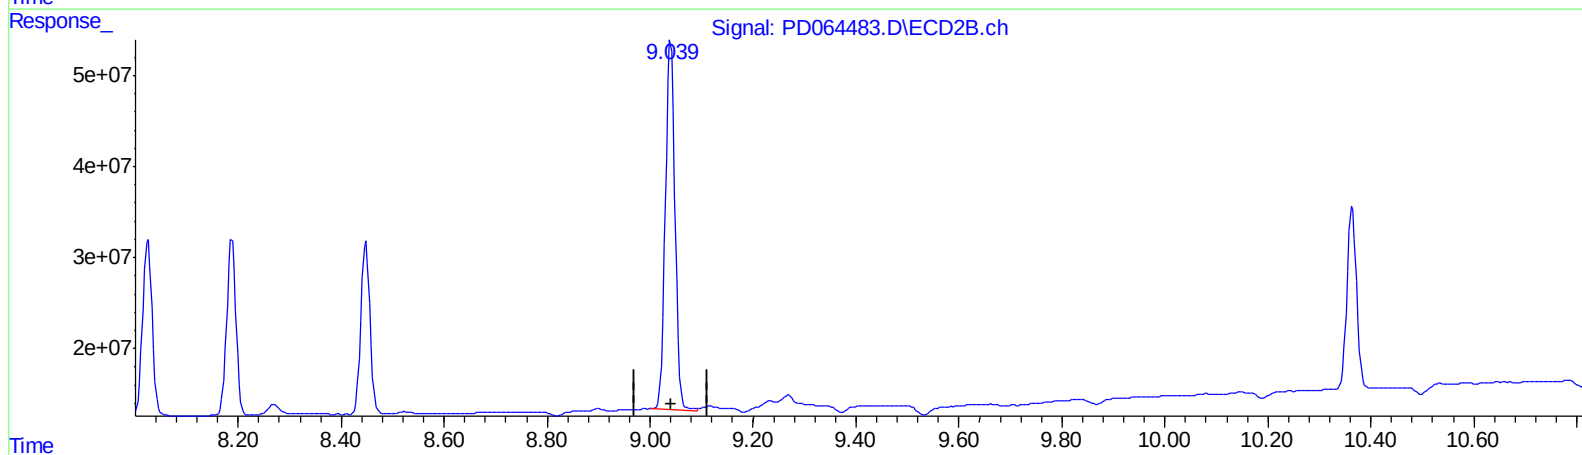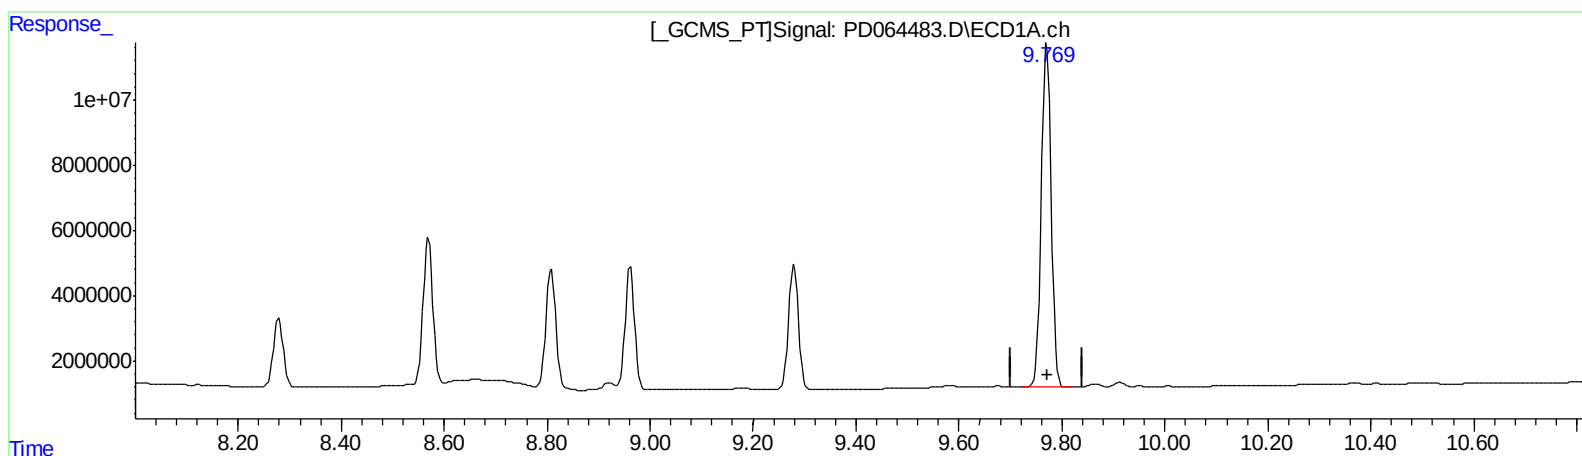

QEdit

(20) Methoxychlor (A)
9.771min 197.610 ng/ml
response 141402199

(20) Methoxychlor #2 (A)
9.040min 207.287 ng/ml
response 530778836

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072821\
Data File : PD064483.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jul 2021 02:20
Operator : AR\AJ
Sample : INDA335
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_D
LabSampleId :
INDA335

Manual Integrations
APPROVED

mohammad
7/30/2021 2:24:03 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 06:11:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 28 07:07:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

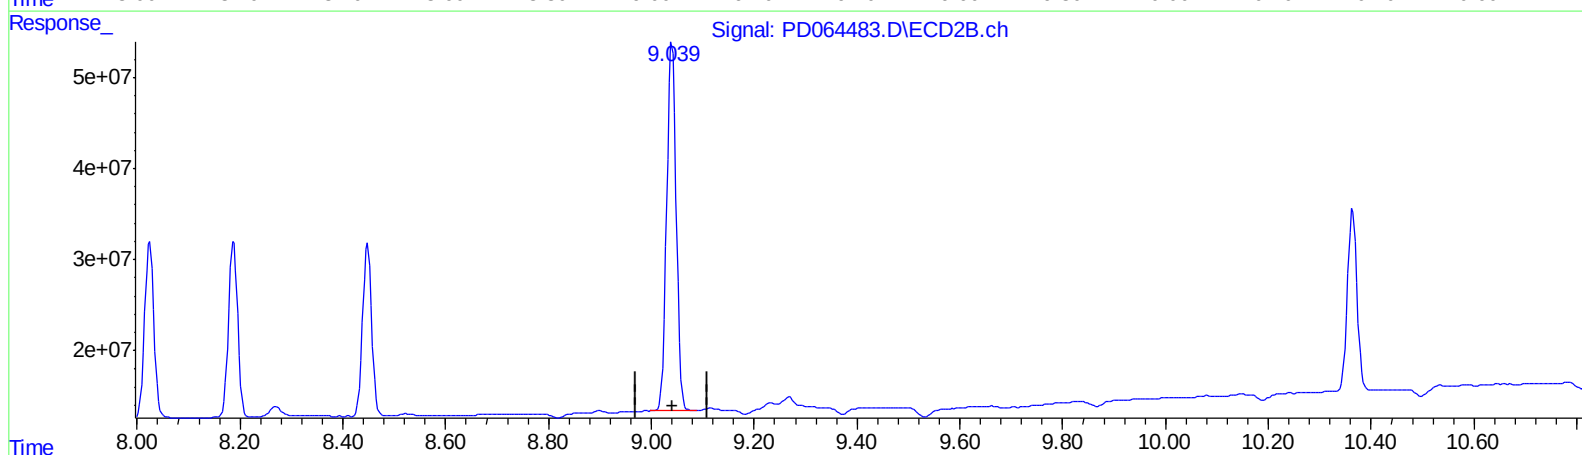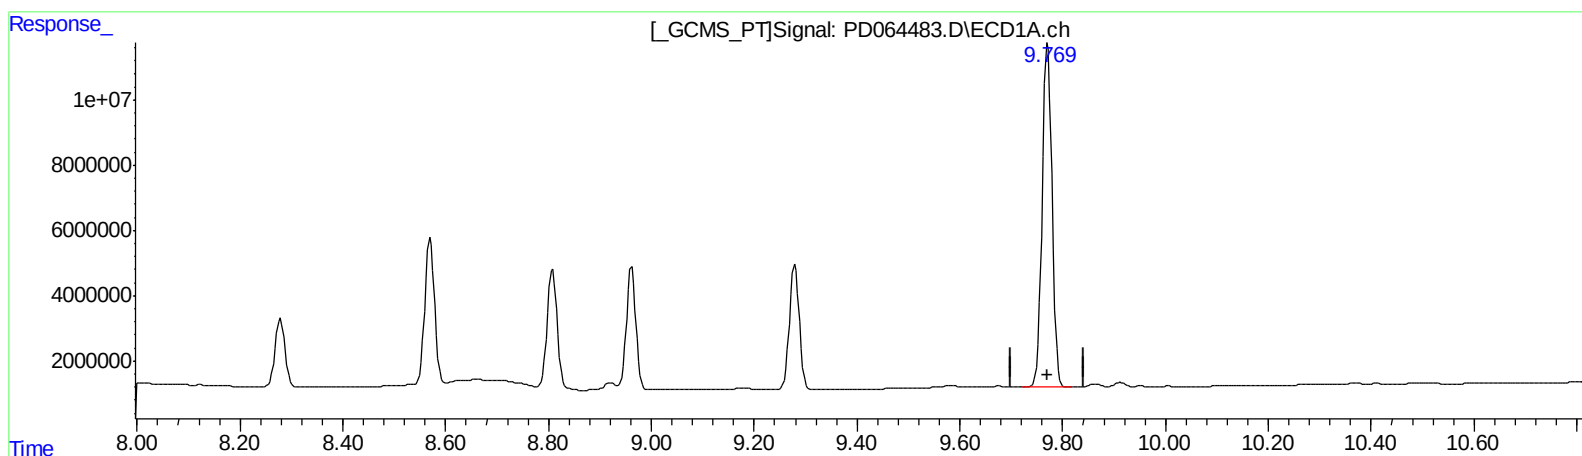

QEdit

(20) Methoxychlor (A)
9.771min 197.610 ng/ml
response 141402199

(20) Methoxychlor #2 (A)
9.039min 204.725 ng/ml m
response 524219039

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072821\
 Data File : PD064483.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2021 02:20
 Operator : AR\AJ
 Sample : INDA335
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_D
 LabSampleId :
 INDA335

Manual Integrations
 APPROVED

mohammad
 7/30/2021 2:24:03 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 06:11:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 28 07:07:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.406	4.619	24381124	201.4E6	20.439	22.037
27) SA Decachlor...	11.305	10.364	52859697	260.3E6	40.155	43.772
Target Compounds						
2) A alpha-BHC	5.988	5.321	32892173	269.9E6	20.191	21.901
3) MA gamma-BHC...	6.385	5.741	32006855	251.7E6	20.408	22.068
4) MA Heptachlor	7.036	6.151	33936593	247.1E6	20.193	21.795
9) A Endosulfan I	8.279	7.449	28456679	164.2E6	20.187	21.349
13) MA Dieldrin	8.570	7.735	58859286	338.4E6	39.469	42.136
14) MA Endrin	8.808	8.025	50821728	242.7E6	39.692	42.245
16) A 4,4'-DDD	8.962	8.188	48846522	241.2E6	39.792	41.885
17) MA 4,4'-DDT	9.280	8.448	51320517	234.3E6	39.312	42.561
20) A Methoxychlor	9.771	9.039	141.4E6	524.2E6	197.610	204.725m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

AJ
 08/02/21