

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072821\
 Data File : PD064512.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2021 10:32
 Operator : AR\AJ
 Sample : M3084-21
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0040

Manual Integrations
 APPROVED

mohammad
 7/30/2021 2:28:51 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 01:36:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 28 07:07:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	5.405	4.618	16658341	143.3E6	13.965	15.684
27) SA Decachlor...	11.301	10.363	33702706	189.4E6	25.602m	31.844
Target Compounds						
12) B 4,4'-DDE	8.421	7.604	10841620	23011605	7.522	3.050 #
13) MA Dieldrin	8.569	7.739	15040381	39710357	10.086m	4.944m#
14) MA Endrin	8.813	8.037	5379179	33824254	4.201	5.888m#
15) B Endosulfa...	9.026	8.329	8461179	27316222	6.516m	4.732 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072821\
Data File : PD064512.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jul 2021 10:32
Operator : AR\AJ
Sample : M3084-21
Misc :
ALS Vial : 33 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 01:36:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 28 07:07:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

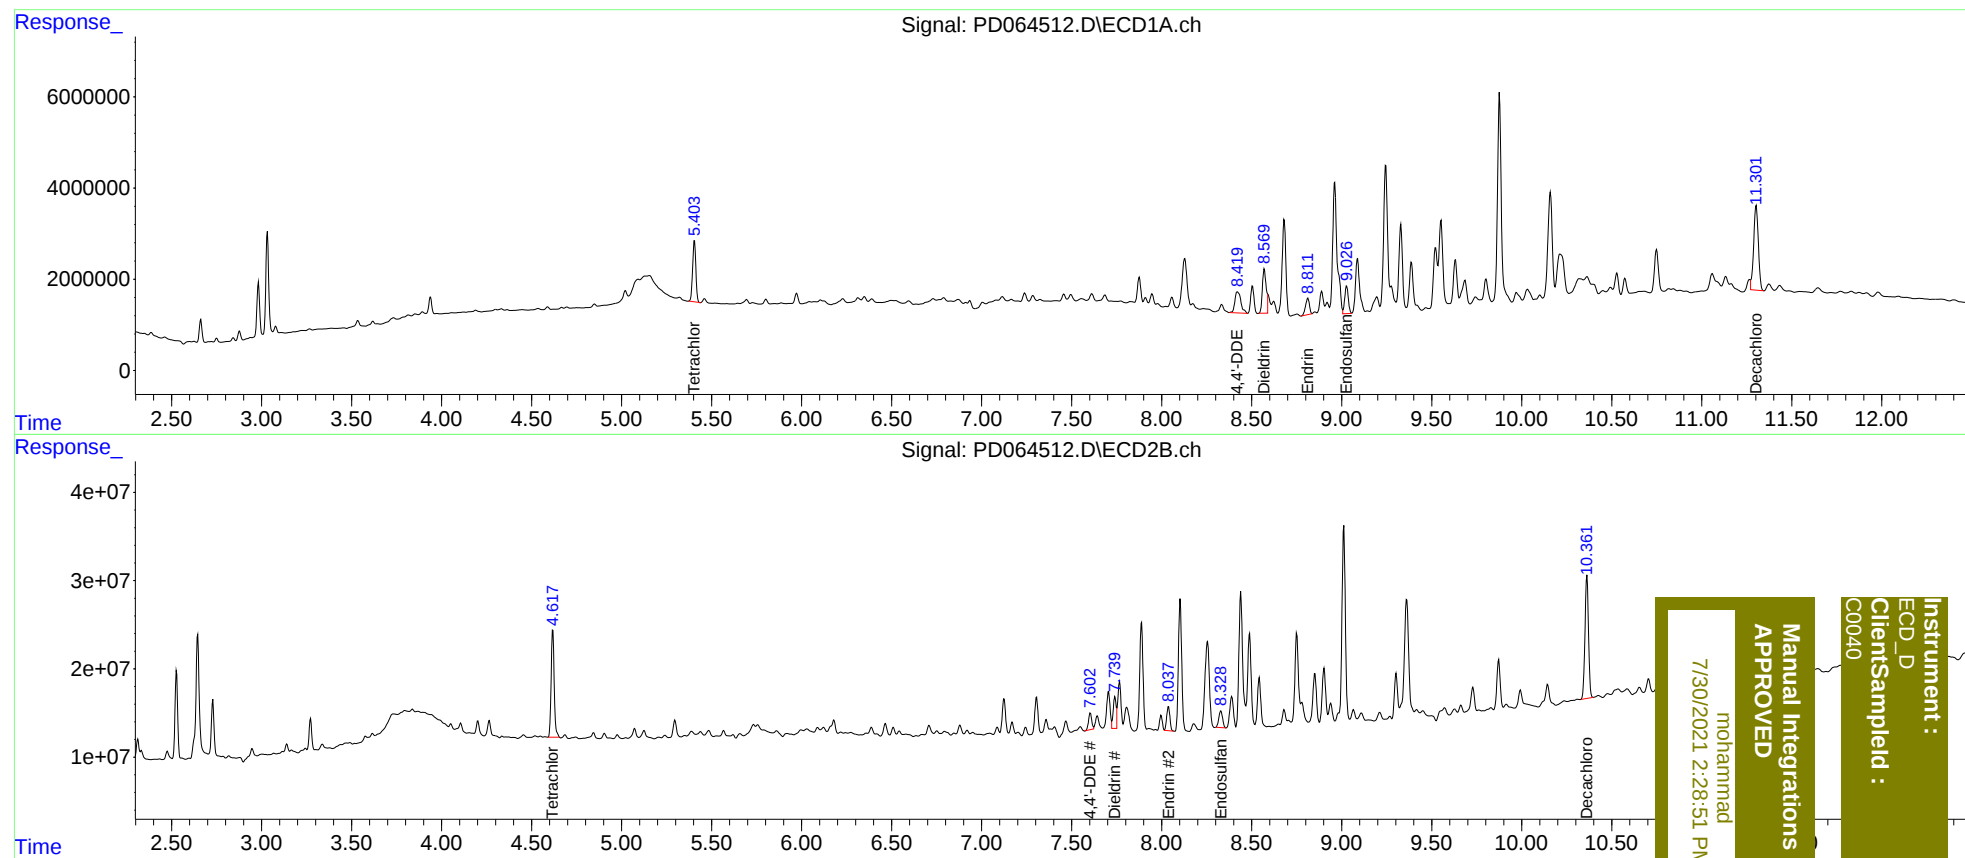

Manual Integrations
APPROVED

mohammad
7/30/2021 2:28:51 PM

Instrument :
ECD_D
ClientSampled :
C0040