

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072822\
 Data File : PD071209.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2022 13:08
 Operator : AR\AJ
 Sample : N3741-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 H0B13

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/28/2022
 Supervised By : Ankita Jodhani 07/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 28 00:09:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 14 05:14:58 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.472	4.125	43687015	478.8E6	18.156	20.400
2)	SA Decachlor...	8.239	9.320	65569417	246.2E6	25.827	26.658
Target Compounds							
10)	B trans-Chl...	5.415	6.281	1860558	24403353	0.535m	1.621 #
11)	B cis-Chlor...	5.475	6.356	3820969	48612459	1.118	3.366 #
12)	B 4,4'-DDE	5.639	6.511	2254878	14434816	0.701m	1.052 #
15)	B Endosulfa...	6.319	7.104	1392875	6068566	0.508m	0.527

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072822\
Data File : PD071209.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2022 13:08
Operator : AR\AJ
Sample : N3741-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 00:09:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 14 05:14:58 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

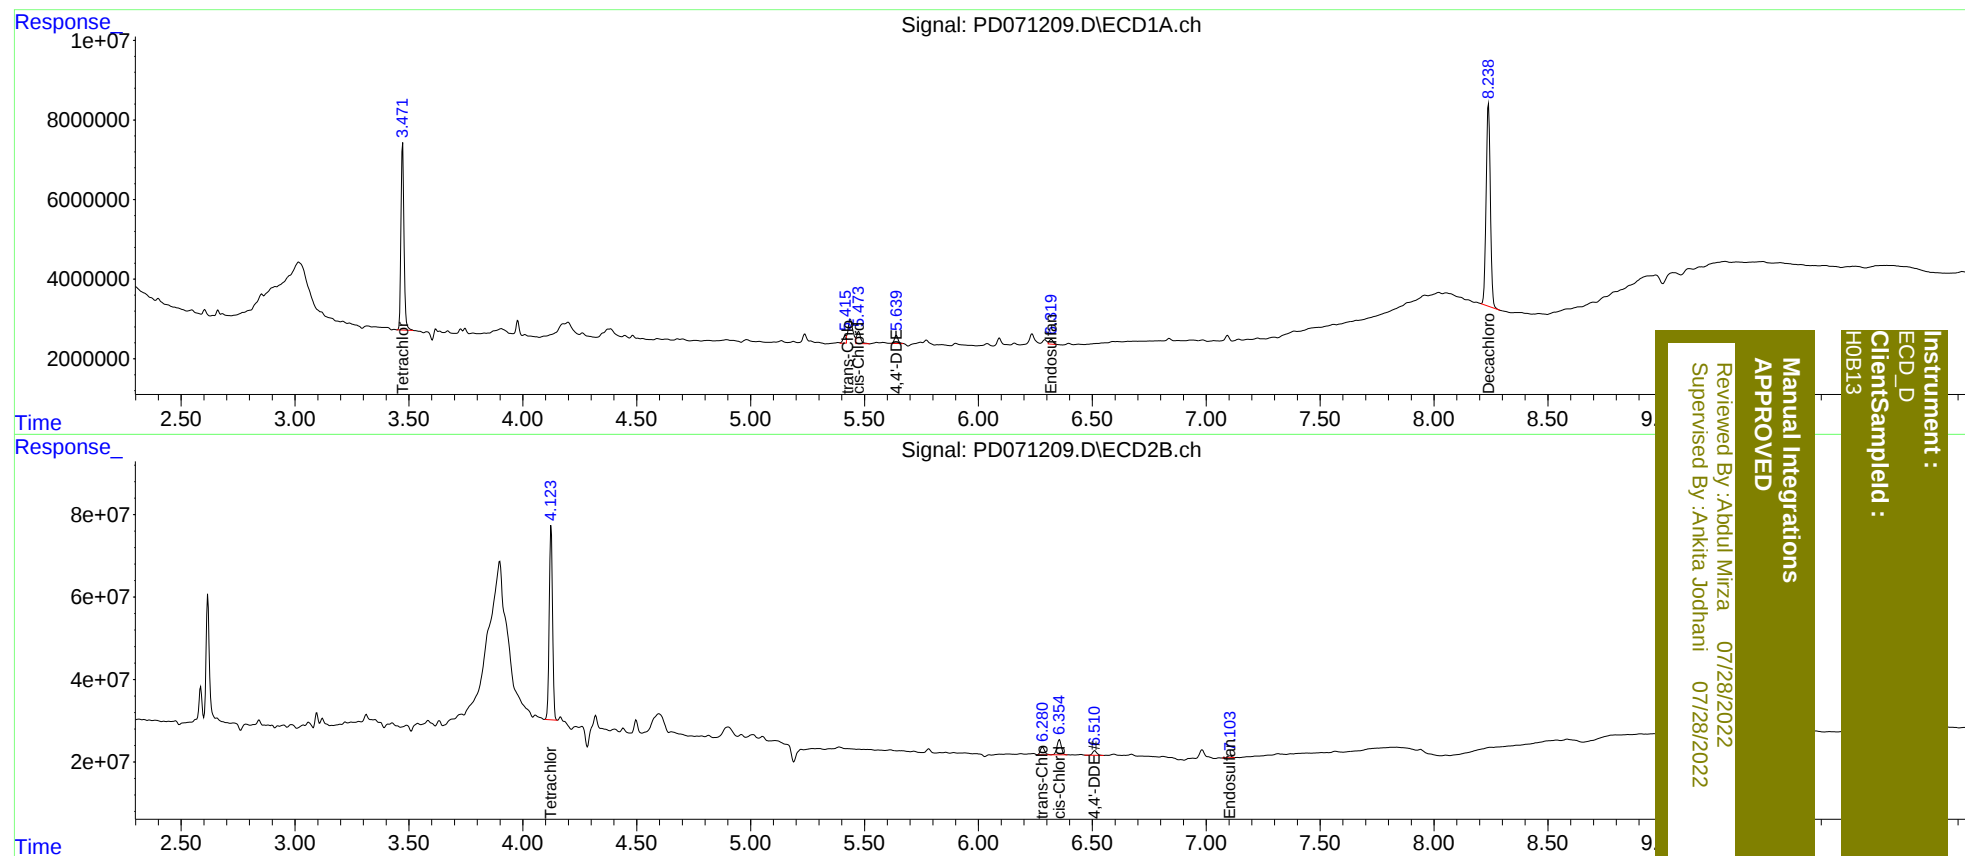

Reviewed By: Abdul Mirza 07/28/2022
Supervised By: Ankita Jodhani 07/28/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
HOB13